

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
 Data File : PP040941.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2021 1:59
 Operator : AJ\MA
 Sample : PB140661BL
 Misc :
 ALS Vial : 38 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 02:04:28 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.765	430370	573172	21.244	23.884
2) SA Decachlor...	10.664	9.030	425667	323832	19.987	18.544
Target Compounds						
8) L2 AR-1221-1	5.011f	0.000	26039	0	114.024	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
Data File : PP040941.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2021 1:59
Operator : AJ\MA
Sample : PB140661BL
Misc :
ALS Vial : 38 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 02:04:28 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

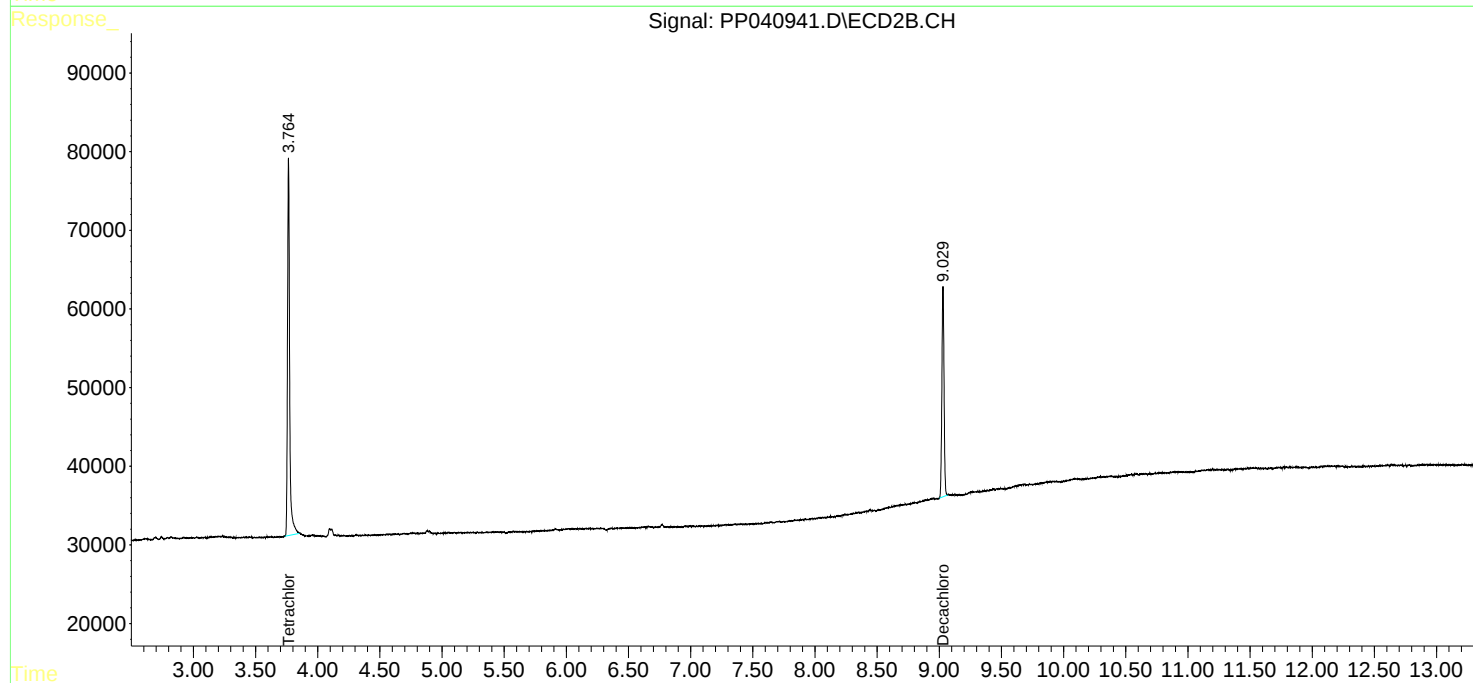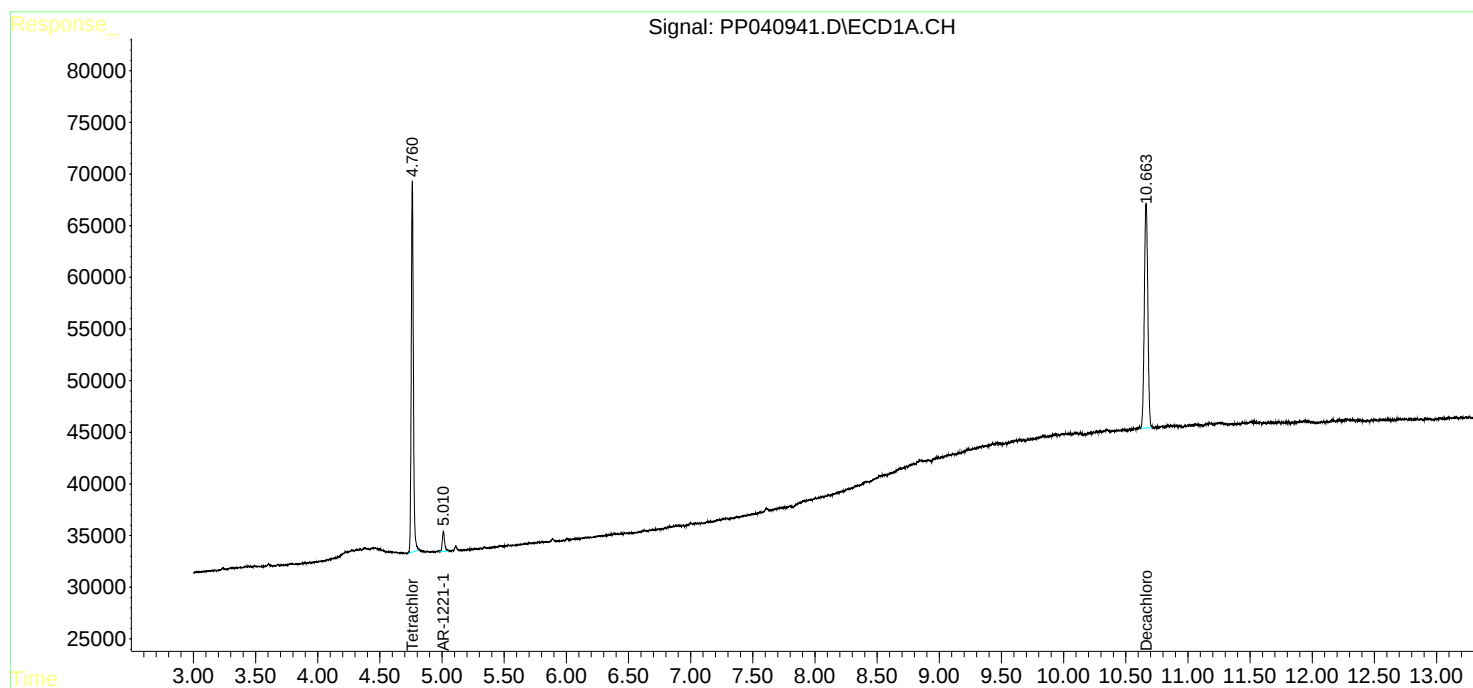


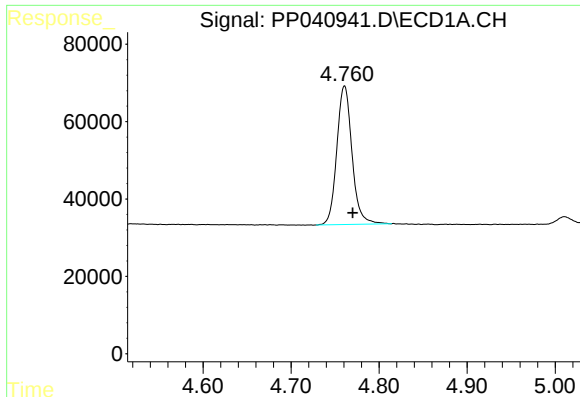

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 430370
Conc: 21.24 ng/ml

Instrument :
ECD_P
ClientSampleId :

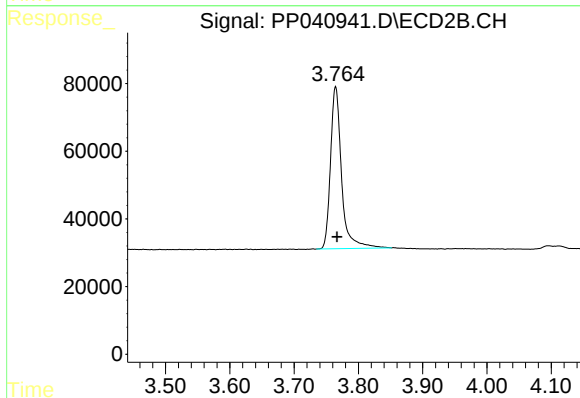


#1 Tetrachloro-m-xylene

R.T.: 3.765 min
Delta R.T.: -0.002 min
Response: 573172
Conc: 23.88 ng/ml

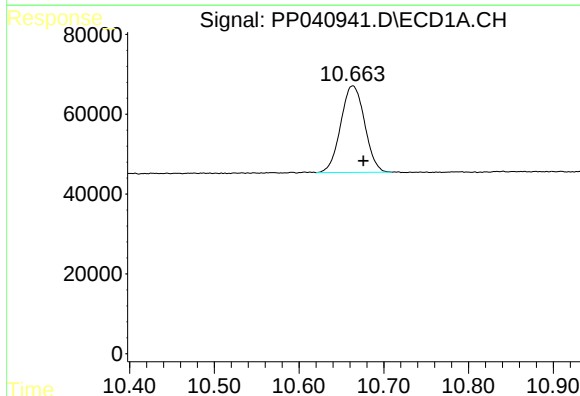


#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.012 min
Response: 425667
Conc: 19.99 ng/ml

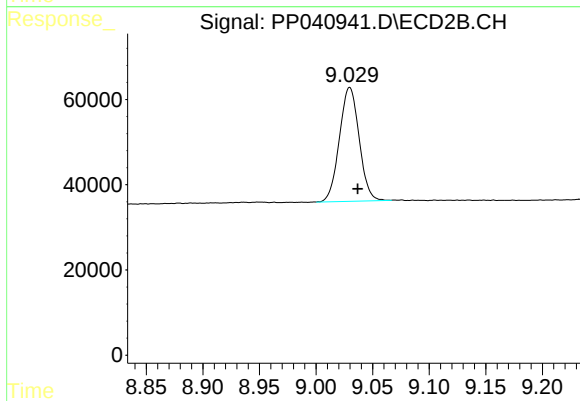

#2 Decachlorobiphenyl


R.T.: 9.030 min
Delta R.T.: -0.007 min
Response: 323832
Conc: 18.54 ng/ml

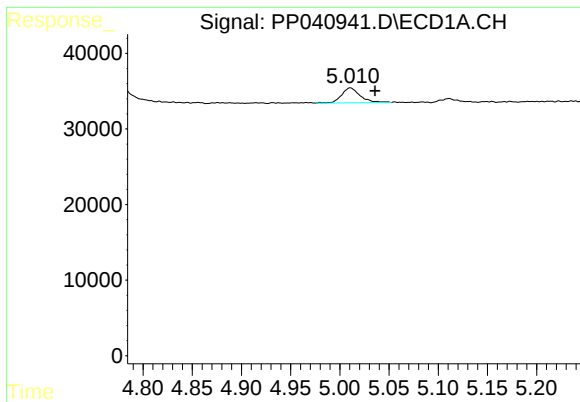

#8 AR-1221-1

R.T.: 5.011 min
Delta R.T.: -0.025 min
Response: 26039
Conc: 114.02 ng/ml

Instrument :
ECD_P
ClientSampleId :

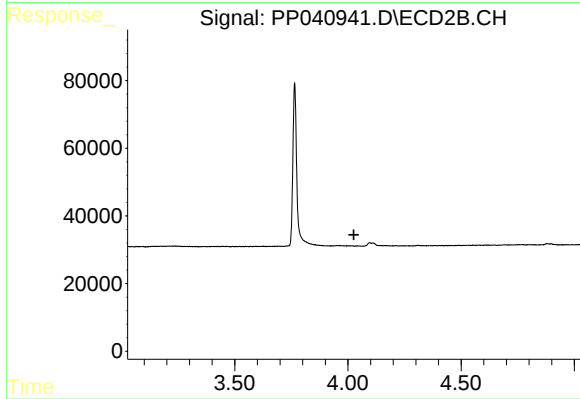

#8 AR-1221-1

R.T.: 0.000 min
Exp R.T. : 4.027 min
Response: 0
Conc: N.D.