

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
Data File : PP040913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 17:44
Operator : AJ\MA
Sample : M4590-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IRV-2021-8A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 01:04:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.764	39112	56586	1.931	2.358
2) SA Decachlor...	10.664	9.032	51439	38221	2.415	2.189

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111021\
Data File : PP040913.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 10 Nov 2021 17:44
Operator : AJ\MA
Sample : M4590-04 10X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
IRV-2021-8A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 01:04:50 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

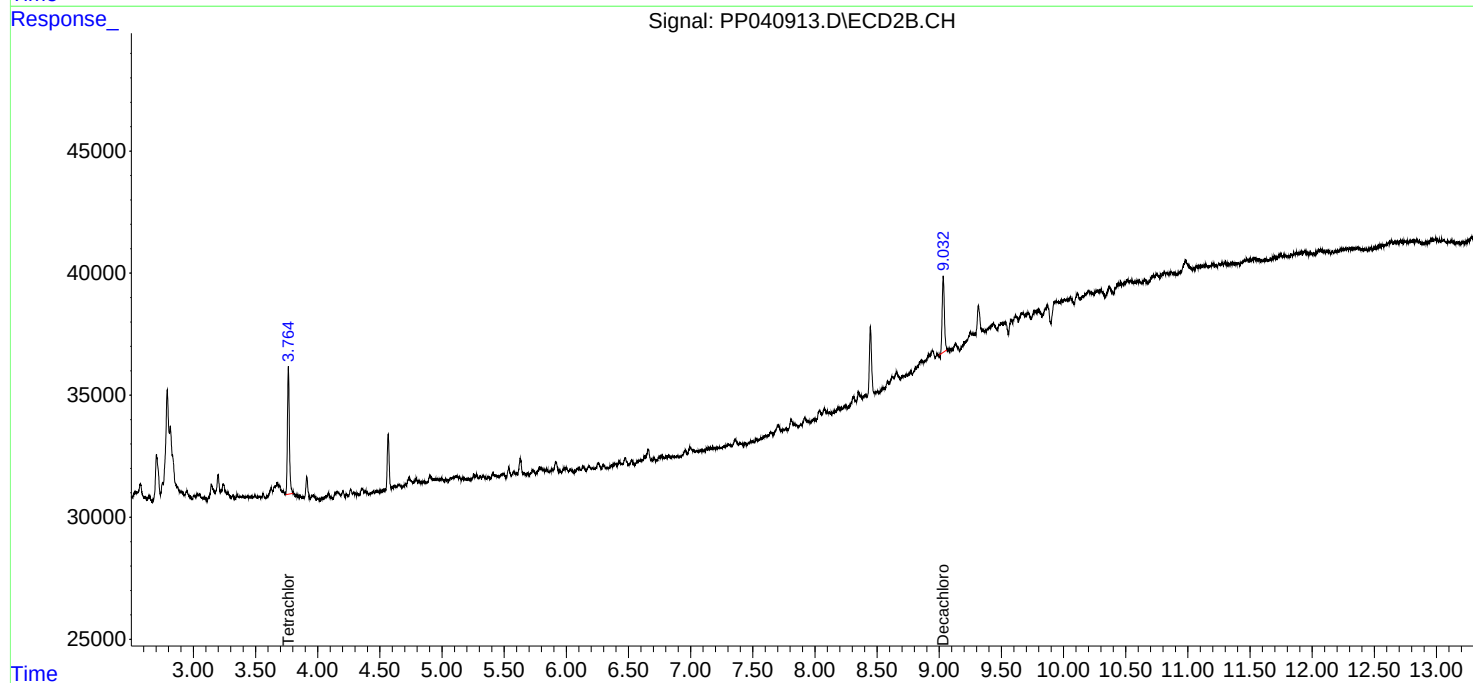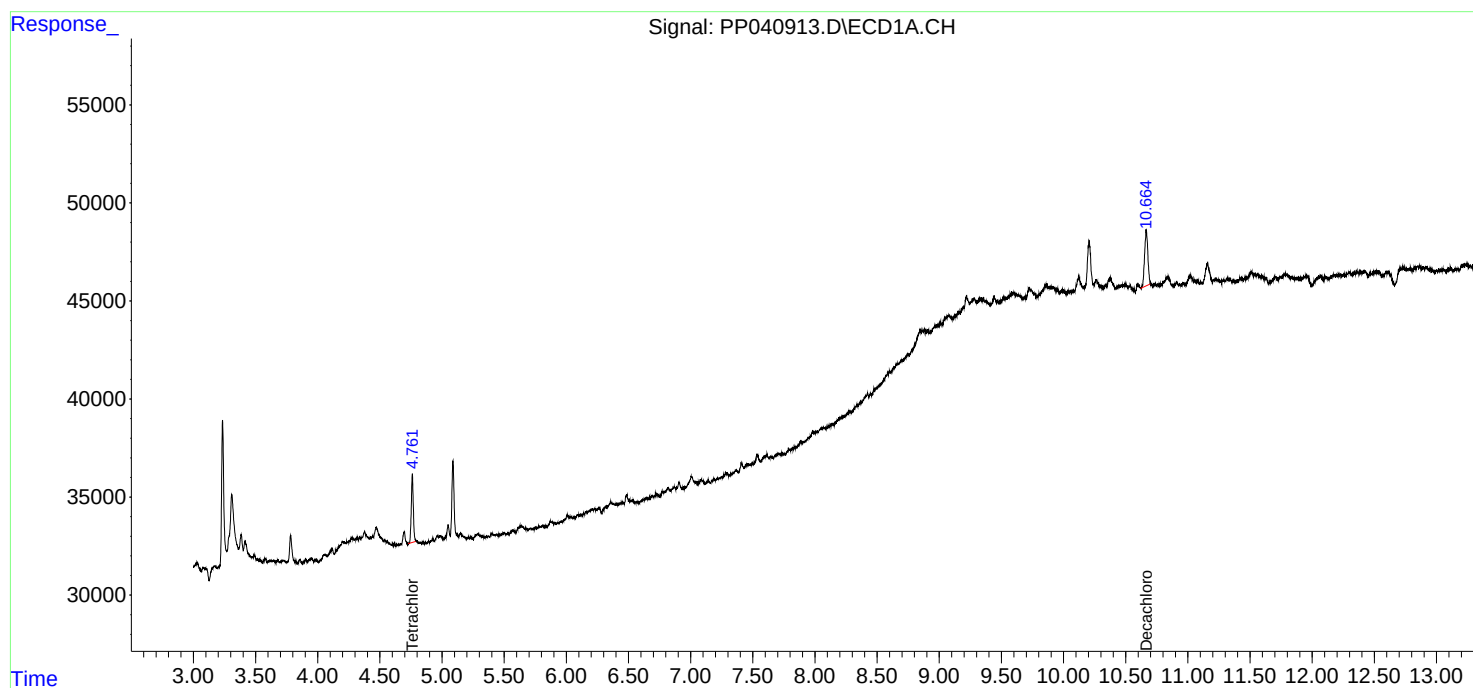


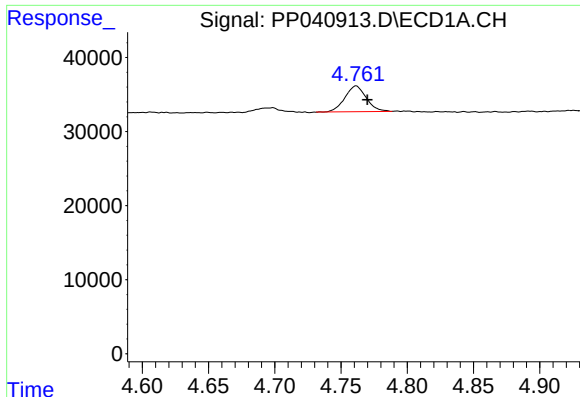

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 39112
Conc: 1.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
IRV-2021-8A

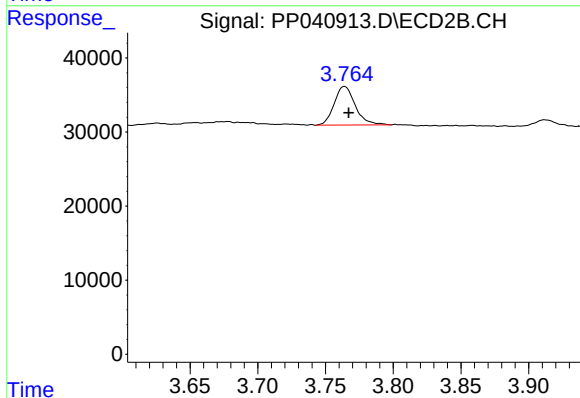


#1 Tetrachloro-m-xylene

R.T.: 3.764 min
Delta R.T.: -0.003 min
Response: 56586
Conc: 2.36 ng/ml

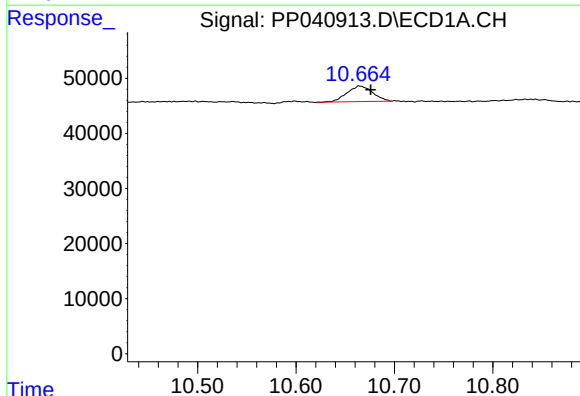

#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.012 min
Response: 51439
Conc: 2.42 ng/ml

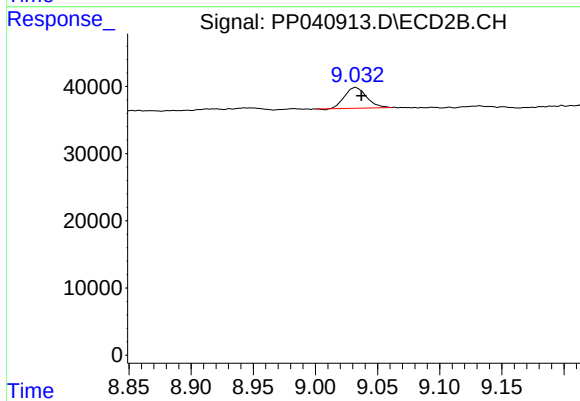

#2 Decachlorobiphenyl

R.T.: 9.032 min
Delta R.T.: -0.005 min
Response: 38221
Conc: 2.19 ng/ml