

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111022\
 Data File : PP053266.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2022 23:27
 Operator : YP\AJ
 Sample : N5553-04
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TOTE-COMP

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/11/2022
 Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 03:51:09 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.413	3.636	590.6E6	720.6E6	307.221m	479.068m#
2) SA Decachlor...	10.202	8.727	21311733	22835687	15.717	12.183

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111022\
Data File : PP053266.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2022 23:27
Operator : YP\AJ
Sample : N5553-04
Misc :
ALS Vial : 35 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 03:51:09 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

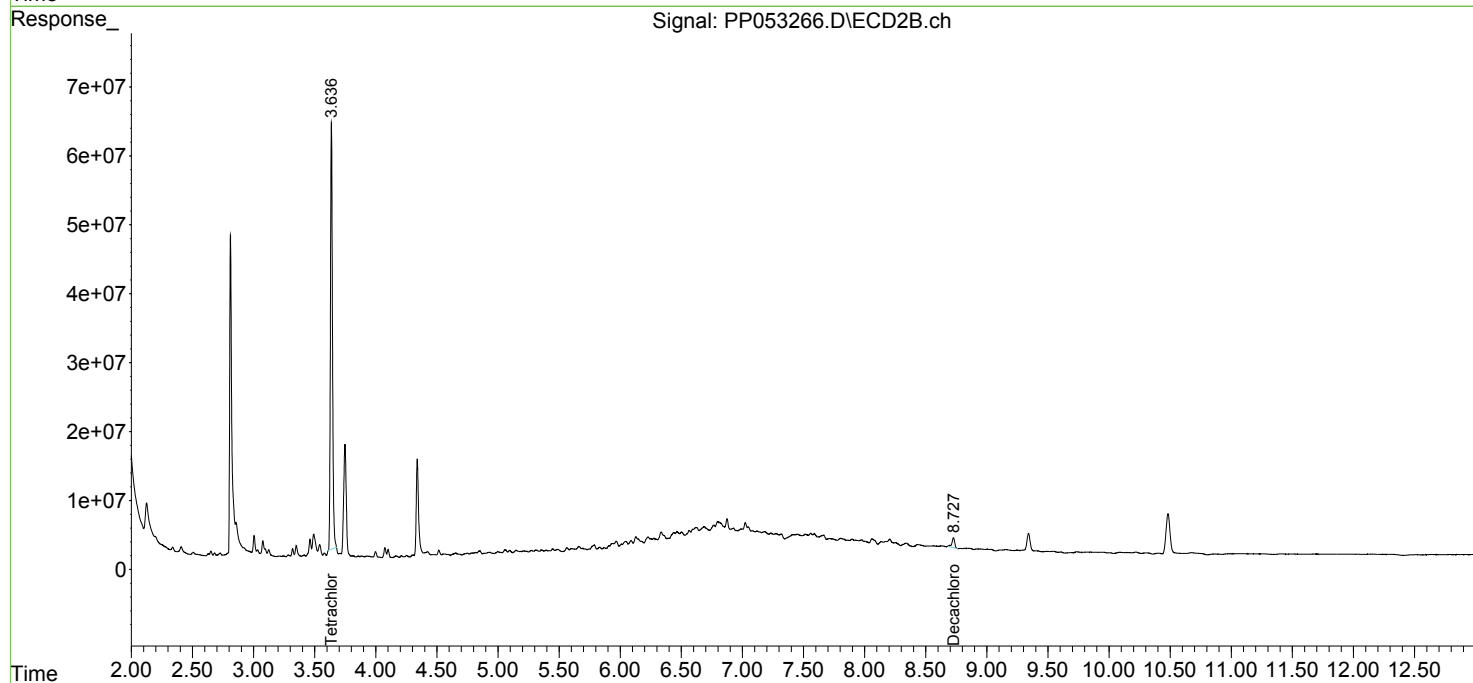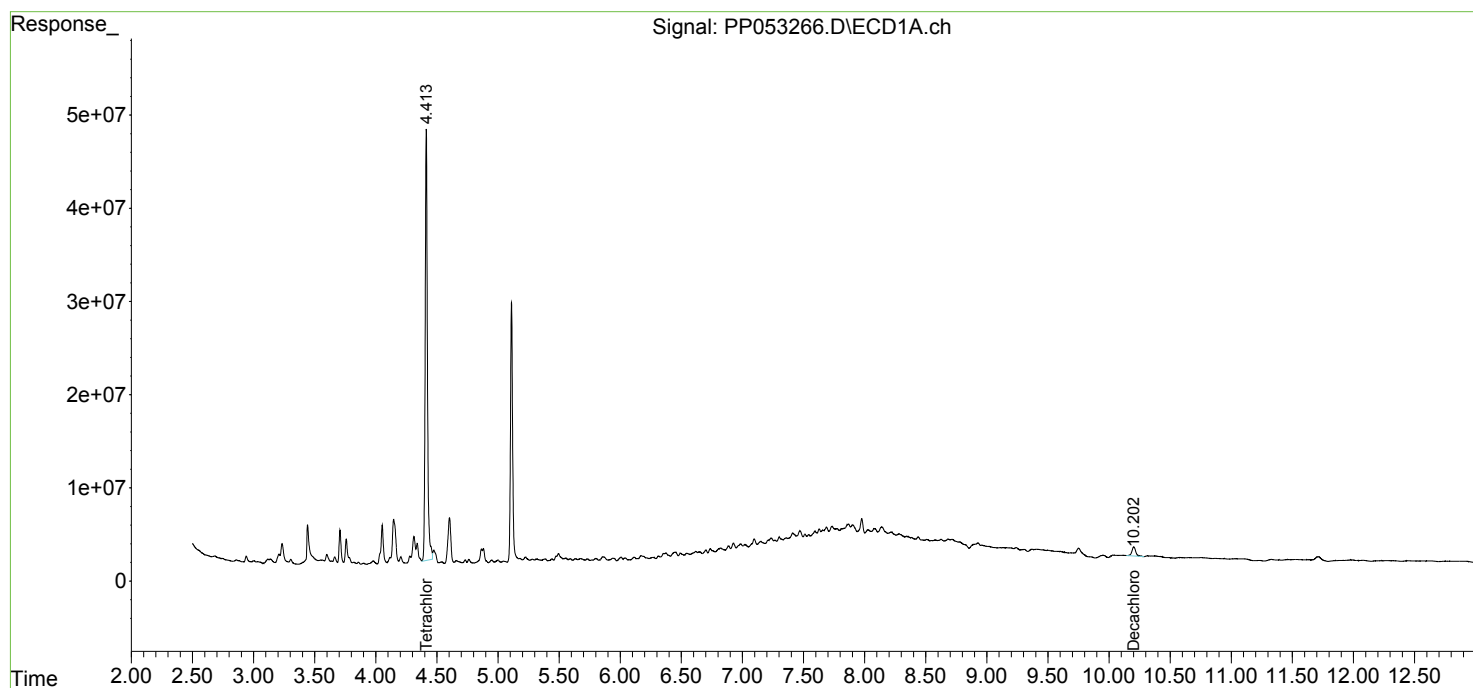

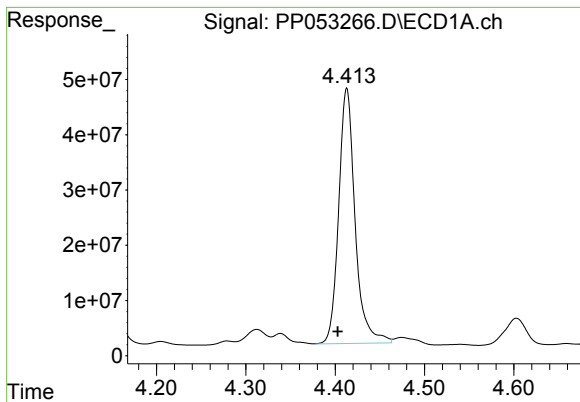


#1 Tetrachloro-m-xylene

R.T.: 4.413 min
Delta R.T.: 0.010 min
Response: 590582958
Conc: 307.22 ng/ml

Instrument :
ECD_P
ClientSampleId :
TOTE-COMP


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/11/2022
Supervised By :Ankita Jodhani 11/11/2022

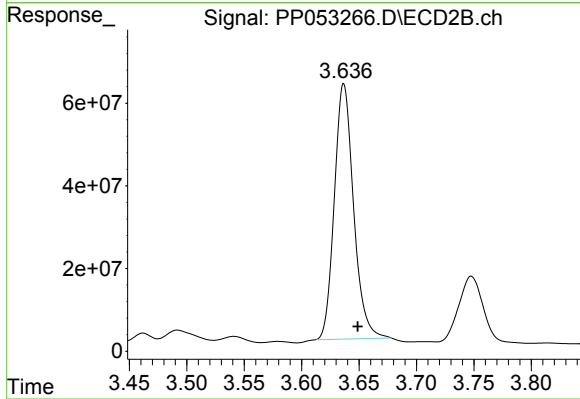


#1 Tetrachloro-m-xylene

R.T.: 3.636 min
Delta R.T.: -0.013 min
Response: 720637950
Conc: 479.07 ng/ml m

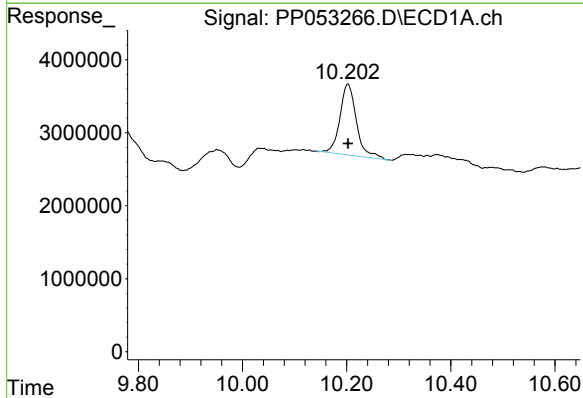

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: 0.000 min
Response: 21311733
Conc: 15.72 ng/ml

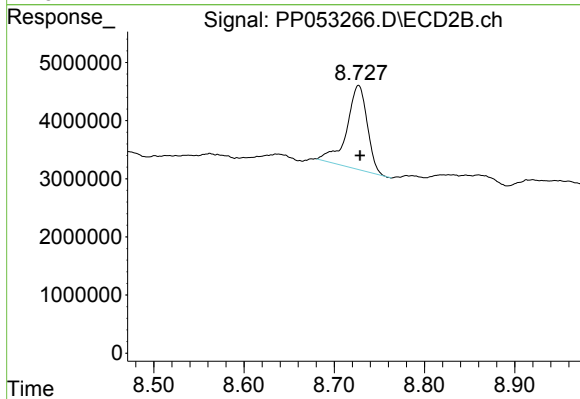

#2 Decachlorobiphenyl

R.T.: 8.727 min
Delta R.T.: -0.002 min
Response: 22835687
Conc: 12.18 ng/ml