

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111025\
 Data File : PP076403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Nov 2025 13:27
 Operator : YP\AJ
 Sample : Q3563-01 10X
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 81525-a

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/11/2025
 Supervised By :Yogesh Patel 11/11/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 10 15:46:54 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.640	3.784	2522243	8812753	1.765m	1.332
2) SA Decachlor...	10.417	8.777	1718044	9399224	1.596	1.143 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111025\
Data File : PP076403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Nov 2025 13:27
Operator : YP\AJ
Sample : Q3563-01 10X
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
81525-a


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/11/2025
Supervised By :Yogesh Patel 11/11/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 10 15:46:54 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

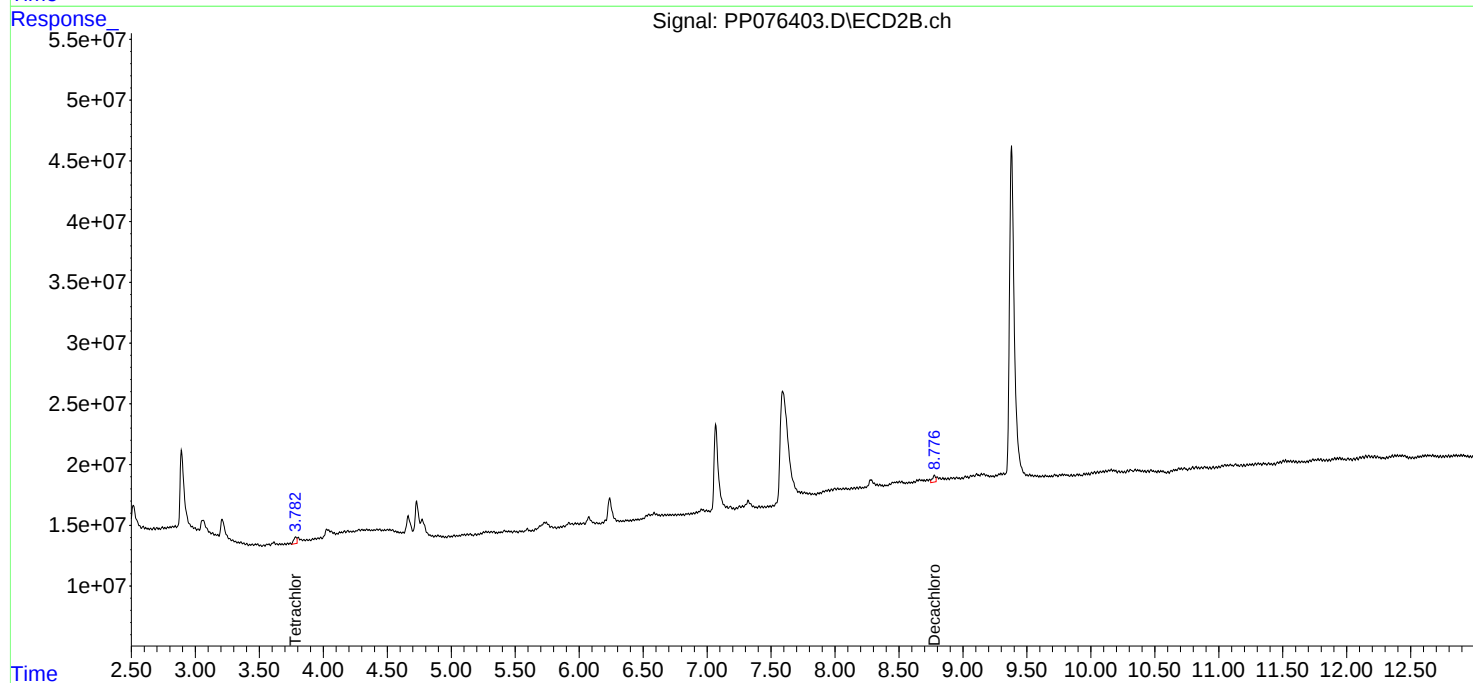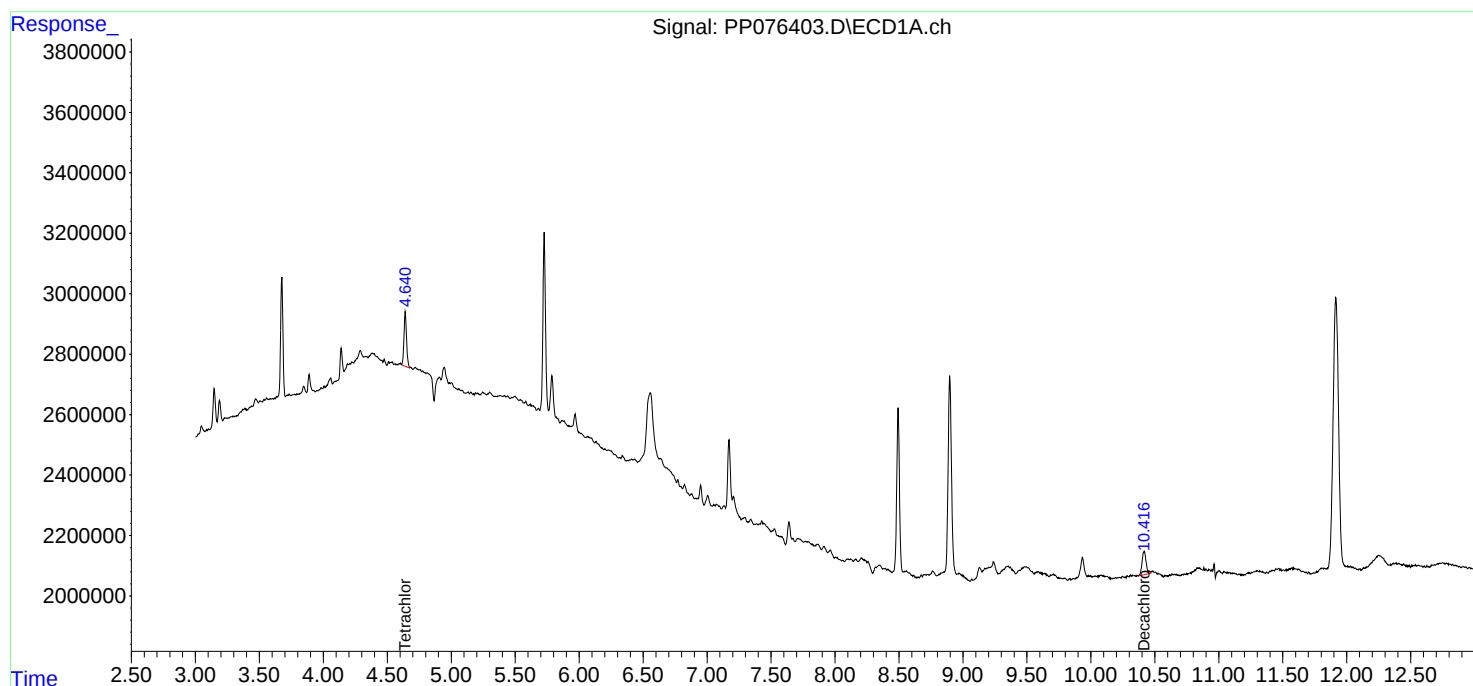

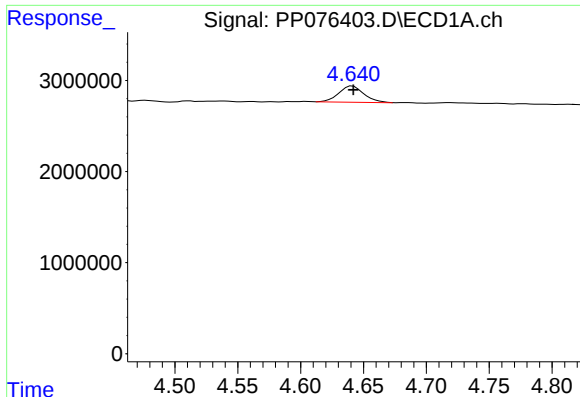


#1 Tetrachloro-m-xylene

R.T.: 4.640 min
Delta R.T.: -0.002 min
Response: 2522243
Conc: 1.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
81525-a


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/11/2025
Supervised By :Yogesh Patel 11/11/2025

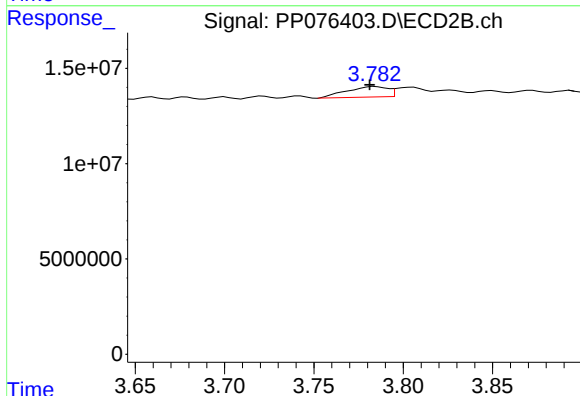


#1 Tetrachloro-m-xylene

R.T.: 3.784 min
Delta R.T.: 0.003 min
Response: 8812753
Conc: 1.33 ng/ml

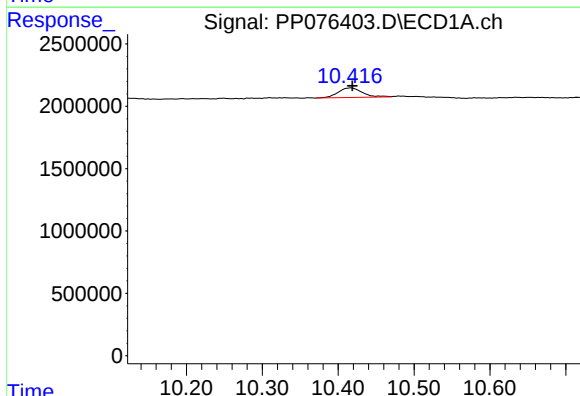

#2 Decachlorobiphenyl

R.T.: 10.417 min
Delta R.T.: -0.002 min
Response: 1718044
Conc: 1.60 ng/ml

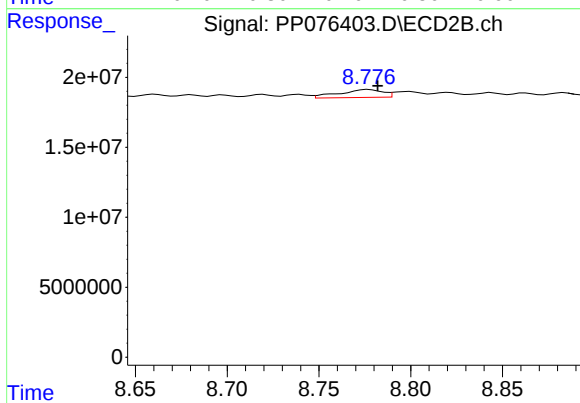

#2 Decachlorobiphenyl

R.T.: 8.777 min
Delta R.T.: -0.005 min
Response: 9399224
Conc: 1.14 ng/ml