

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111120\
 Data File : PP031225.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2020 12:59
 Operator : DD\AJ
 Sample : PB132938BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 16:03:31 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.799	4.072	1077208	987950	16.128	14.863
2)	SA Decachlor...	10.686	9.392	729984	776228	18.257	18.590
Target Compounds							
9)	L2 AR-1221-2	0.000	4.425	0	14082	N.D.	32.890 #
35)	L7 AR-1260-5	0.000	7.994f	0	1620	N.D.	0.360 #
36)	L8 AR-1262-1	0.000	7.518	0	17638	N.D.	7.593 #
37)	L8 AR-1262-2	0.000	7.994f	0	1620	N.D.	0.391 #
42)	L9 AR-1268-2	0.000	8.395f	0	1969	N.D.	0.414 #
43)	L9 AR-1268-3	0.000	8.601f	0	1510	N.D.	0.377 #
45)	L9 AR-1268-5	0.000	9.144	0	1585	N.D.	0.118 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111120\
Data File : PP031225.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2020 12:59
Operator : DD\AJ
Sample : PB132938BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 16:03:31 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

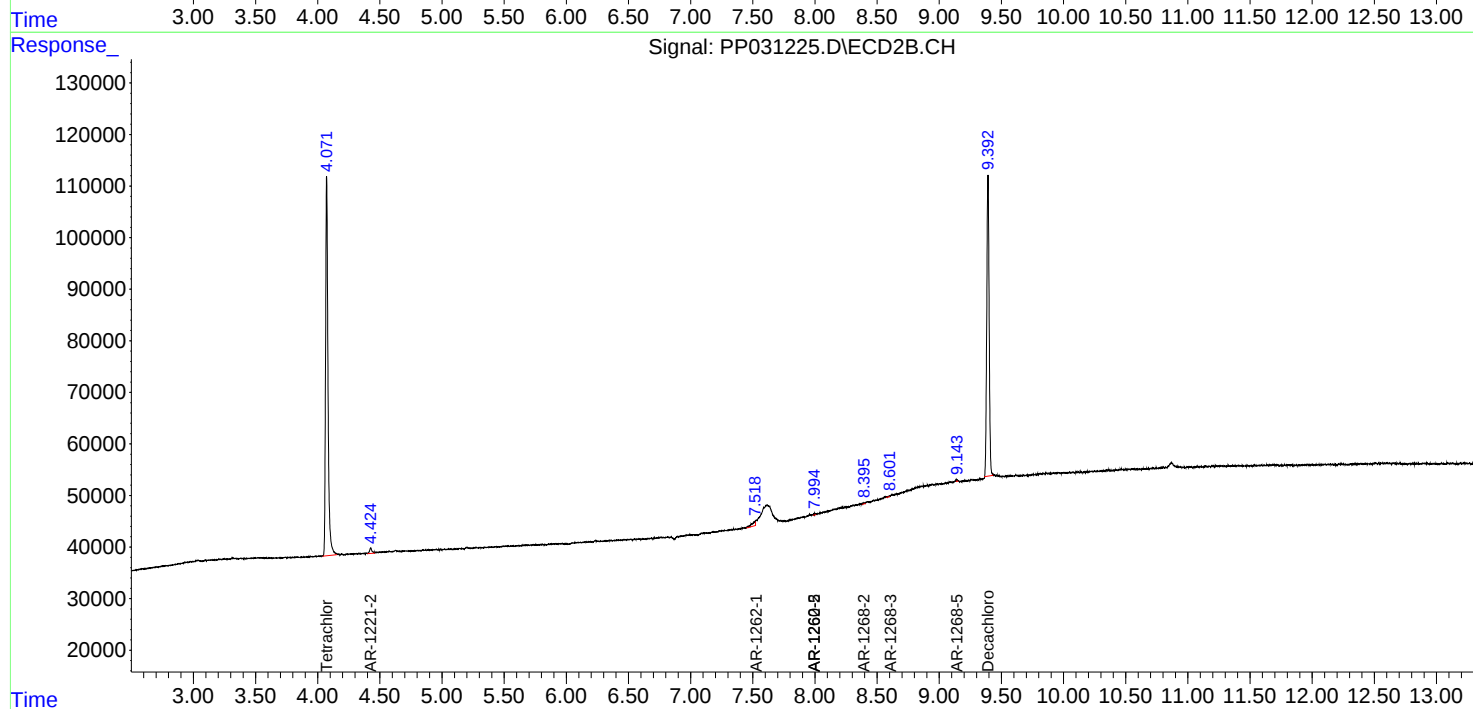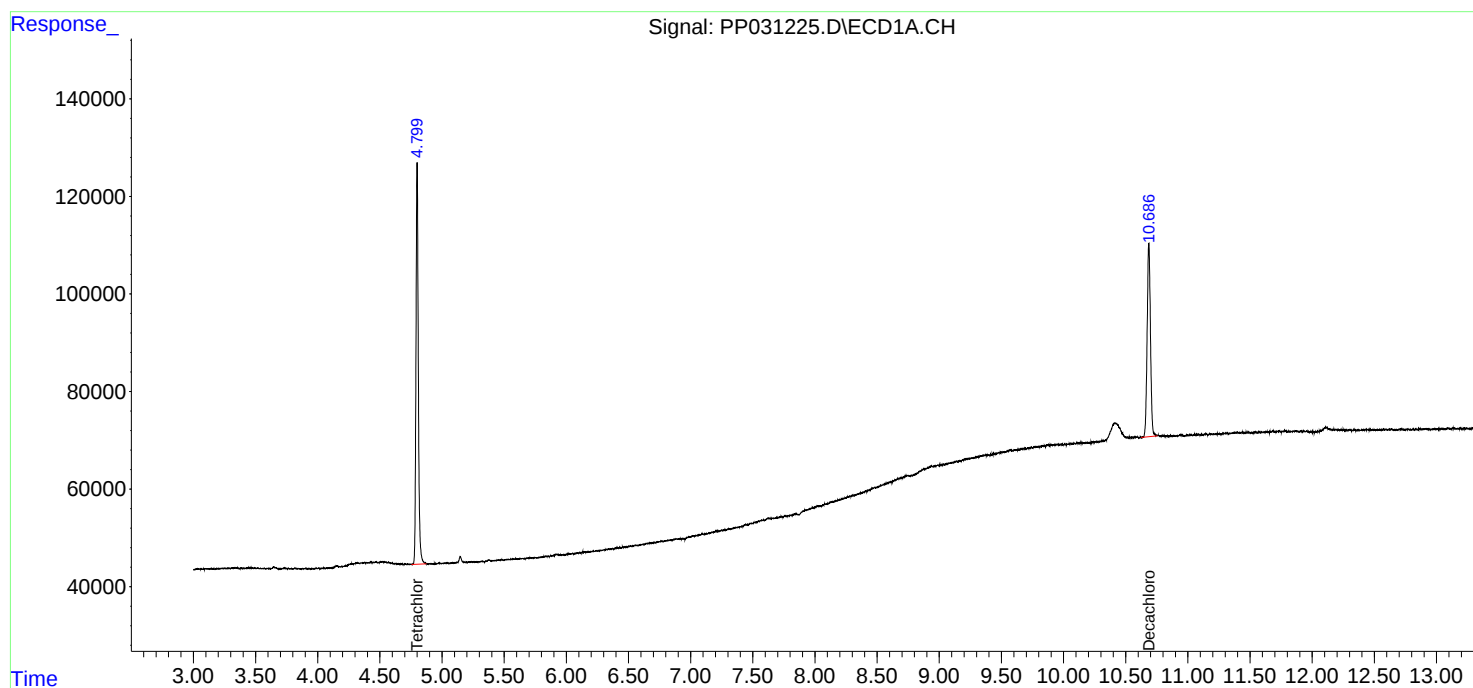


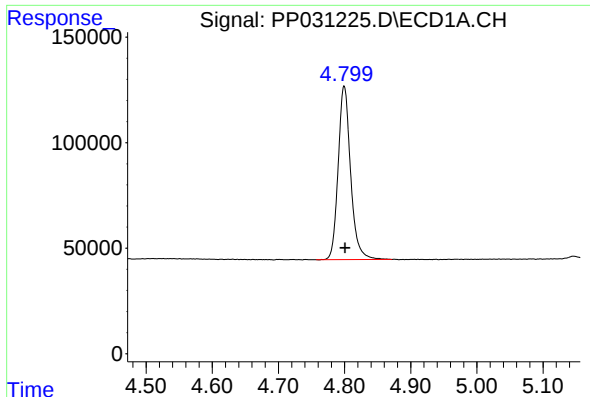

#1 Tetrachloro-m-xylene


R.T.: 4.799 min
Delta R.T.: -0.002 min
Response: 1077208
Conc: 16.13 ng/ml

Instrument :
ECD_P
ClientSampleId :

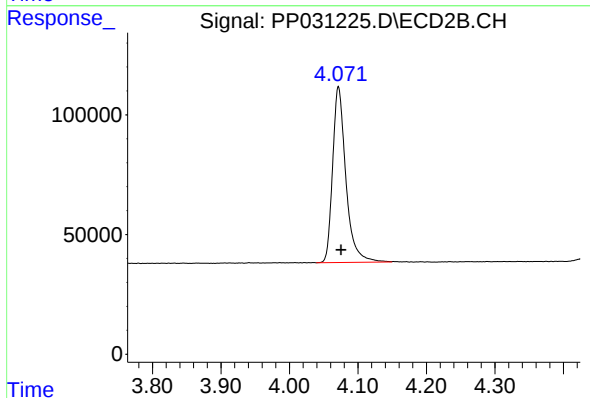


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: -0.004 min
Response: 987950
Conc: 14.86 ng/ml

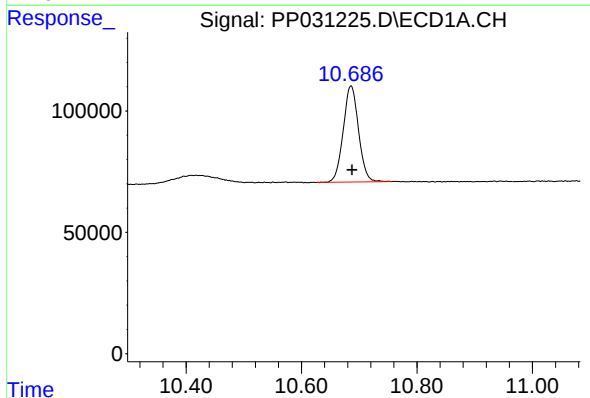


#2 Decachlorobiphenyl

R.T.: 10.686 min
Delta R.T.: -0.002 min
Response: 729984
Conc: 18.26 ng/ml

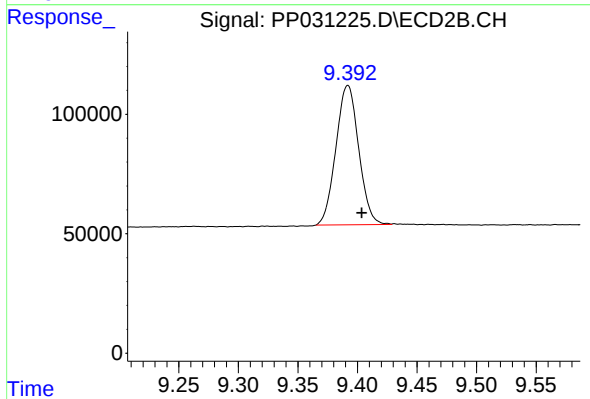

#2 Decachlorobiphenyl


R.T.: 9.392 min
Delta R.T.: -0.012 min
Response: 776228
Conc: 18.59 ng/ml

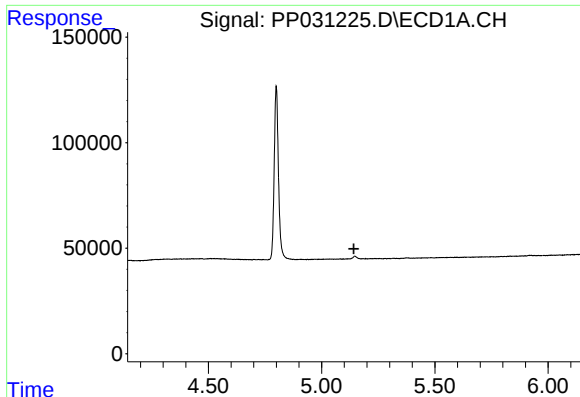

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

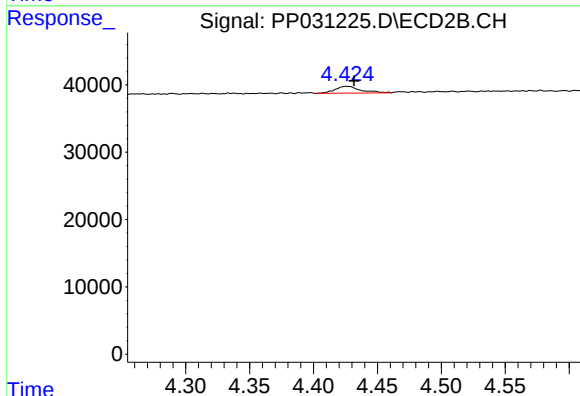


#9 AR-1221-2

R.T.: 4.425 min
Delta R.T.: -0.007 min
Response: 14082
Conc: 32.89 ng/ml

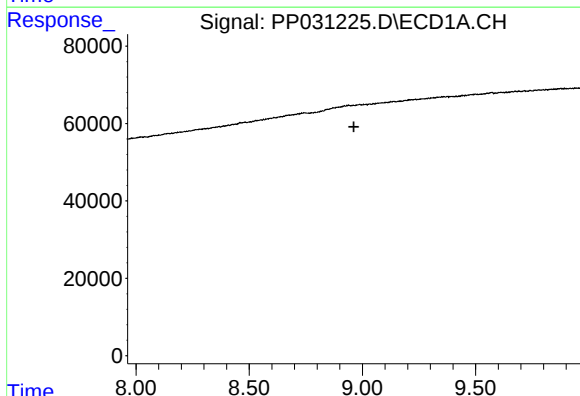


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.962 min
Response: 0
Conc: N.D.

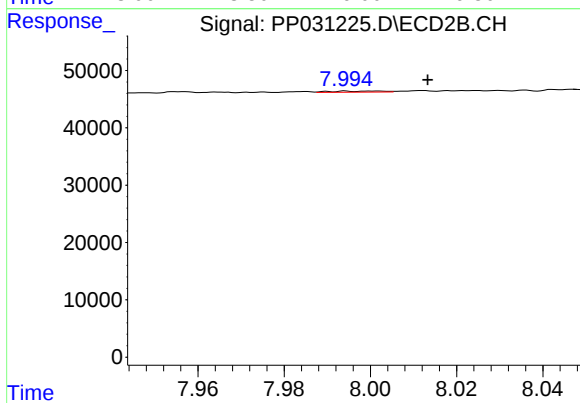

#35 AR-1260-5


R.T.: 7.994 min
Delta R.T.: -0.019 min
Response: 1620
Conc: 0.36 ng/ml

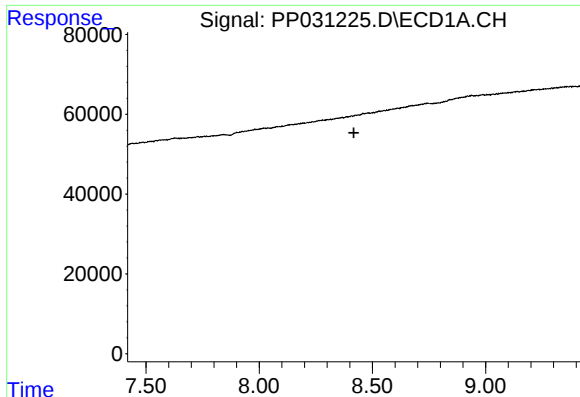

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.419 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

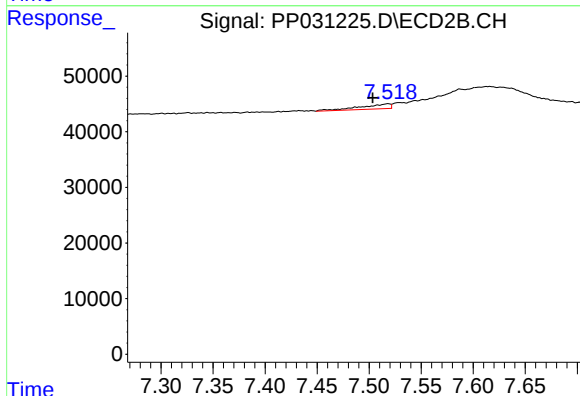


#36 AR-1262-1

R.T.: 7.518 min
Delta R.T.: 0.015 min
Response: 17638
Conc: 7.59 ng/ml

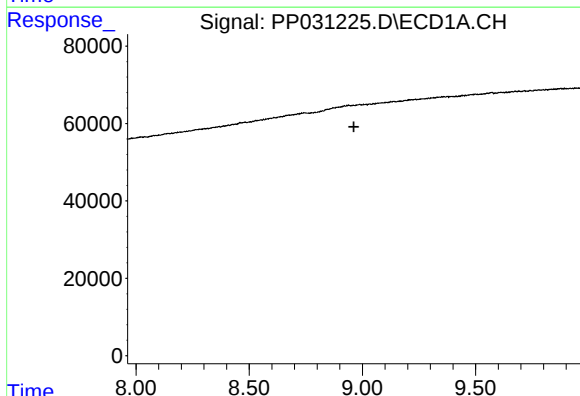


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.963 min
Response: 0
Conc: N.D.

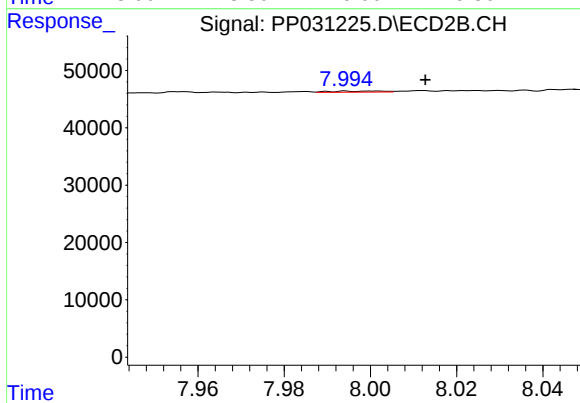

#37 AR-1262-2


R.T.: 7.994 min
Delta R.T.: -0.018 min
Response: 1620
Conc: 0.39 ng/ml

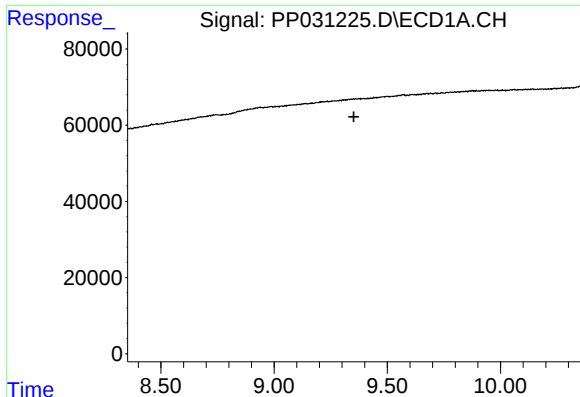

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.352 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

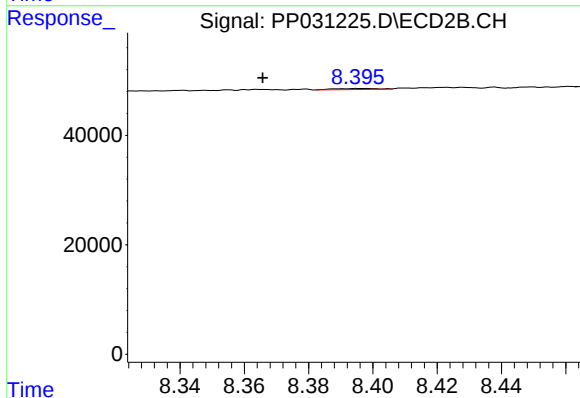


#42 AR-1268-2

R.T.: 8.395 min
Delta R.T.: 0.030 min
Response: 1969
Conc: 0.41 ng/ml

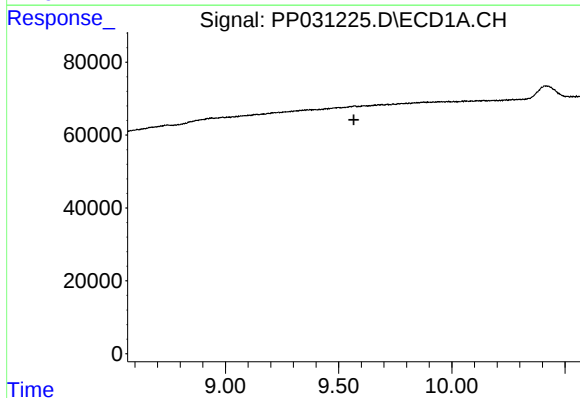


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.568 min
Response: 0
Conc: N.D.

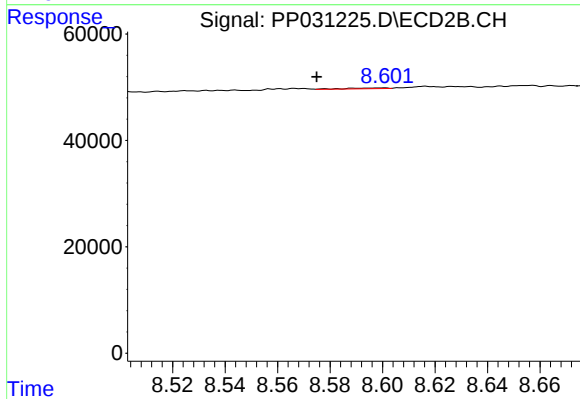

#43 AR-1268-3


R.T.: 8.601 min
Delta R.T.: 0.026 min
Response: 1510
Conc: 0.38 ng/ml

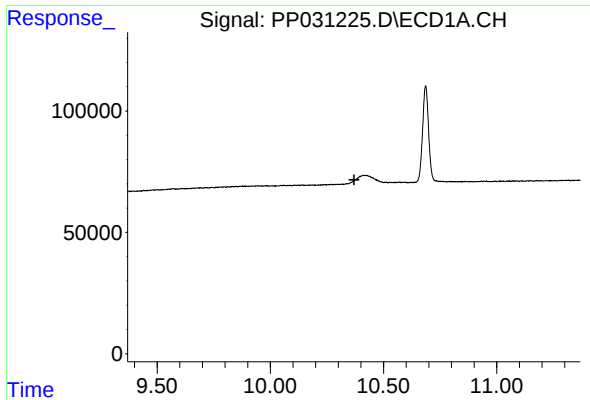

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

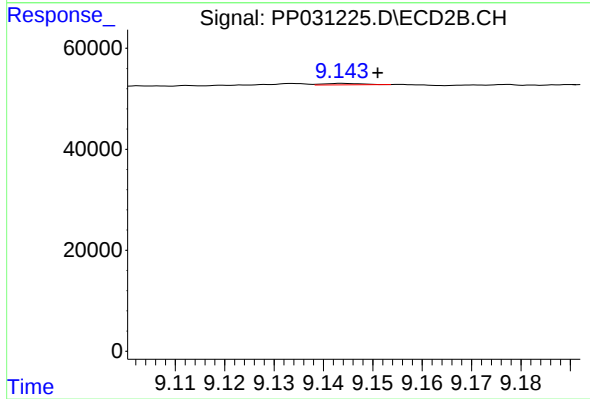

#45 AR-1268-5

R.T.: 9.144 min
Delta R.T.: -0.007 min
Response: 1585
Conc: 0.12 ng/ml