

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP111120\  
 Data File : PP031231.D  
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
 Acq On : 11 Nov 2020 14:39  
 Operator : DD\AJ  
 Sample : L4697-03  
 Misc :  
 ALS Vial : 10 Sample Multiplier: 1

Instrument :  
 ECD\_P  
 ClientSampleId :  
 TP-2-S

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Nov 11 16:06:12 2020  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP110420.M  
 Quant Title : GC EXTRACTABLES  
 QLast Update : Thu Nov 05 13:03:18 2020  
 Response via : Initial Calibration  
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

| Compound                    | RT#1   | RT#2  | Resp#1  | Resp#2  | ng/ml  | ng/ml  |
|-----------------------------|--------|-------|---------|---------|--------|--------|
| -----                       |        |       |         |         |        |        |
| System Monitoring Compounds |        |       |         |         |        |        |
| 1) SA Tetrachlo...          | 4.798  | 4.072 | 1465686 | 1386520 | 21.944 | 20.860 |
| 2) SA Decachlor...          | 10.682 | 9.392 | 856156  | 908844  | 21.413 | 21.766 |

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_P\Data\PP111120\  
Data File : PP031231.D  
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH  
Acq On : 11 Nov 2020 14:39  
Operator : DD\AJ  
Sample : L4697-03  
Misc :  
ALS Vial : 10 Sample Multiplier: 1

Instrument :  
ECD\_P  
ClientSampleId :  
TP-2-S

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Nov 11 16:06:12 2020  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_P\methods\PP110420.M  
Quant Title : GC EXTRACTABLES  
QLast Update : Thu Nov 05 13:03:18 2020  
Response via : Initial Calibration  
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

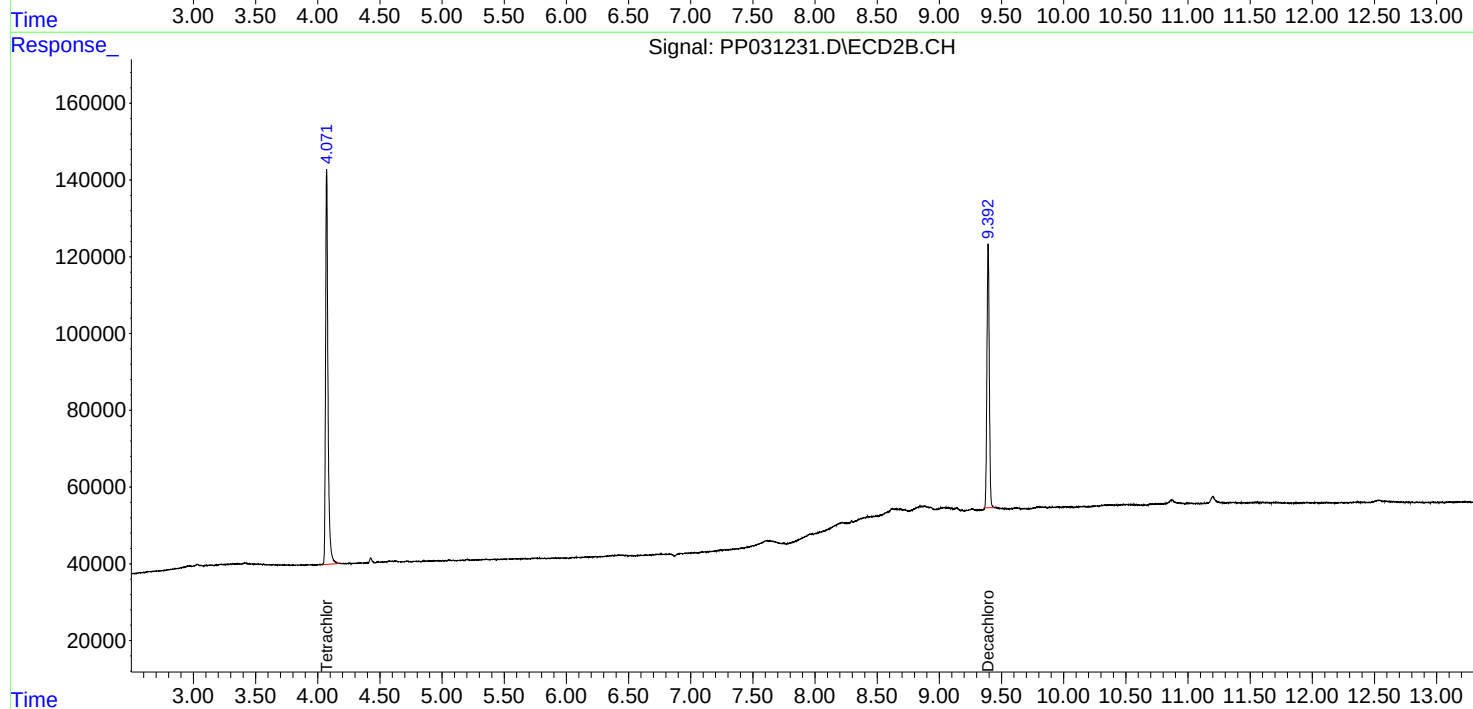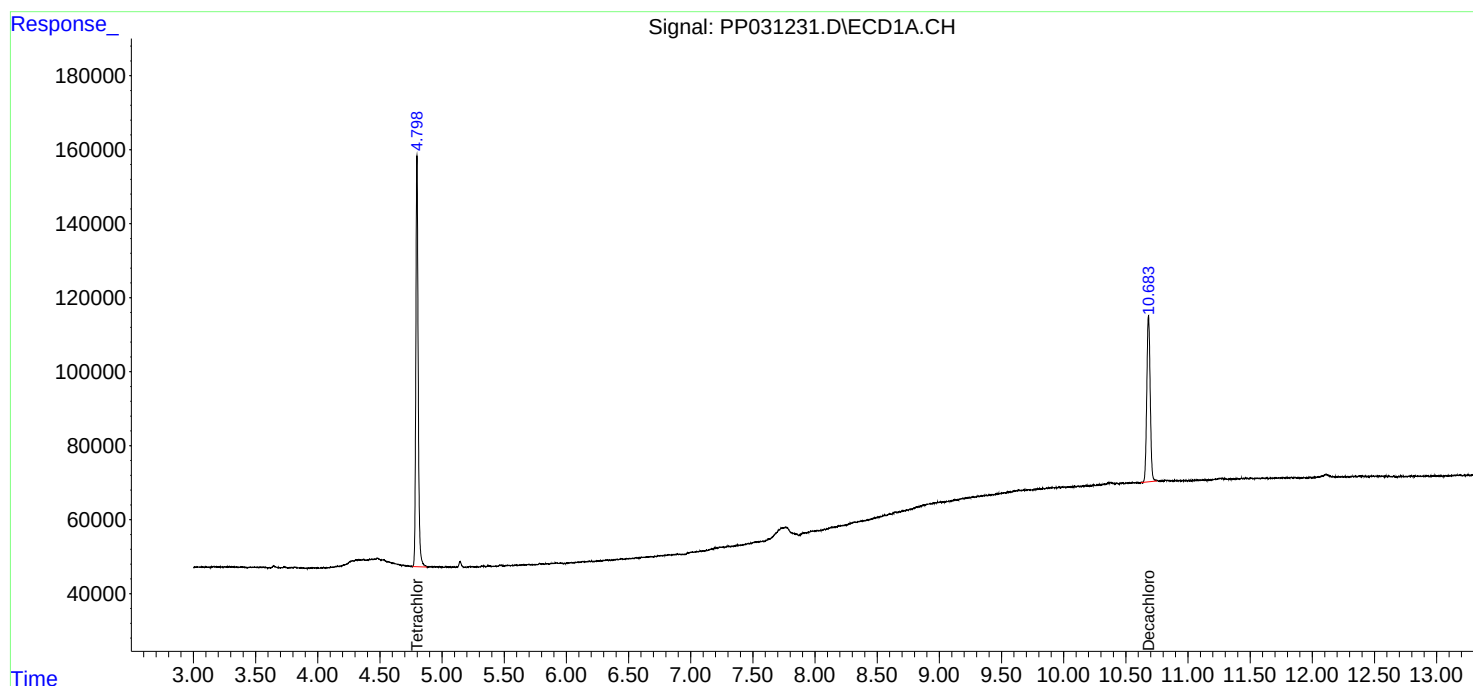


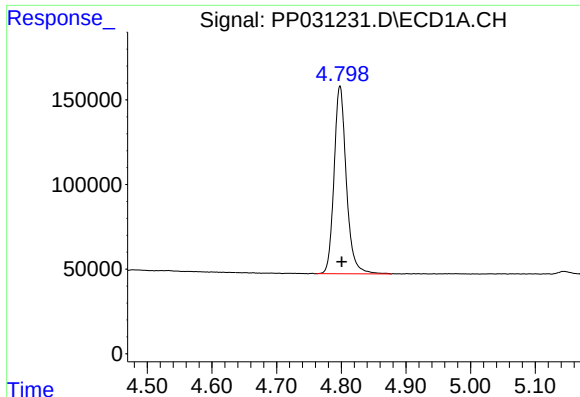

#1 Tetrachloro-m-xylene


R.T.: 4.798 min  
Delta R.T.: -0.003 min  
Response: 1465686  
Conc: 21.94 ng/ml

Instrument :  
ECD\_P  
ClientSampleId :  
TP-2-S

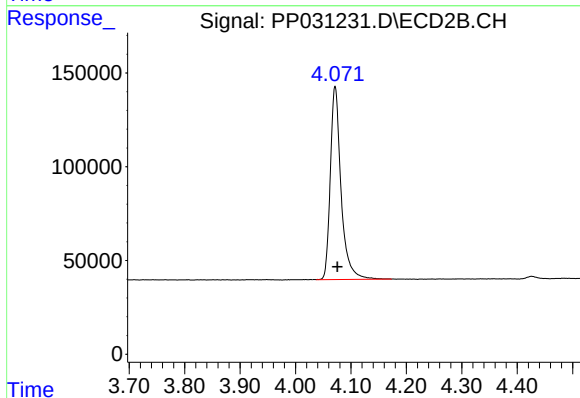


#1 Tetrachloro-m-xylene

R.T.: 4.072 min  
Delta R.T.: -0.004 min  
Response: 1386520  
Conc: 20.86 ng/ml

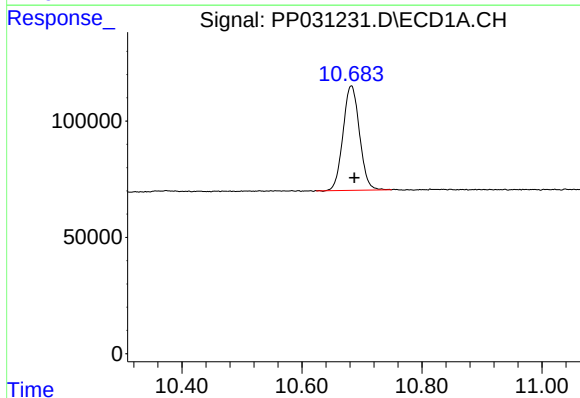

#2 Decachlorobiphenyl

R.T.: 10.682 min  
Delta R.T.: -0.005 min  
Response: 856156  
Conc: 21.41 ng/ml

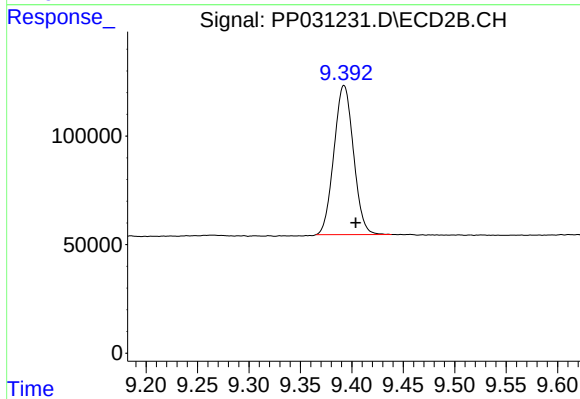

#2 Decachlorobiphenyl

R.T.: 9.392 min  
Delta R.T.: -0.011 min  
Response: 908844  
Conc: 21.77 ng/ml