

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
 Data File : PP040979.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2021 14:03
 Operator : AJ\MA
 Sample : M4607-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 15:32:36 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	3.765	425072	580801	20.982	24.202
2) SA Decachlor...	10.661f	9.028	430786	328948	20.227	18.837
Target Compounds						
9) L2 AR-1221-2	0.000	4.112	0	7484	N.D.	35.576 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
Data File : PP040979.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2021 14:03
Operator : AJ\MA
Sample : M4607-01
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 15:32:36 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

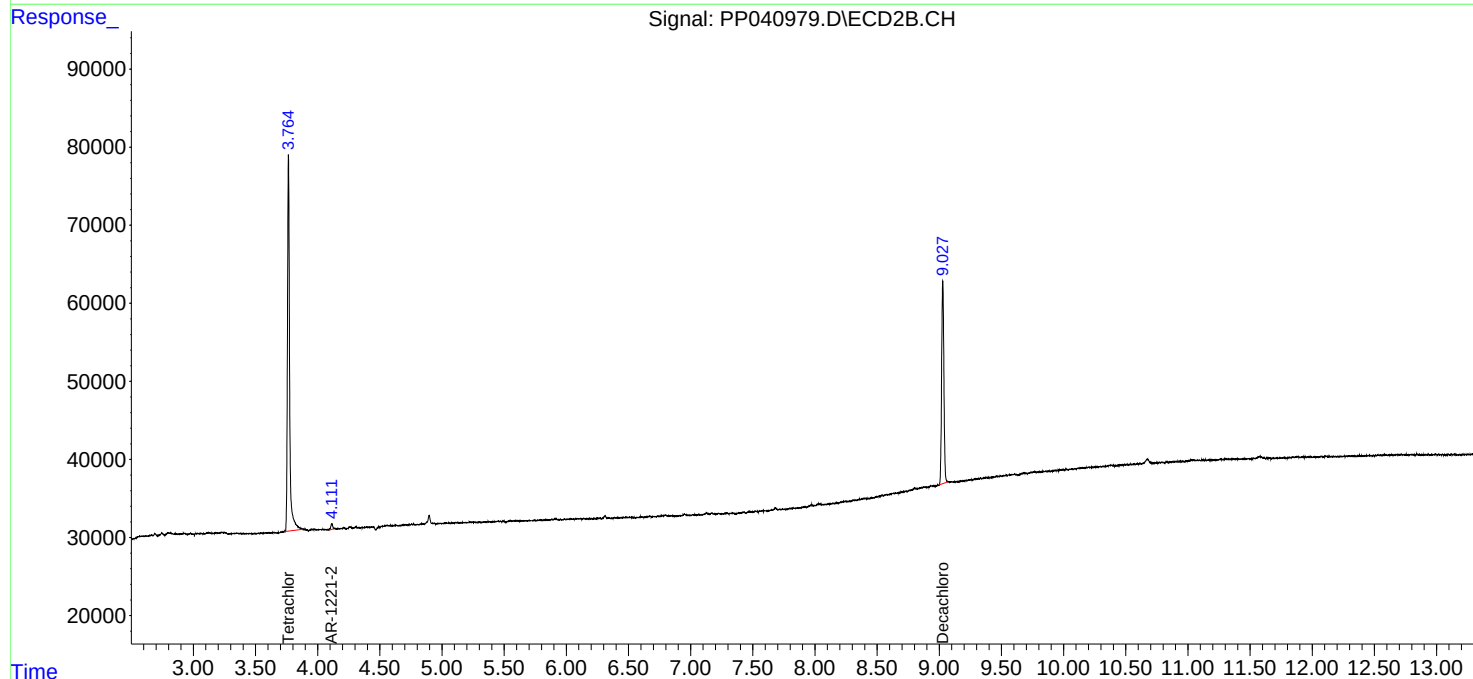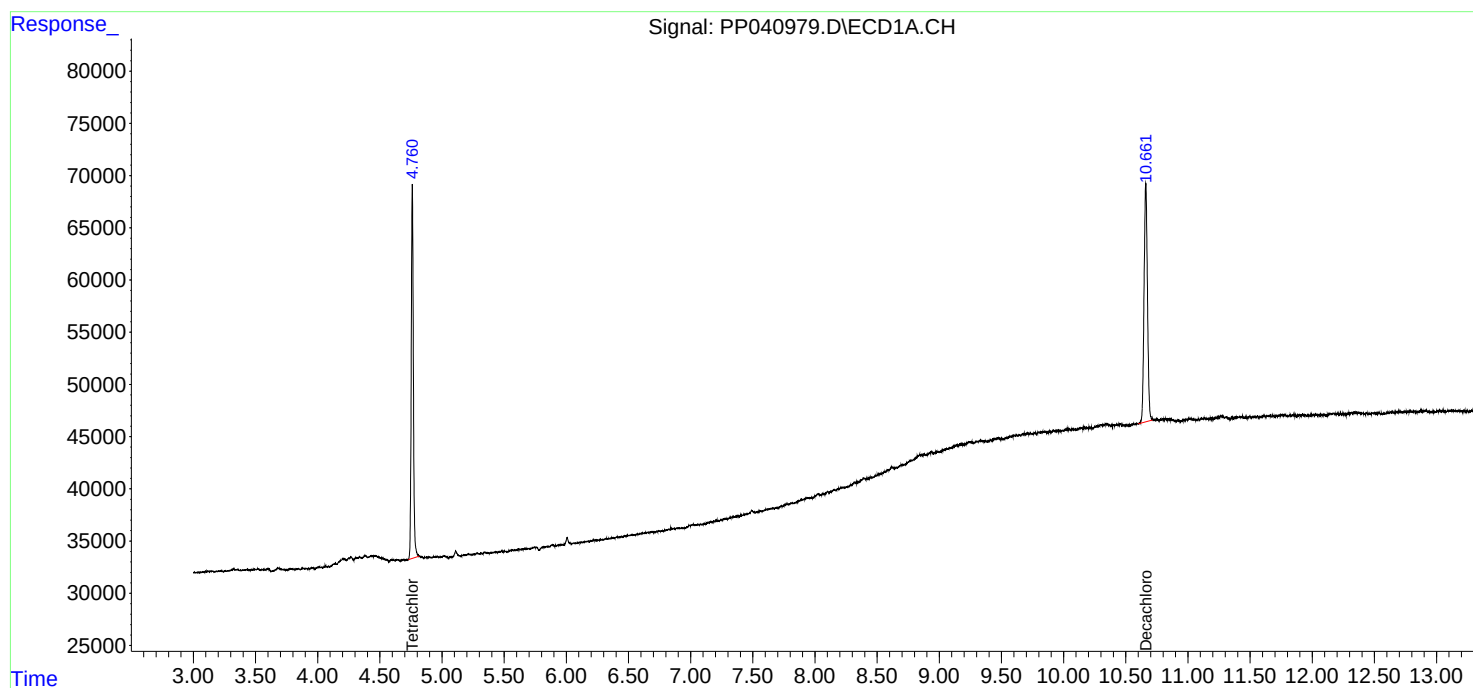


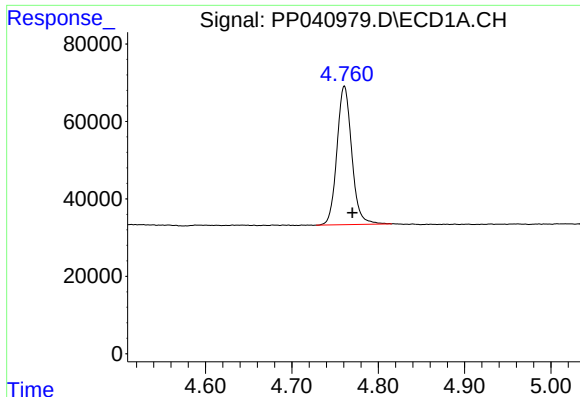

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: -0.009 min
Response: 425072
Conc: 20.98 ng/ml

Instrument :
ECD_P
ClientSampleId :

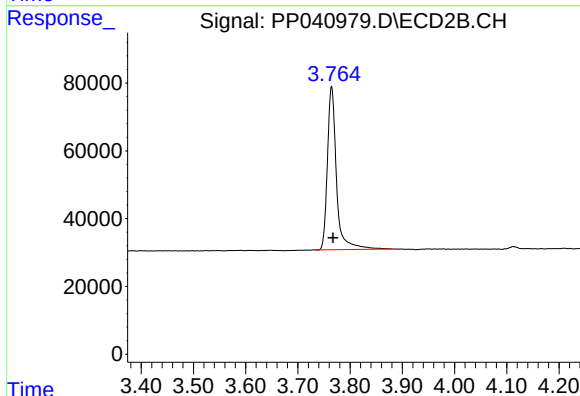


#1 Tetrachloro-m-xylene

R.T.: 3.765 min
Delta R.T.: -0.003 min
Response: 580801
Conc: 24.20 ng/ml

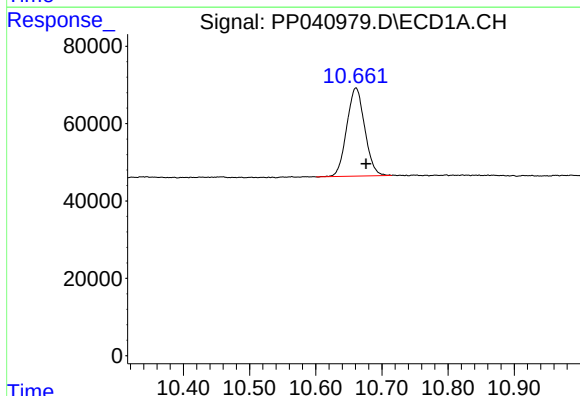


#2 Decachlorobiphenyl

R.T.: 10.661 min
Delta R.T.: -0.015 min
Response: 430786
Conc: 20.23 ng/ml

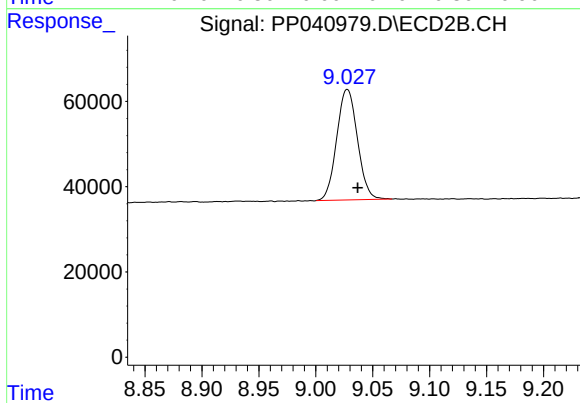

#2 Decachlorobiphenyl


R.T.: 9.028 min
Delta R.T.: -0.009 min
Response: 328948
Conc: 18.84 ng/ml

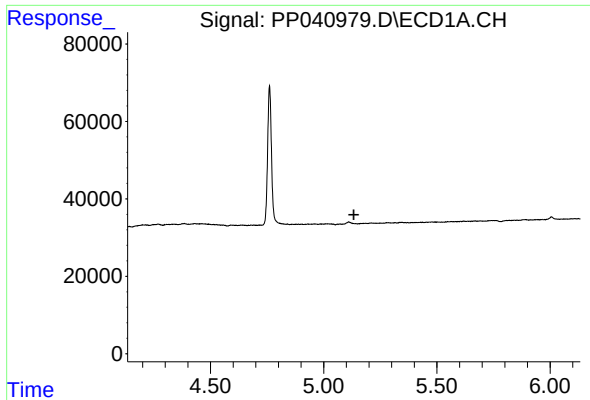

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.133 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

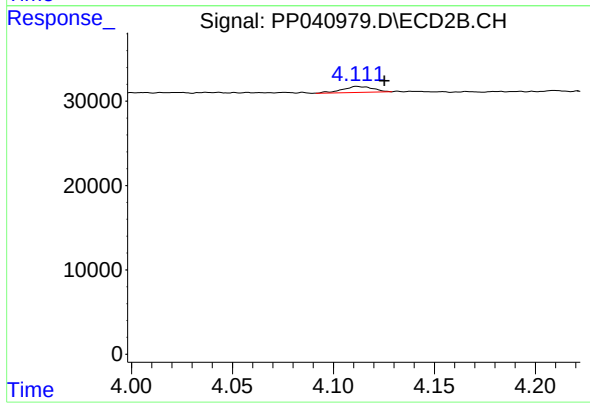

#9 AR-1221-2

R.T.: 4.112 min
Delta R.T.: -0.014 min
Response: 7484
Conc: 35.58 ng/ml