

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
 Data File : PP041001.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2021 20:27
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:51:17 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.760	3.763	447801	601004	22.104	25.044
2)	SA Decachlor...	10.662	9.028	426693	310666	20.035	17.790
Target Compounds							
9)	L2 AR-1221-2	5.146	0.000	19028	0	126.067	N.D. #
10)	L2 AR-1221-3	0.000	4.206	0	29377	N.D.	44.753 #
11)	L3 AR-1232-1	0.000	4.206	0	29377	N.D.	54.432 #
20)	L4 AR-1242-5	0.000	5.906f	0	14142	N.D.	30.705 #
24)	L5 AR-1248-4	6.991f	0.000	27503	0	34.817	N.D. #
25)	L5 AR-1248-5	0.000	5.906f	0	14142	N.D.	22.390 #
26)	L6 AR-1254-1	6.991	5.906f	27503	14142	35.625	14.539 #
28)	L6 AR-1254-3	7.609	0.000	9992	0	7.422	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
Data File : PP041001.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2021 20:27
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:51:17 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

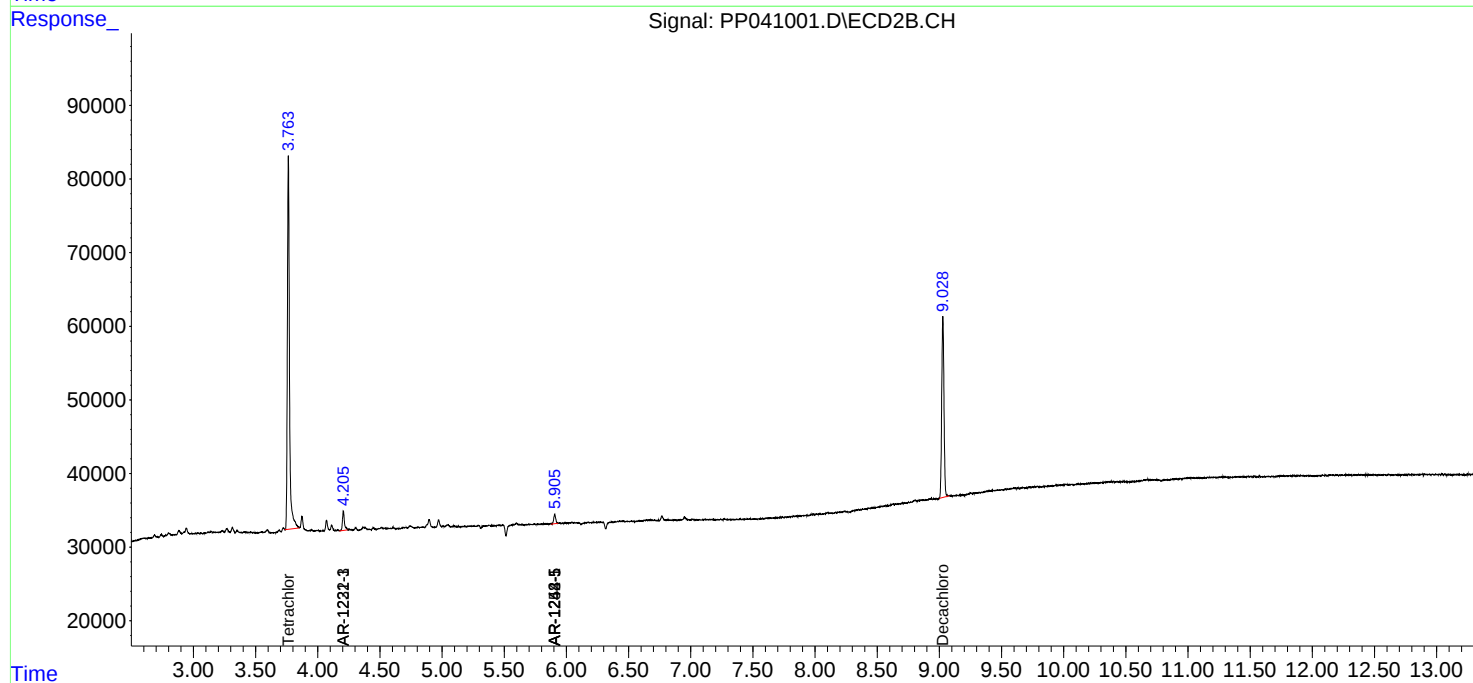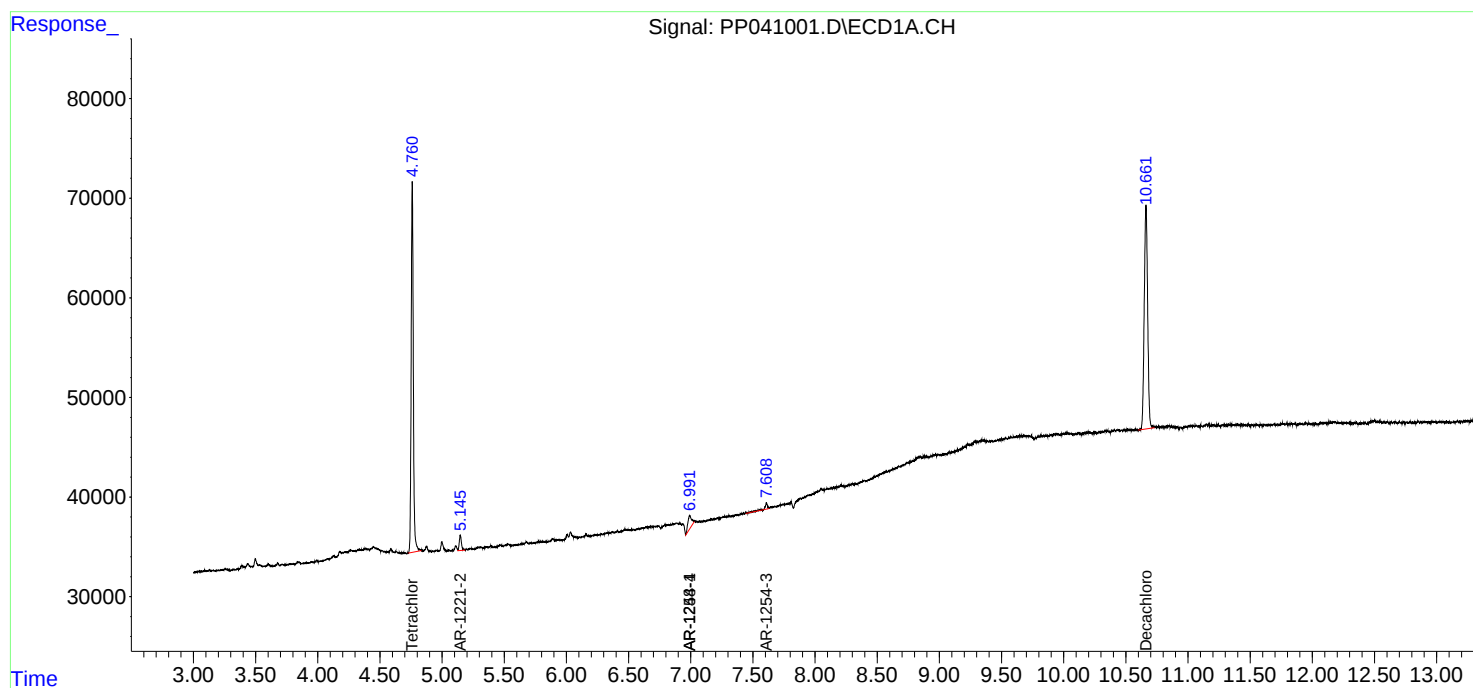


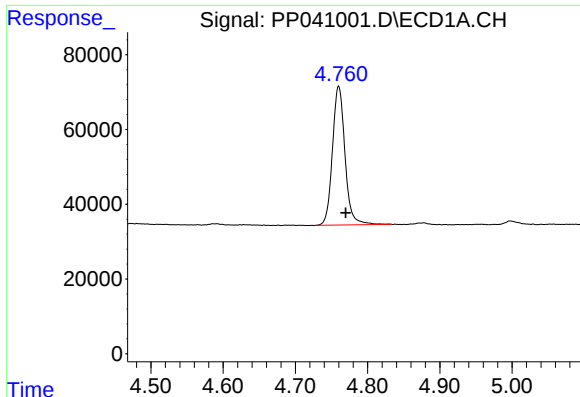

#1 Tetrachloro-m-xylene


R.T.: 4.760 min
Delta R.T.: -0.010 min
Response: 447801
Conc: 22.10 ng/ml

Instrument :
ECD_P
ClientSampleId :

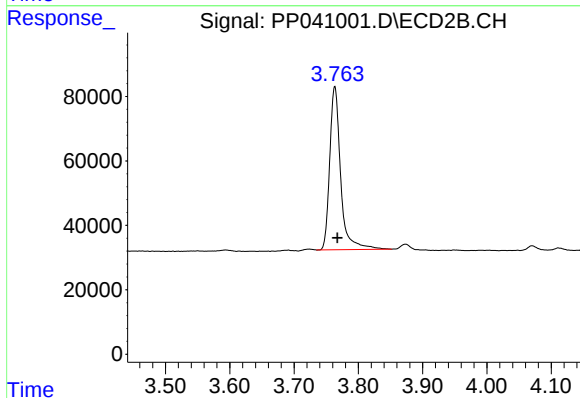


#1 Tetrachloro-m-xylene

R.T.: 3.763 min
Delta R.T.: -0.004 min
Response: 601004
Conc: 25.04 ng/ml

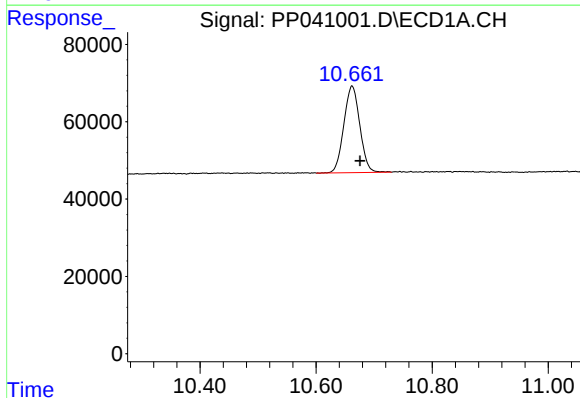


#2 Decachlorobiphenyl

R.T.: 10.662 min
Delta R.T.: -0.014 min
Response: 426693
Conc: 20.04 ng/ml

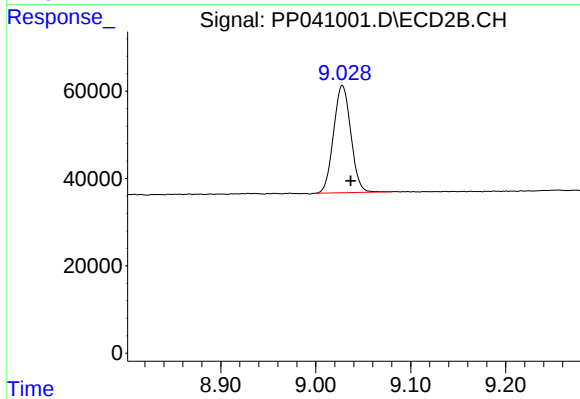

#2 Decachlorobiphenyl


R.T.: 9.028 min
Delta R.T.: -0.009 min
Response: 310666
Conc: 17.79 ng/ml

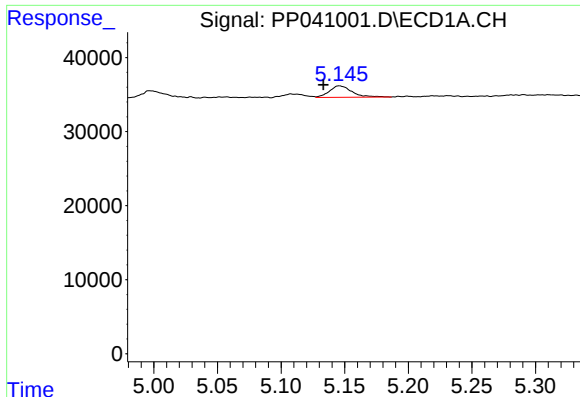

#9 AR-1221-2


R.T.: 5.146 min
Delta R.T.: 0.013 min
Response: 19028
Conc: 126.07 ng/ml

Instrument :
ECD_P
ClientSampleId :

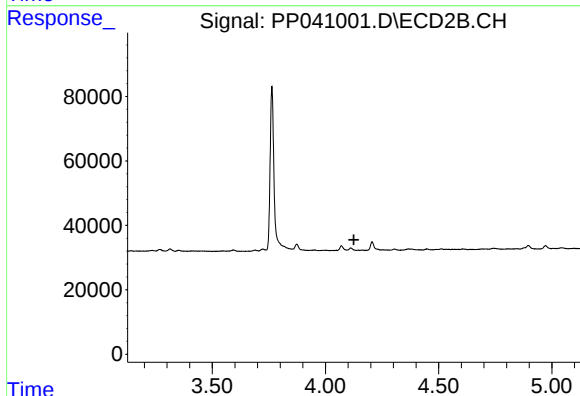


#9 AR-1221-2

R.T.: 0.000 min
Exp R.T. : 4.125 min
Response: 0
Conc: N.D.

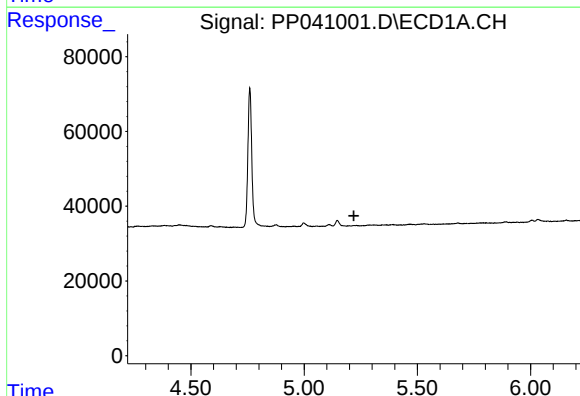


#10 AR-1221-3

R.T.: 0.000 min
Exp R.T. : 5.220 min
Response: 0
Conc: N.D.

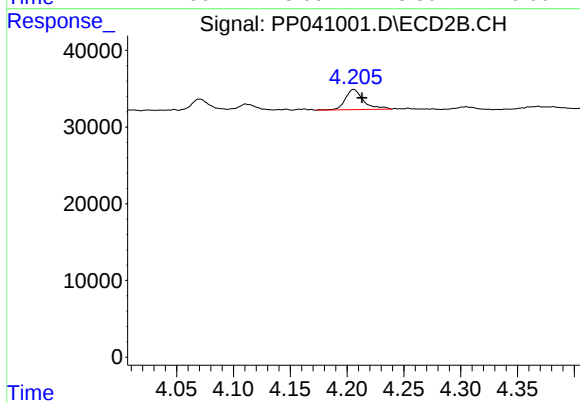

#10 AR-1221-3


R.T.: 4.206 min
Delta R.T.: -0.007 min
Response: 29377
Conc: 44.75 ng/ml

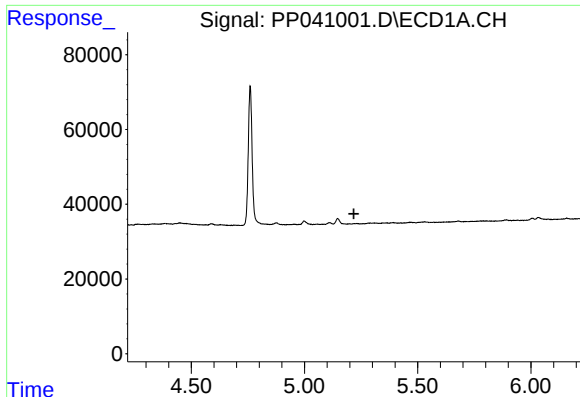

#11 AR-1232-1


R.T.: 0.000 min
Exp R.T.: 5.218 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

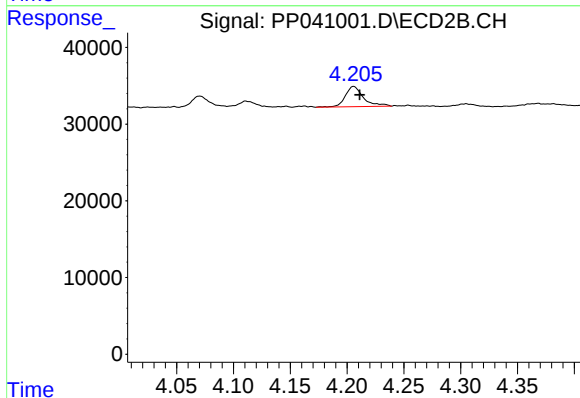


#11 AR-1232-1

R.T.: 4.206 min
Delta R.T.: -0.005 min
Response: 29377
Conc: 54.43 ng/ml

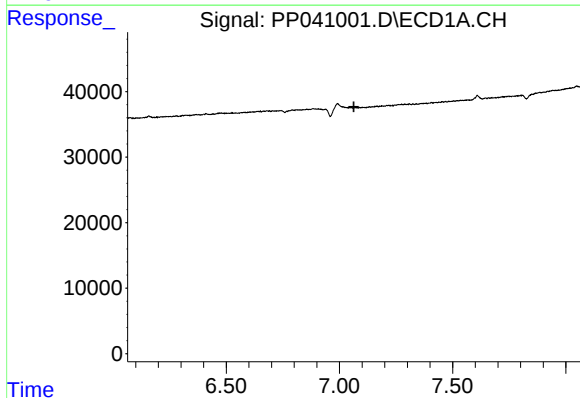


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.064 min
Response: 0
Conc: N.D.

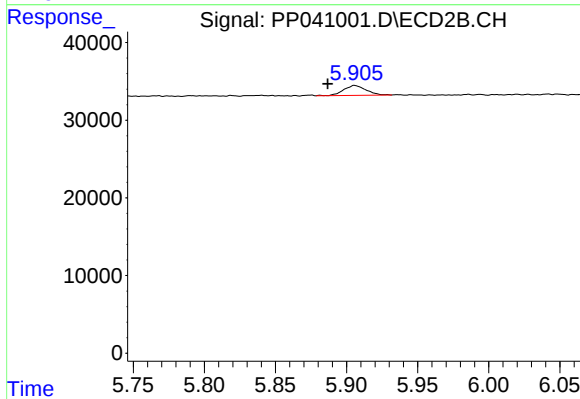

#20 AR-1242-5


R.T.: 5.906 min
Delta R.T.: 0.019 min
Response: 14142
Conc: 30.70 ng/ml

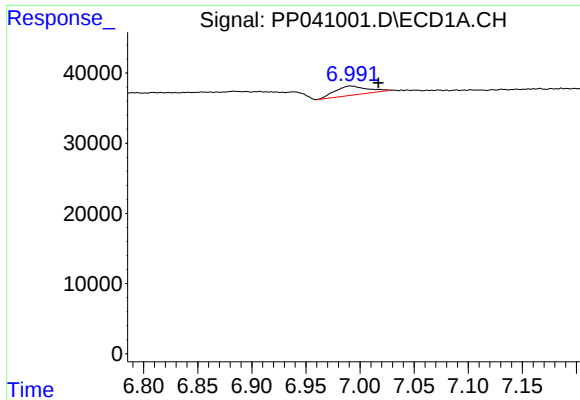

#24 AR-1248-4


R.T.: 6.991 min
Delta R.T.: -0.026 min
Response: 27503
Conc: 34.82 ng/ml

Instrument :
ECD_P
ClientSampleId :

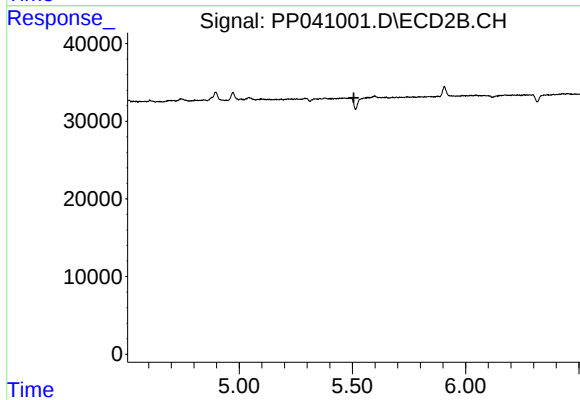


#24 AR-1248-4

R.T.: 0.000 min
Exp R.T. : 5.507 min
Response: 0
Conc: N.D.

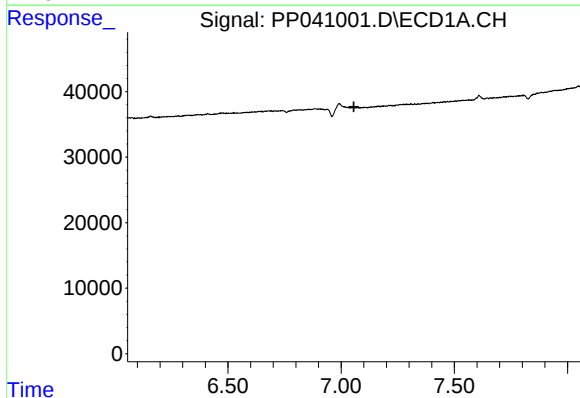


#25 AR-1248-5

R.T.: 0.000 min
Exp R.T. : 7.056 min
Response: 0
Conc: N.D.

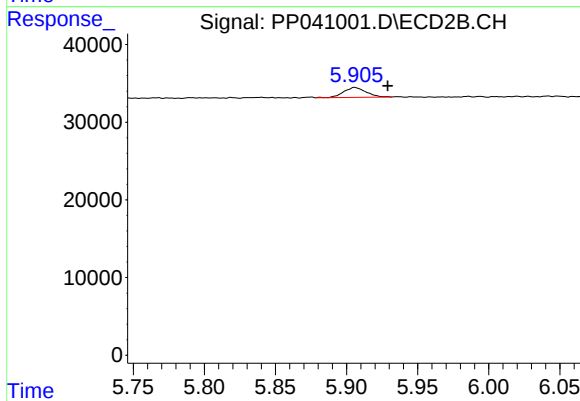

#25 AR-1248-5


R.T.: 5.906 min
Delta R.T.: -0.023 min
Response: 14142
Conc: 22.39 ng/ml

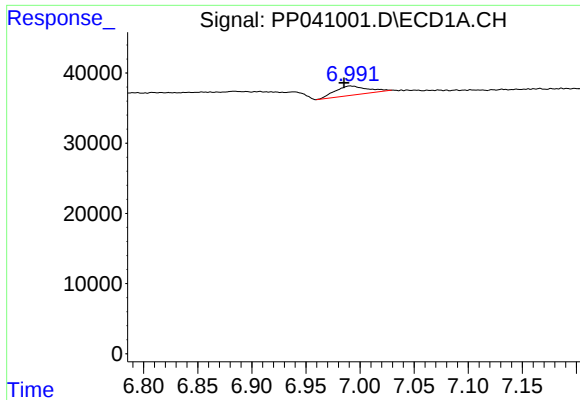

#26 AR-1254-1


R.T.: 6.991 min
Delta R.T.: 0.006 min
Response: 27503
Conc: 35.63 ng/ml

Instrument :
ECD_P
ClientSampleId :

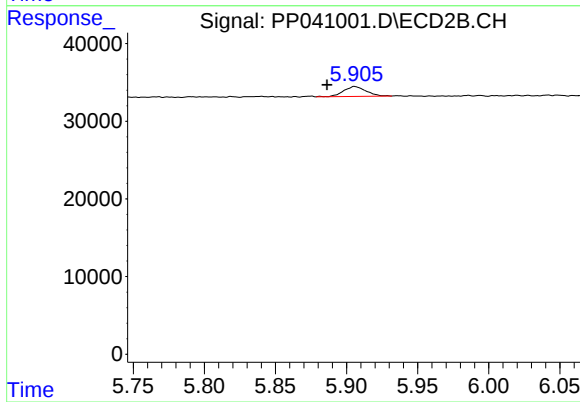


#26 AR-1254-1

R.T.: 5.906 min
Delta R.T.: 0.019 min
Response: 14142
Conc: 14.54 ng/ml

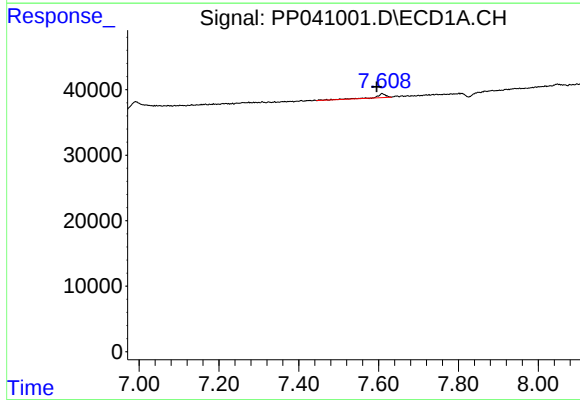

#28 AR-1254-3

R.T.: 7.609 min
Delta R.T.: 0.013 min
Response: 9992
Conc: 7.42 ng/ml

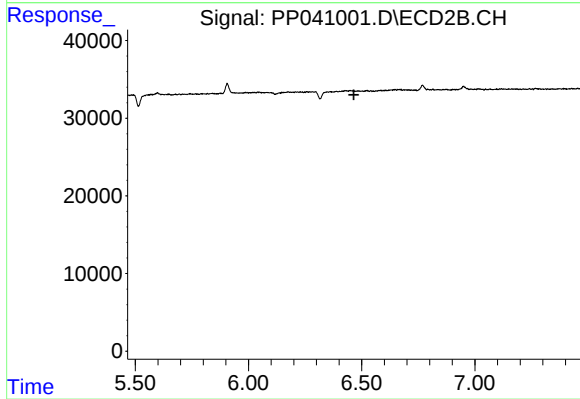

#28 AR-1254-3

R.T.: 0.000 min
Exp R.T. : 6.466 min
Response: 0
Conc: N.D.