

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
 Data File : PP041005.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 11 Nov 2021 21:34
 Operator : AJ\MA
 Sample : M4600-01
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FM786-N34145

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 12 00:52:11 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 04 11:28:51 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.762	3.767	458031	596621	22.609	24.861
2)	SA Decachlor...	10.664	9.029	323653	233455	15.197	13.369

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111121\
Data File : PP041005.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 11 Nov 2021 21:34
Operator : AJ\MA
Sample : M4600-01
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FM786-N34145

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:52:11 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110421.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 04 11:28:51 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

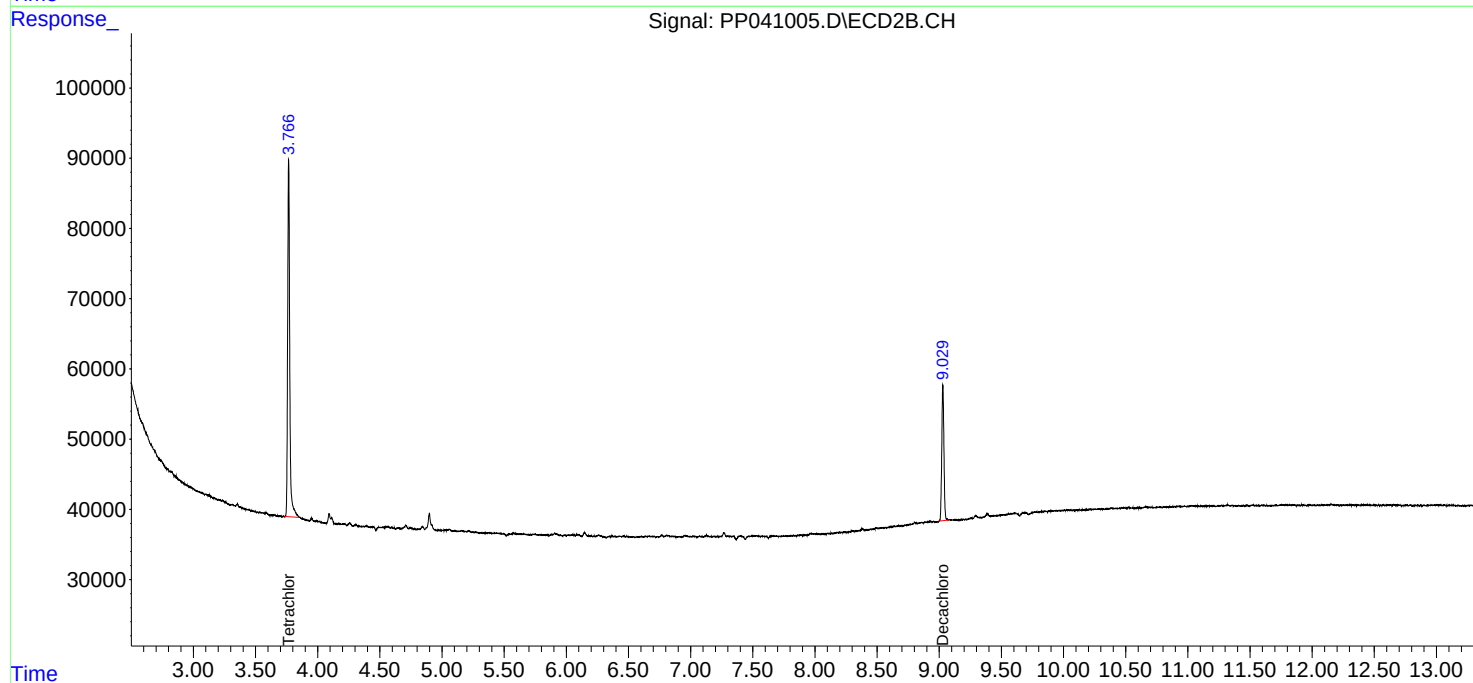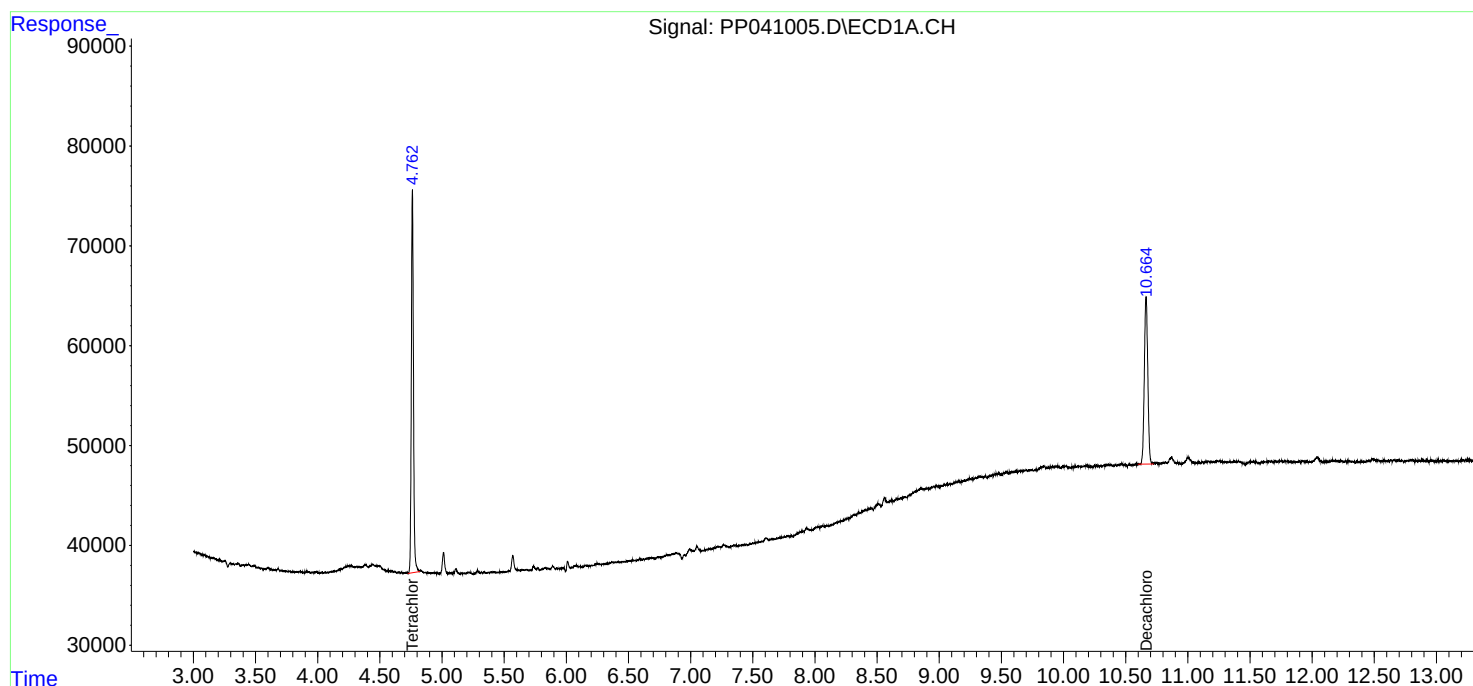


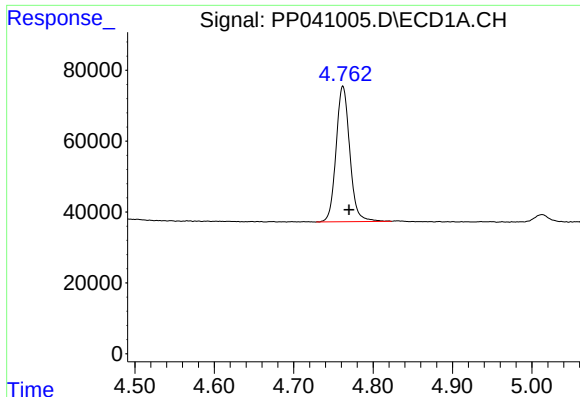

#1 Tetrachloro-m-xylene


R.T.: 4.762 min
Delta R.T.: -0.008 min
Response: 458031
Conc: 22.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
FM786-N34145

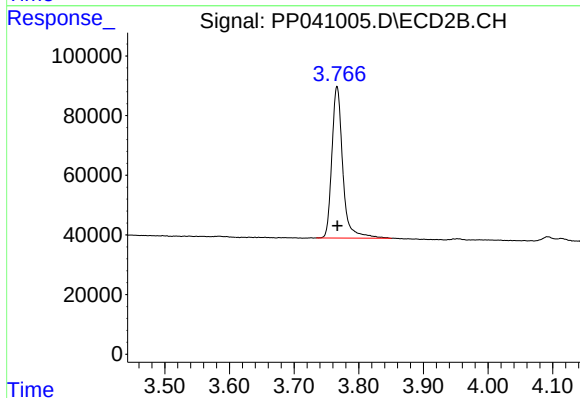


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: 0.000 min
Response: 596621
Conc: 24.86 ng/ml

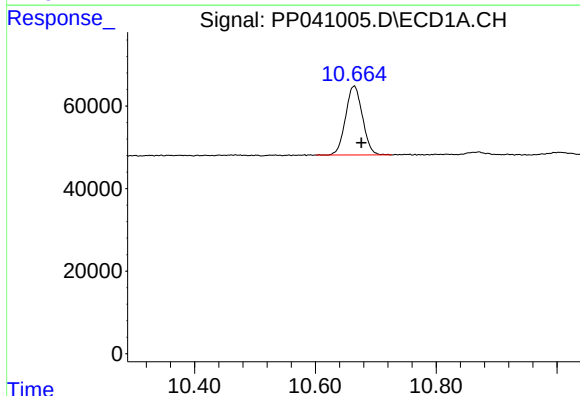

#2 Decachlorobiphenyl

R.T.: 10.664 min
Delta R.T.: -0.012 min
Response: 323653
Conc: 15.20 ng/ml

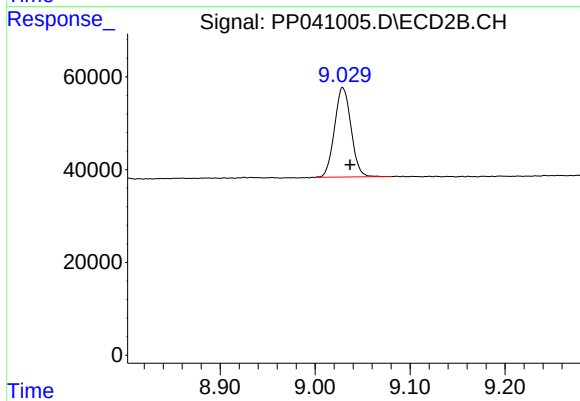

#2 Decachlorobiphenyl

R.T.: 9.029 min
Delta R.T.: -0.008 min
Response: 233455
Conc: 13.37 ng/ml