

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111125\
 Data File : PP076432.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Nov 2025 13:44
 Operator : YP\AJ
 Sample : Q3588-01
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TR-06-11072025

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/12/2025
 Supervised By :Yogesh Patel 11/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 11 14:54:27 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.638	3.776	44745490	197.5E6	31.310m	29.836m
2) SA Decachlor...	10.415	8.775	31272749	187.8E6	29.050	22.840

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111125\
Data File : PP076432.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2025 13:44
Operator : YP\AJ
Sample : Q3588-01
Misc :
ALS Vial : 14 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
TR-06-11072025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/12/2025
Supervised By :Yogesh Patel 11/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 11 14:54:27 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

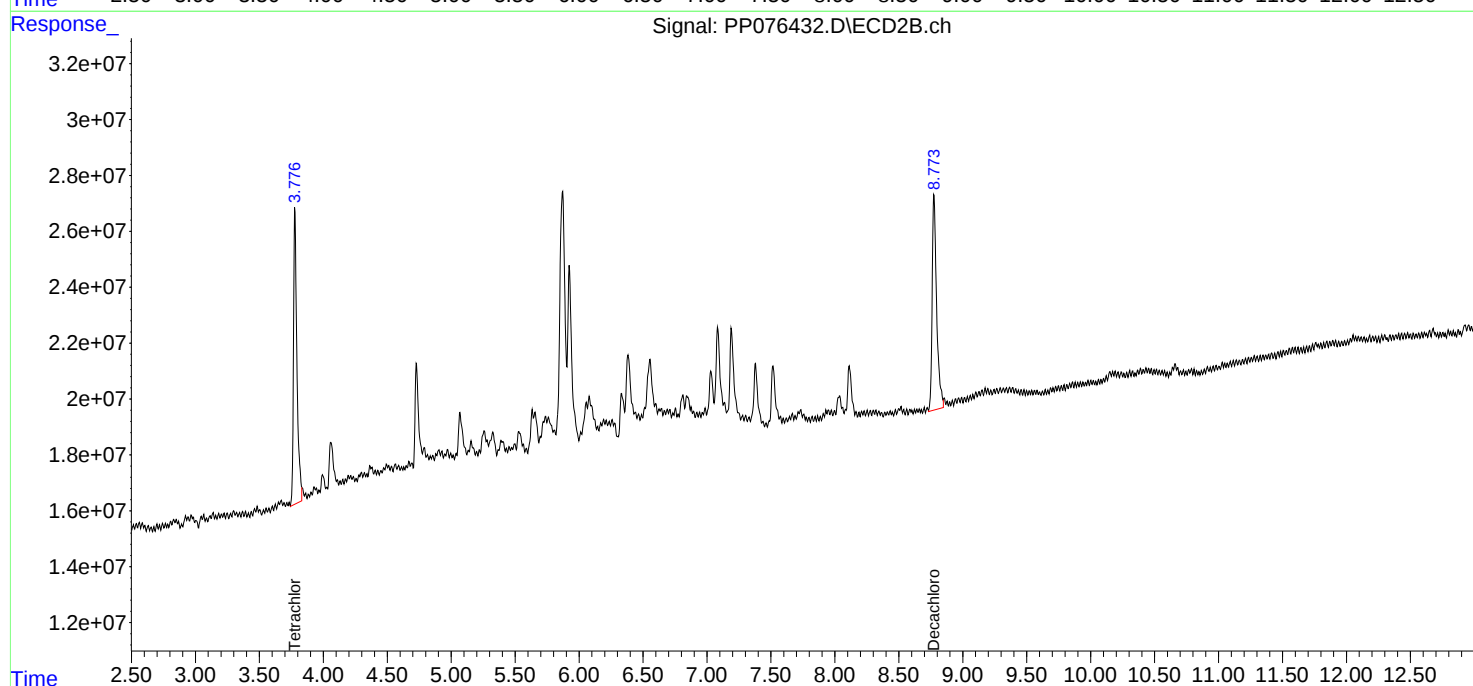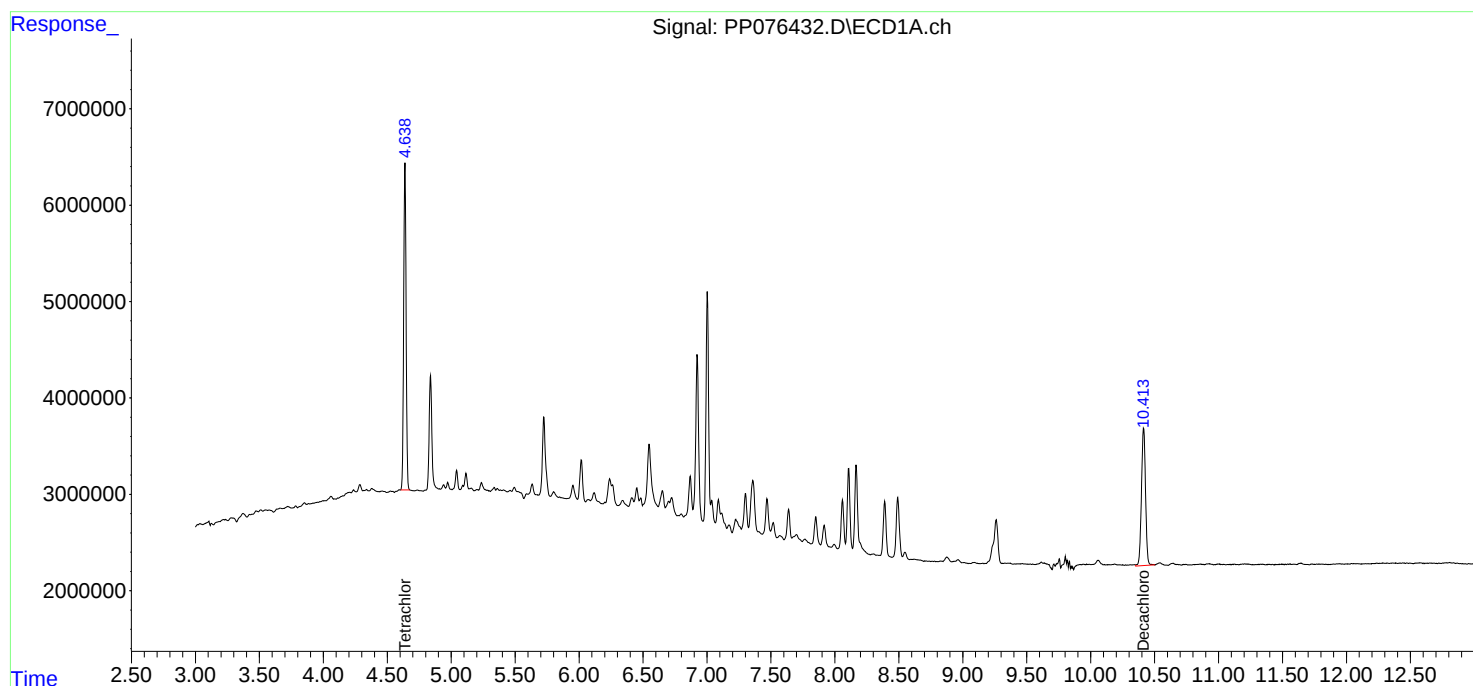

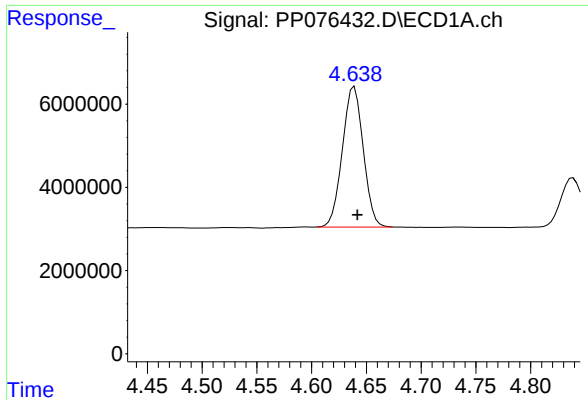


#1 Tetrachloro-m-xylene

R.T.: 4.638 min
Delta R.T.: -0.004 min
Response: 44745490
Conc: 31.31 ng/ml

Instrument :
ECD_P
ClientSampleId :
TR-06-11072025


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/12/2025
Supervised By :Yogesh Patel 11/12/2025

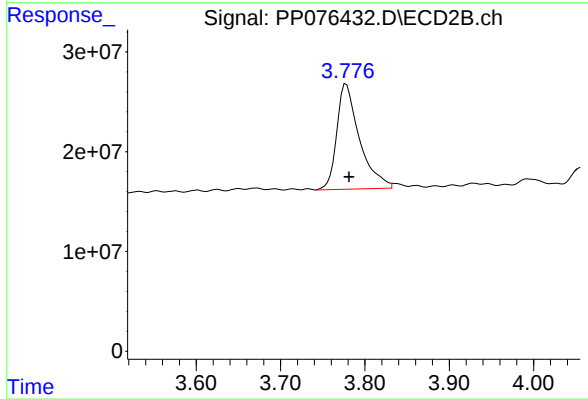


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.005 min
Response: 197465086
Conc: 29.84 ng/ml m

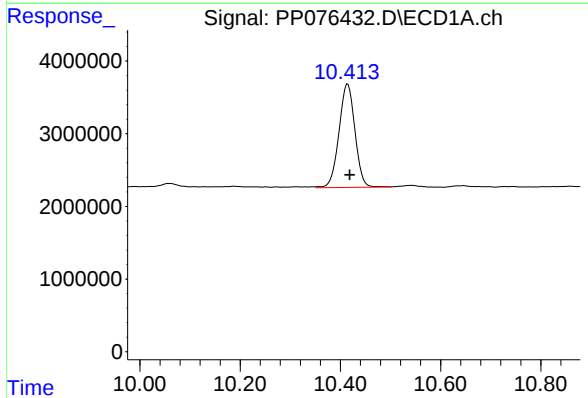

#2 Decachlorobiphenyl

R.T.: 10.415 min
Delta R.T.: -0.004 min
Response: 31272749
Conc: 29.05 ng/ml

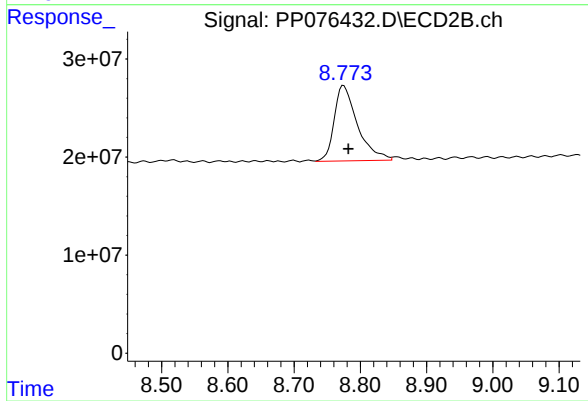

#2 Decachlorobiphenyl

R.T.: 8.775 min
Delta R.T.: -0.007 min
Response: 187810208
Conc: 22.84 ng/ml