

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111125\
Data File : PP076442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2025 17:16
Operator : YP\AJ
Sample : Q3593-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
C-LAW-25-0156-0166-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:25:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.639	3.779	23878280	132.7E6	16.709	20.058
2) SA Decachlor...	10.412	8.771	26724283	184.1E6	24.825	22.393

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111125\
Data File : PP076442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Nov 2025 17:16
Operator : YP\AJ
Sample : Q3593-08
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
C-LAW-25-0156-0166-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 12 00:25:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

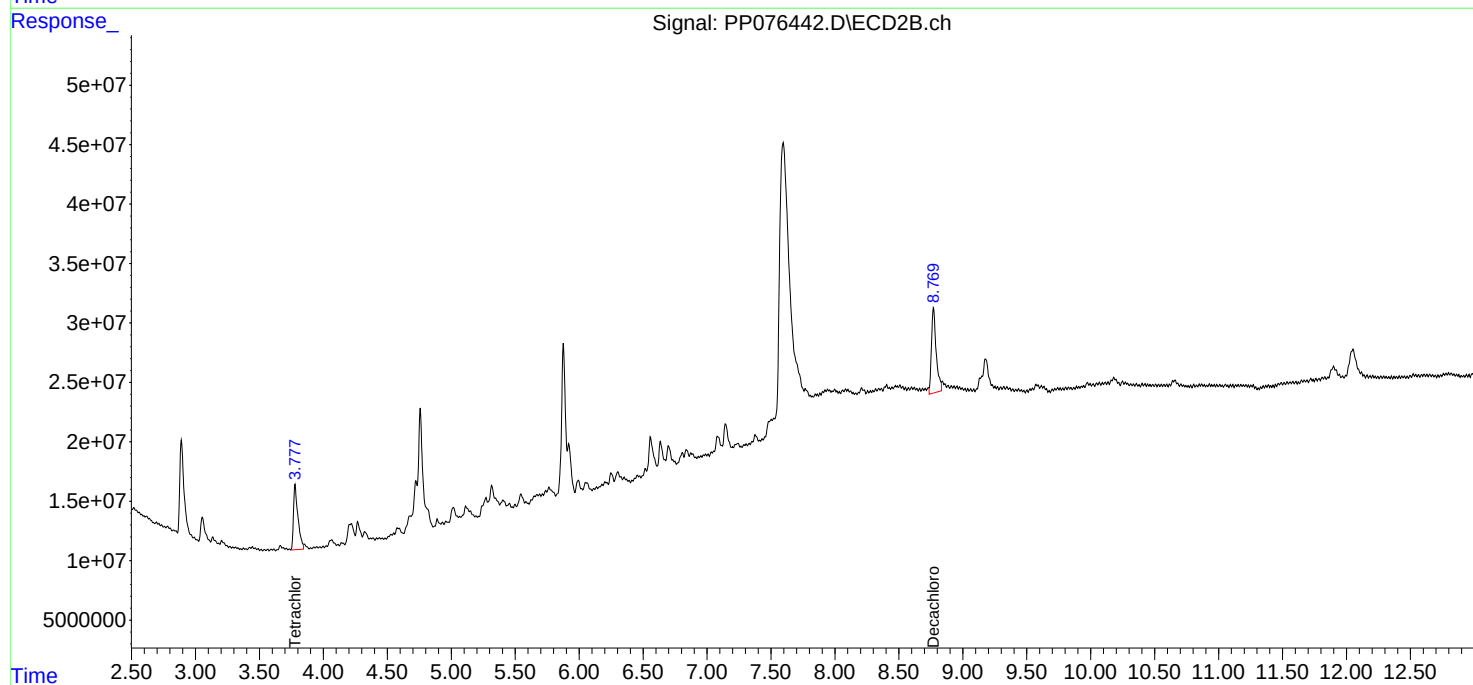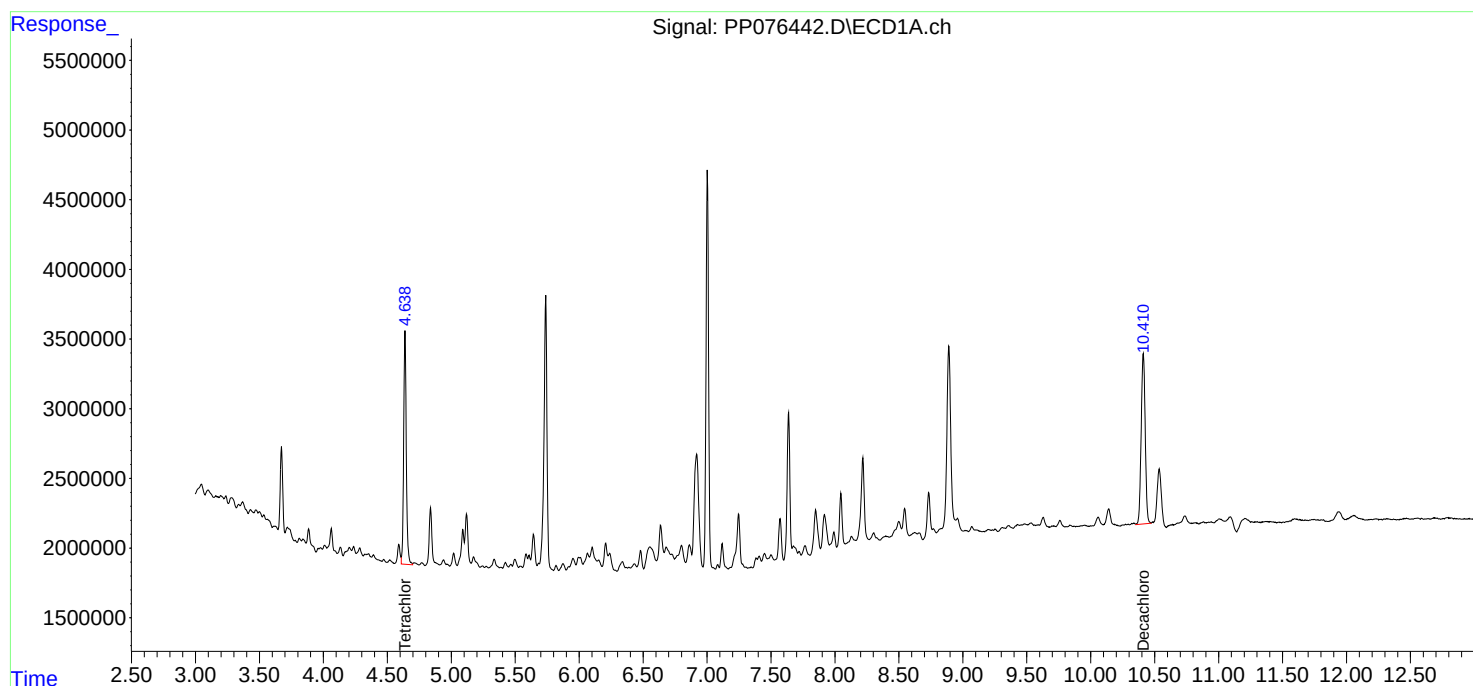


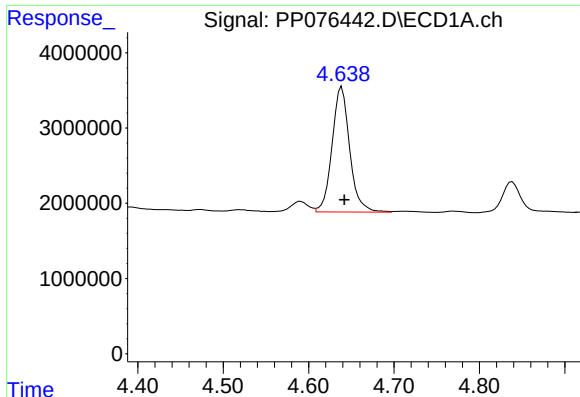

#1 Tetrachloro-m-xylene


R.T.: 4.639 min
Delta R.T.: -0.003 min
Response: 23878280
Conc: 16.71 ng/ml

Instrument :
ECD_P
ClientSampleId :
C-LAW-25-0156-0166-COMP

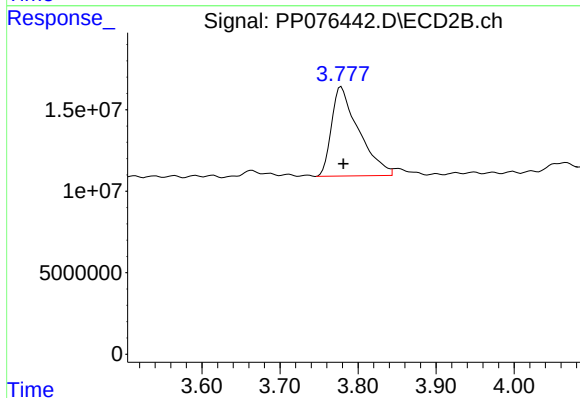


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.003 min
Response: 132749173
Conc: 20.06 ng/ml

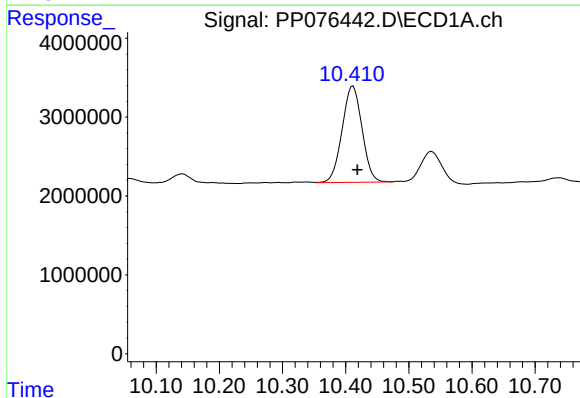

#2 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.007 min
Response: 26724283
Conc: 24.82 ng/ml

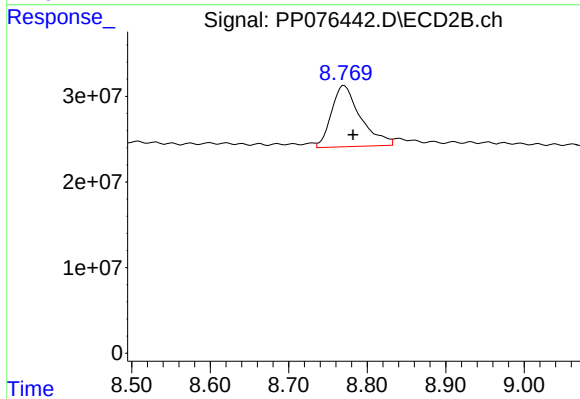

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.011 min
Response: 184135311
Conc: 22.39 ng/ml