

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111224\
 Data File : PP068449.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 11:03
 Operator : YP\AJ
 Sample : P4791-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 HINCHMAN-OILY-WATER

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :Ankita Jodhani 11/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 02:17:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.754	4.049	6390133	5800239	6.584m	5.990m
2) SA Decachlor...	10.666	9.205	7461925	5318474	5.962	4.702

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111224\
Data File : PP068449.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 11:03
Operator : YP\AJ
Sample : P4791-02
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
HINCHMAN-OILY-WATER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :Ankita Jodhani 11/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 02:17:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

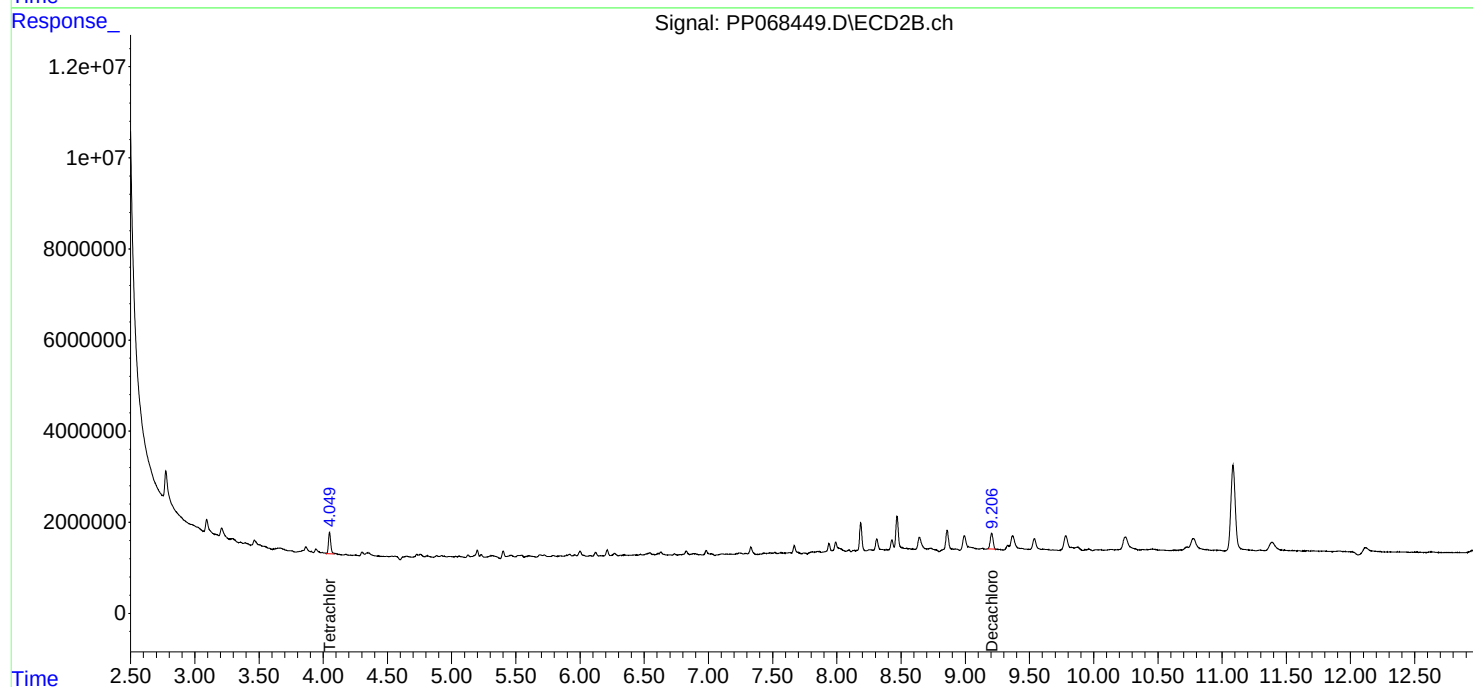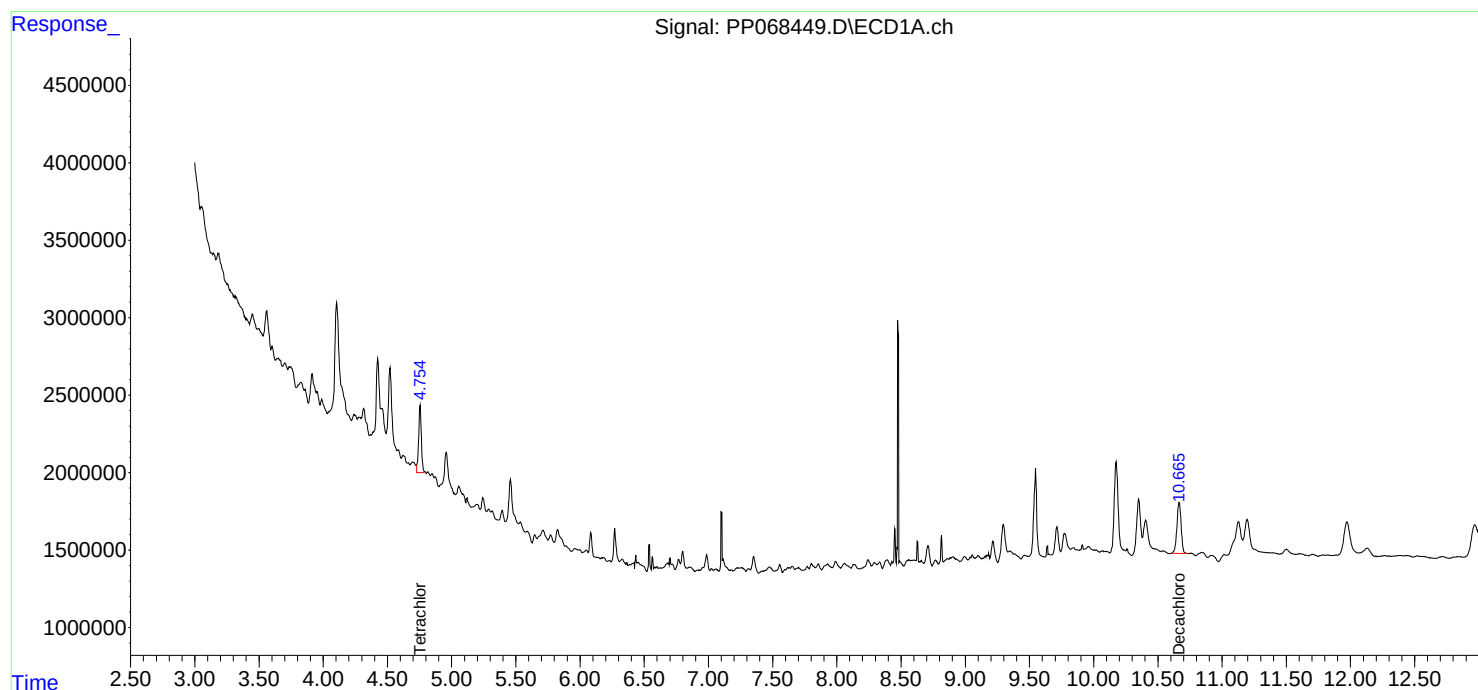

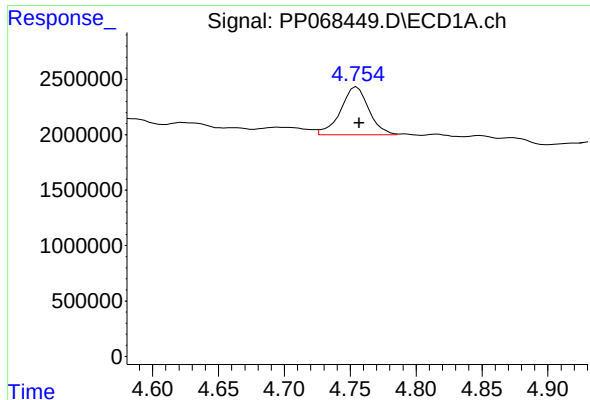


#1 Tetrachloro-m-xylene

R.T.: 4.754 min
Delta R.T.: -0.003 min
Response: 6390133
Conc: 6.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
HINCHMAN-OILY-WATER


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :Ankita Jodhani 11/13/2024

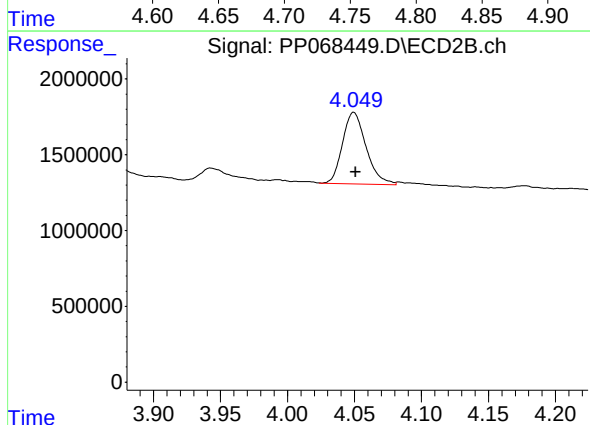


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 5800239
Conc: 5.99 ng/ml

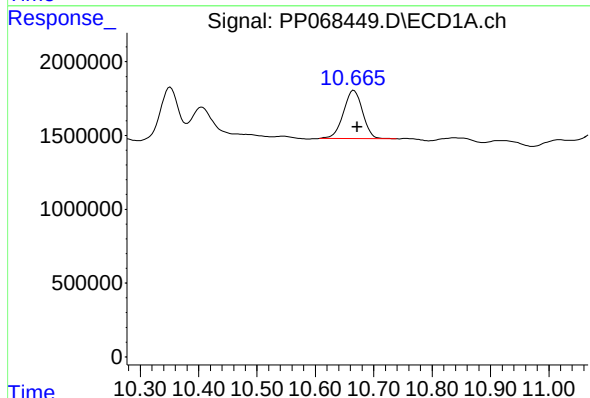

#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.006 min
Response: 7461925
Conc: 5.96 ng/ml

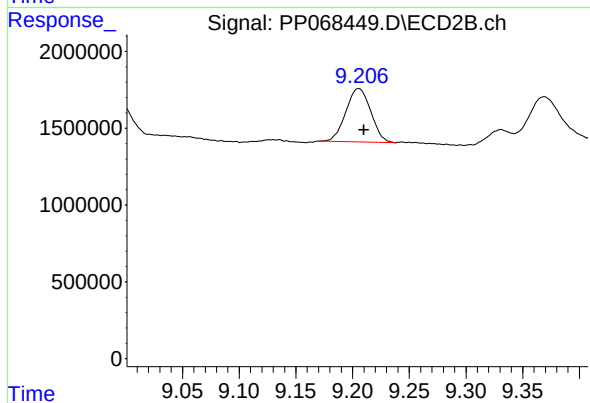

#2 Decachlorobiphenyl

R.T.: 9.205 min
Delta R.T.: -0.004 min
Response: 5318474
Conc: 4.70 ng/ml