

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111224\
 Data File : PP068465.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2024 16:28
 Operator : YP\AJ
 Sample : P4815-03 10X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC271332-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/13/2024
 Supervised By :Ankita Jodhani 11/13/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 02:26:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.755	4.049	2439804	2909401	2.514m	3.005m
2) SA Decachlor...	10.671	9.205	2869977	2424734	2.293	2.144

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111224\
Data File : PP068465.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2024 16:28
Operator : YP\AJ
Sample : P4815-03 10X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :

ECD_P

ClientSampleId :

BC271332-1-1

Manual Integrations



APPROVED


Reviewed By :Yogesh Patel 11/13/2024

Supervised By :Ankita Jodhani 11/13/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 02:26:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

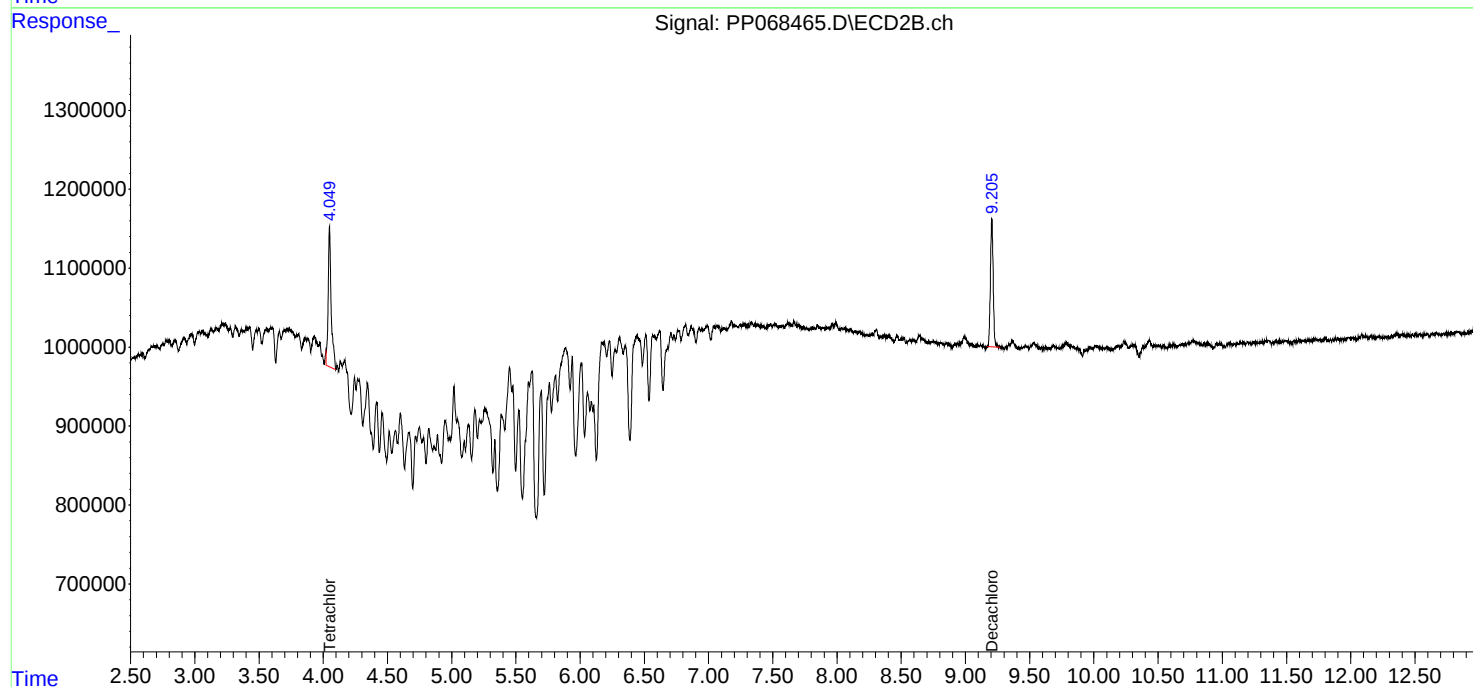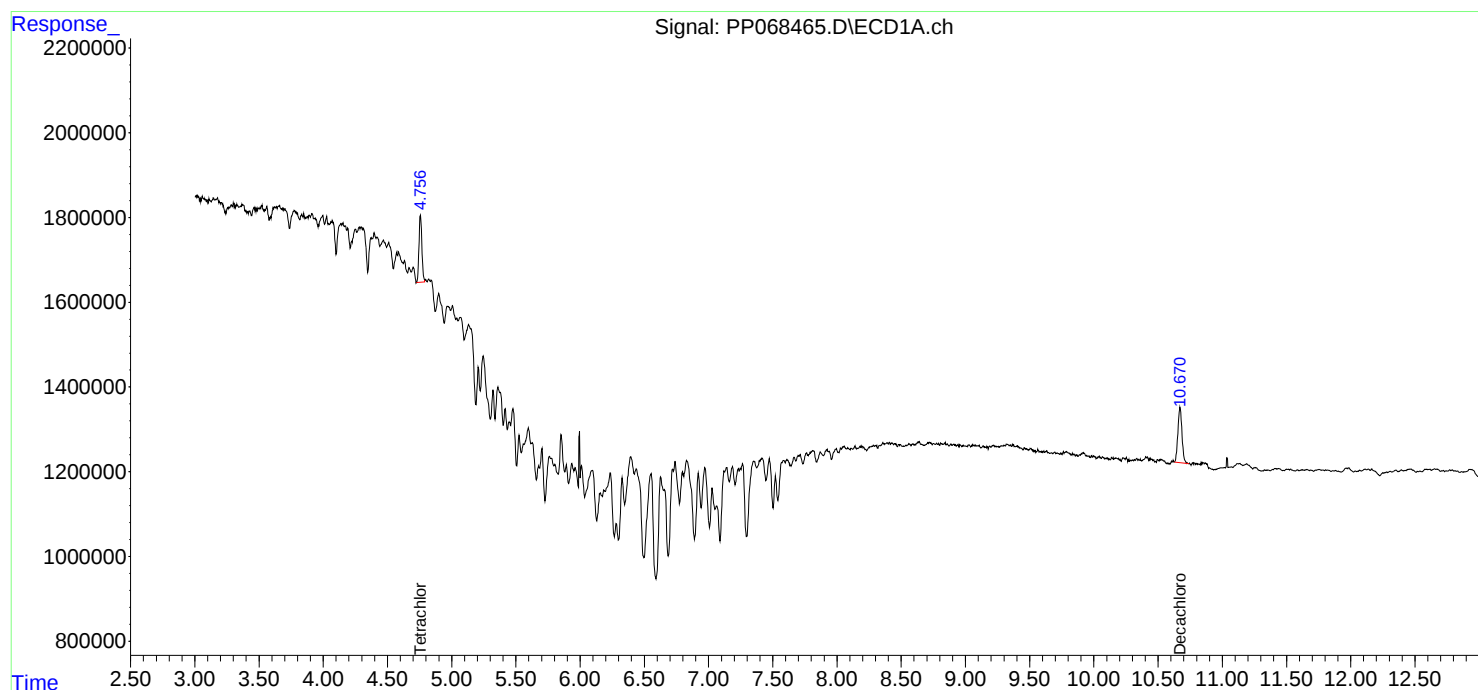

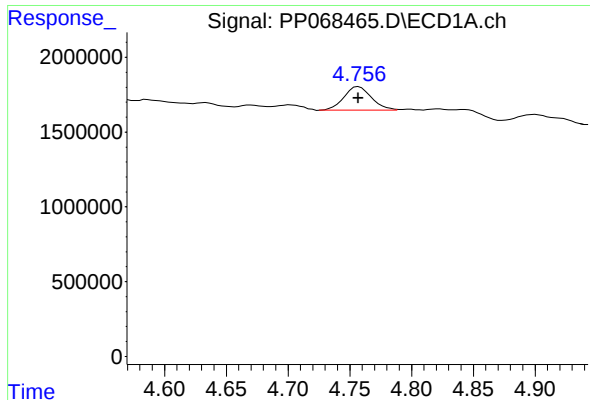


#1 Tetrachloro-m-xylene

R.T.: 4.755 min
Delta R.T.: -0.002 min
Response: 2439804
Conc: 2.51 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC271332-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/13/2024
Supervised By :Ankita Jodhani 11/13/2024

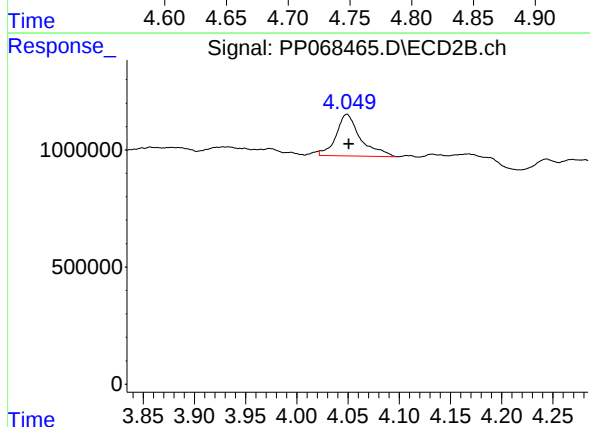


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 2909401
Conc: 3.00 ng/ml

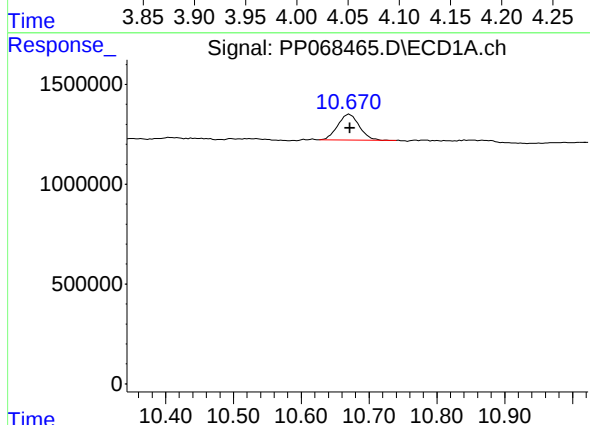

#2 Decachlorobiphenyl

R.T.: 10.671 min
Delta R.T.: -0.001 min
Response: 2869977
Conc: 2.29 ng/ml

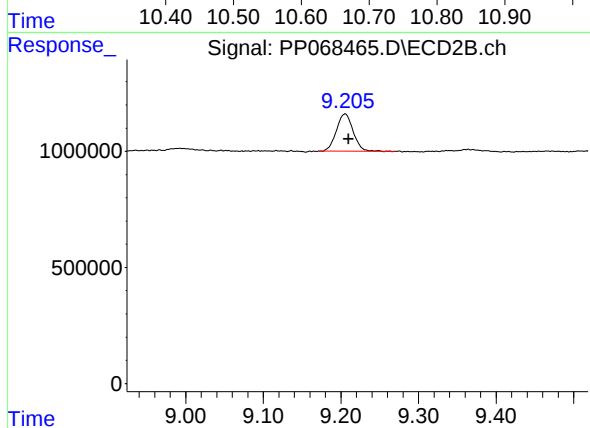

#2 Decachlorobiphenyl

R.T.: 9.205 min
Delta R.T.: -0.005 min
Response: 2424734
Conc: 2.14 ng/ml