

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111225\
 Data File : PP076476.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Nov 2025 17:25
 Operator : YP\AJ
 Sample : Q3598-01
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 EO-CONCRETE

Manual Integrations
 APPROVED

Reviewed By :Rahul Chavli 11/13/2025
 Supervised By :Yogesh Patel 11/13/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 10:49:44 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.636	3.775	34110454	190.5E6	23.869m	28.786
2) SA Decachlor...	10.410	8.769	24337193	162.5E6	22.607	19.762

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111225\
Data File : PP076476.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Nov 2025 17:25
Operator : YP\AJ
Sample : Q3598-01
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
EO-CONCRETE


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Yogesh Patel 11/13/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 10:49:44 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

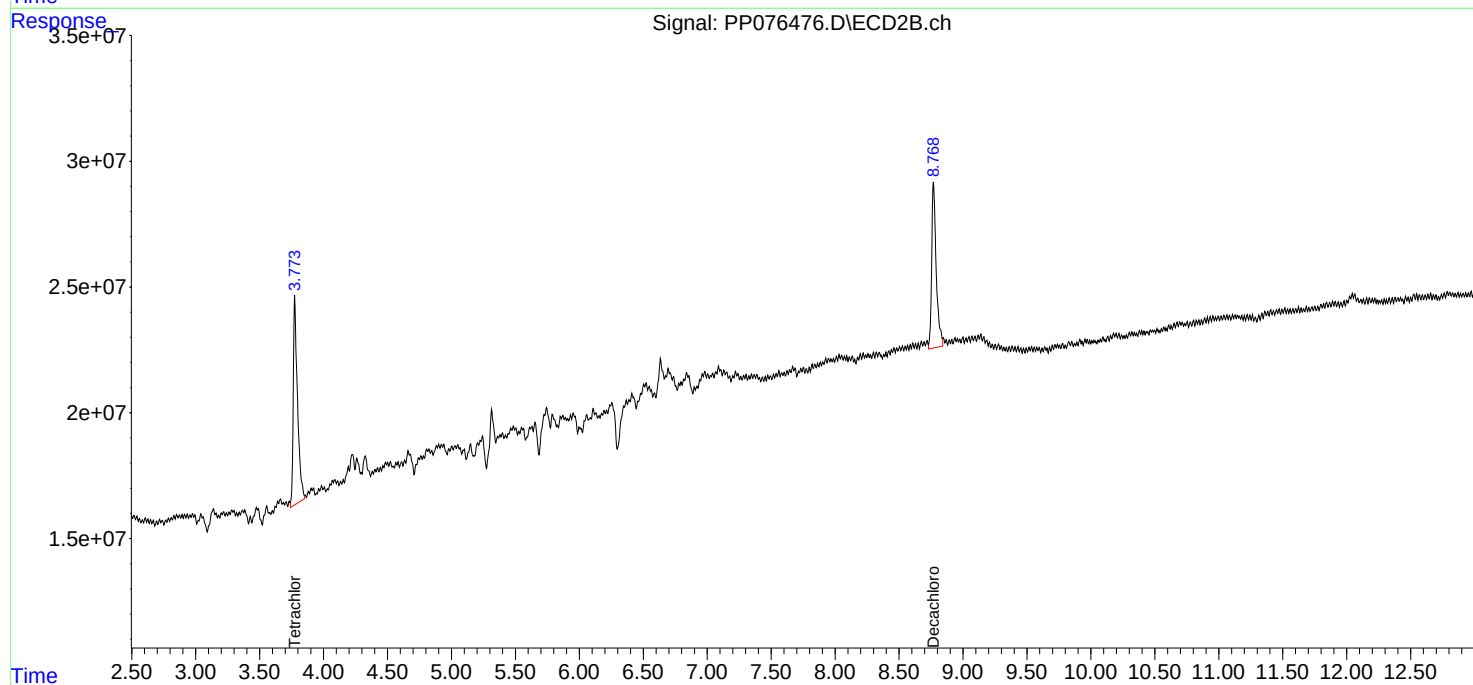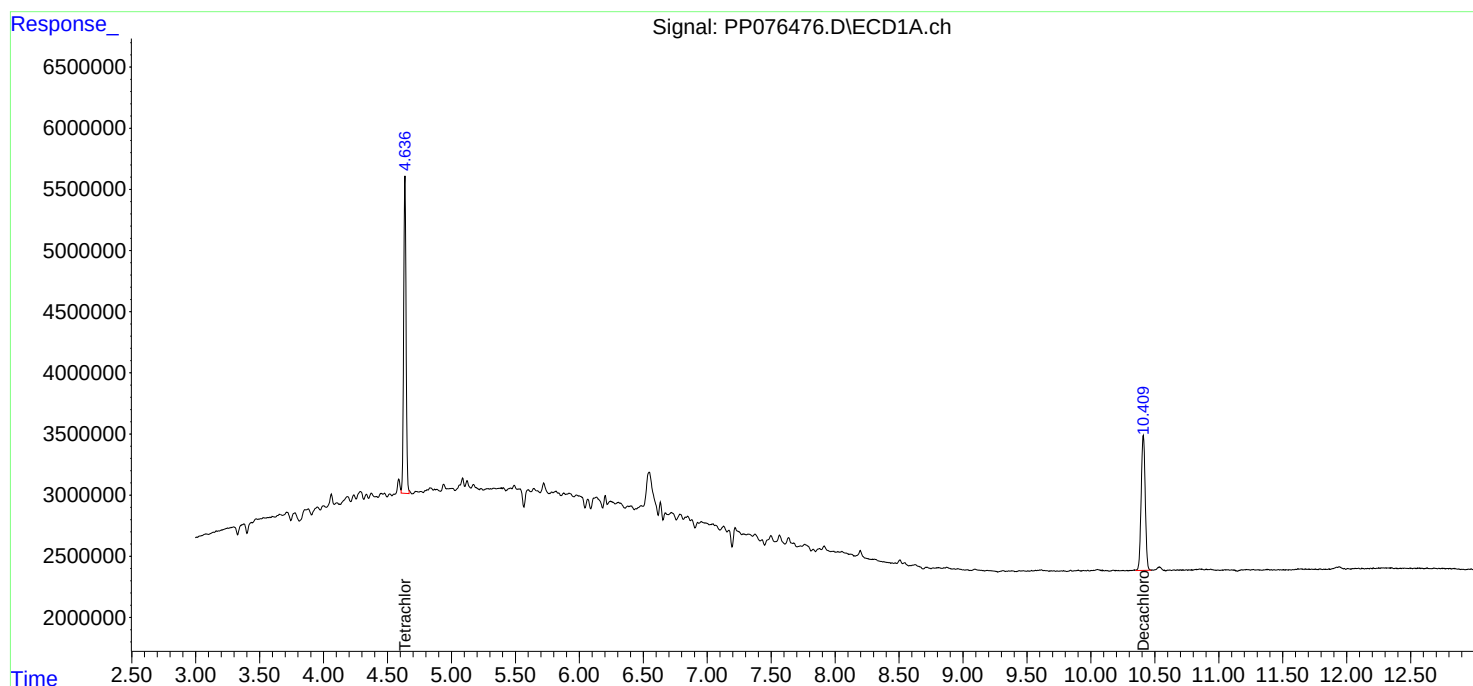

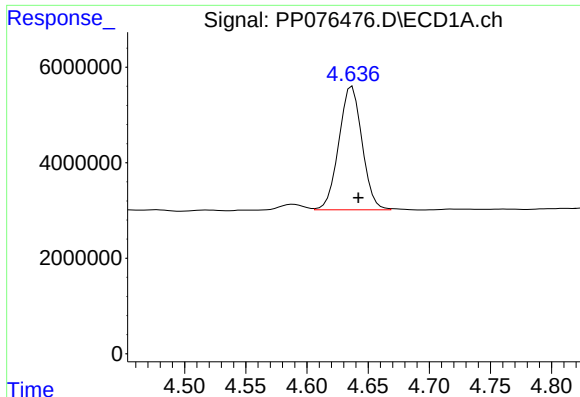


#1 Tetrachloro-m-xylene

R.T.: 4.636 min
Delta R.T.: -0.006 min
Response: 34110454
Conc: 23.87 ng/ml

Instrument :
ECD_P
ClientSampleId :
EO-CONCRETE


Manual Integrations
APPROVED

Reviewed By :Rahul Chavli 11/13/2025
Supervised By :Yogesh Patel 11/13/2025

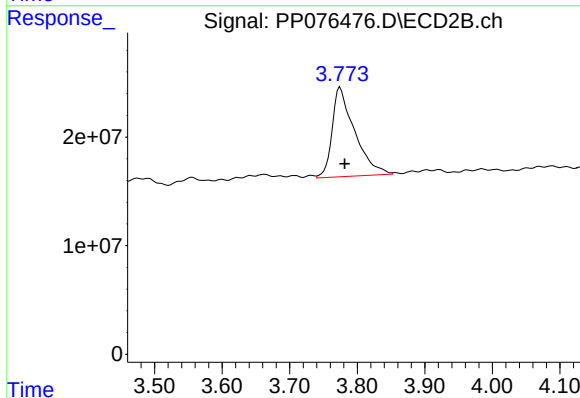


#1 Tetrachloro-m-xylene

R.T.: 3.775 min
Delta R.T.: -0.006 min
Response: 190514203
Conc: 28.79 ng/ml

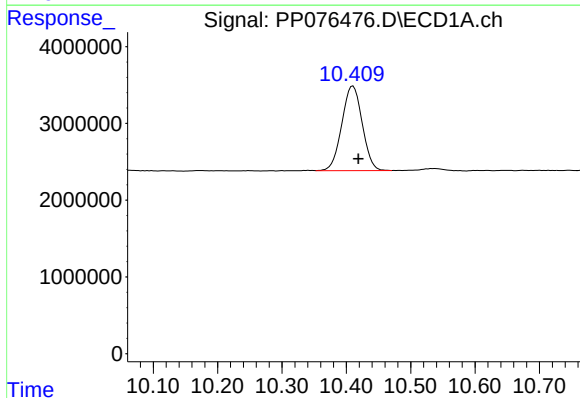

#2 Decachlorobiphenyl

R.T.: 10.410 min
Delta R.T.: -0.009 min
Response: 24337193
Conc: 22.61 ng/ml

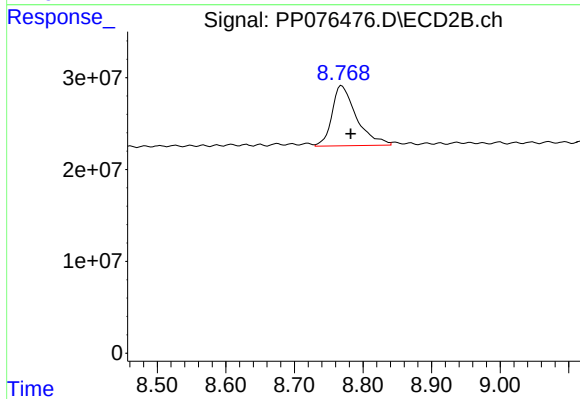

#2 Decachlorobiphenyl

R.T.: 8.769 min
Delta R.T.: -0.013 min
Response: 162503463
Conc: 19.76 ng/ml