

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111320\
 Data File : PP031269.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2020 14:33
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 14:33:57 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.798	4.071	1310496	1269050	19.621	19.092
2)	SA Decachlor...	10.683	9.391	751958	793773	18.807	19.010
Target Compounds							
9)	L2 AR-1221-2	0.000	4.426	0	13174	N.D.	30.768 #
20)	L4 AR-1242-5	0.000	6.230f	0	6145	N.D.	6.173 #
25)	L5 AR-1248-5	0.000	6.230f	0	6145	N.D.	4.865 #
26)	L6 AR-1254-1	0.000	6.230f	0	6145	N.D.	3.124 #
28)	L6 AR-1254-3	0.000	6.780	0	1688	N.D.	0.616 #
32)	L7 AR-1260-2	0.000	7.119	0	3822	N.D.	1.632 #
45)	L9 AR-1268-5	0.000	9.140	0	12300	N.D.	0.917 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111320\
Data File : PP031269.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2020 14:33
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 14:33:57 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

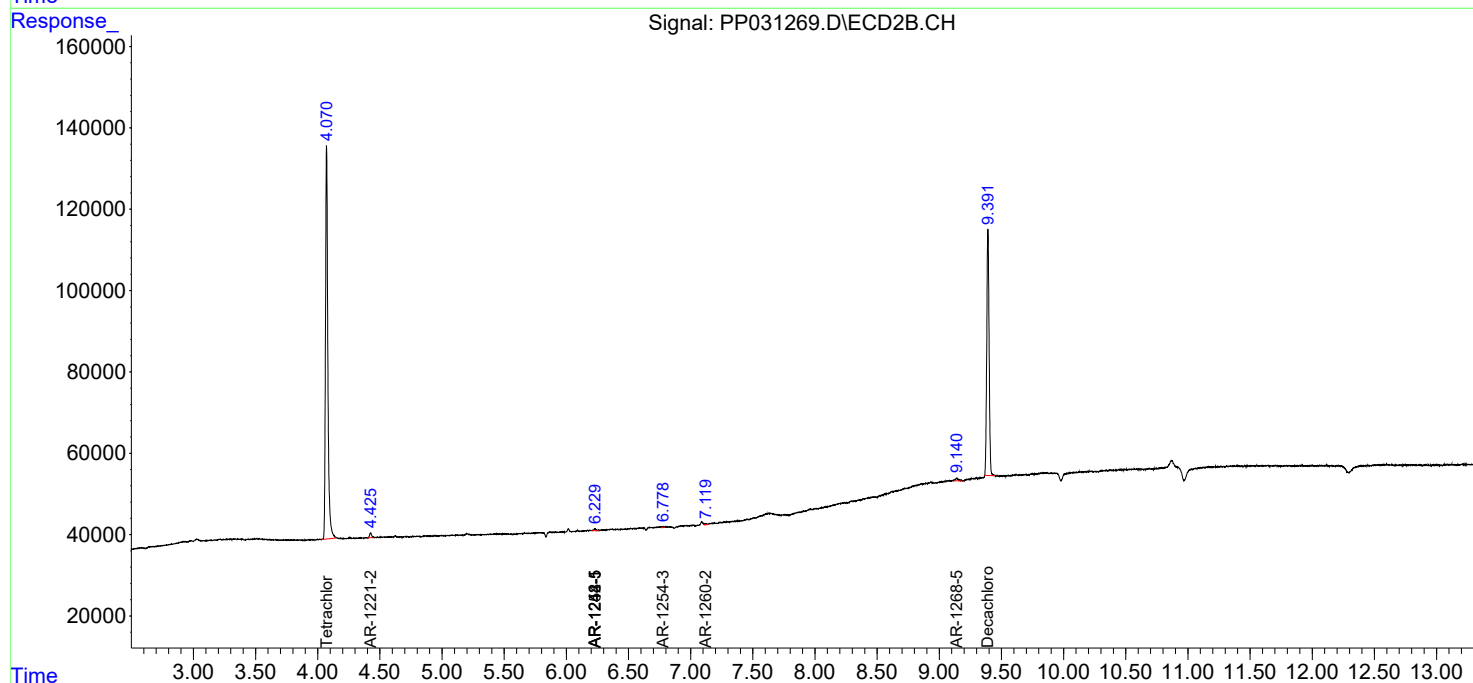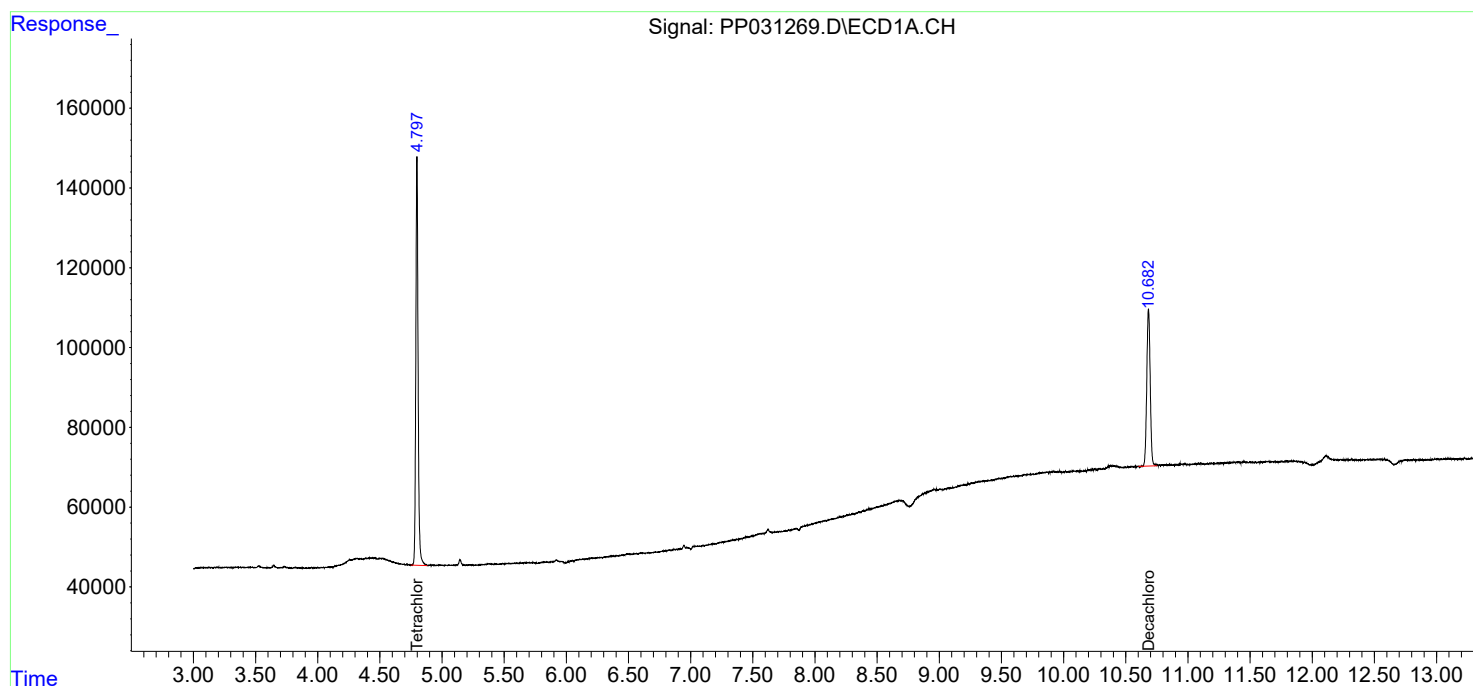


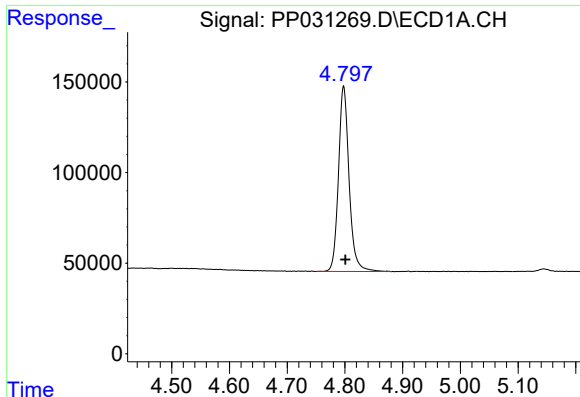

#1 Tetrachloro-m-xylene


R.T.: 4.798 min
Delta R.T.: -0.003 min
Response: 1310496
Conc: 19.62 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

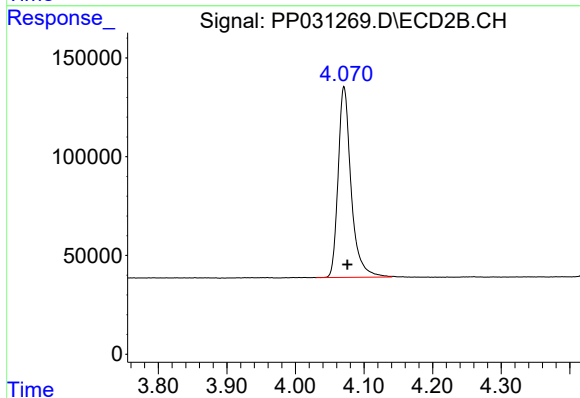


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.005 min
Response: 1269050
Conc: 19.09 ng/ml

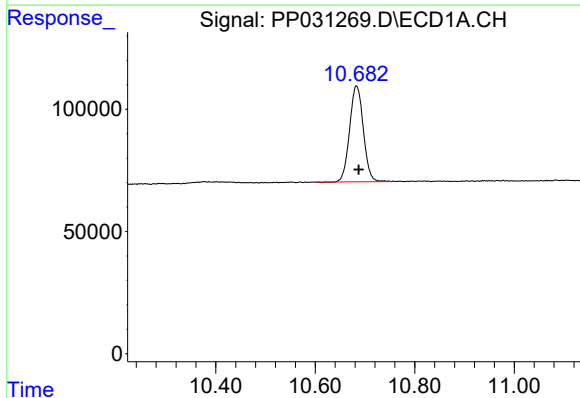


#2 Decachlorobiphenyl

R.T.: 10.683 min
Delta R.T.: -0.005 min
Response: 751958
Conc: 18.81 ng/ml

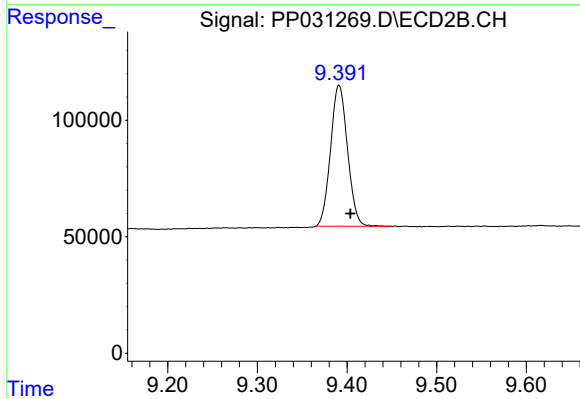

#2 Decachlorobiphenyl


R.T.: 9.391 min
Delta R.T.: -0.013 min
Response: 793773
Conc: 19.01 ng/ml

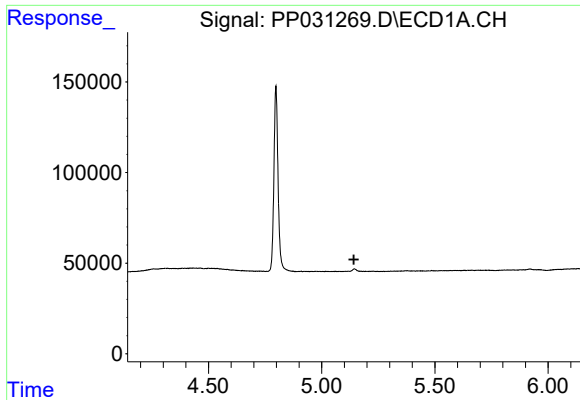

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

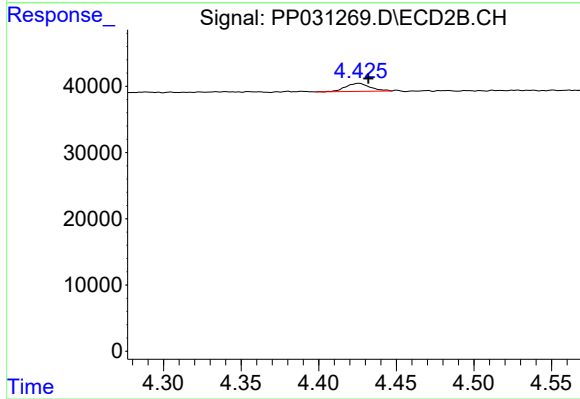


#9 AR-1221-2

R.T.: 4.426 min
Delta R.T.: -0.006 min
Response: 13174
Conc: 30.77 ng/ml

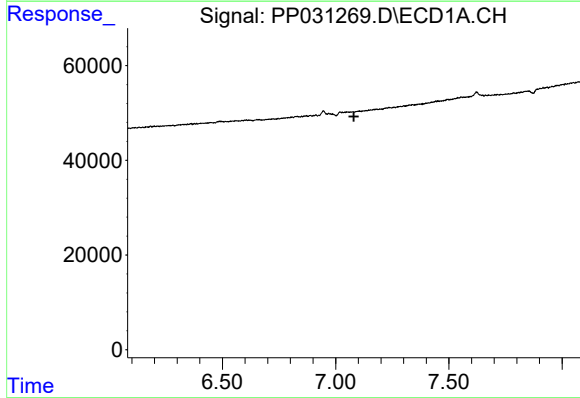


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.081 min
Response: 0
Conc: N.D.

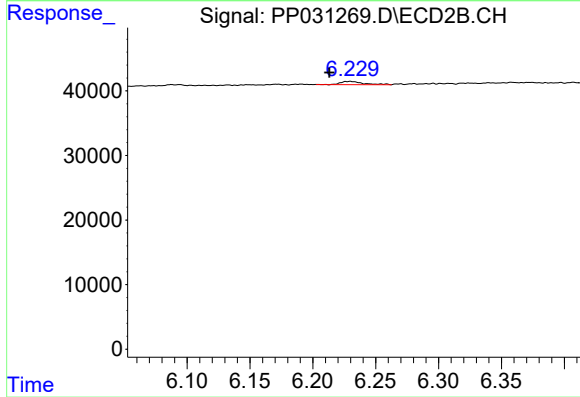

#20 AR-1242-5


R.T.: 6.230 min
Delta R.T.: 0.017 min
Response: 6145
Conc: 6.17 ng/ml

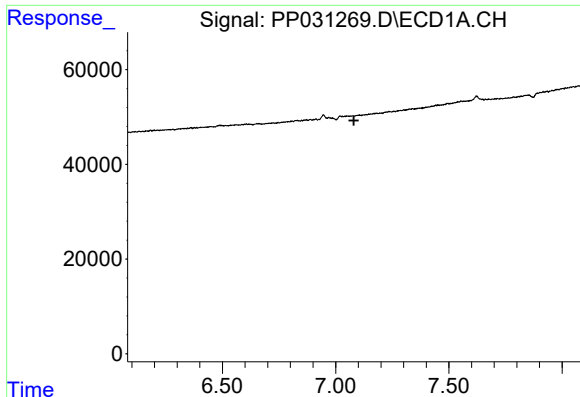

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.080 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

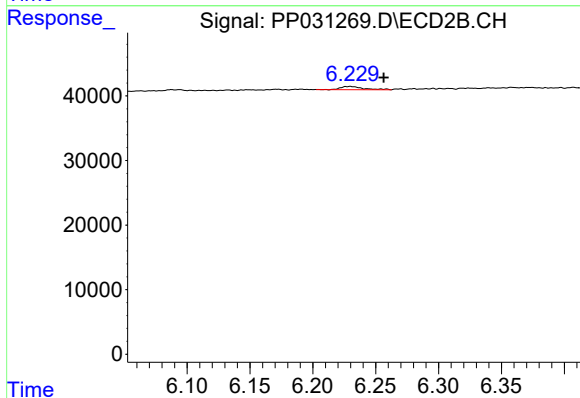


#25 AR-1248-5

R.T.: 6.230 min
Delta R.T.: -0.027 min
Response: 6145
Conc: 4.87 ng/ml

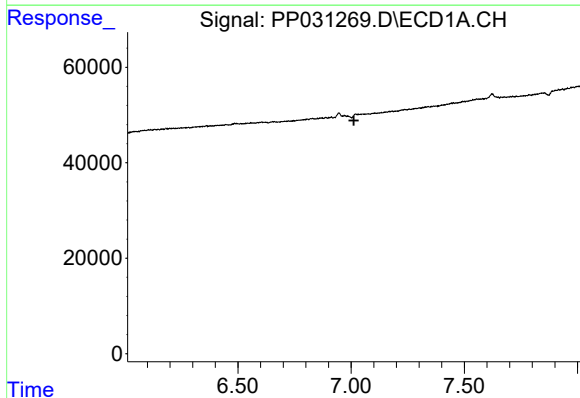


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.013 min
Response: 0
Conc: N.D.

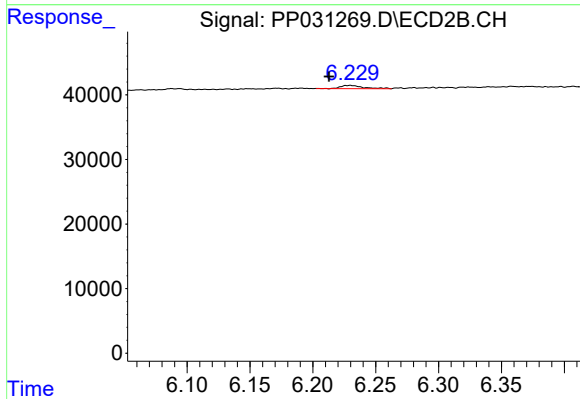

#26 AR-1254-1


R.T.: 6.230 min
Delta R.T.: 0.017 min
Response: 6145
Conc: 3.12 ng/ml

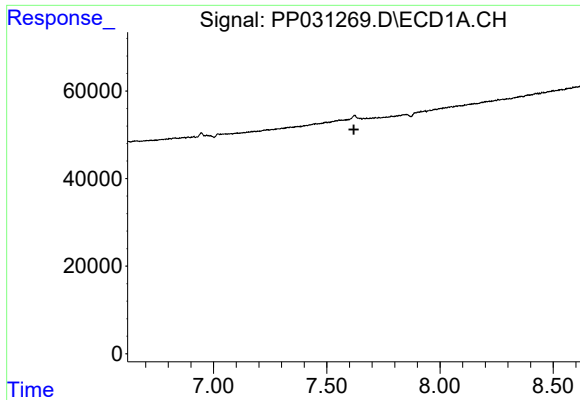

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 7.620 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

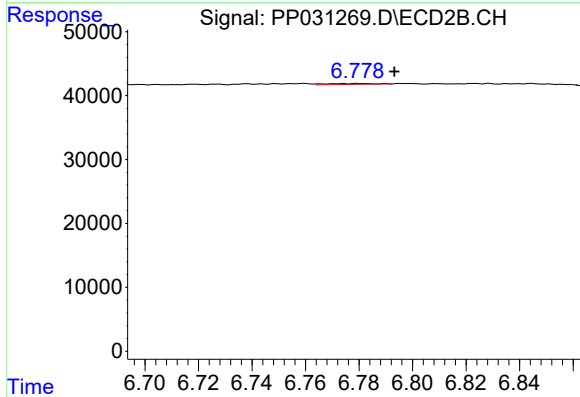


#28 AR-1254-3

R.T.: 6.780 min
Delta R.T.: -0.014 min
Response: 1688
Conc: 0.62 ng/ml

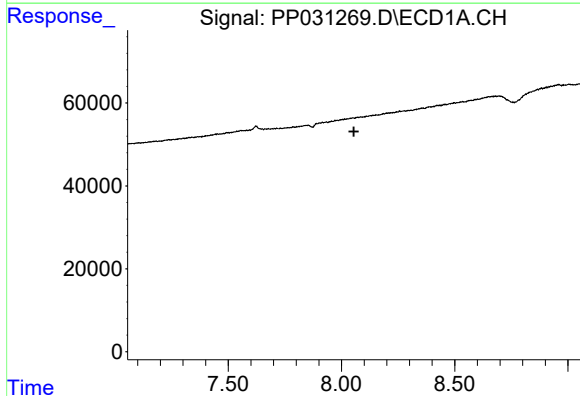


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.054 min
Response: 0
Conc: N.D.

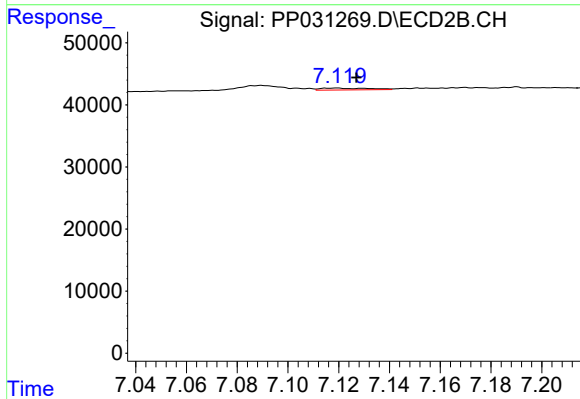

#32 AR-1260-2


R.T.: 7.119 min
Delta R.T.: -0.008 min
Response: 3822
Conc: 1.63 ng/ml

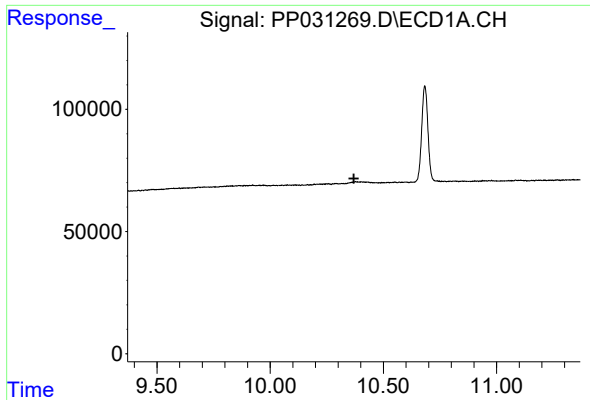

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

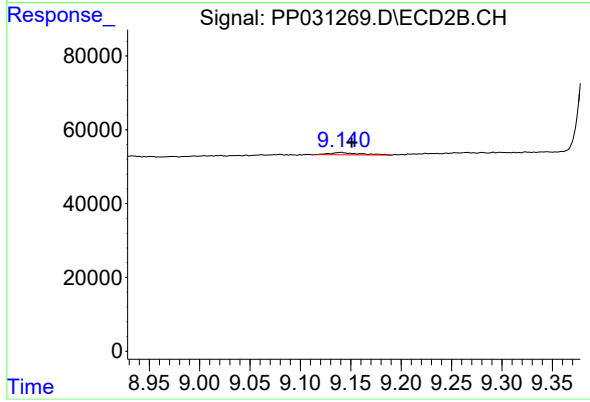

#45 AR-1268-5

R.T.: 9.140 min
Delta R.T.: -0.011 min
Response: 12300
Conc: 0.92 ng/ml