

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111320\
 Data File : PP031270.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 13 Nov 2020 14:49
 Operator : DD\AJ
 Sample : L4719-11
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 TP-3A-S

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 15:34:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 05 13:03:18 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.797	4.071	1467506	1419005	21.971	21.348
2)	SA Decachlor...	10.682	9.391	751506	792217	18.795	18.972
Target Compounds							
9)	L2 AR-1221-2	0.000	4.426	0	18028	N.D.	42.105 #
30)	L6 AR-1254-5	0.000	7.452	0	6949	N.D.	3.174 #
35)	L7 AR-1260-5	0.000	8.001	0	1483	N.D.	0.329 #
36)	L8 AR-1262-1	0.000	7.498	0	2812	N.D.	1.211 #
37)	L8 AR-1262-2	0.000	8.001	0	1483	N.D.	0.358 #
38)	L8 AR-1262-3	0.000	8.292	0	5464	N.D.	3.223 #
39)	L8 AR-1262-4	0.000	8.365	0	2017	N.D.	0.635 #
40)	L8 AR-1262-5	0.000	8.851	0	1865	N.D.	1.161 #
41)	L9 AR-1268-1	0.000	8.292	0	5464	N.D.	1.116 #
42)	L9 AR-1268-2	0.000	8.365	0	2017	N.D.	0.424 #
43)	L9 AR-1268-3	0.000	8.567	0	2003	N.D.	0.501 #
44)	L9 AR-1268-4	0.000	8.851	0	1865	N.D.	1.101 #
45)	L9 AR-1268-5	0.000	9.142	0	2910	N.D.	0.217 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111320\
Data File : PP031270.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 13 Nov 2020 14:49
Operator : DD\AJ
Sample : L4719-11
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
TP-3A-S

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 15:34:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110420.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 05 13:03:18 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

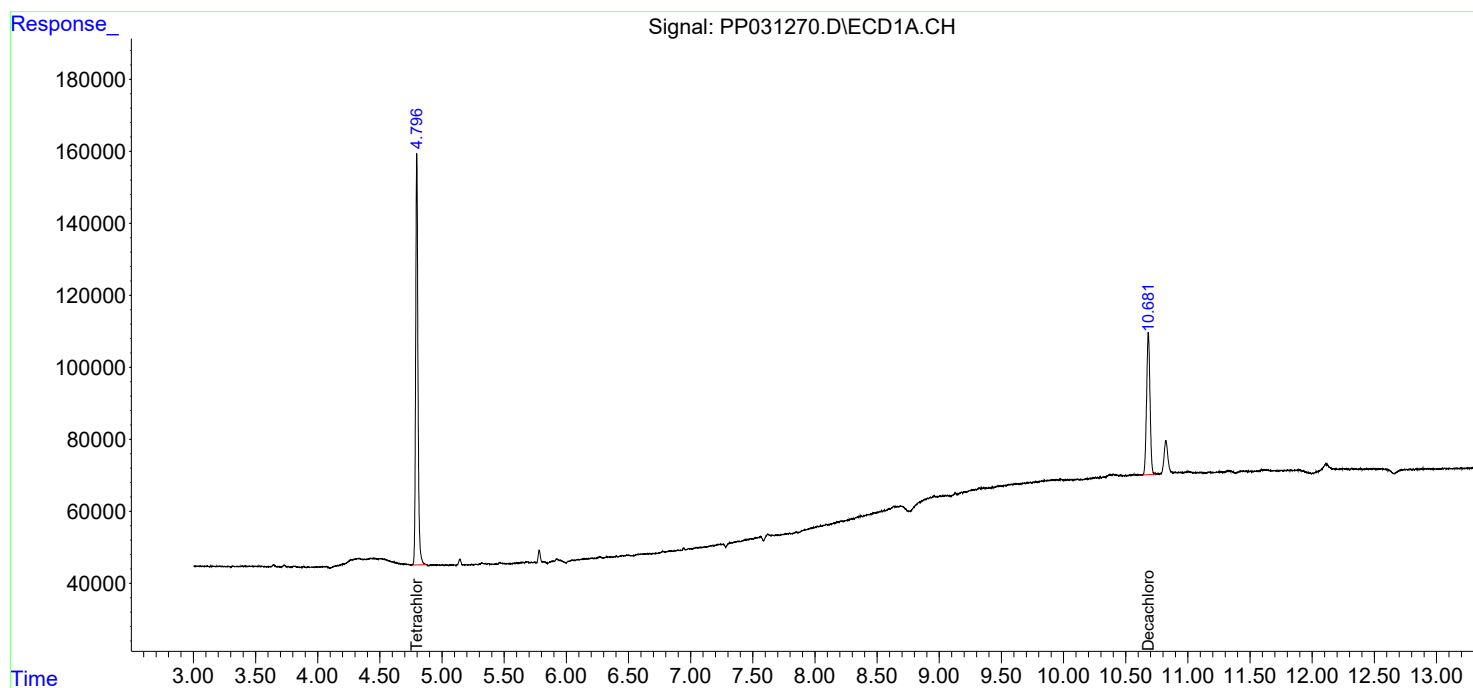


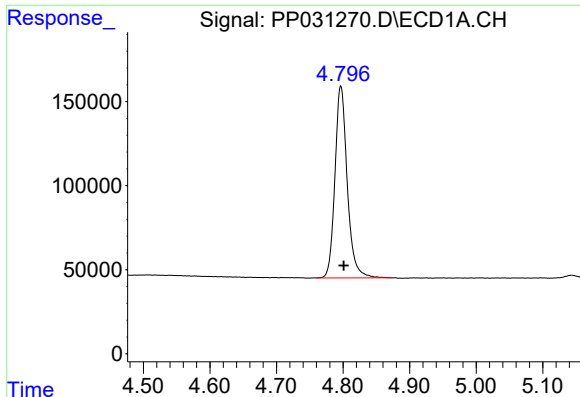

#1 Tetrachloro-m-xylene


R.T.: 4.797 min
Delta R.T.: -0.004 min
Response: 1467506
Conc: 21.97 ng/ml

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

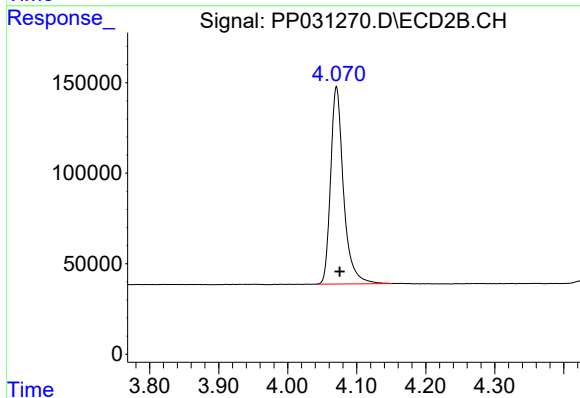


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.005 min
Response: 1419005
Conc: 21.35 ng/ml

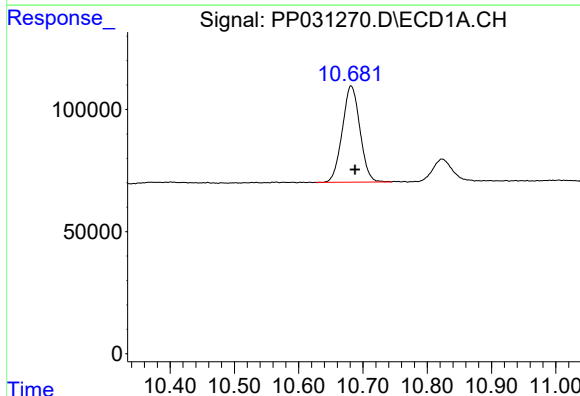


#2 Decachlorobiphenyl

R.T.: 10.682 min
Delta R.T.: -0.006 min
Response: 751506
Conc: 18.80 ng/ml

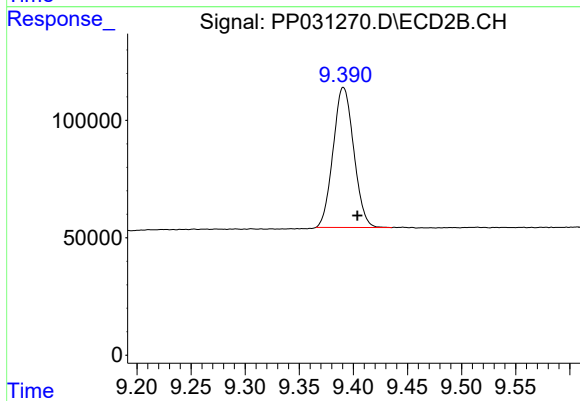

#2 Decachlorobiphenyl


R.T.: 9.391 min
Delta R.T.: -0.013 min
Response: 792217
Conc: 18.97 ng/ml

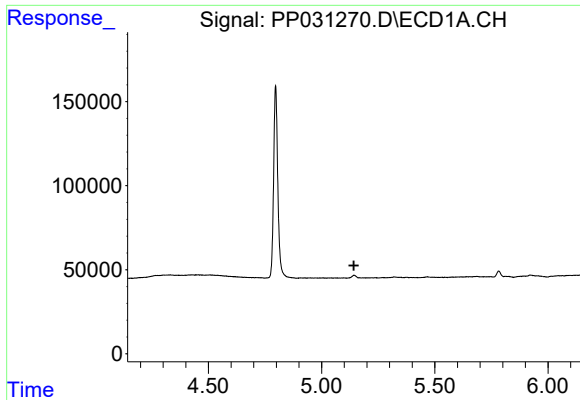

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.143 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

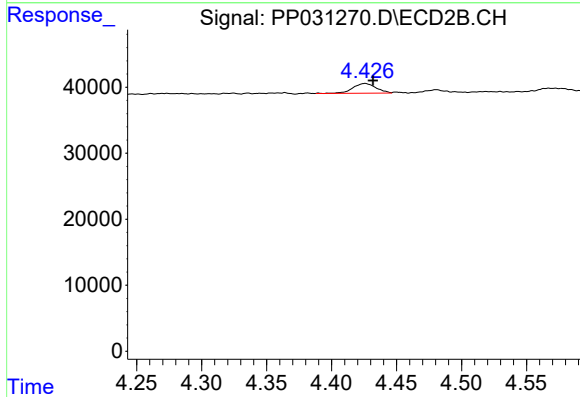


#9 AR-1221-2

R.T.: 4.426 min
Delta R.T.: -0.006 min
Response: 18028
Conc: 42.10 ng/ml

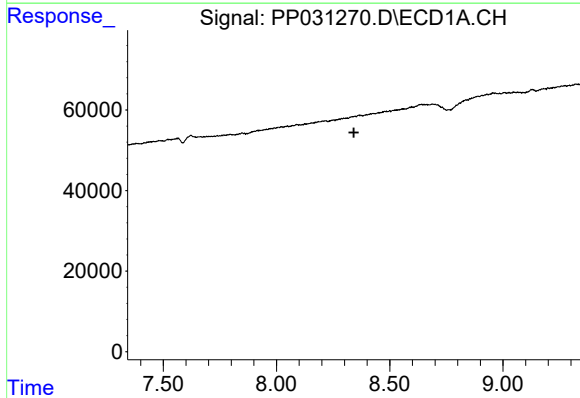


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T.: 8.341 min
Response: 0
Conc: N.D.

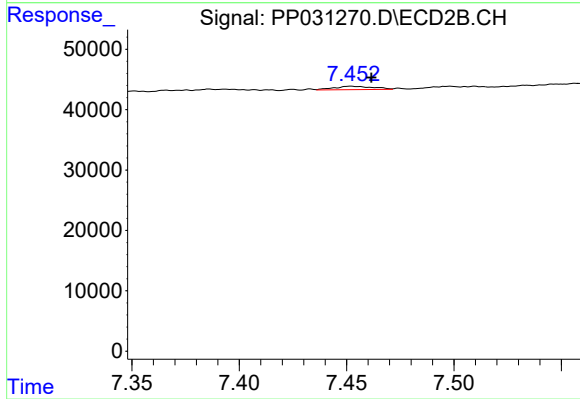

#30 AR-1254-5


R.T.: 7.452 min
Delta R.T.: -0.009 min
Response: 6949
Conc: 3.17 ng/ml

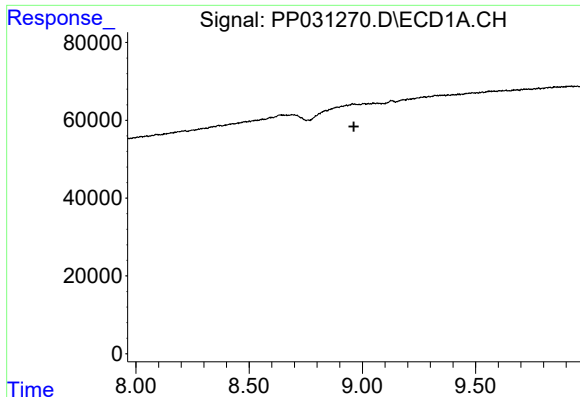

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.962 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

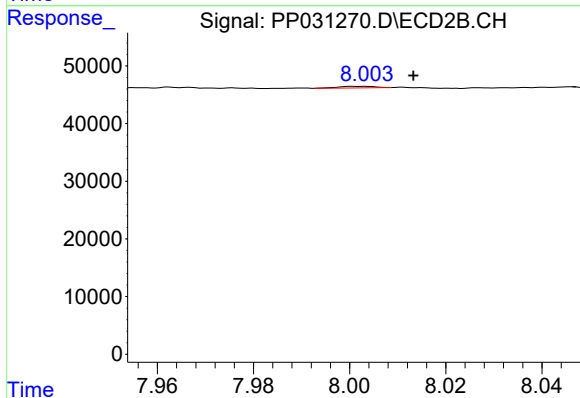


#35 AR-1260-5

R.T.: 8.001 min
Delta R.T.: -0.013 min
Response: 1483
Conc: 0.33 ng/ml

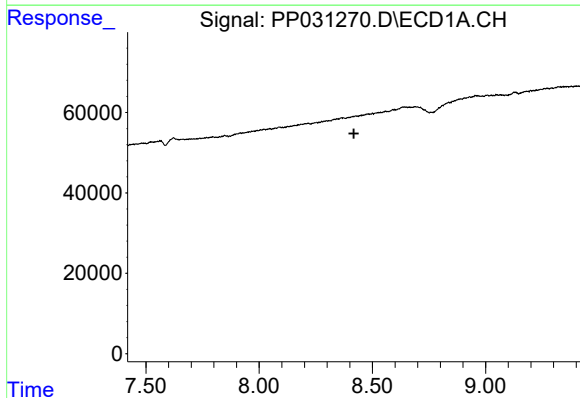


#36 AR-1262-1

R.T.: 0.000 min
Exp R.T. : 8.419 min
Response: 0
Conc: N.D.

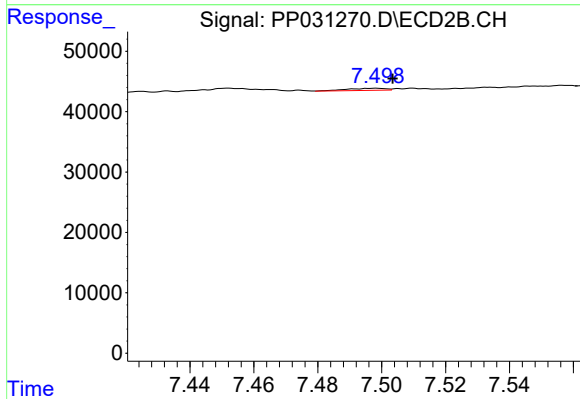

#36 AR-1262-1


R.T.: 7.498 min
Delta R.T.: -0.005 min
Response: 2812
Conc: 1.21 ng/ml

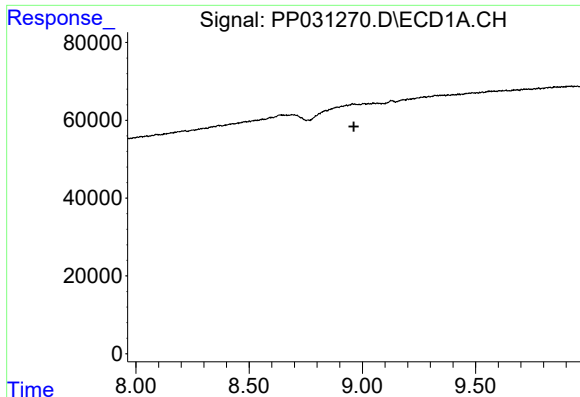

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T. : 8.963 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

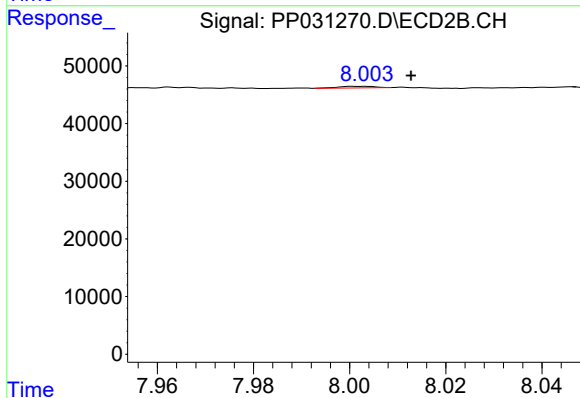


#37 AR-1262-2

R.T.: 8.001 min
Delta R.T.: -0.012 min
Response: 1483
Conc: 0.36 ng/ml

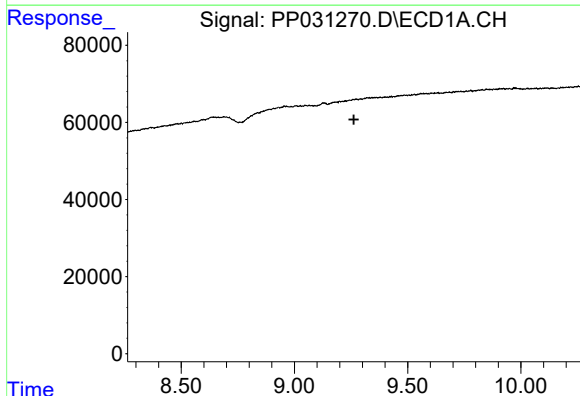


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T. : 9.262 min
Response: 0
Conc: N.D.

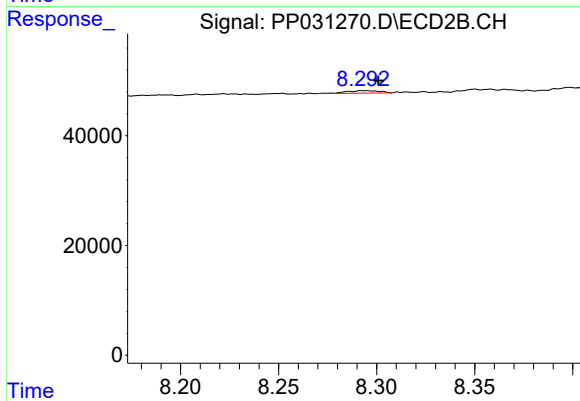

#38 AR-1262-3


R.T.: 8.292 min
Delta R.T.: -0.009 min
Response: 5464
Conc: 3.22 ng/ml

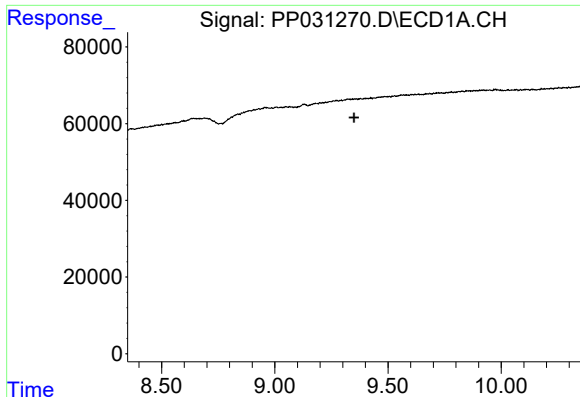

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.350 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

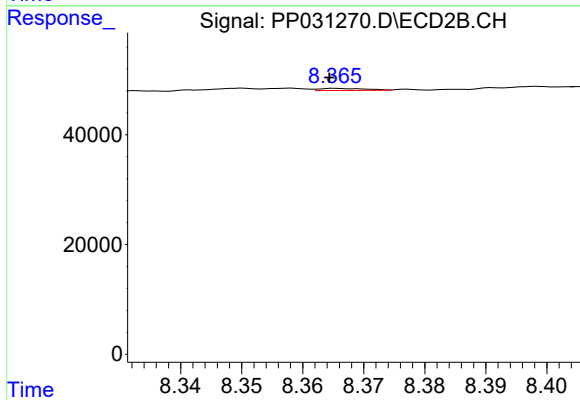


#39 AR-1262-4

R.T.: 8.365 min
Delta R.T.: 0.001 min
Response: 2017
Conc: 0.64 ng/ml

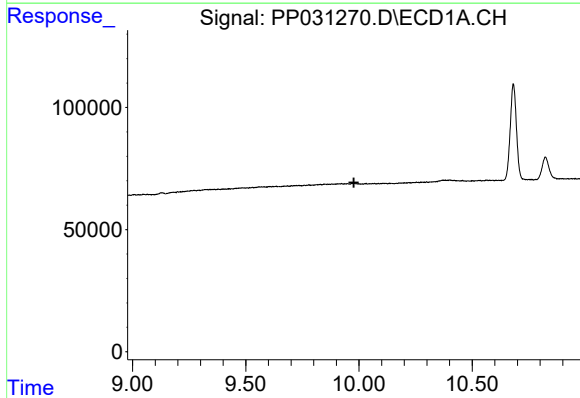


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.978 min
Response: 0
Conc: N.D.

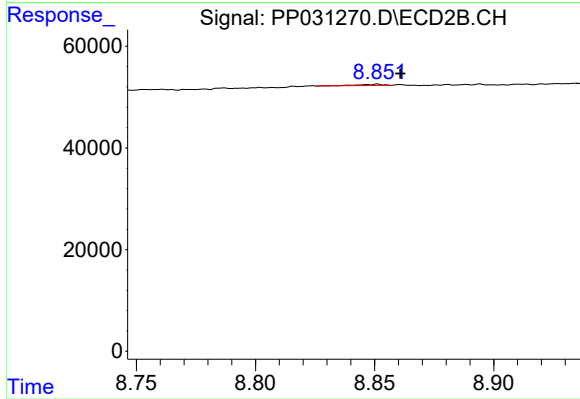

#40 AR-1262-5


R.T.: 8.851 min
Delta R.T.: -0.009 min
Response: 1865
Conc: 1.16 ng/ml

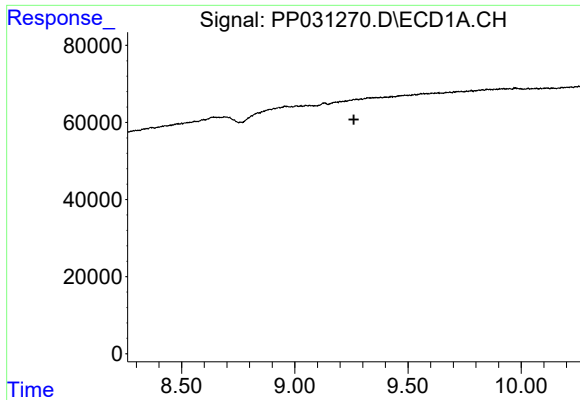

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.261 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

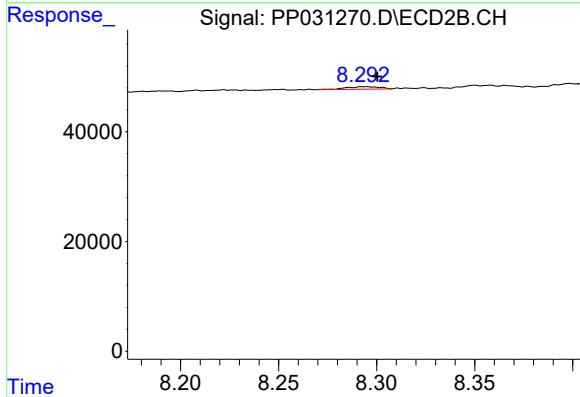


#41 AR-1268-1

R.T.: 8.292 min
Delta R.T.: -0.008 min
Response: 5464
Conc: 1.12 ng/ml

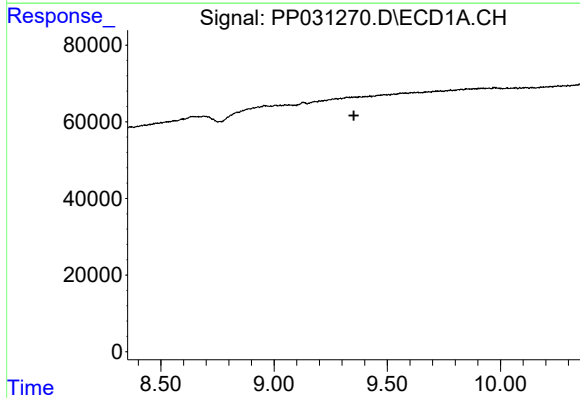


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T. : 9.352 min
Response: 0
Conc: N.D.

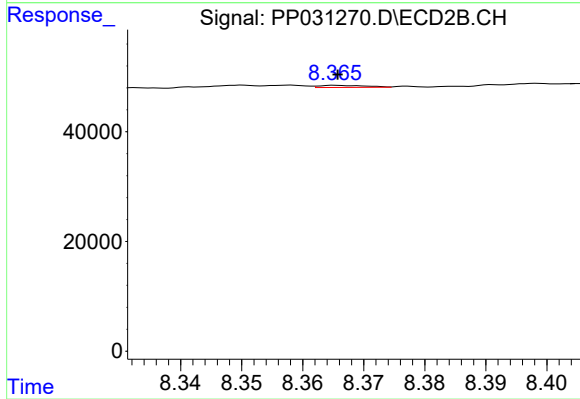

#42 AR-1268-2


R.T.: 8.365 min
Delta R.T.: 0.000 min
Response: 2017
Conc: 0.42 ng/ml

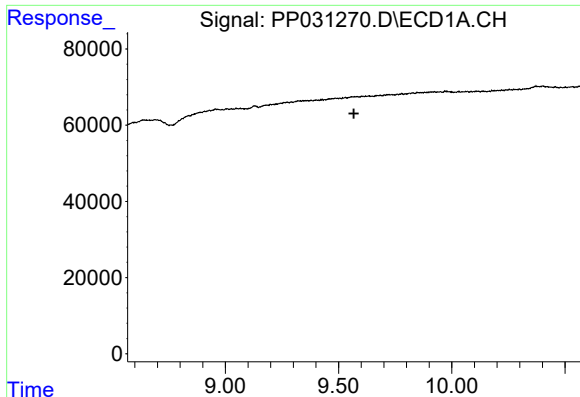

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.568 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

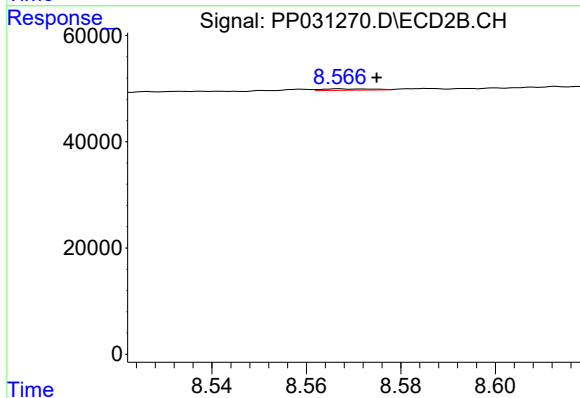


#43 AR-1268-3

R.T.: 8.567 min
Delta R.T.: -0.008 min
Response: 2003
Conc: 0.50 ng/ml

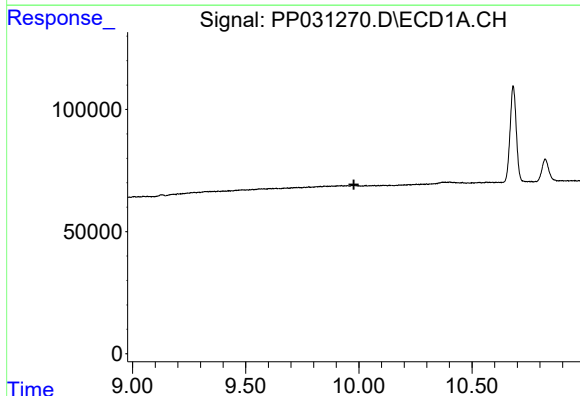


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.978 min
Response: 0
Conc: N.D.

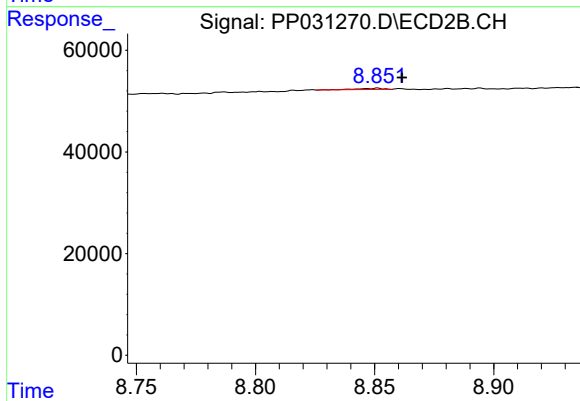

#44 AR-1268-4


R.T.: 8.851 min
Delta R.T.: -0.010 min
Response: 1865
Conc: 1.10 ng/ml

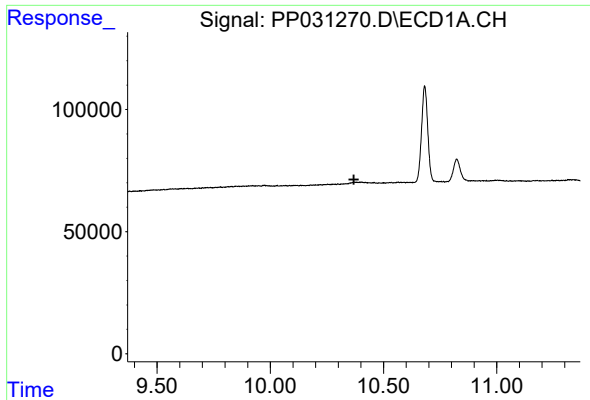

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.369 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
TP-3A-S

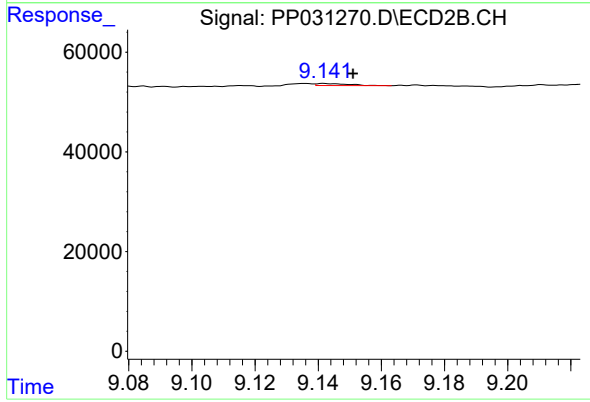

#45 AR-1268-5

R.T.: 9.142 min
Delta R.T.: -0.009 min
Response: 2910
Conc: 0.22 ng/ml