

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
 Data File : PP061623.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2023 09:14
 Operator : YP\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 11:03:59 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 13 03:41:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

7) L1	AR-1016-5	0.000	5.356	0	15397	N.D.	0.254 #
15) L3	AR-1232-5	0.000	5.356	0	15397	N.D.	0.578 #
24) L5	AR-1248-4	0.000	5.356	0	15397	N.D.	0.189 #
28) L6	AR-1254-3	7.140	0.000	446855	0	7.089	N.D. #
32) L7	AR-1260-2	0.000	6.584f	0	755541	N.D.	5.455 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
Data File : PP061623.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2023 09:14
Operator : YP\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 11:03:59 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 13 03:41:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

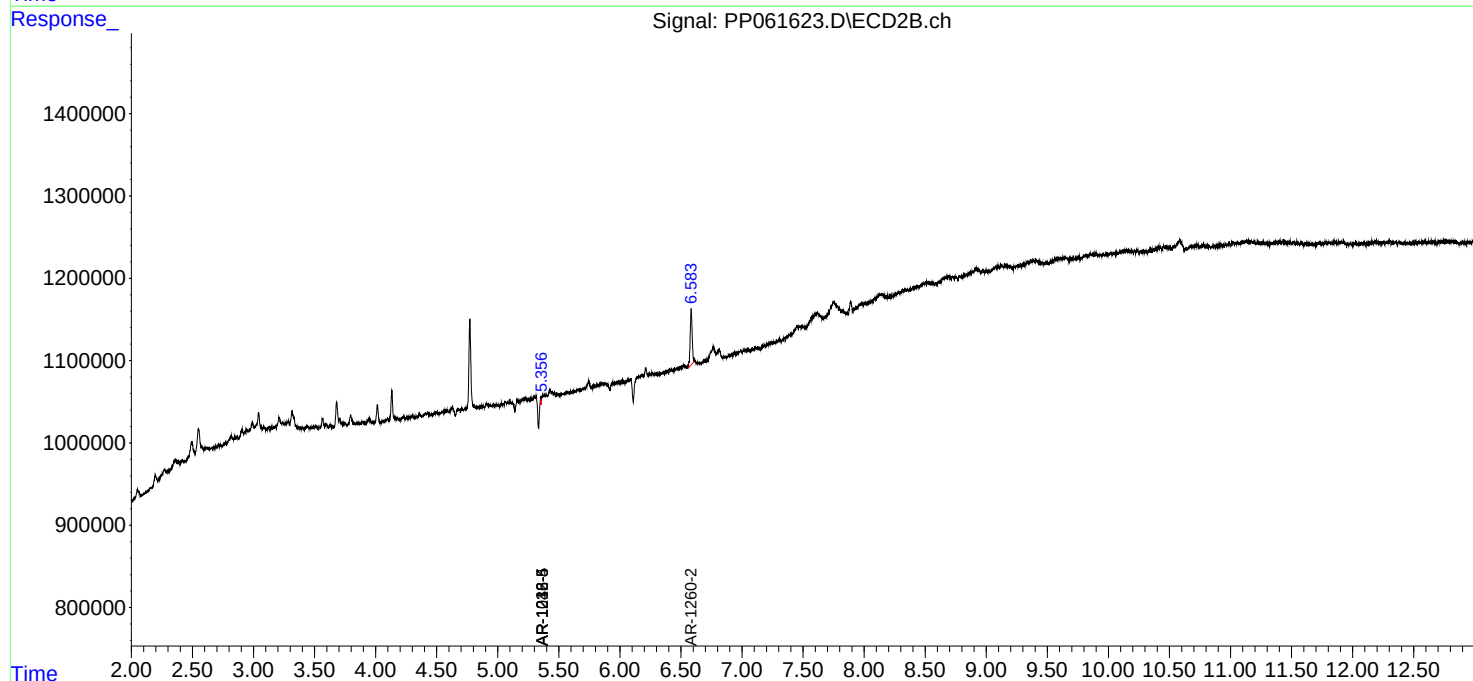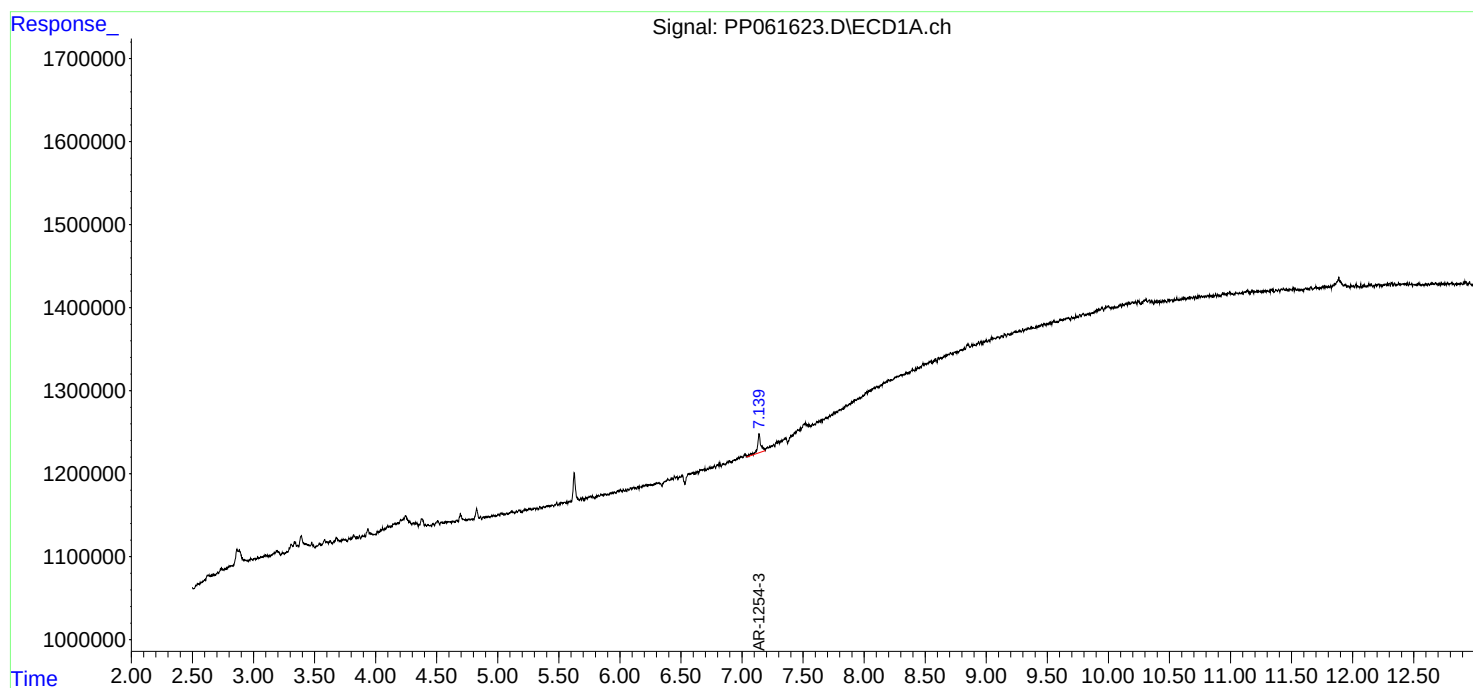


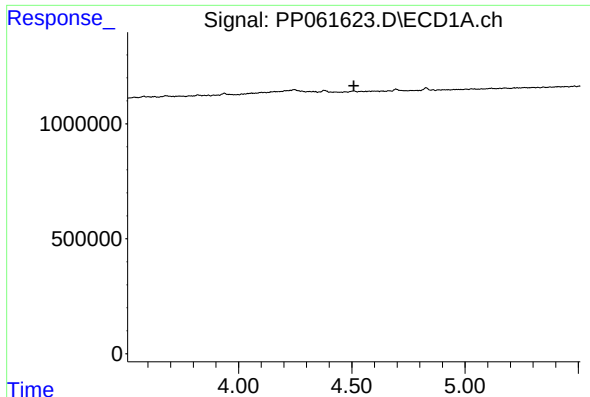

#1 Tetrachloro-m-xylene


R.T.: 0.000 min
Exp R.T. : 4.509 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

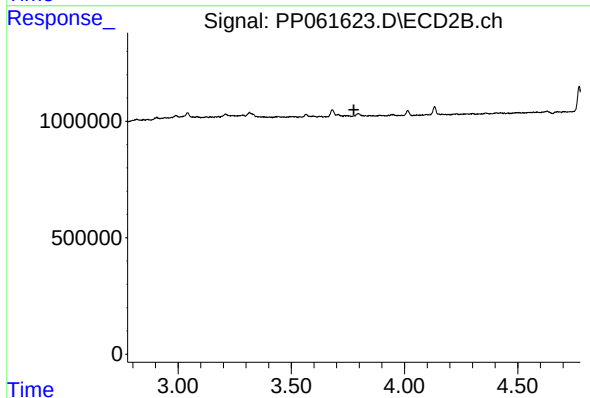


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.776 min
Response: 0
Conc: N.D.

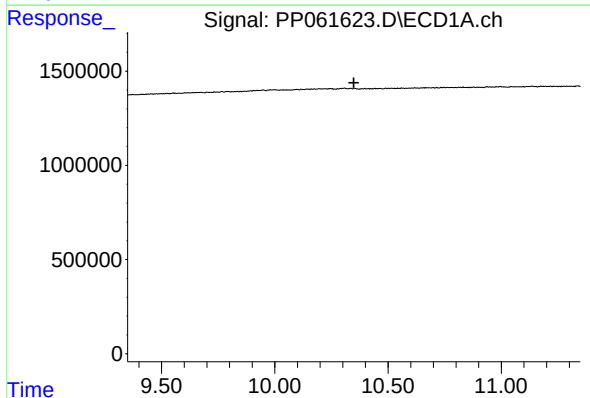


#2 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 10.349 min
Response: 0
Conc: N.D.

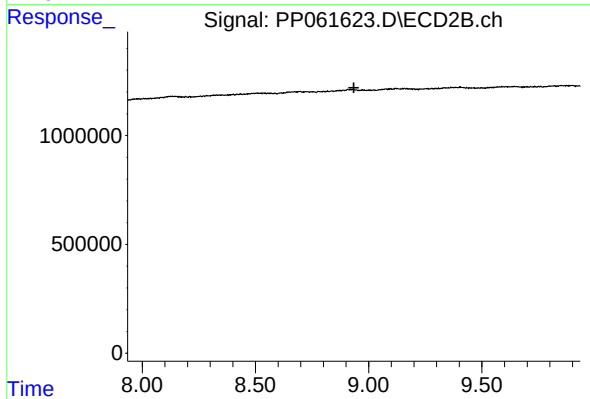

#2 Decachlorobiphenyl


R.T.: 0.000 min
Exp R.T. : 8.935 min
Response: 0
Conc: N.D.

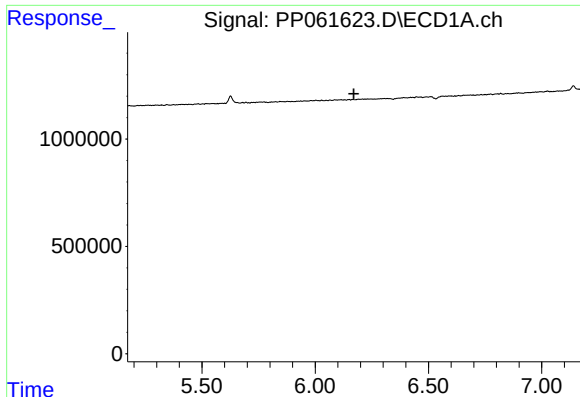

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.170 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

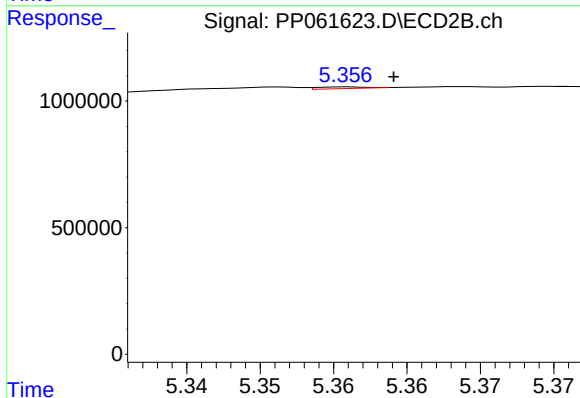


#7 AR-1016-5

R.T.: 5.356 min
Delta R.T.: -0.003 min
Response: 15397
Conc: 0.25 ng/ml

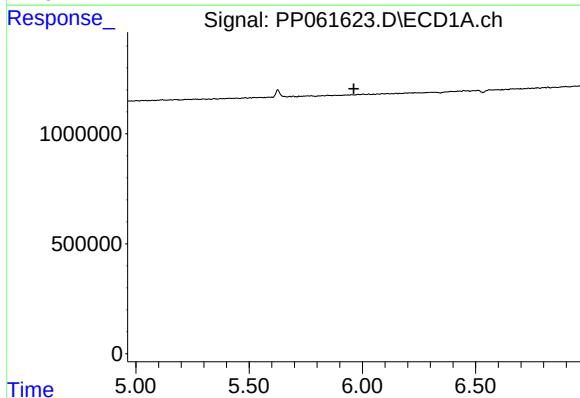


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T.: 5.962 min
Response: 0
Conc: N.D.

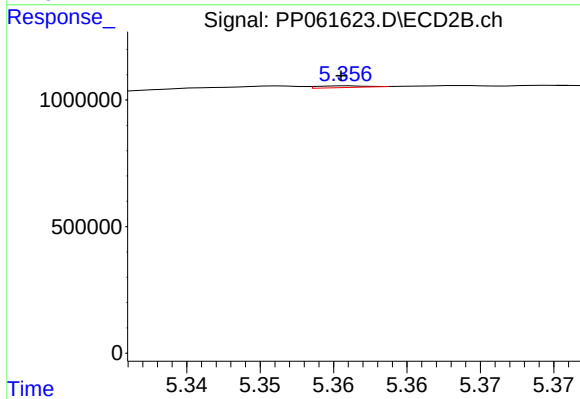

#15 AR-1232-5


R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 15397
Conc: 0.58 ng/ml

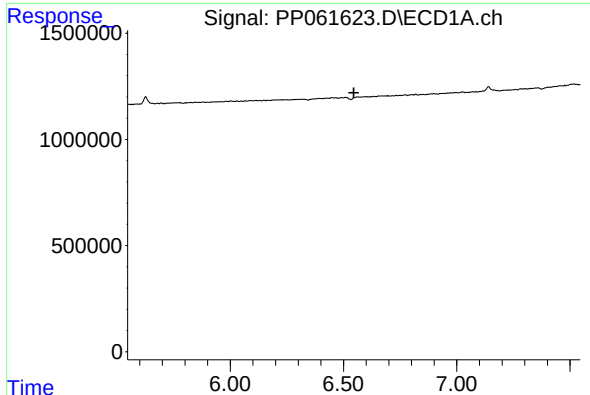

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T.: 6.546 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

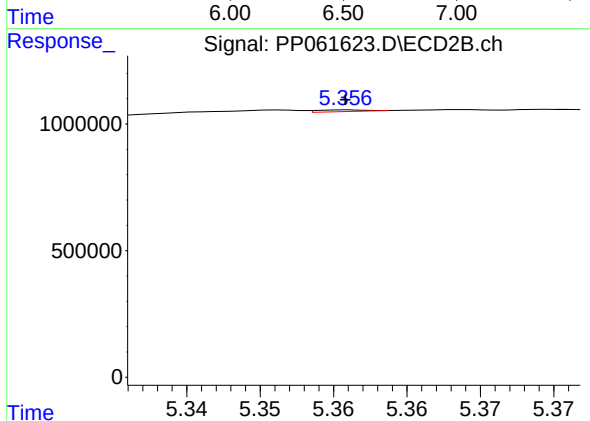


#24 AR-1248-4

R.T.: 5.356 min
Delta R.T.: 0.000 min
Response: 15397
Conc: 0.19 ng/ml

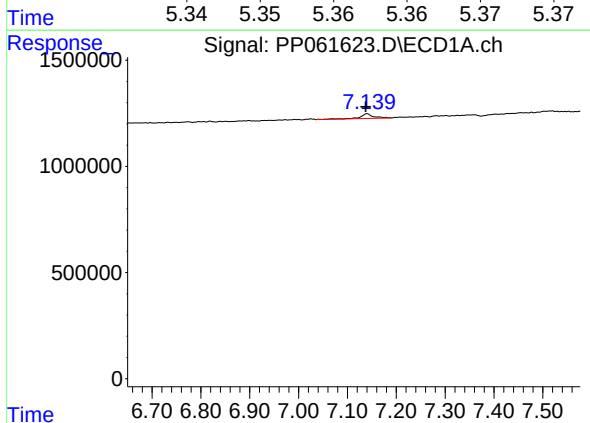


#28 AR-1254-3

R.T.: 7.140 min
Delta R.T.: 0.002 min
Response: 446855
Conc: 7.09 ng/ml

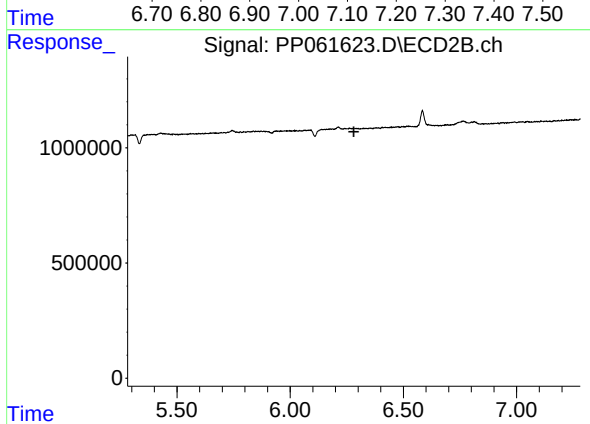

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T.: 6.282 min
Response: 0
Conc: N.D.

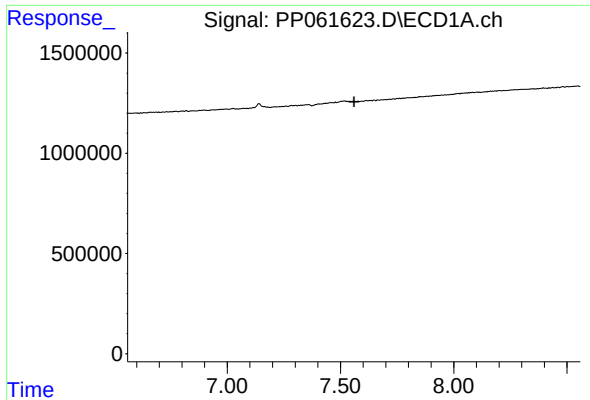

#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.560 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

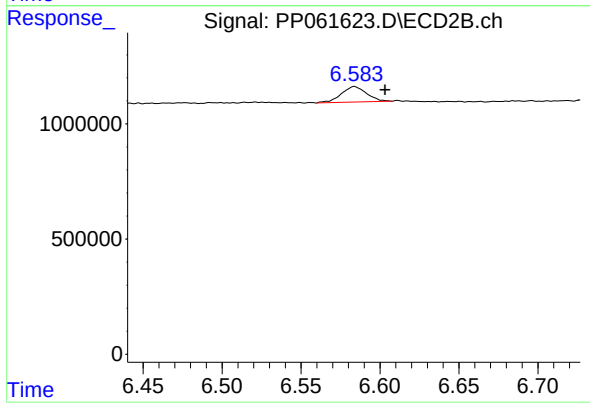

#32 AR-1260-2

R.T.: 6.584 min
Delta R.T.: -0.019 min
Response: 755541
Conc: 5.45 ng/ml