

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
 Data File : PP061656.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2023 18:24
 Operator : YP\AJ
 Sample : 05316-01
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 NWB-1978

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 14 04:29:19 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 13 03:41:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.505	3.772	21939347	34063852	17.826	16.487
2) SA Decachlor...	10.337	8.918	14360439	24273122	16.752	13.346

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
Data File : PP061656.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2023 18:24
Operator : YP\AJ
Sample : 05316-01
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
NWB-1978


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 14 04:29:19 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 13 03:41:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

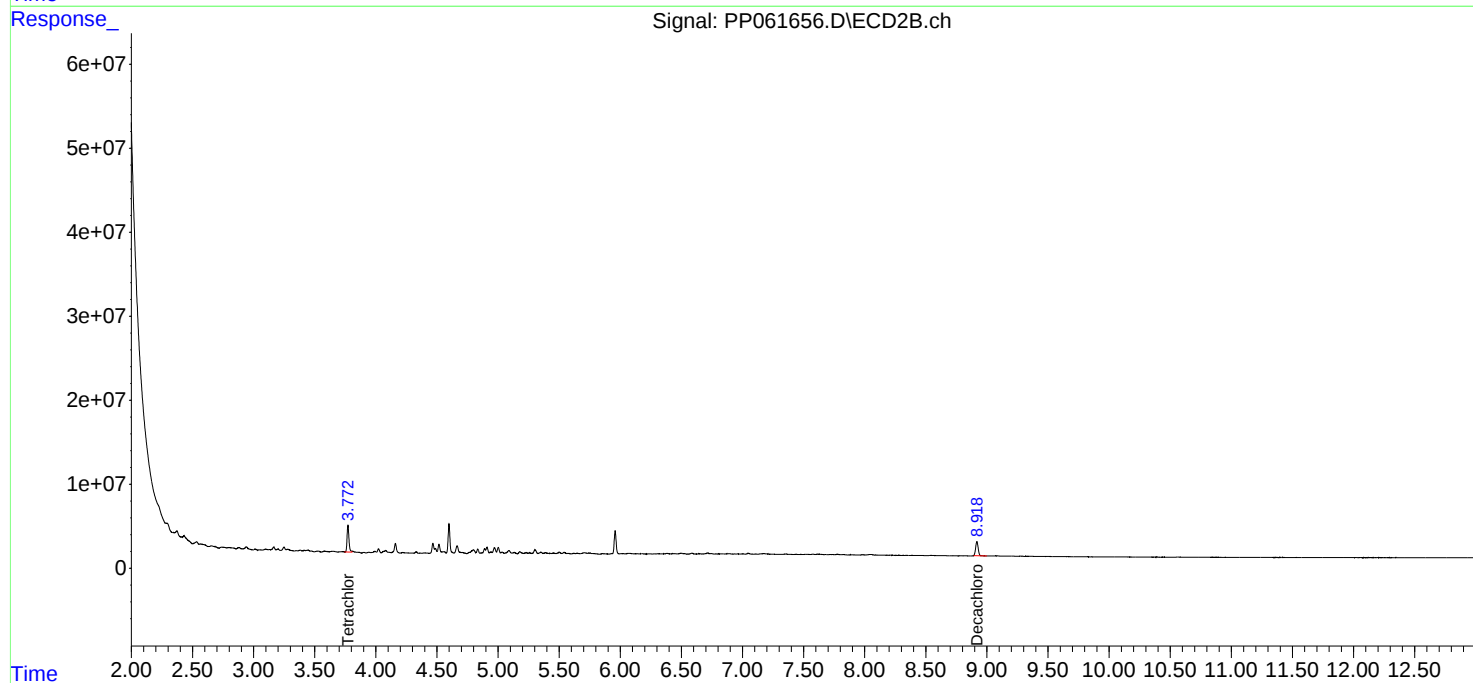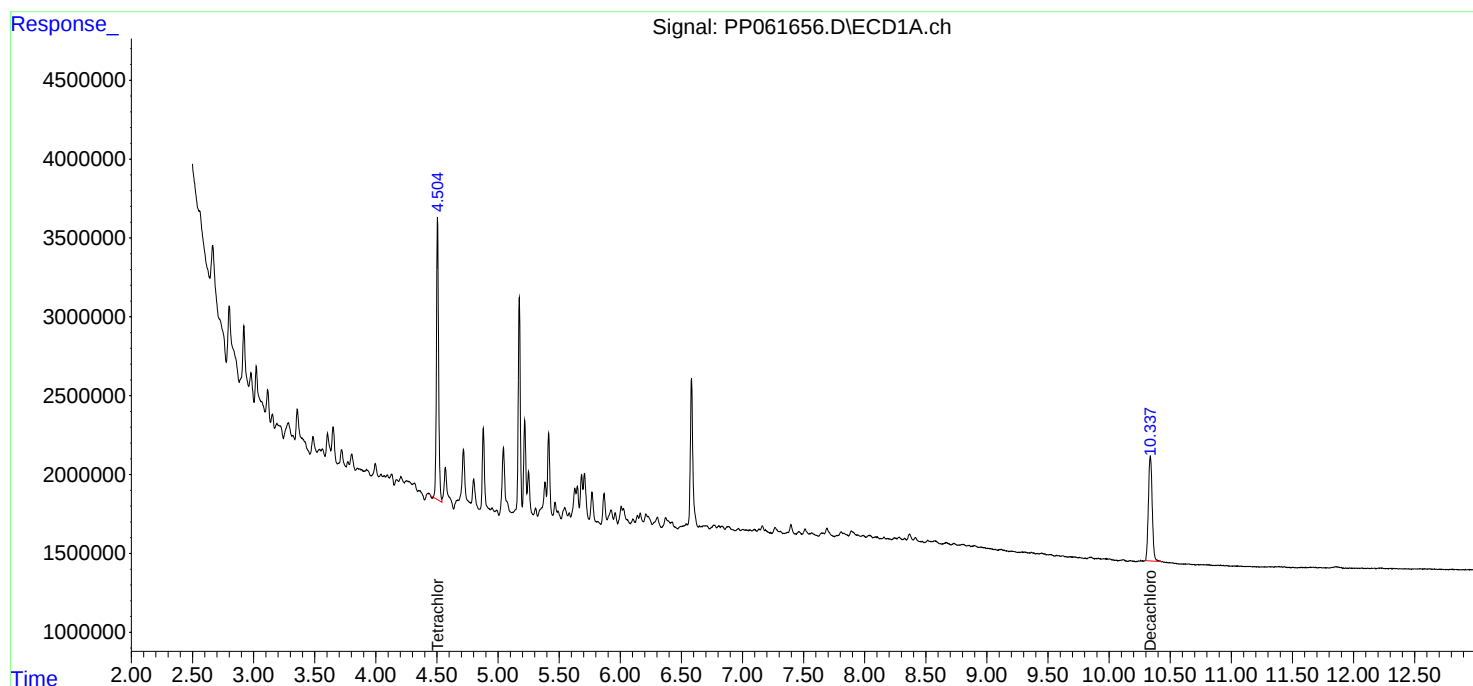

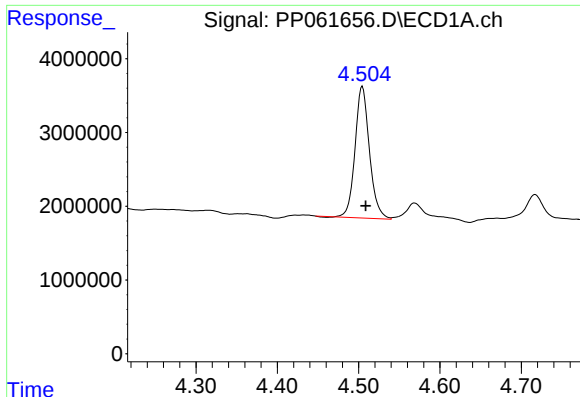


#1 Tetrachloro-m-xylene

R.T.: 4.505 min
Delta R.T.: -0.004 min
Response: 21939347
Conc: 17.83 ng/ml

Instrument :
ECD_P
ClientSampleId :
NWB-1978


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

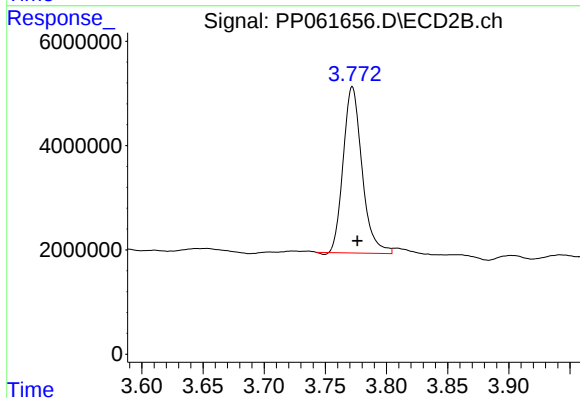


#1 Tetrachloro-m-xylene

R.T.: 3.772 min
Delta R.T.: -0.004 min
Response: 34063852
Conc: 16.49 ng/ml

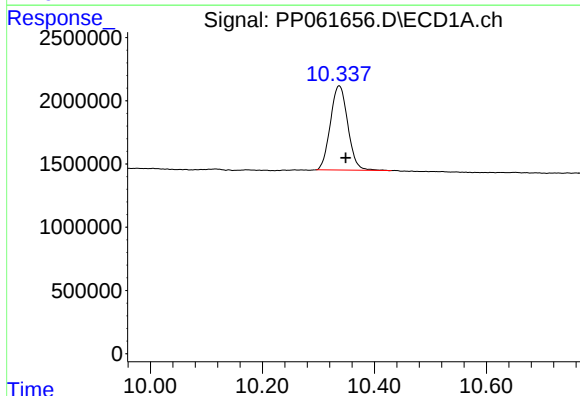

#2 Decachlorobiphenyl

R.T.: 10.337 min
Delta R.T.: -0.012 min
Response: 14360439
Conc: 16.75 ng/ml

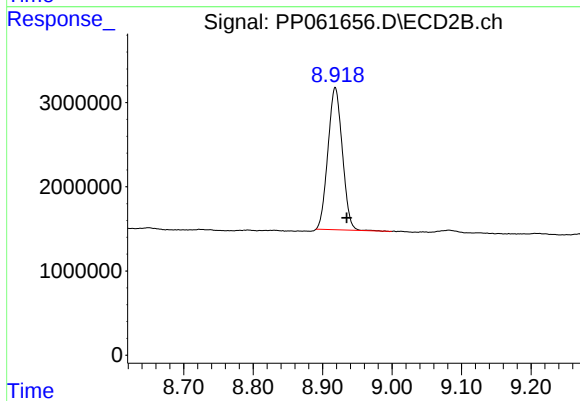

#2 Decachlorobiphenyl

R.T.: 8.918 min
Delta R.T.: -0.017 min
Response: 24273122
Conc: 13.35 ng/ml