

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
 Data File : PP061659.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Nov 2023 19:13
 Operator : YP\AJ
 Sample : 05354-03
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 OILY-WATER-TOTE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/14/2023
 Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 13 20:12:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Mon Nov 13 03:41:25 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.499	3.767	16931502	27165296	13.757	13.148
2) SA Decachlor...	10.325	8.910	8897878	15130931	10.379m	8.319m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111323\
Data File : PP061659.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Nov 2023 19:13
Operator : YP\AJ
Sample : 05354-03
Misc :
ALS Vial : 26 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
OILY-WATER-TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 13 20:12:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111123.M
Quant Title : GC EXTRACTABLES
QLast Update : Mon Nov 13 03:41:25 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

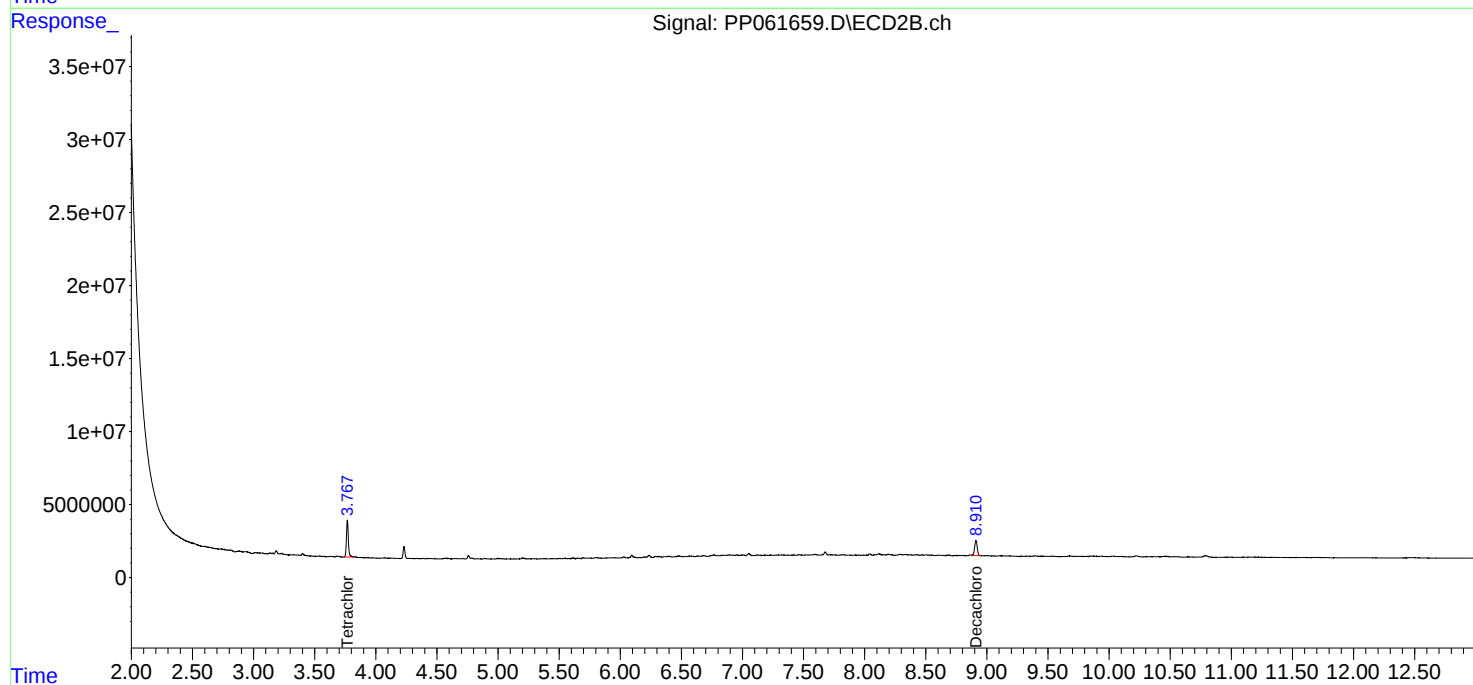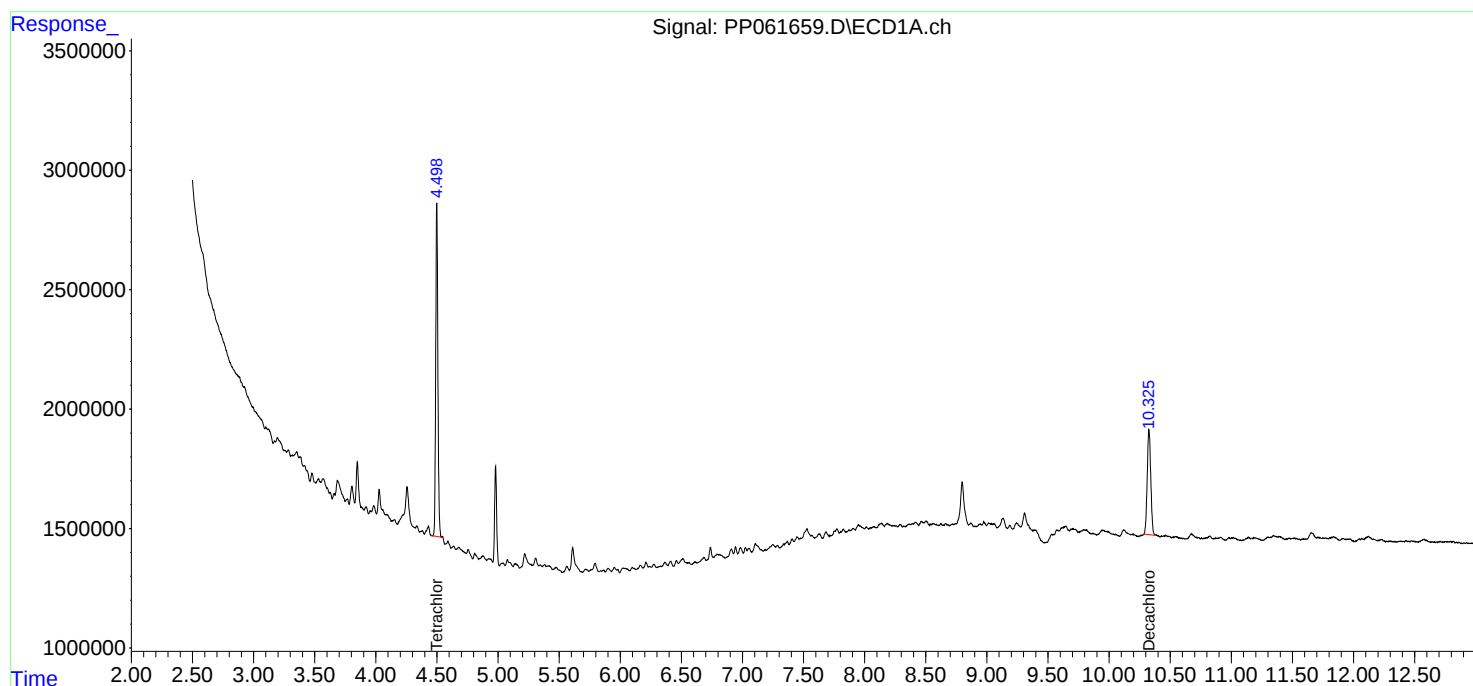

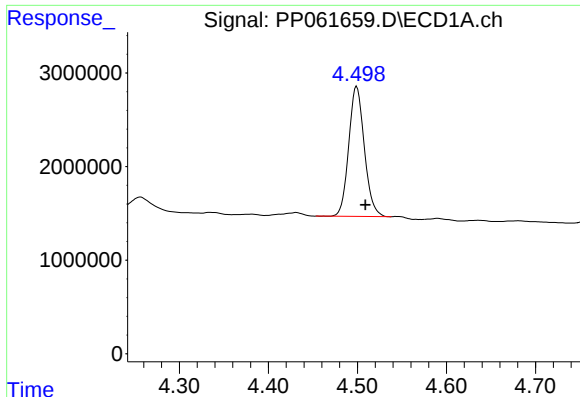


#1 Tetrachloro-m-xylene

R.T.: 4.499 min
Delta R.T.: -0.010 min
Response: 16931502
Conc: 13.76 ng/ml

Instrument :
ECD_P
ClientSampleId :
OILY-WATER-TOTE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/14/2023
Supervised By :Ankita Jodhani 11/14/2023

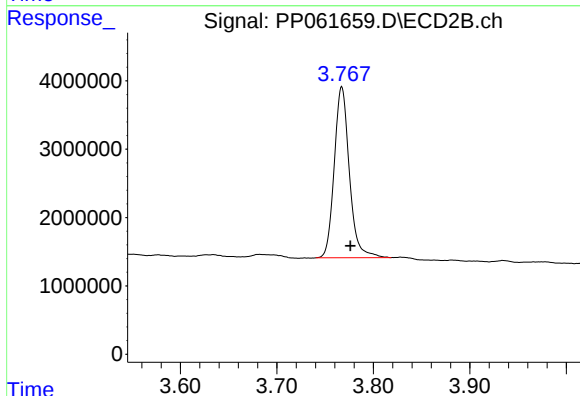


#1 Tetrachloro-m-xylene

R.T.: 3.767 min
Delta R.T.: -0.009 min
Response: 27165296
Conc: 13.15 ng/ml

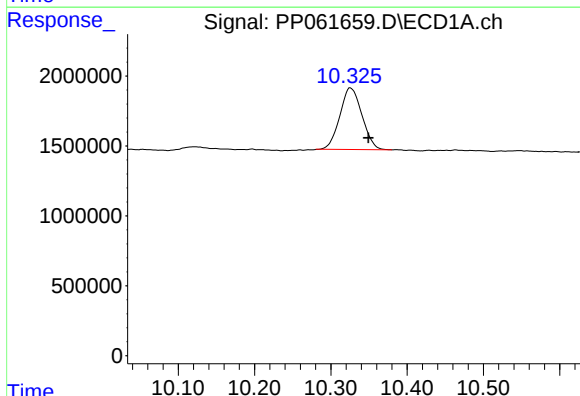

#2 Decachlorobiphenyl

R.T.: 10.325 min
Delta R.T.: -0.025 min
Response: 8897878
Conc: 10.38 ng/ml m

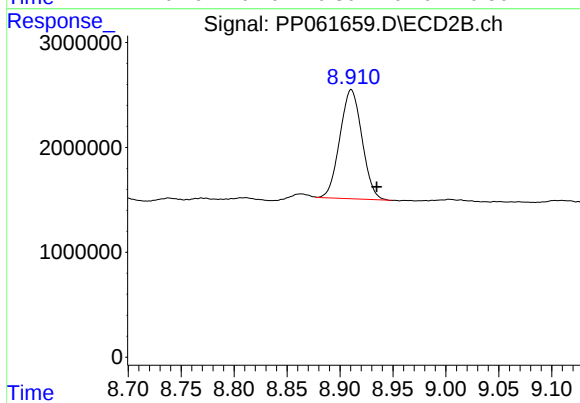

#2 Decachlorobiphenyl

R.T.: 8.910 min
Delta R.T.: -0.025 min
Response: 15130931
Conc: 8.32 ng/ml m