

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
 Data File : PP068488.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2024 12:17
 Operator : YP\AJ
 Sample : P4858-02 10X
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BC258780-1-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 01:34:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.758	4.050	1602375	1430985	1.651	1.478
2)	SA Decachlor...	10.677	9.208	2477203	1682191	1.979	1.487
Target Compounds							
27)	L6 AR-1254-2	7.026	0.000	152423	0	2.234	N.D. #
28)	L6 AR-1254-3	7.313f	0.000	28161	0	0.394	N.D. #
30)	L6 AR-1254-5	0.000	7.177	0	78340	N.D.	1.050 #
32)	L7 AR-1260-2	0.000	6.826	0	127000	N.D.	1.917 #
36)	L8 AR-1262-1	0.000	7.177f	0	78340	N.D.	1.010 #
39)	L8 AR-1262-4	9.150	8.094	108398	52494	1.419	0.507 #
42)	L9 AR-1268-2	9.150	8.094	108398	52494	0.774	0.371 #
45)	L9 AR-1268-5	0.000	8.931	0	86873	N.D.	0.231 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
Data File : PP068488.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 12:17
Operator : YP\AJ
Sample : P4858-02 10X
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:34:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

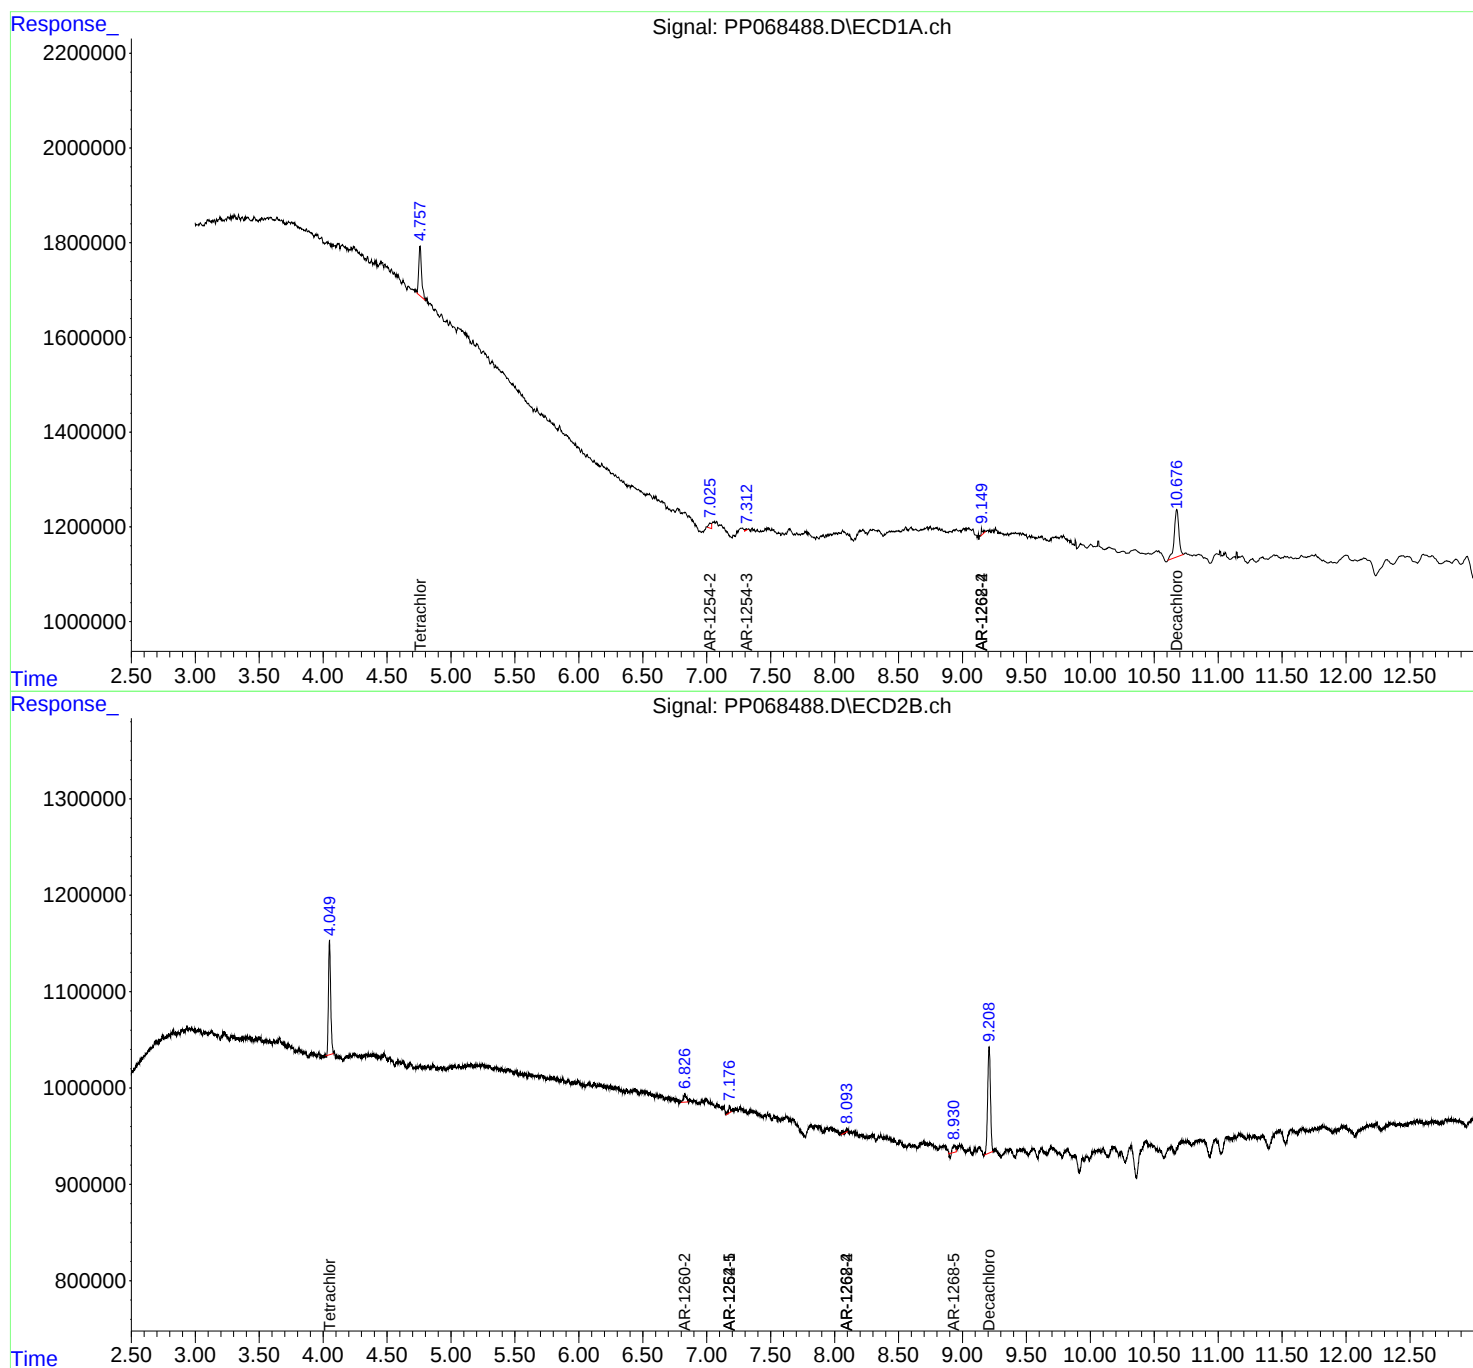


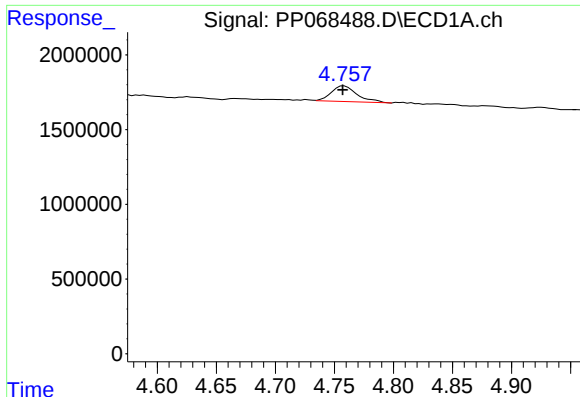

#1 Tetrachloro-m-xylene


R.T.: 4.758 min
Delta R.T.: 0.001 min
Response: 1602375
Conc: 1.65 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

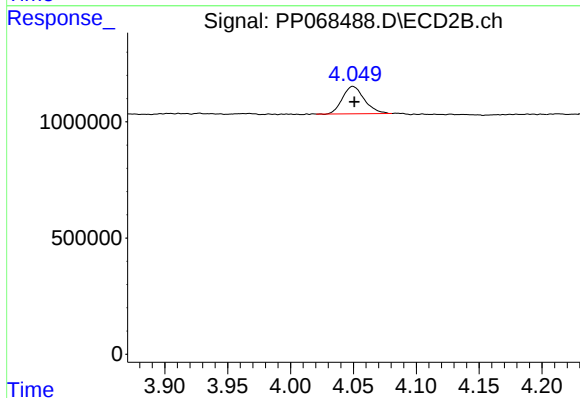


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: -0.001 min
Response: 1430985
Conc: 1.48 ng/ml

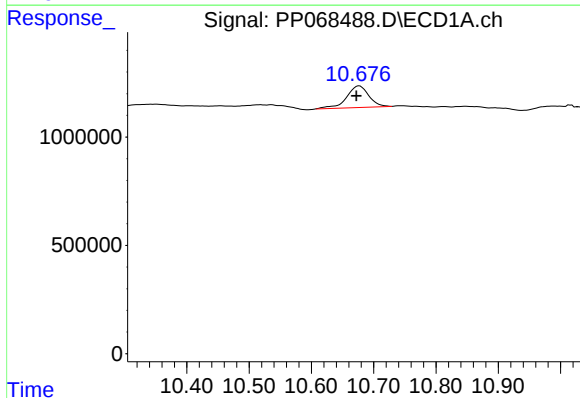


#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.005 min
Response: 2477203
Conc: 1.98 ng/ml

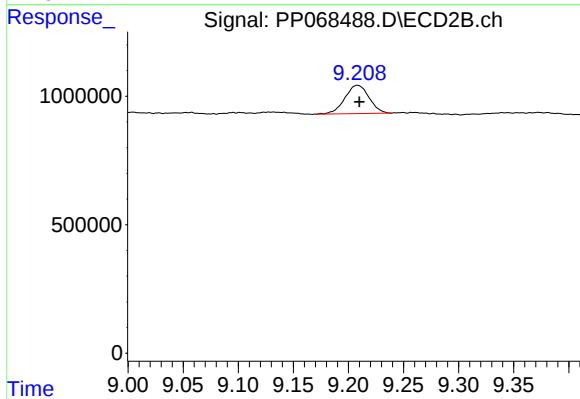

#2 Decachlorobiphenyl


R.T.: 9.208 min
Delta R.T.: -0.002 min
Response: 1682191
Conc: 1.49 ng/ml

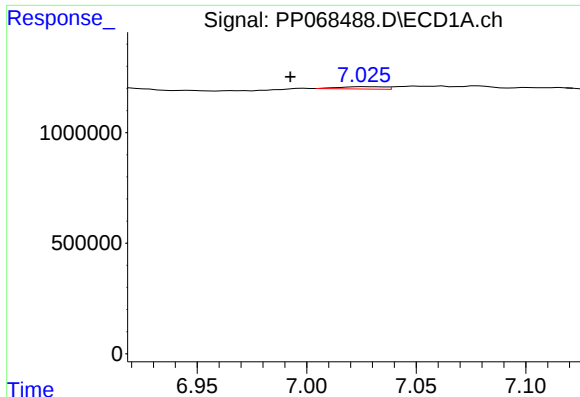

#27 AR-1254-2


R.T.: 7.026 min
Delta R.T.: 0.033 min
Response: 152423
Conc: 2.23 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

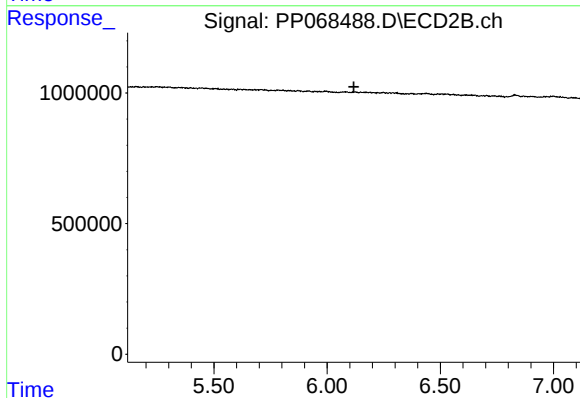


#27 AR-1254-2

R.T.: 0.000 min
Exp R.T. : 6.118 min
Response: 0
Conc: N.D.

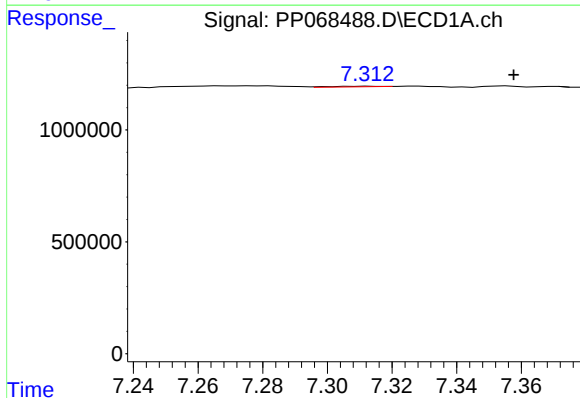


#28 AR-1254-3

R.T.: 7.313 min
Delta R.T.: -0.045 min
Response: 28161
Conc: 0.39 ng/ml

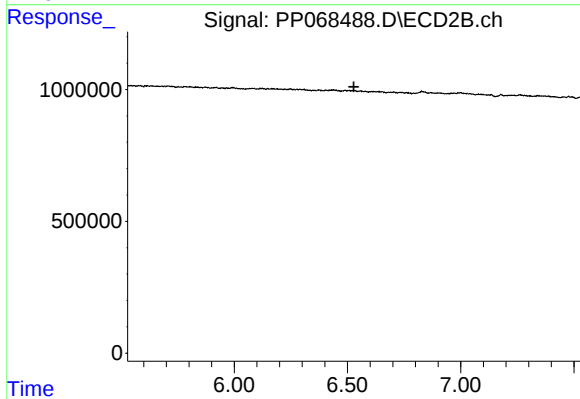

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 6.528 min
Response: 0
Conc: N.D.

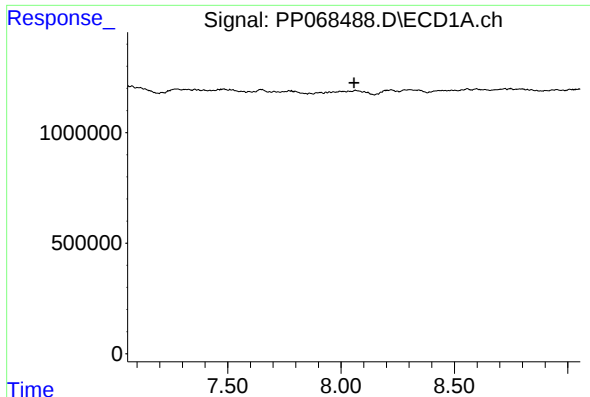

#30 AR-1254-5


R.T.: 0.000 min
Exp R.T.: 8.057 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

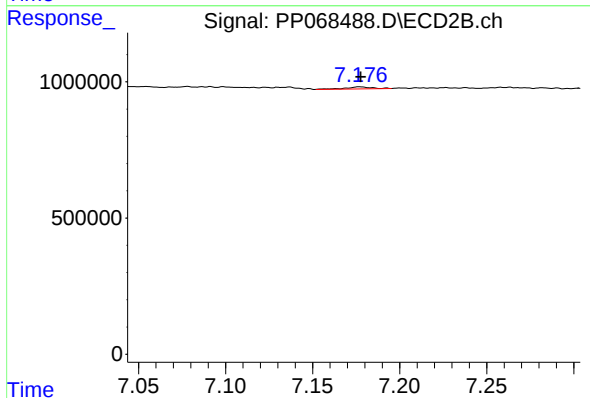


#30 AR-1254-5

R.T.: 7.177 min
Delta R.T.: 0.000 min
Response: 78340
Conc: 1.05 ng/ml

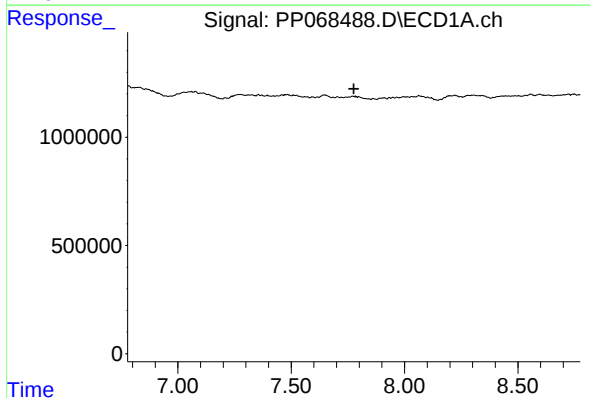


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 7.776 min
Response: 0
Conc: N.D.

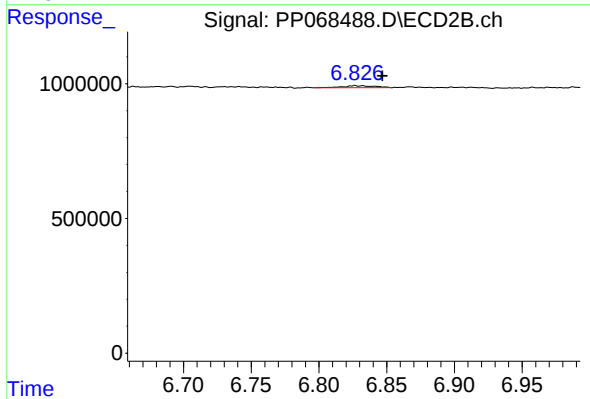

#32 AR-1260-2


R.T.: 6.826 min
Delta R.T.: -0.020 min
Response: 127000
Conc: 1.92 ng/ml

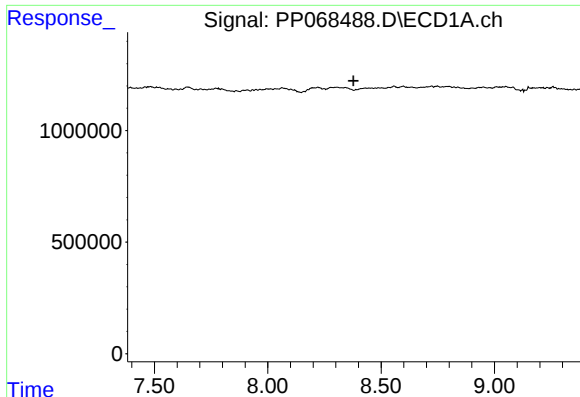

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T.: 8.379 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

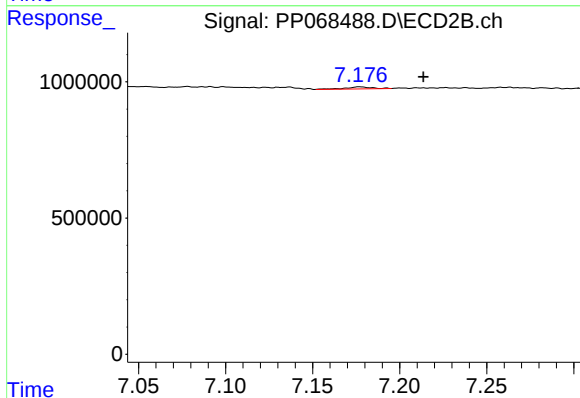


#36 AR-1262-1

R.T.: 7.177 min
Delta R.T.: -0.036 min
Response: 78340
Conc: 1.01 ng/ml

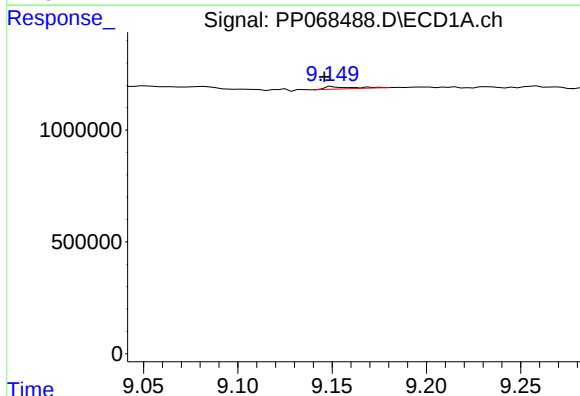


#39 AR-1262-4

R.T.: 9.150 min
Delta R.T.: 0.004 min
Response: 108398
Conc: 1.42 ng/ml

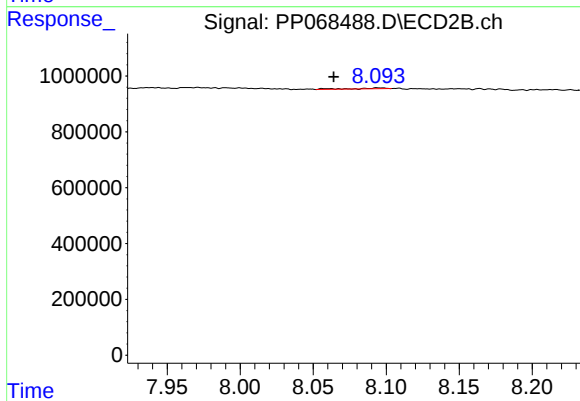

#39 AR-1262-4


R.T.: 8.094 min
Delta R.T.: 0.030 min
Response: 52494
Conc: 0.51 ng/ml

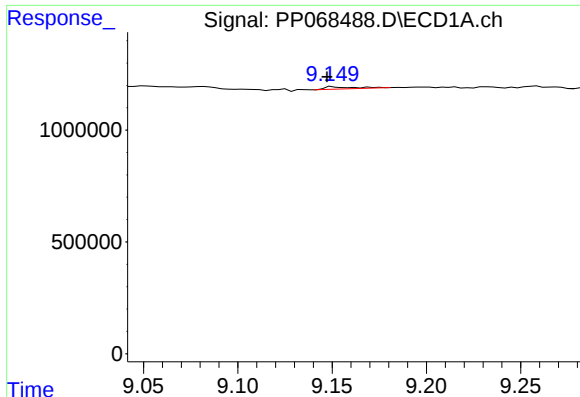

#42 AR-1268-2


R.T.: 9.150 min
Delta R.T.: 0.003 min
Response: 108398
Conc: 0.77 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC258780-1-2

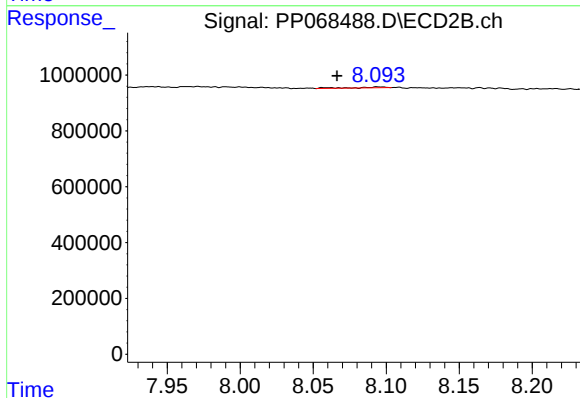


#42 AR-1268-2

R.T.: 8.094 min
Delta R.T.: 0.028 min
Response: 52494
Conc: 0.37 ng/ml

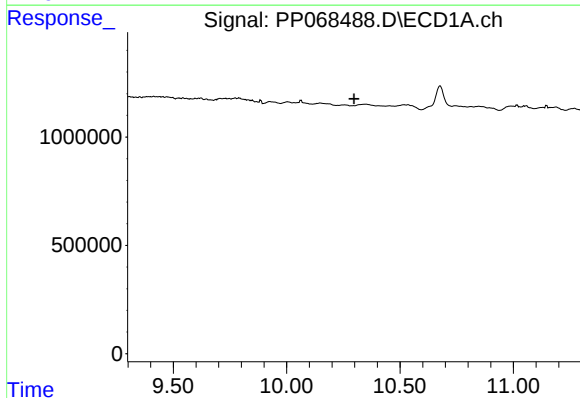

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.297 min
Response: 0
Conc: N.D.

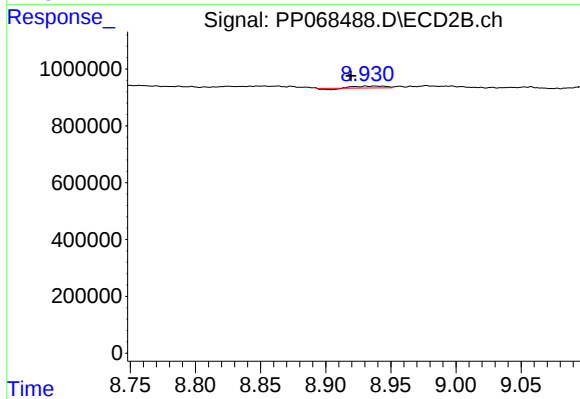

#45 AR-1268-5

R.T.: 8.931 min
Delta R.T.: 0.011 min
Response: 86873
Conc: 0.23 ng/ml