

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
Data File : PP068502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 17:09
Operator : YP\AJ
Sample : P4858-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
BC225734-1-2

Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:39:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.756	4.050	1502402	1325189	1.548	1.369
2) SA Decachlor...	10.675	9.210	1962084	1397974	1.568	1.236m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
Data File : PP068502.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 17:09
Operator : YP\AJ
Sample : P4858-08 10X
Misc :
ALS Vial : 19 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BC225734-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:39:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

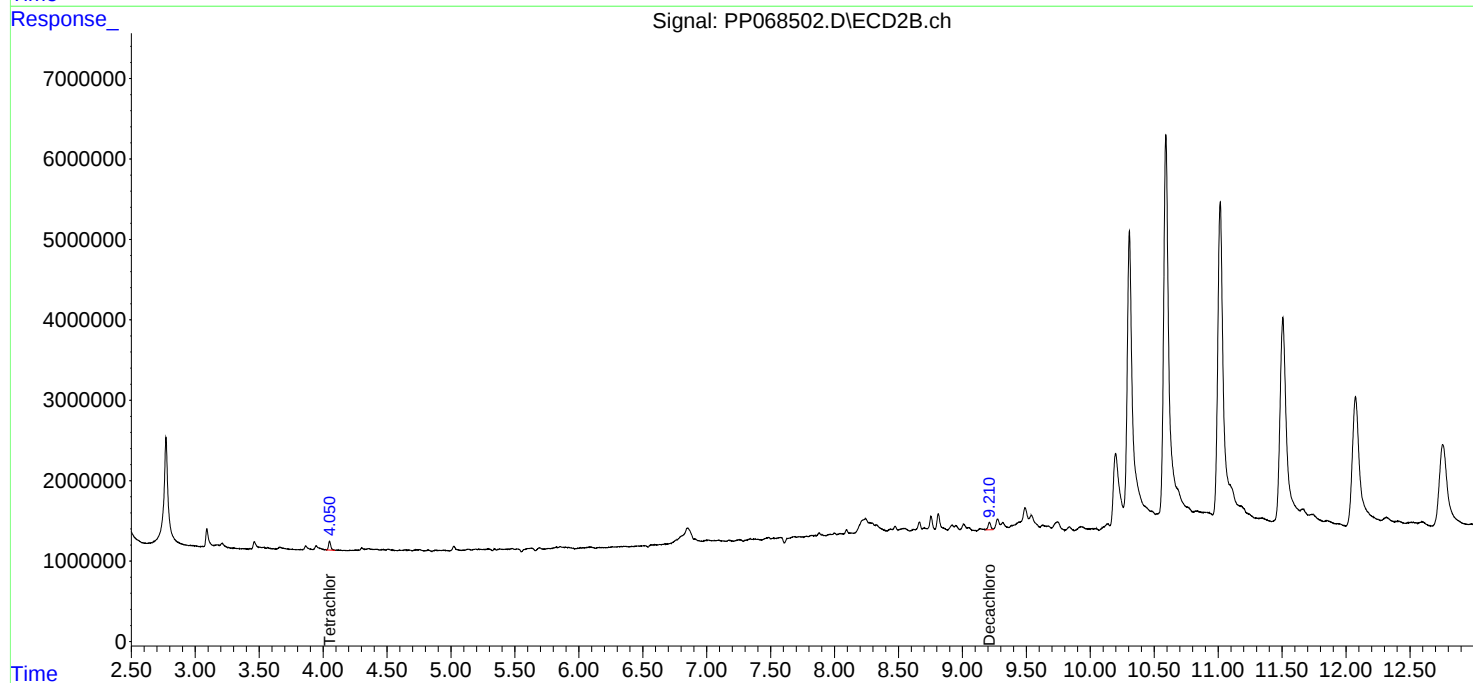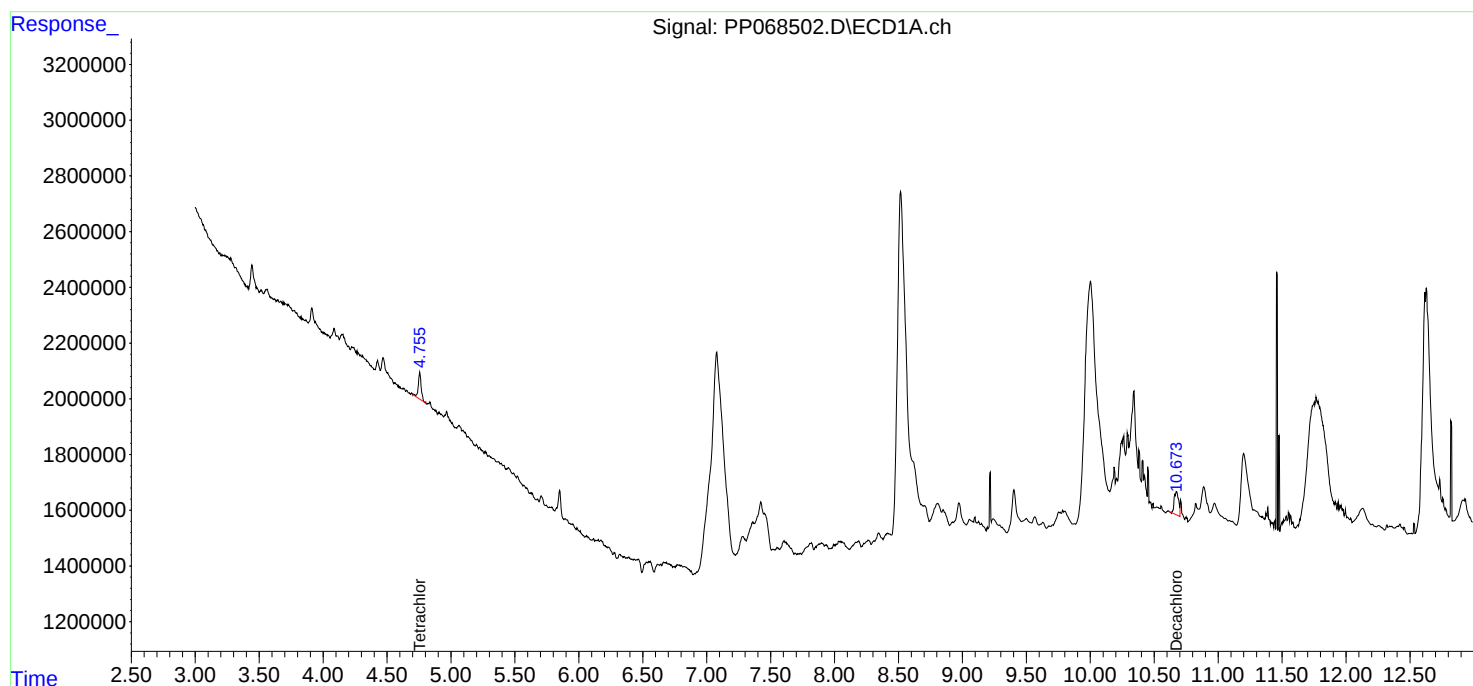

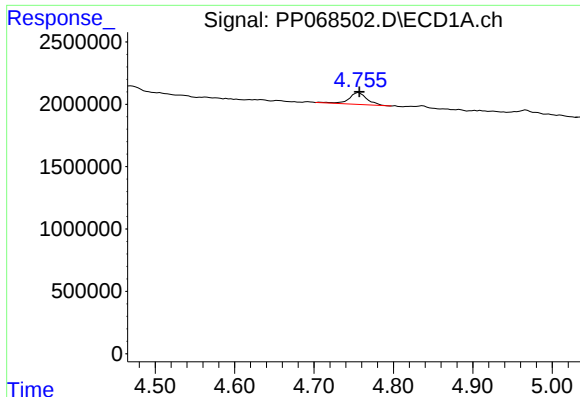


#1 Tetrachloro-m-xylene

R.T.: 4.756 min
Delta R.T.: 0.000 min
Response: 1502402
Conc: 1.55 ng/ml

Instrument :
ECD_P
ClientSampleId :
BC225734-1-2


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

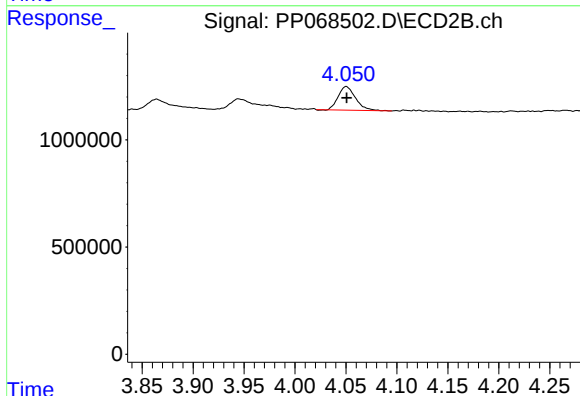


#1 Tetrachloro-m-xylene

R.T.: 4.050 min
Delta R.T.: 0.000 min
Response: 1325189
Conc: 1.37 ng/ml

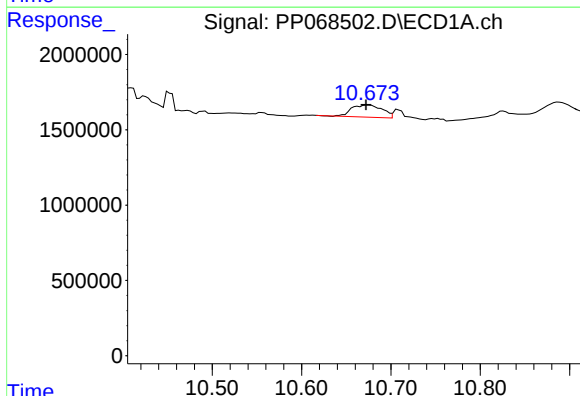

#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: 0.003 min
Response: 1962084
Conc: 1.57 ng/ml

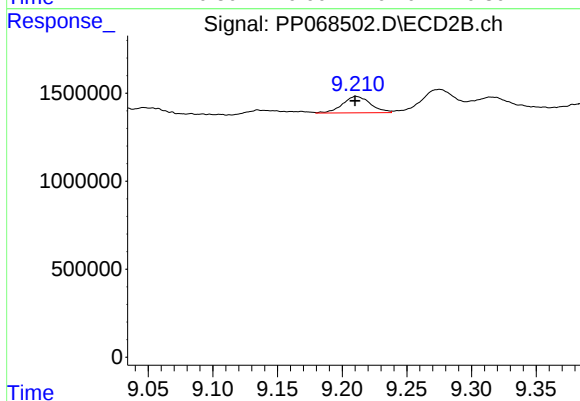

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: 0.000 min
Response: 1397974
Conc: 1.24 ng/ml m