

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
 Data File : PP068504.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Nov 2024 17:42
 Operator : YP\AJ
 Sample : P4858-13 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2309-0044-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/18/2024
 Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 16 01:39:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.760	4.051	1734386	1619496	1.787	1.673
2) SA Decachlor...	10.676	9.210	2576049	1413894	2.058m	1.250 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111524\
Data File : PP068504.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Nov 2024 17:42
Operator : YP\AJ
Sample : P4858-13 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2309-0044-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 16 01:39:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

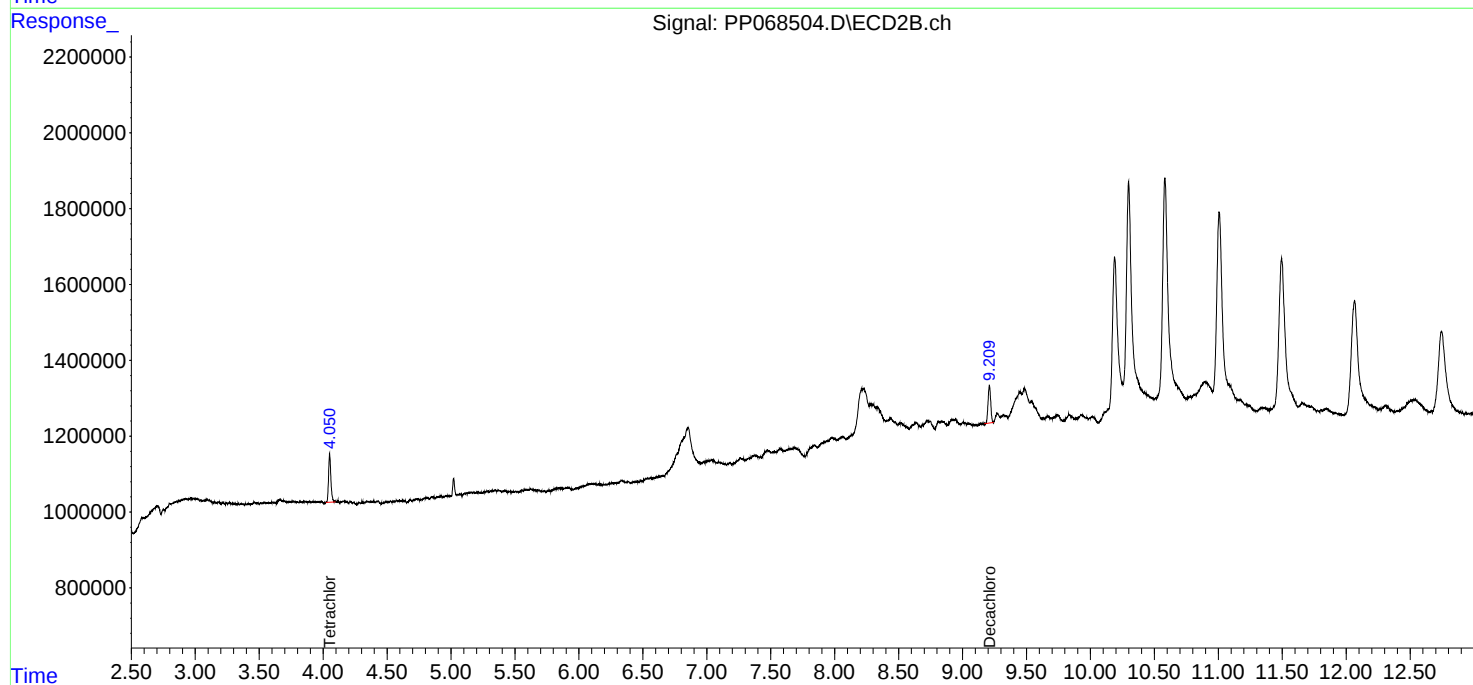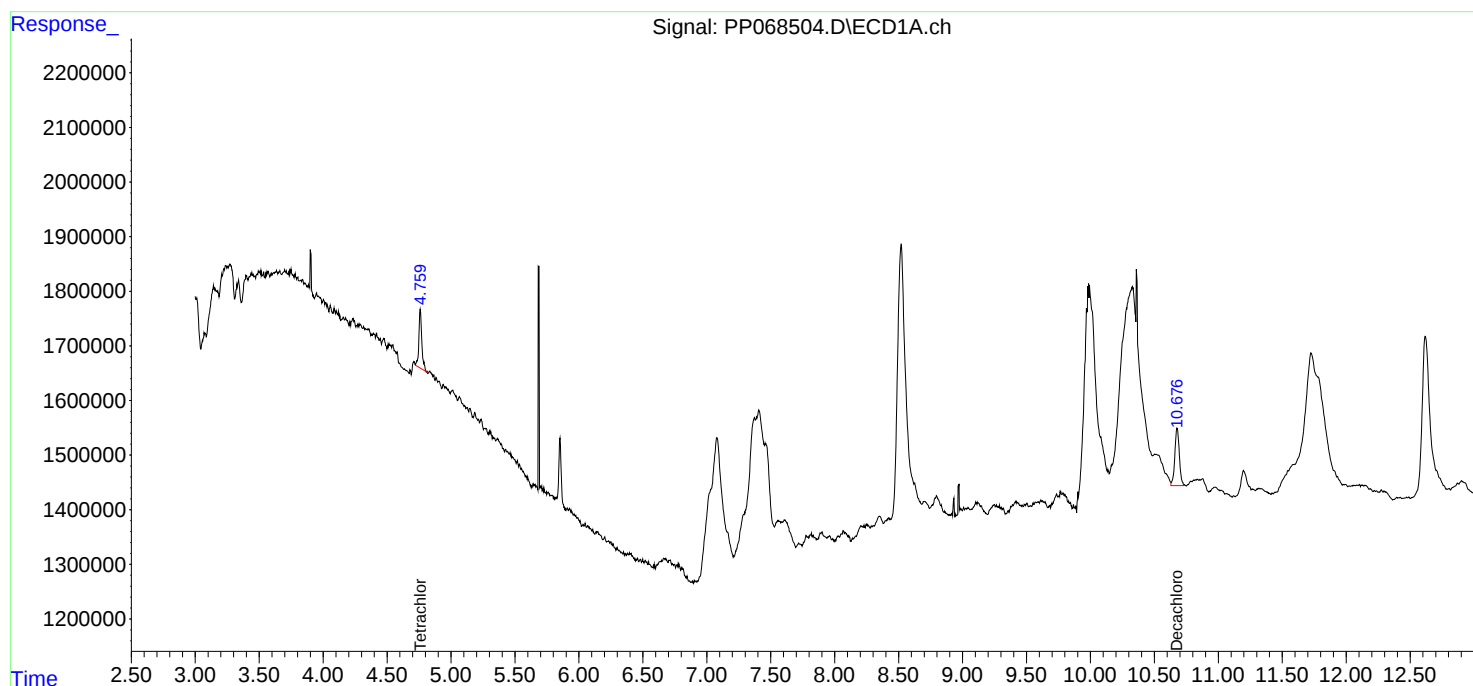

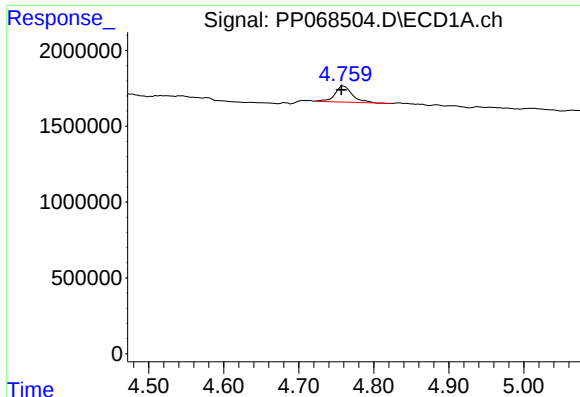


#1 Tetrachloro-m-xylene

R.T.: 4.760 min
Delta R.T.: 0.003 min
Response: 1734386
Conc: 1.79 ng/ml

Instrument :
ECD_P
ClientSampleId :
Y2309-0044-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/18/2024
Supervised By :Ankita Jodhani 11/18/2024

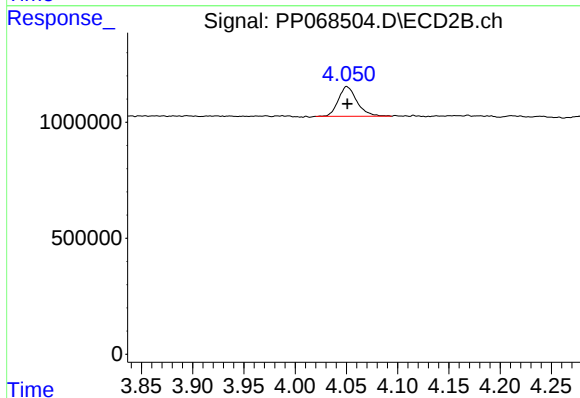


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 1619496
Conc: 1.67 ng/ml

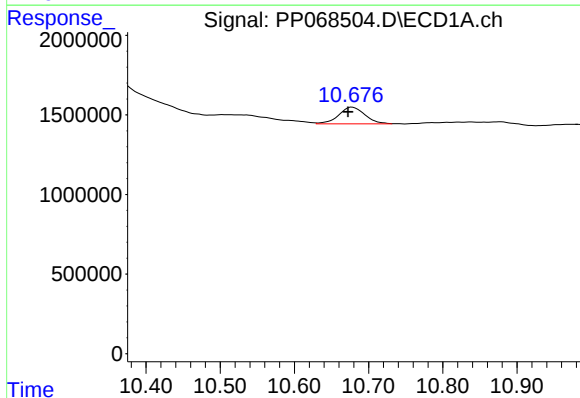

#2 Decachlorobiphenyl

R.T.: 10.676 min
Delta R.T.: 0.004 min
Response: 2576049
Conc: 2.06 ng/ml m

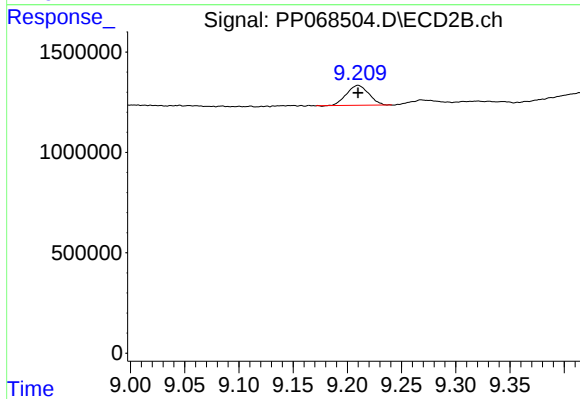

#2 Decachlorobiphenyl

R.T.: 9.210 min
Delta R.T.: 0.000 min
Response: 1413894
Conc: 1.25 ng/ml