

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031301.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 17:15
 Operator : DD\AJ
 Sample : L4745-01
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CV-OS

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:39:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.797	4.072	964989	900152	23.687	21.531
2)	SA Decachlor...	10.677	9.386	724698	816309	23.595	24.378
Target Compounds							
9)	L2 AR-1221-2	0.000	4.421	0	24937	N.D.	70.618 #
20)	L4 AR-1242-5	0.000	6.227f	0	10104	N.D.	11.432 #
25)	L5 AR-1248-5	0.000	6.227f	0	10104	N.D.	8.044 #
26)	L6 AR-1254-1	0.000	6.227f	0	10104	N.D.	5.309 #
32)	L7 AR-1260-2	0.000	7.107	0	921	N.D.	0.452 #
34)	L7 AR-1260-4	0.000	7.764	0	5689	N.D.	3.528 #
35)	L7 AR-1260-5	0.000	7.997	0	7193	N.D.	1.821 #
37)	L8 AR-1262-2	0.000	7.997	0	7193	N.D.	1.749 #
38)	L8 AR-1262-3	0.000	8.288	0	18497	N.D.	11.605 #
39)	L8 AR-1262-4	0.000	8.359	0	3464	N.D.	1.106 #
40)	L8 AR-1262-5	0.000	8.848	0	1052	N.D.	0.746 #
41)	L9 AR-1268-1	0.000	8.288	0	18497	N.D.	3.758 #
42)	L9 AR-1268-2	0.000	8.359	0	3464	N.D.	0.712 #
43)	L9 AR-1268-3	0.000	8.562	0	2582	N.D.	0.620 #
44)	L9 AR-1268-4	0.000	8.848	0	1052	N.D.	0.632 #
45)	L9 AR-1268-5	0.000	9.140	0	7771	N.D.	0.595 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031301.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 17:15
Operator : DD\AJ
Sample : L4745-01
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CV-OS

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:39:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

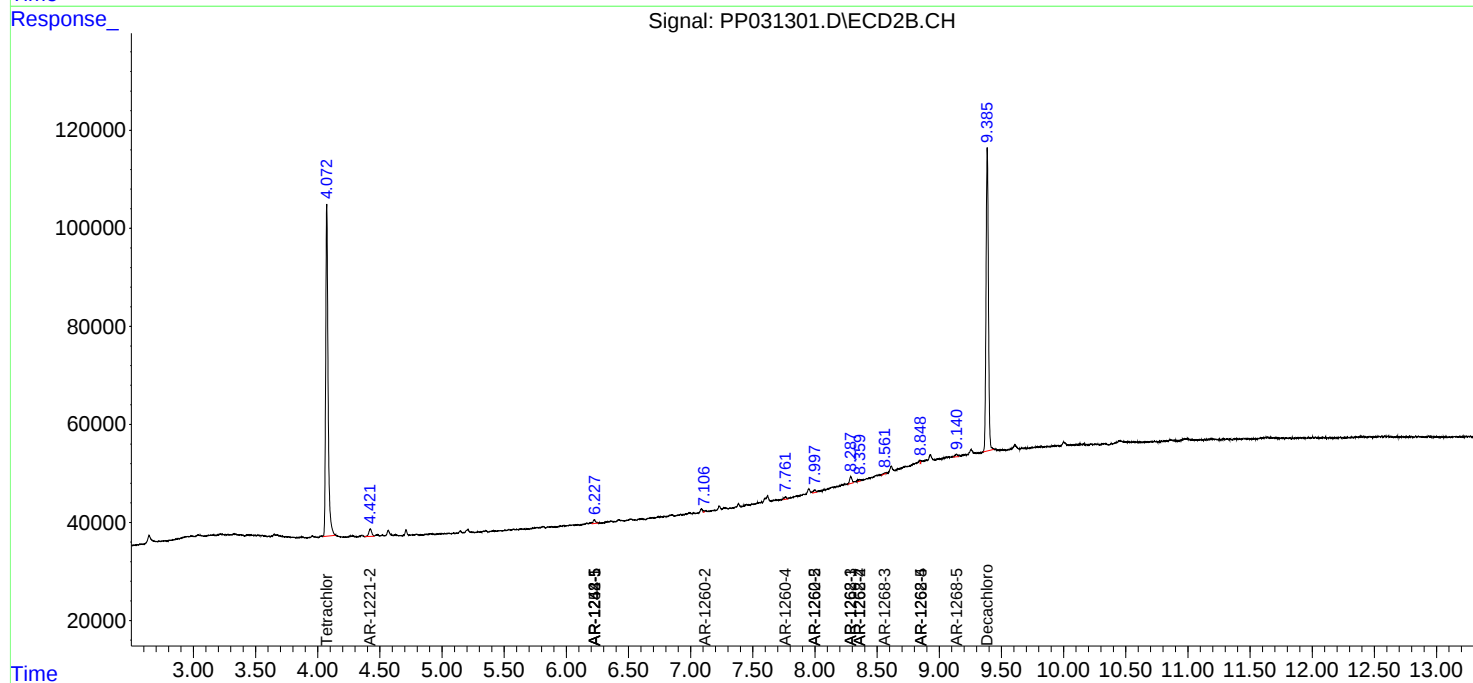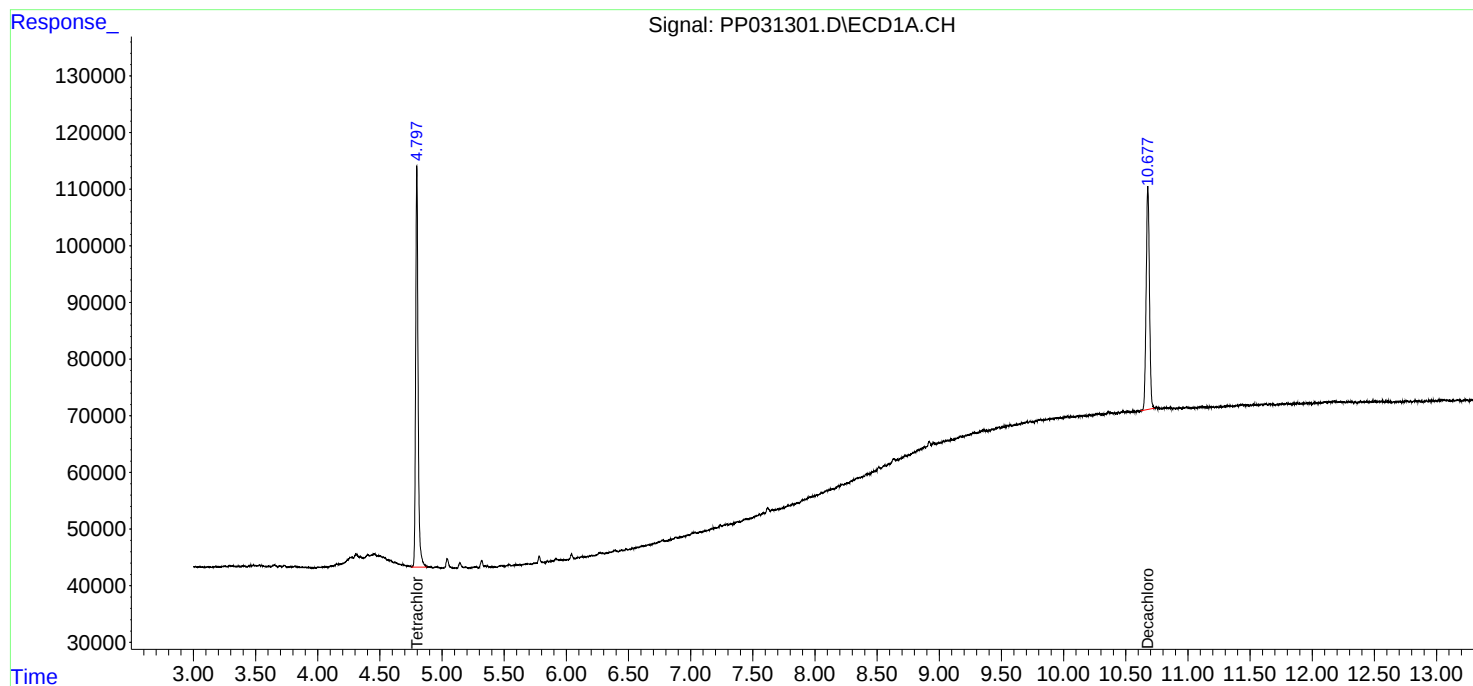


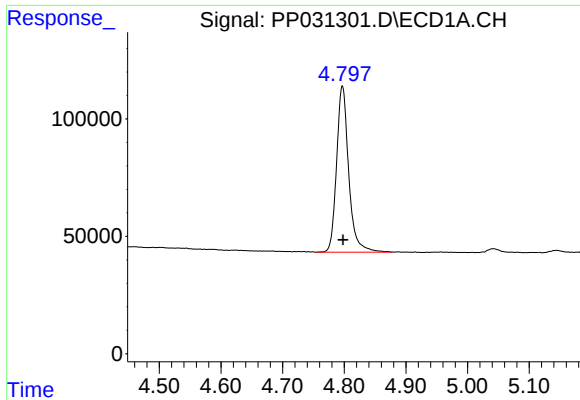

#1 Tetrachloro-m-xylene


R.T.: 4.797 min
Delta R.T.: 0.000 min
Response: 964989
Conc: 23.69 ng/ml

Instrument :
ECD_P
ClientSampleId :
CV-OS

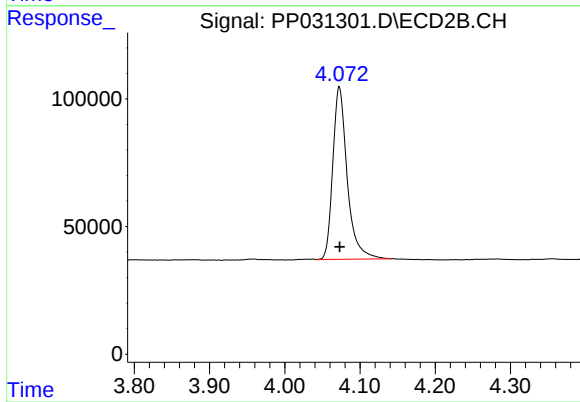


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: 0.000 min
Response: 900152
Conc: 21.53 ng/ml

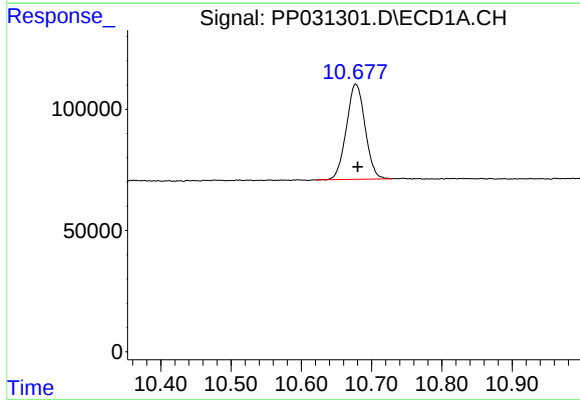


#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: -0.003 min
Response: 724698
Conc: 23.60 ng/ml

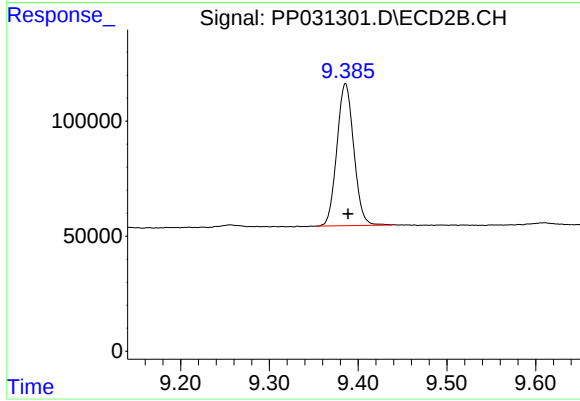

#2 Decachlorobiphenyl


R.T.: 9.386 min
Delta R.T.: -0.003 min
Response: 816309
Conc: 24.38 ng/ml

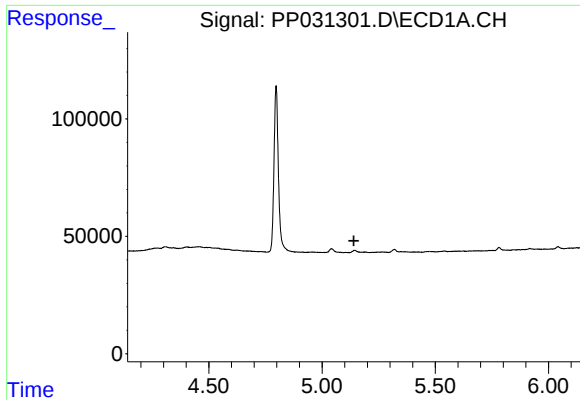

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

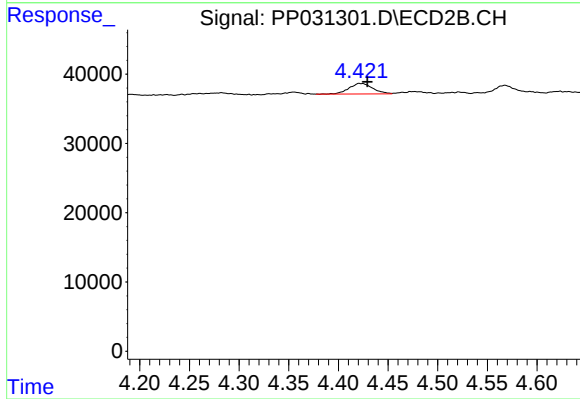


#9 AR-1221-2

R.T.: 4.421 min
Delta R.T.: -0.008 min
Response: 24937
Conc: 70.62 ng/ml

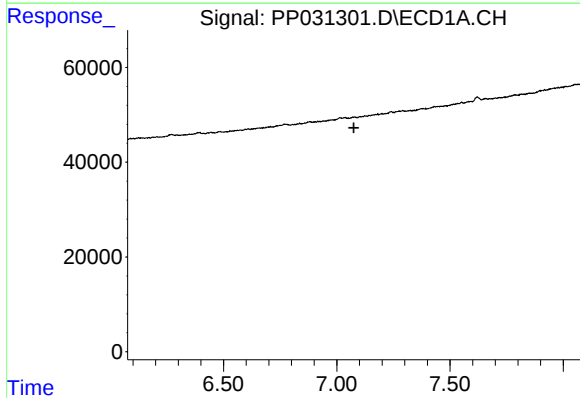


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T.: 7.076 min
Response: 0
Conc: N.D.

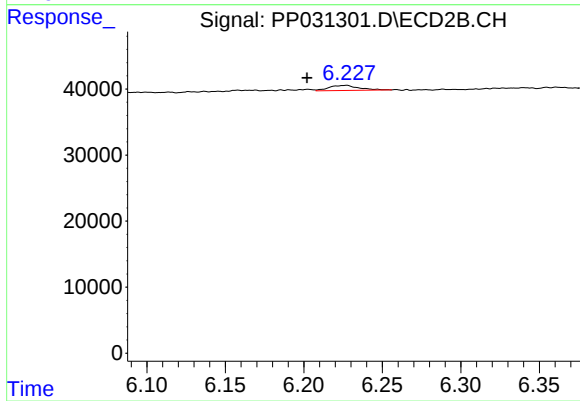

#20 AR-1242-5


R.T.: 6.227 min
Delta R.T.: 0.025 min
Response: 10104
Conc: 11.43 ng/ml

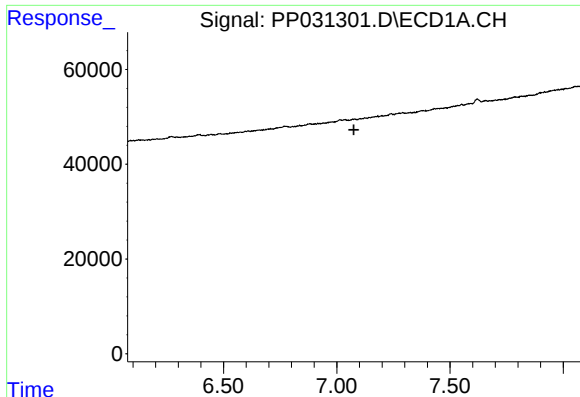

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T.: 7.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

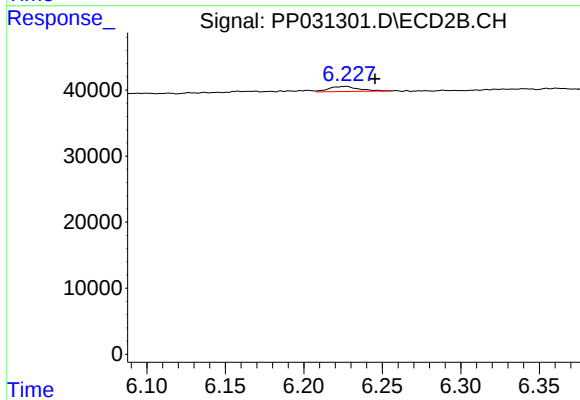


#25 AR-1248-5

R.T.: 6.227 min
Delta R.T.: -0.018 min
Response: 10104
Conc: 8.04 ng/ml

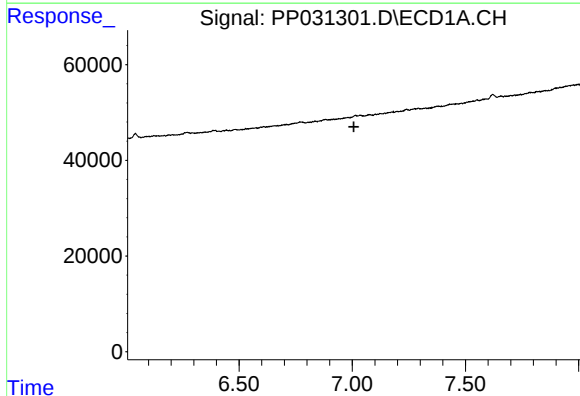


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T.: 7.008 min
Response: 0
Conc: N.D.

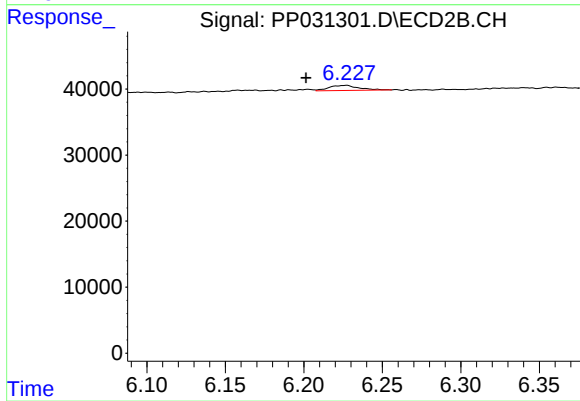

#26 AR-1254-1


R.T.: 6.227 min
Delta R.T.: 0.026 min
Response: 10104
Conc: 5.31 ng/ml

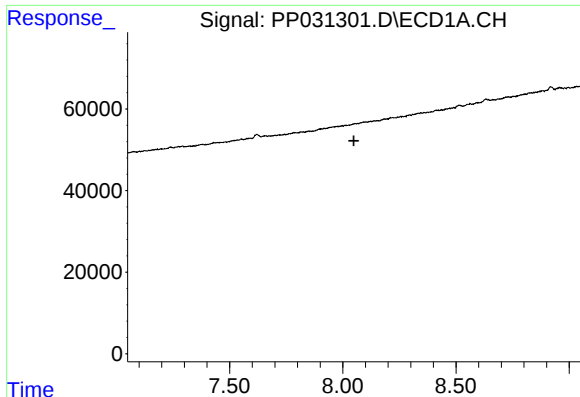

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T.: 8.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

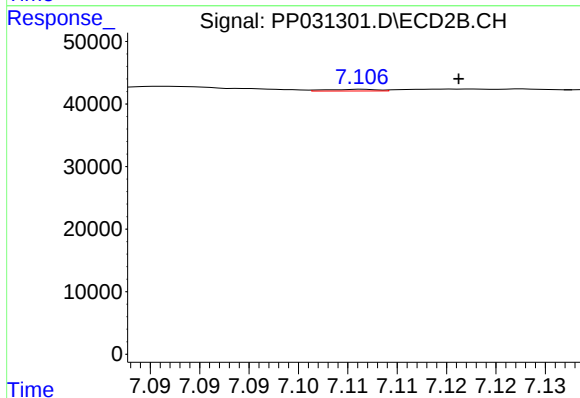


#32 AR-1260-2

R.T.: 7.107 min
Delta R.T.: -0.010 min
Response: 921
Conc: 0.45 ng/ml

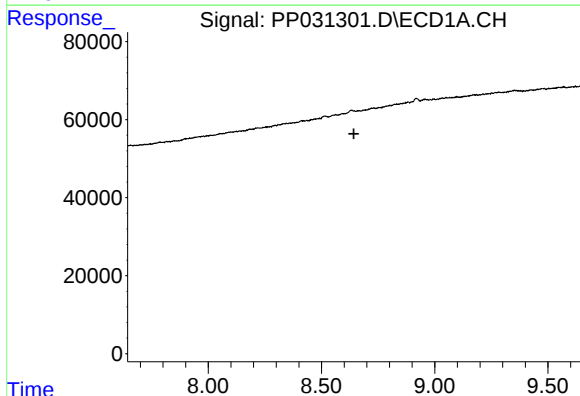


#34 AR-1260-4

R.T.: 0.000 min
Exp R.T.: 8.643 min
Response: 0
Conc: N.D.

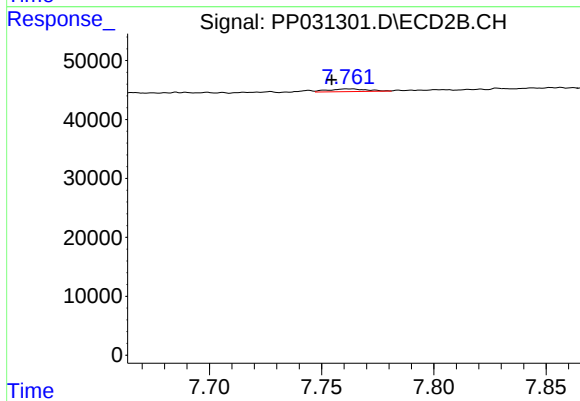

#34 AR-1260-4


R.T.: 7.764 min
Delta R.T.: 0.009 min
Response: 5689
Conc: 3.53 ng/ml

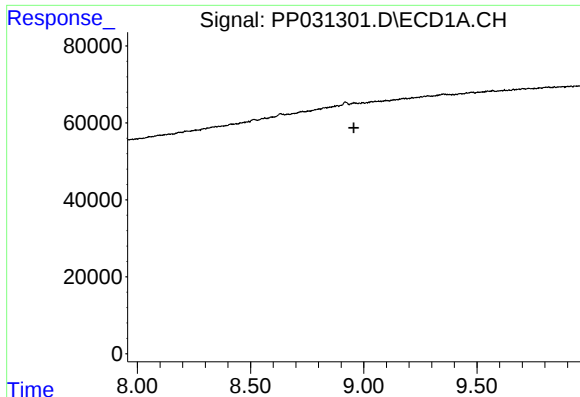

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T.: 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

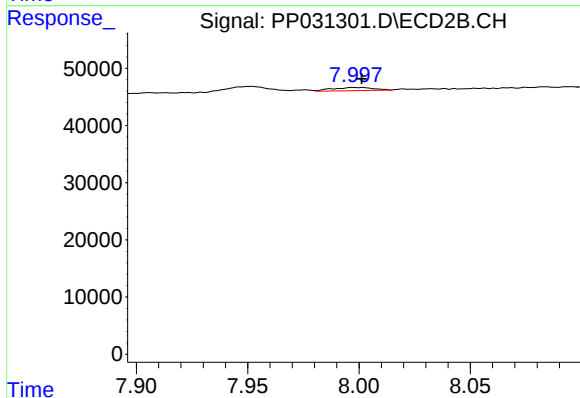


#35 AR-1260-5

R.T.: 7.997 min
Delta R.T.: -0.004 min
Response: 7193
Conc: 1.82 ng/ml

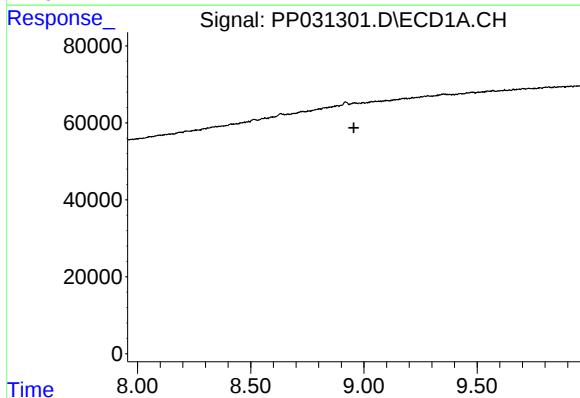


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T.: 8.956 min
Response: 0
Conc: N.D.

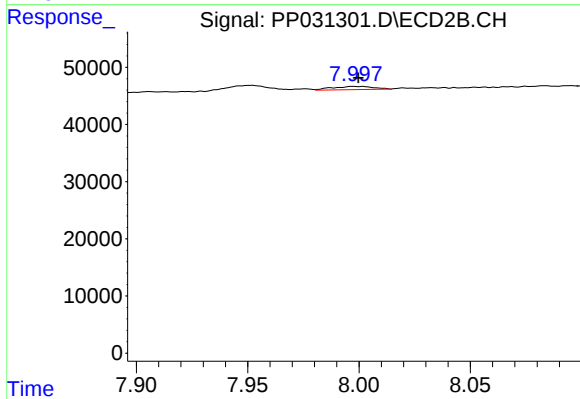

#37 AR-1262-2


R.T.: 7.997 min
Delta R.T.: -0.003 min
Response: 7193
Conc: 1.75 ng/ml

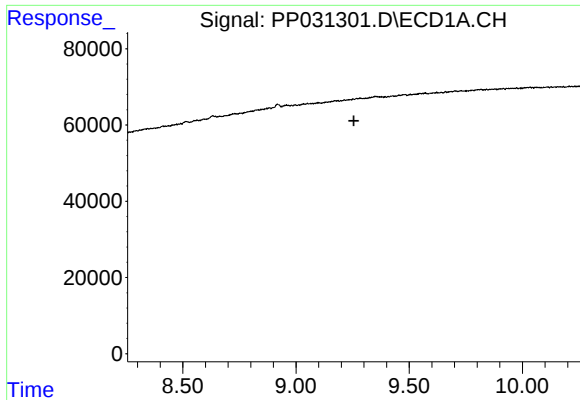

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

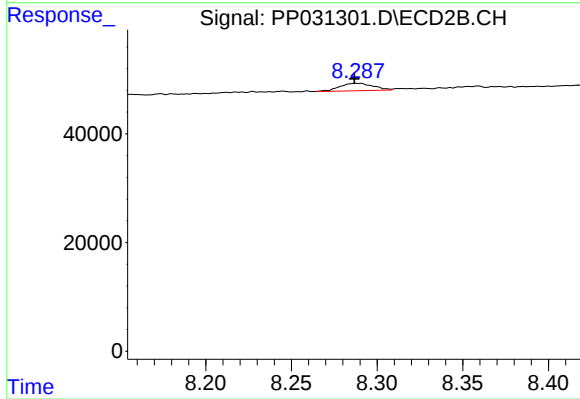


#38 AR-1262-3

R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 18497
Conc: 11.61 ng/ml

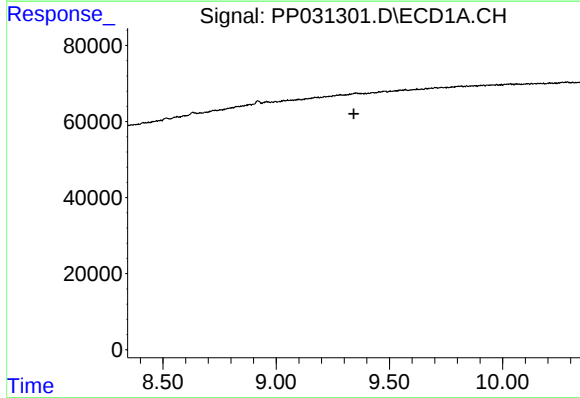


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.343 min
Response: 0
Conc: N.D.

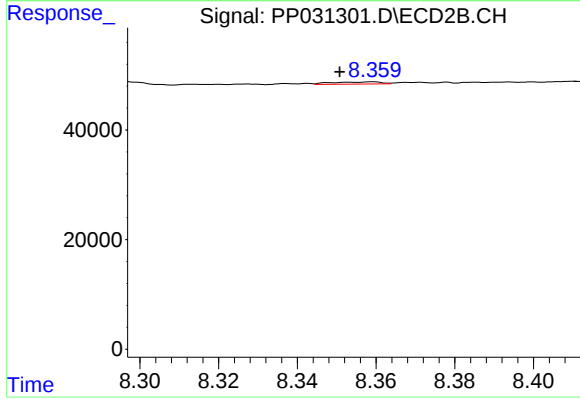

#39 AR-1262-4


R.T.: 8.359 min
Delta R.T.: 0.008 min
Response: 3464
Conc: 1.11 ng/ml

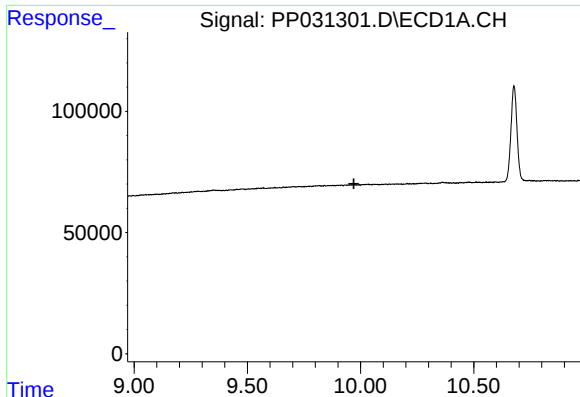

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T.: 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

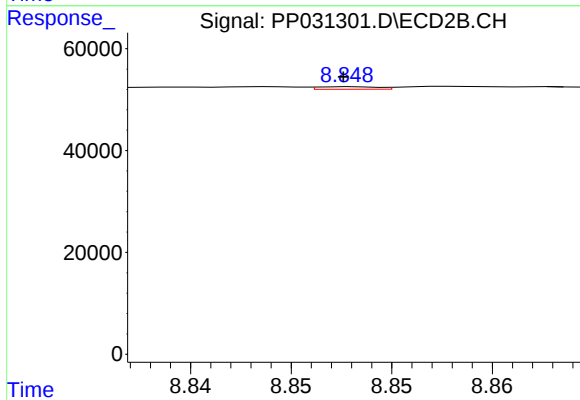


#40 AR-1262-5

R.T.: 8.848 min
Delta R.T.: 0.000 min
Response: 1052
Conc: 0.75 ng/ml

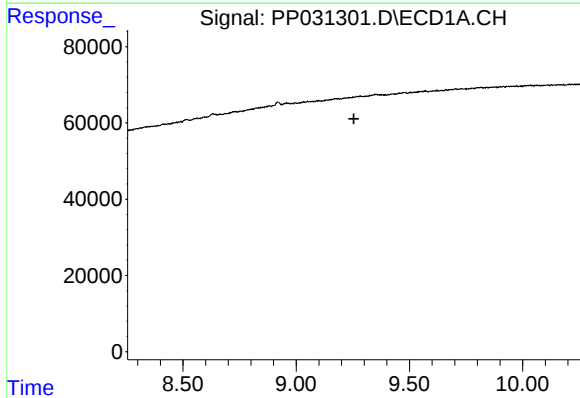


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T.: 9.255 min
Response: 0
Conc: N.D.

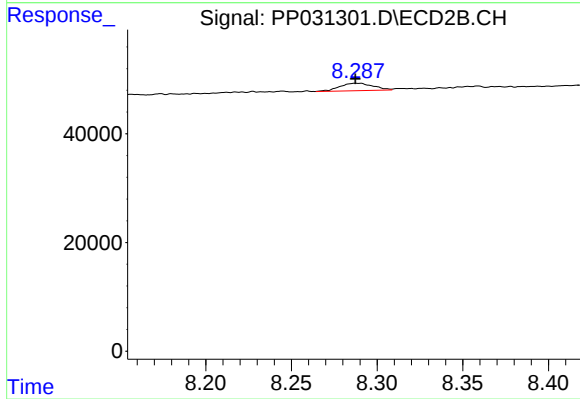

#41 AR-1268-1


R.T.: 8.288 min
Delta R.T.: 0.000 min
Response: 18497
Conc: 3.76 ng/ml

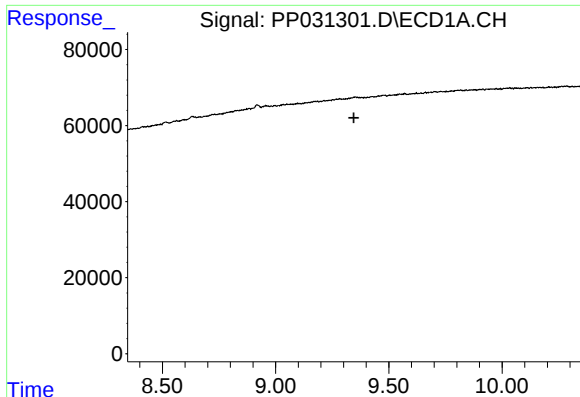

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

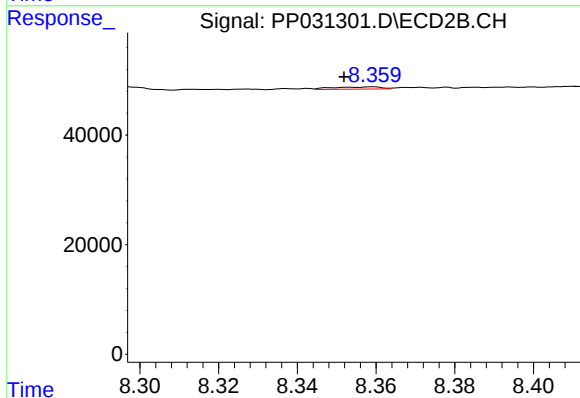


#42 AR-1268-2

R.T.: 8.359 min
Delta R.T.: 0.007 min
Response: 3464
Conc: 0.71 ng/ml

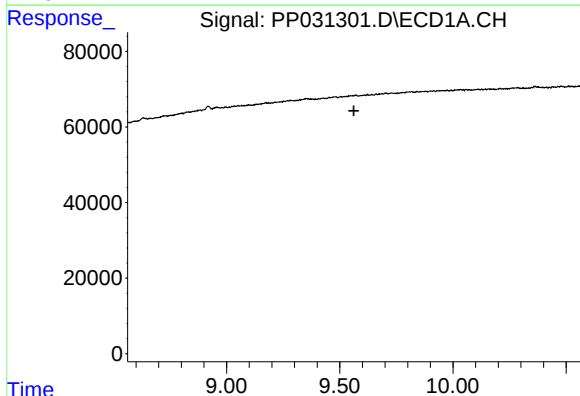


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.562 min
Response: 0
Conc: N.D.

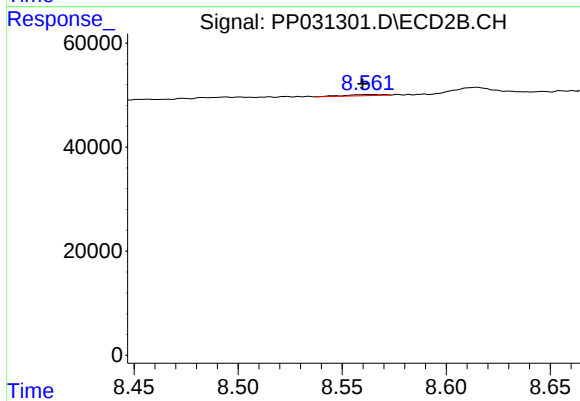

#43 AR-1268-3


R.T.: 8.562 min
Delta R.T.: 0.002 min
Response: 2582
Conc: 0.62 ng/ml

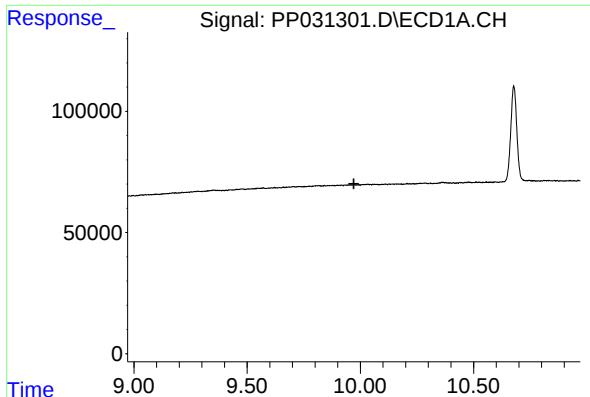

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
CV-OS

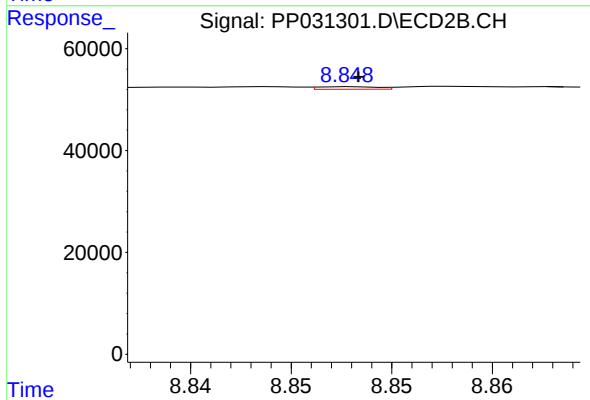


#44 AR-1268-4

R.T.: 8.848 min
Delta R.T.: 0.000 min
Response: 1052
Conc: 0.63 ng/ml

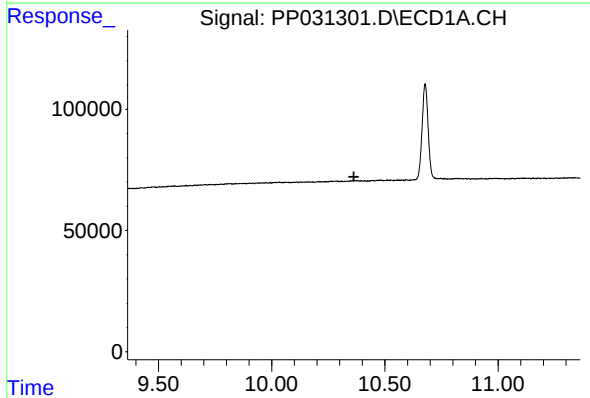

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.363 min
Response: 0
Conc: N.D.

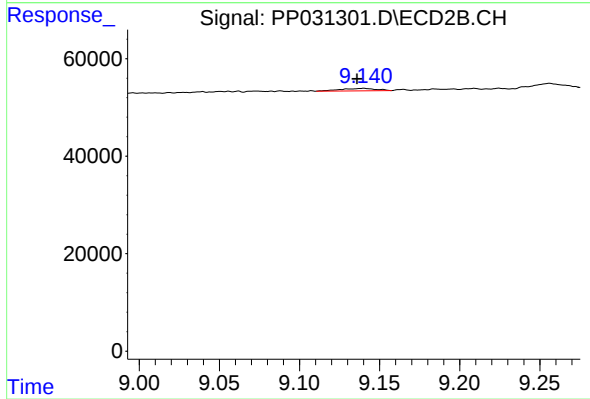

#45 AR-1268-5

R.T.: 9.140 min
Delta R.T.: 0.004 min
Response: 7771
Conc: 0.60 ng/ml