

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031305.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 18:21
 Operator : DD\AJ
 Sample : PB133046BL
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB133046BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:41:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.797	4.072	856305	829331	21.019	19.837
2)	SA Decachlor...	10.677	9.386	605693	671159	19.720	20.044
Target Compounds							
9)	L2 AR-1221-2	0.000	4.424	0	13164	N.D.	37.279 #
35)	L7 AR-1260-5	0.000	8.003	0	3375	N.D.	0.854 #
37)	L8 AR-1262-2	0.000	8.003	0	3375	N.D.	0.821 #
38)	L8 AR-1262-3	0.000	8.287	0	2170	N.D.	1.362 #
40)	L8 AR-1262-5	0.000	8.851	0	239	N.D.	0.170 #
41)	L9 AR-1268-1	0.000	8.287	0	2170	N.D.	0.441 #
44)	L9 AR-1268-4	0.000	8.851	0	239	N.D.	0.144 #
45)	L9 AR-1268-5	0.000	9.135	0	2655	N.D.	0.203 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031305.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 18:21
Operator : DD\AJ
Sample : PB133046BL
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB133046BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:41:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

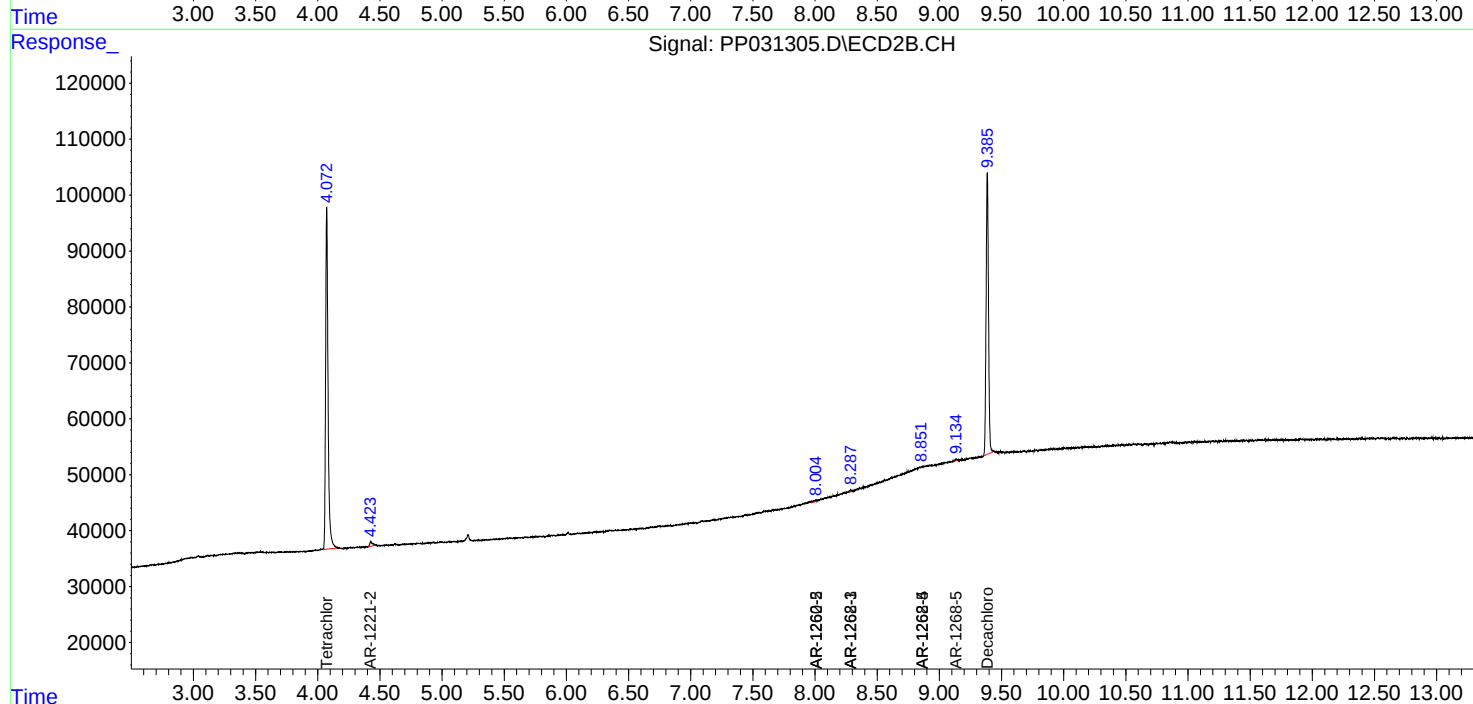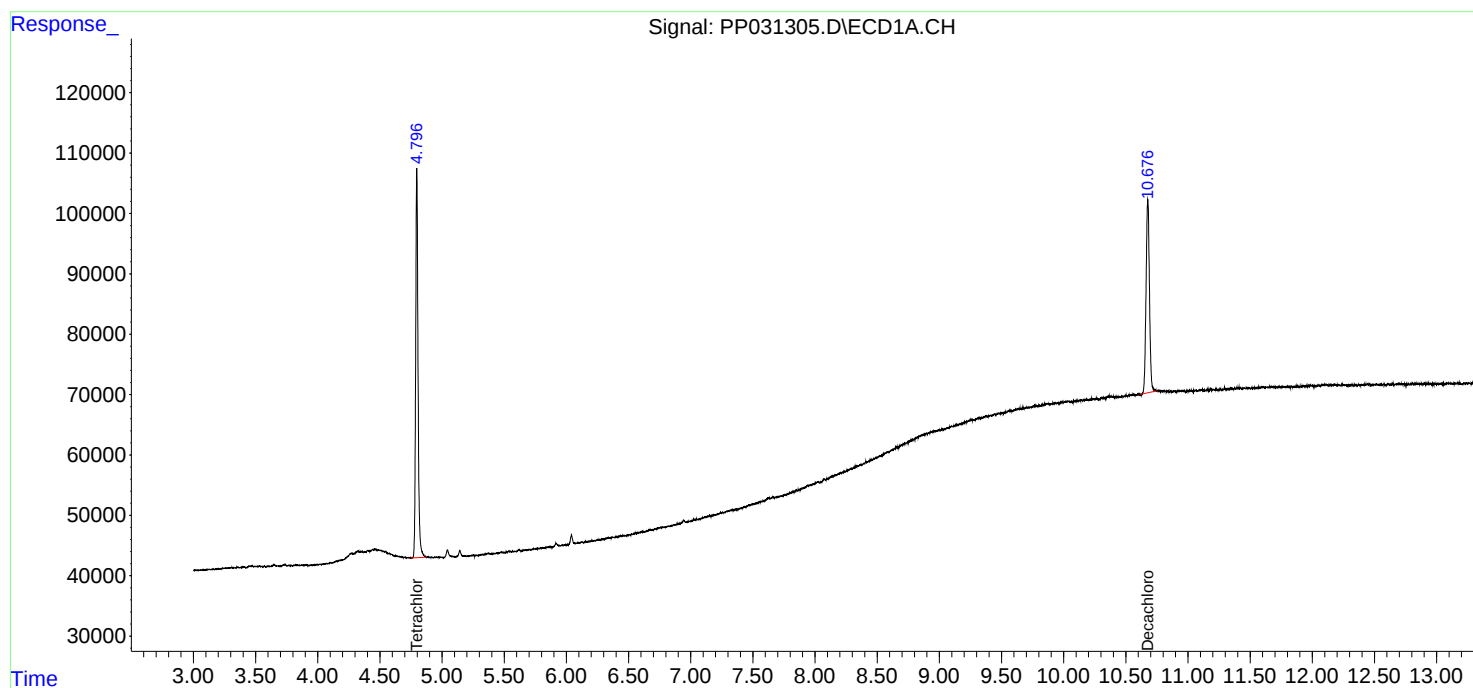


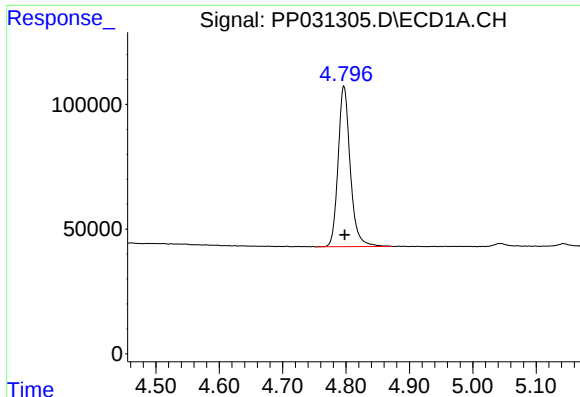

#1 Tetrachloro-m-xylene


R.T.: 4.797 min
Delta R.T.: -0.001 min
Response: 856305
Conc: 21.02 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB133046BL

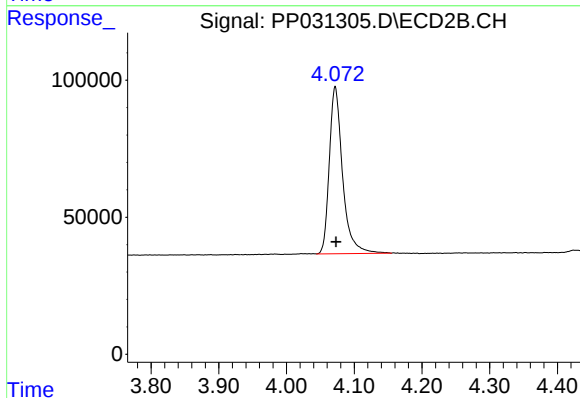


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: -0.001 min
Response: 829331
Conc: 19.84 ng/ml

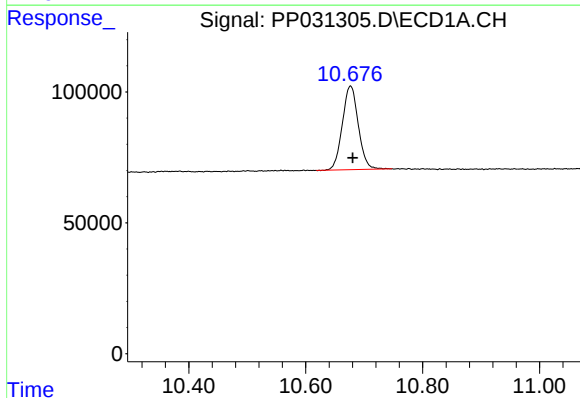


#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: -0.004 min
Response: 605693
Conc: 19.72 ng/ml

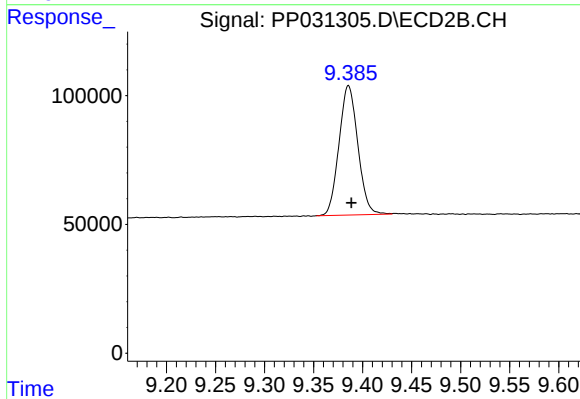

#2 Decachlorobiphenyl


R.T.: 9.386 min
Delta R.T.: -0.003 min
Response: 671159
Conc: 20.04 ng/ml

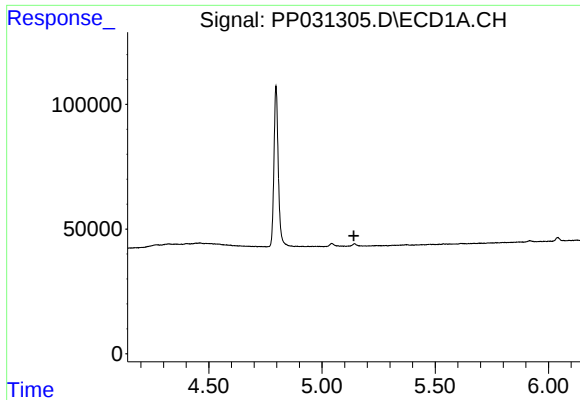

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB133046BL

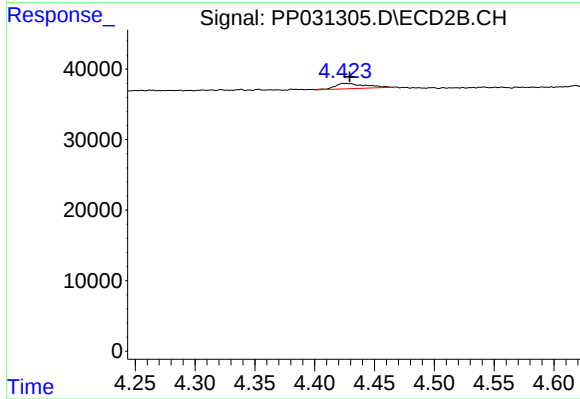


#9 AR-1221-2

R.T.: 4.424 min
Delta R.T.: -0.005 min
Response: 13164
Conc: 37.28 ng/ml

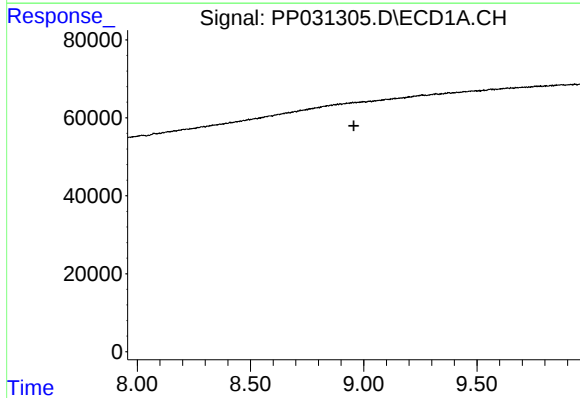


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.957 min
Response: 0
Conc: N.D.

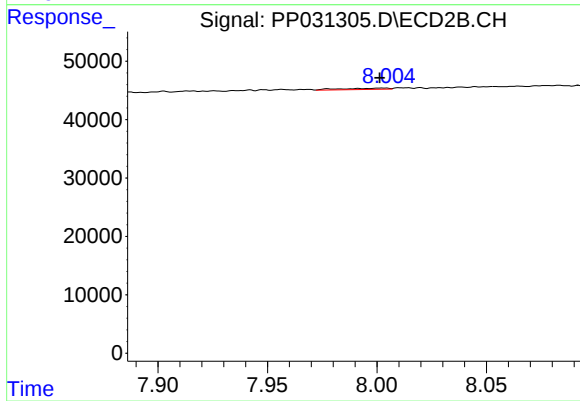

#35 AR-1260-5


R.T.: 8.003 min
Delta R.T.: 0.002 min
Response: 3375
Conc: 0.85 ng/ml

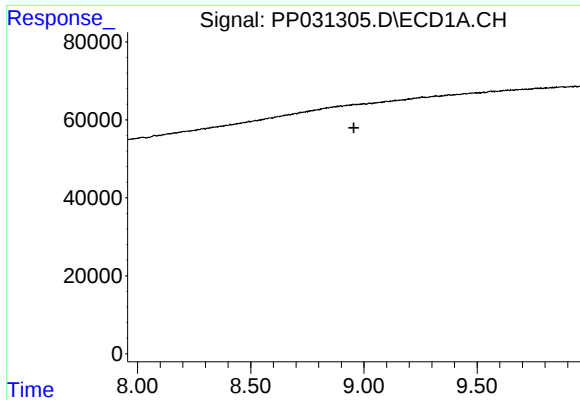

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB133046BL

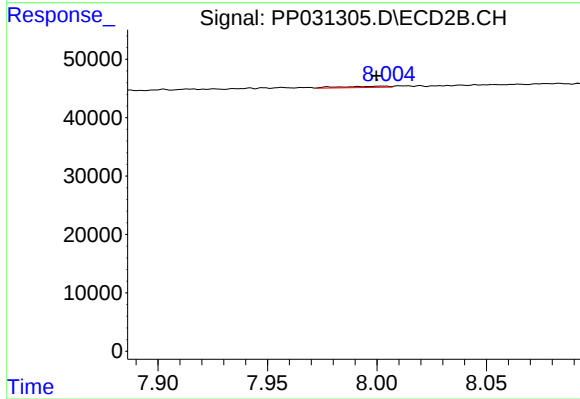


#37 AR-1262-2

R.T.: 8.003 min
Delta R.T.: 0.003 min
Response: 3375
Conc: 0.82 ng/ml

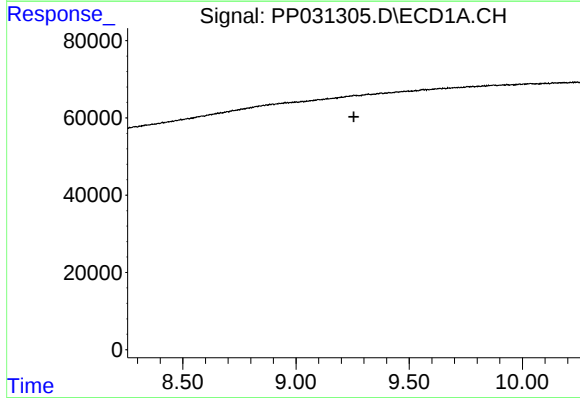


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.256 min
Response: 0
Conc: N.D.

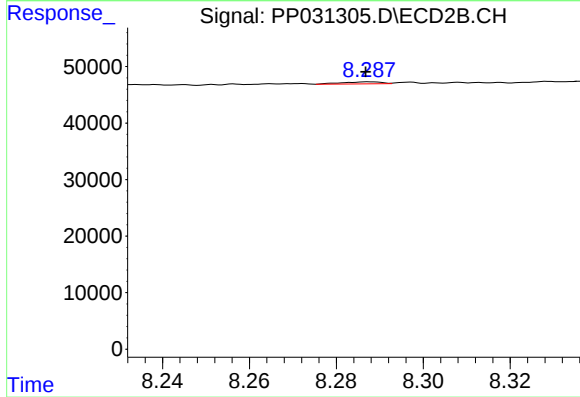

#38 AR-1262-3


R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 2170
Conc: 1.36 ng/ml

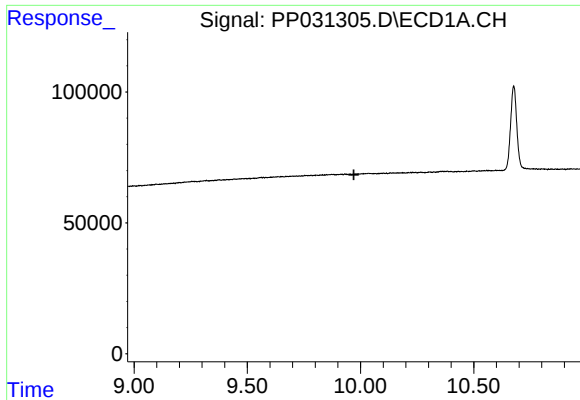

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB133046BL

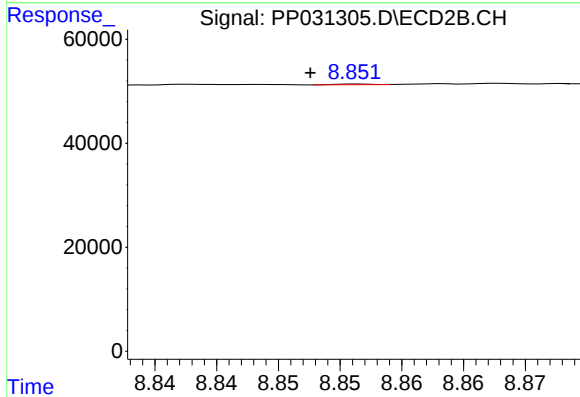


#40 AR-1262-5

R.T.: 8.851 min
Delta R.T.: 0.004 min
Response: 239
Conc: 0.17 ng/ml

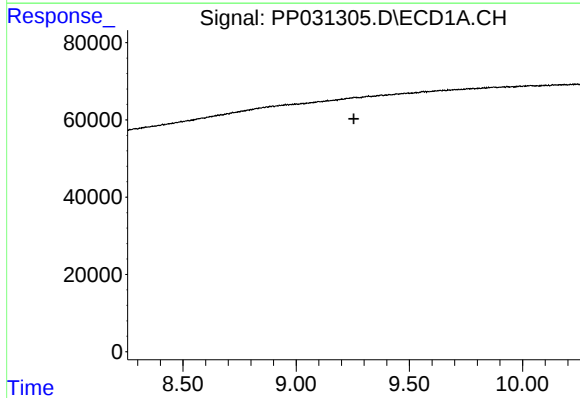


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.255 min
Response: 0
Conc: N.D.

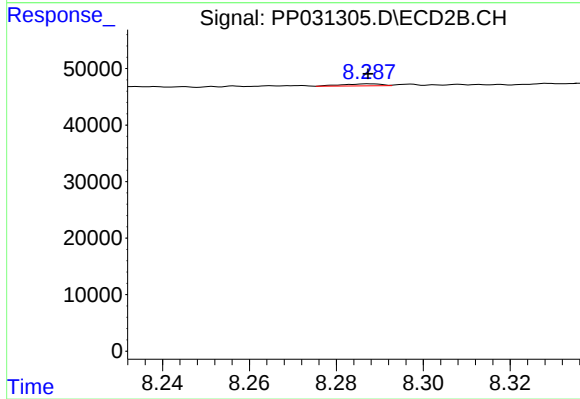

#41 AR-1268-1


R.T.: 8.287 min
Delta R.T.: 0.000 min
Response: 2170
Conc: 0.44 ng/ml

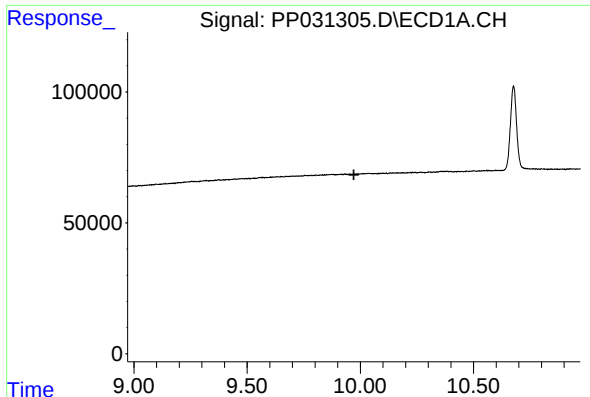

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T.: 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
PB133046BL

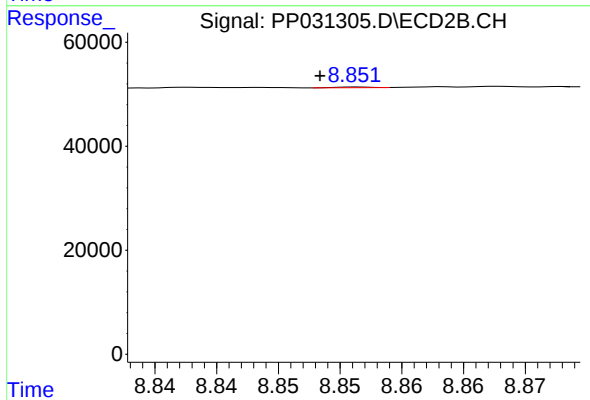


#44 AR-1268-4

R.T.: 8.851 min
Delta R.T.: 0.003 min
Response: 239
Conc: 0.14 ng/ml

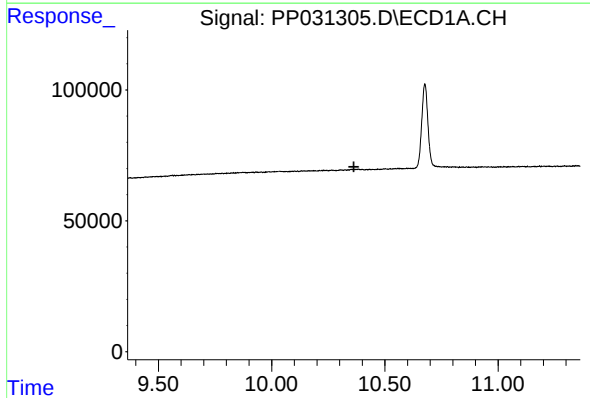

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.363 min
Response: 0
Conc: N.D.

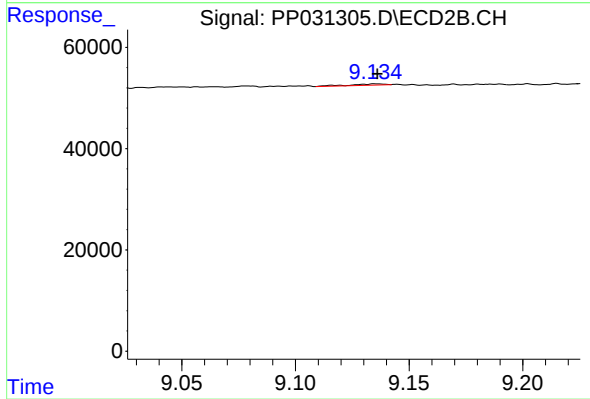

#45 AR-1268-5

R.T.: 9.135 min
Delta R.T.: -0.001 min
Response: 2655
Conc: 0.20 ng/ml