

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031320.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 22:32
 Operator : DD\AJ
 Sample : L4737-02
 Misc :
 ALS Vial : 34 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MS-MSD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:47:49 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.798	4.073	997702	980583	24.490	23.454
2)	SA Decachlor...	10.676	9.387	602241	603180	19.608	18.013
Target Compounds							
9)	L2 AR-1221-2	0.000	4.426	0	11266	N.D.	31.903 #
32)	L7 AR-1260-2	0.000	7.090f	0	2043	N.D.	1.004 #
33)	L7 AR-1260-3	0.000	7.280	0	3099	N.D.	1.606 #
38)	L8 AR-1262-3	0.000	8.289	0	4088	N.D.	2.565 #
40)	L8 AR-1262-5	0.000	8.851	0	4273	N.D.	3.028 #
41)	L9 AR-1268-1	0.000	8.289	0	4088	N.D.	0.830 #
43)	L9 AR-1268-3	0.000	8.564	0	1484	N.D.	0.356 #
44)	L9 AR-1268-4	0.000	8.851	0	4273	N.D.	2.564 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031320.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 22:32
Operator : DD\AJ
Sample : L4737-02
Misc :
ALS Vial : 34 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MS-MSD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:47:49 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

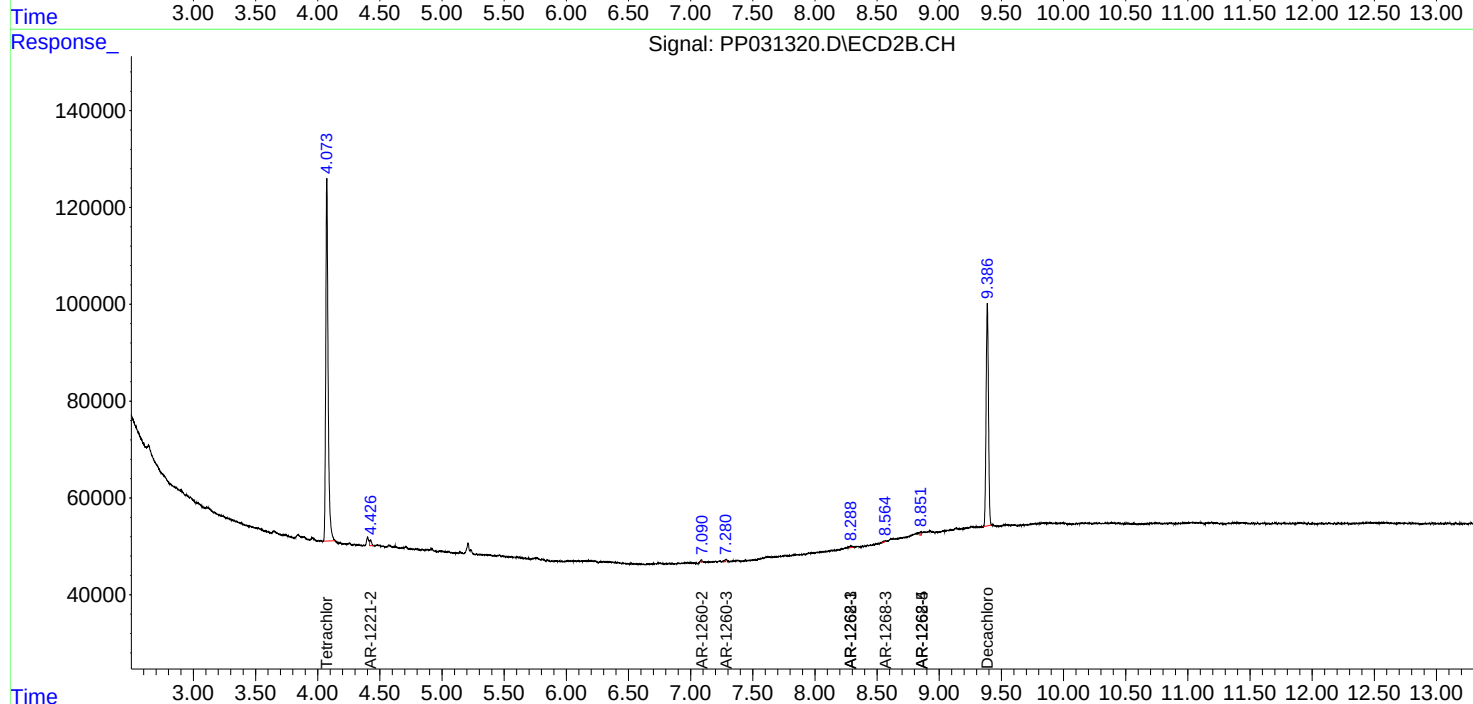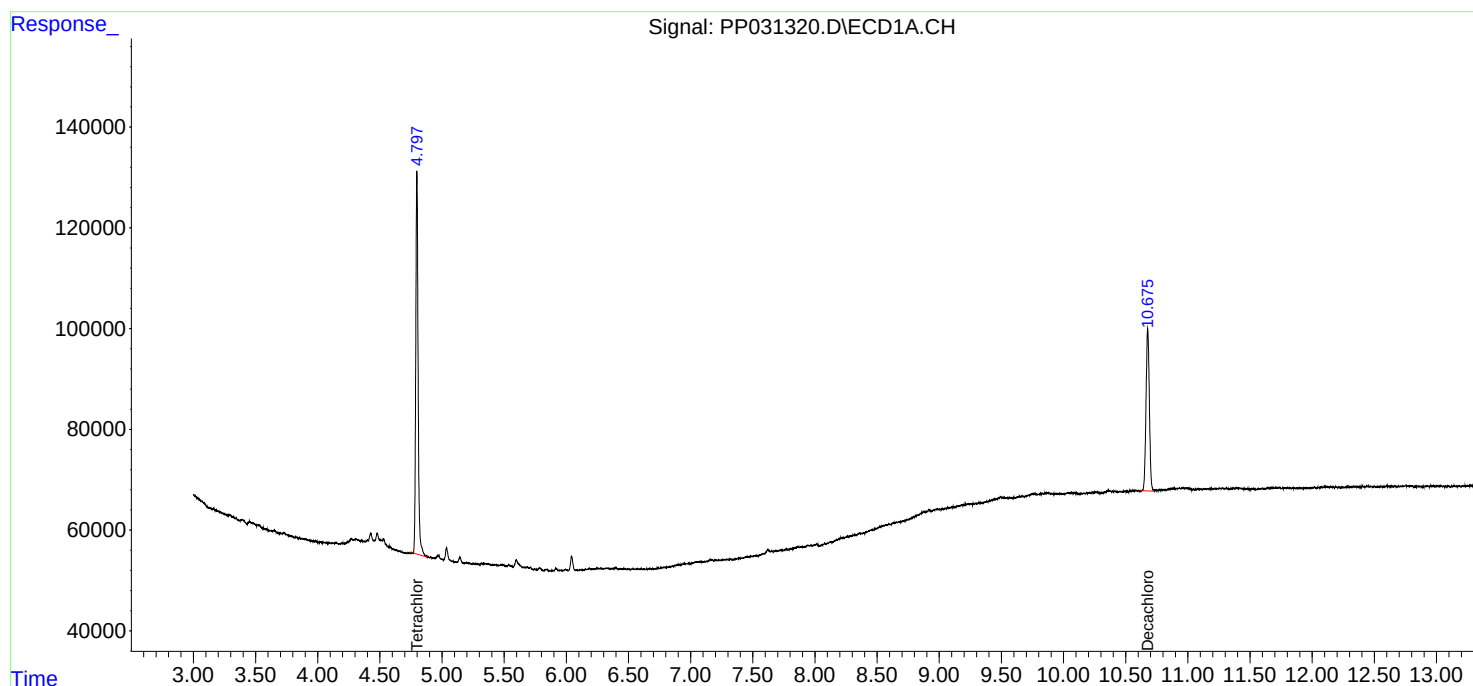


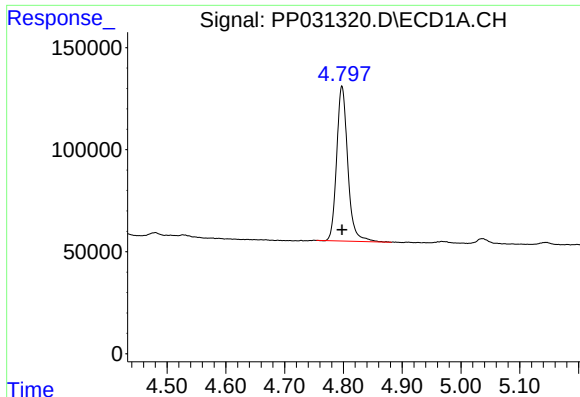

#1 Tetrachloro-m-xylene


R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 997702
Conc: 24.49 ng/ml

Instrument :
ECD_P
ClientSampleId :
MS-MSD

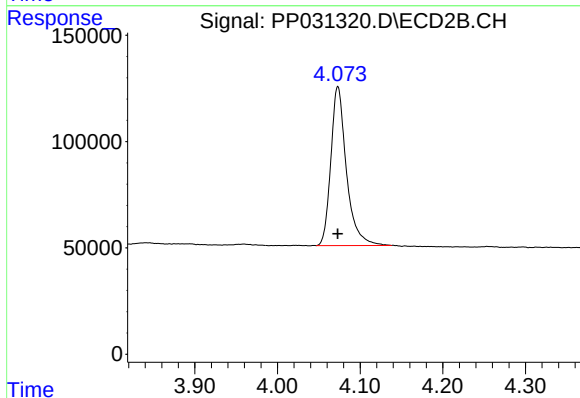


#1 Tetrachloro-m-xylene

R.T.: 4.073 min
Delta R.T.: 0.000 min
Response: 980583
Conc: 23.45 ng/ml

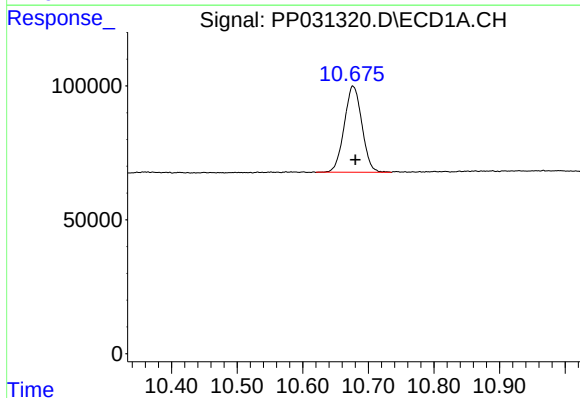


#2 Decachlorobiphenyl

R.T.: 10.676 min
Delta R.T.: -0.004 min
Response: 602241
Conc: 19.61 ng/ml

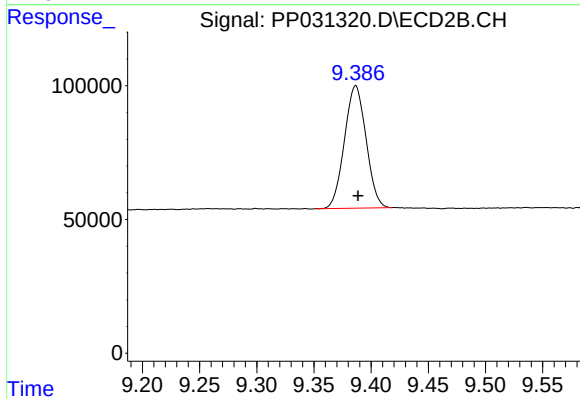

#2 Decachlorobiphenyl


R.T.: 9.387 min
Delta R.T.: -0.002 min
Response: 603180
Conc: 18.01 ng/ml

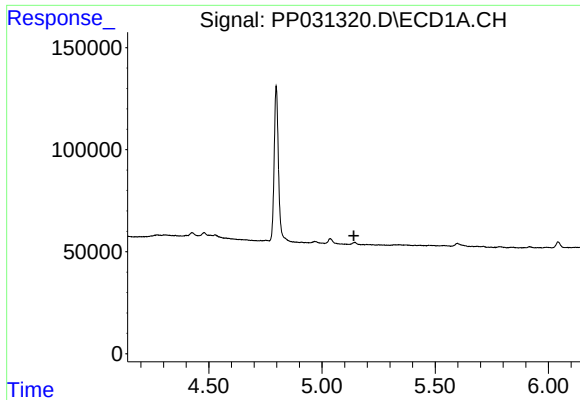

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-MSD

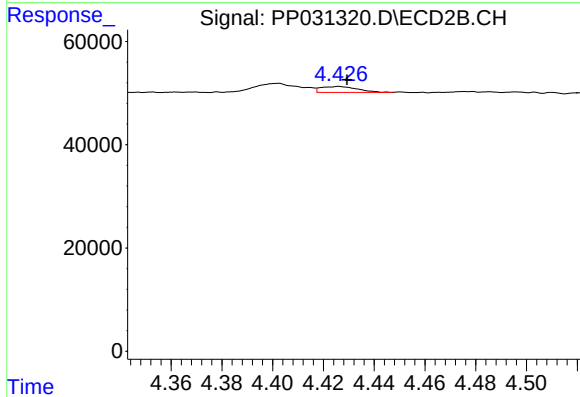


#9 AR-1221-2

R.T.: 4.426 min
Delta R.T.: -0.003 min
Response: 11266
Conc: 31.90 ng/ml

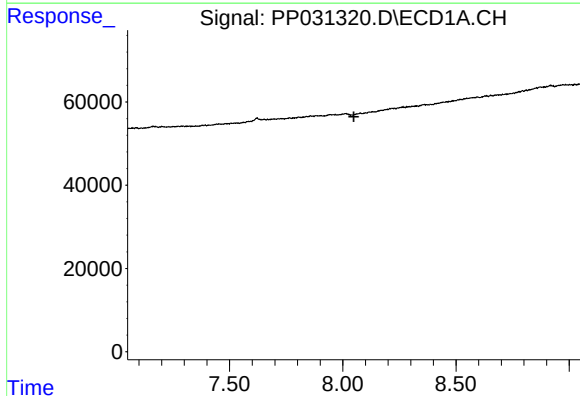


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T.: 8.049 min
Response: 0
Conc: N.D.

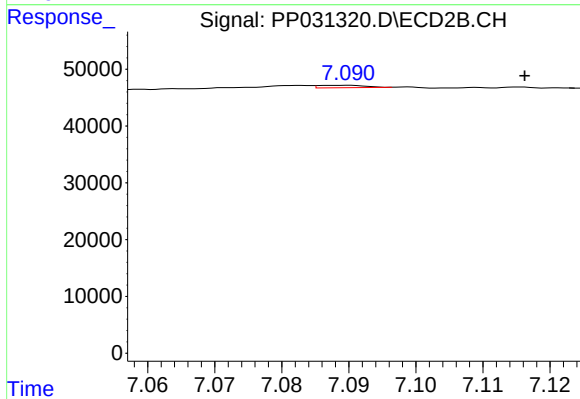

#32 AR-1260-2


R.T.: 7.090 min
Delta R.T.: -0.026 min
Response: 2043
Conc: 1.00 ng/ml

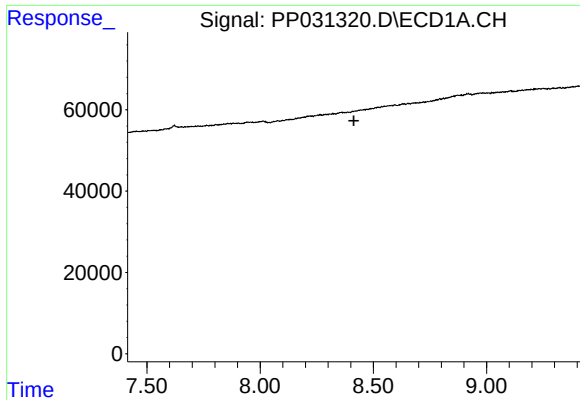

#33 AR-1260-3


R.T.: 0.000 min
Exp R.T.: 8.414 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-MSD

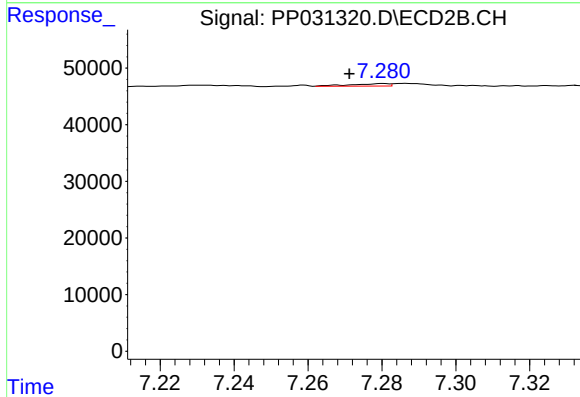


#33 AR-1260-3

R.T.: 7.280 min
Delta R.T.: 0.009 min
Response: 3099
Conc: 1.61 ng/ml

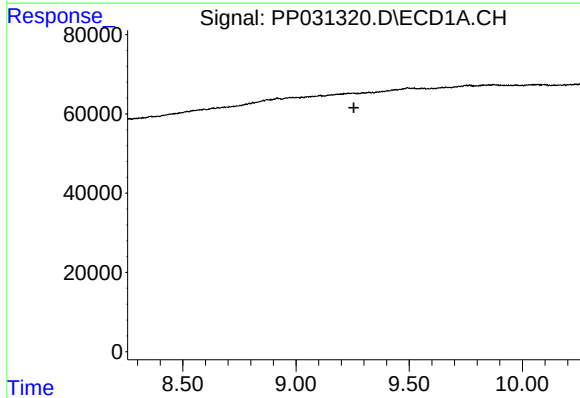


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.256 min
Response: 0
Conc: N.D.

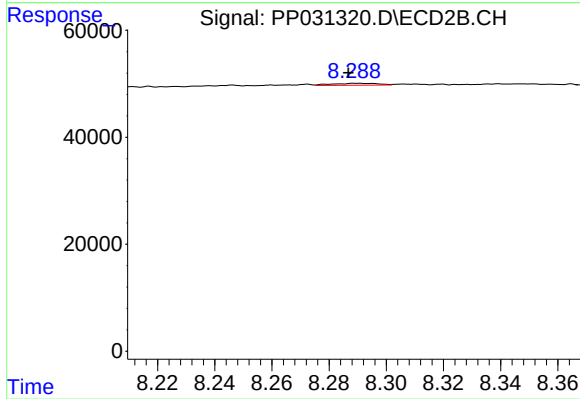

#38 AR-1262-3


R.T.: 8.289 min
Delta R.T.: 0.002 min
Response: 4088
Conc: 2.56 ng/ml

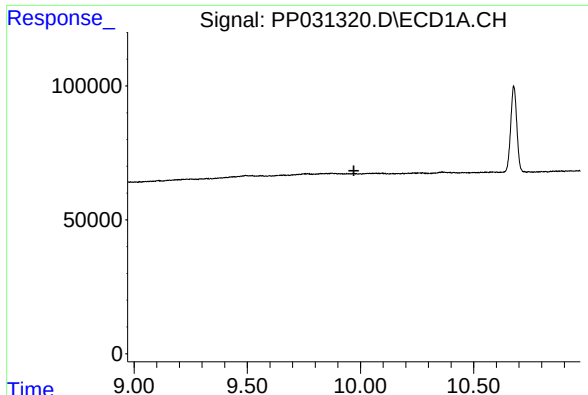

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-MSD

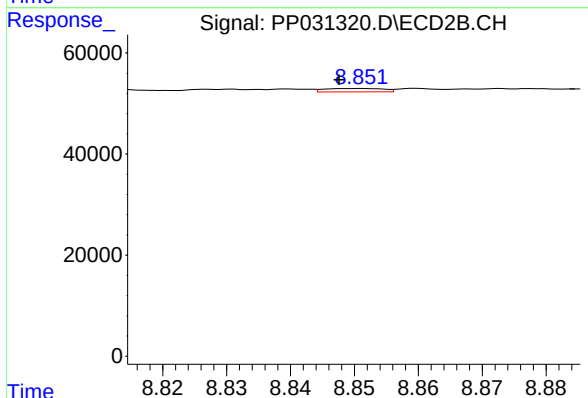


#40 AR-1262-5

R.T.: 8.851 min
Delta R.T.: 0.003 min
Response: 4273
Conc: 3.03 ng/ml

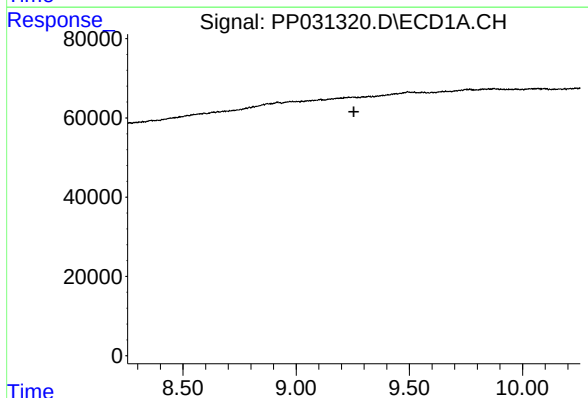


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.255 min
Response: 0
Conc: N.D.

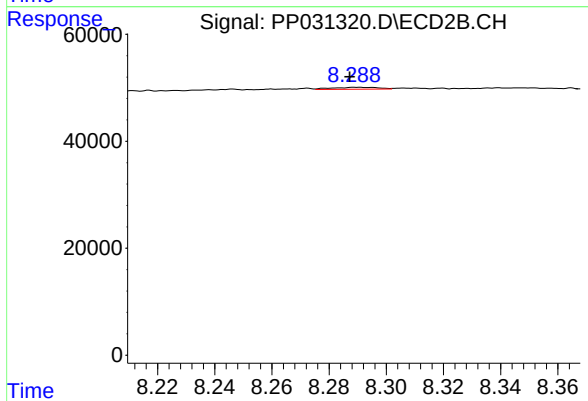

#41 AR-1268-1


R.T.: 8.289 min
Delta R.T.: 0.002 min
Response: 4088
Conc: 0.83 ng/ml

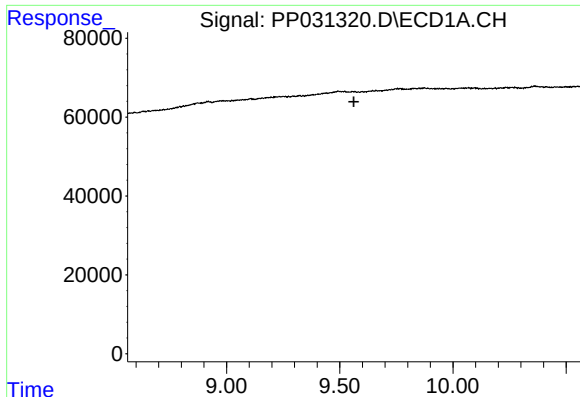

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.562 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
MS-MSD

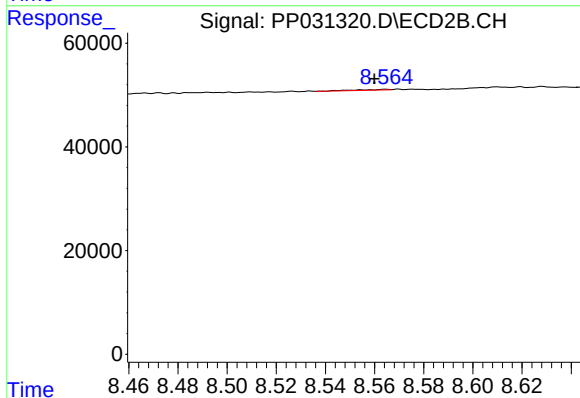


#43 AR-1268-3

R.T.: 8.564 min
Delta R.T.: 0.004 min
Response: 1484
Conc: 0.36 ng/ml

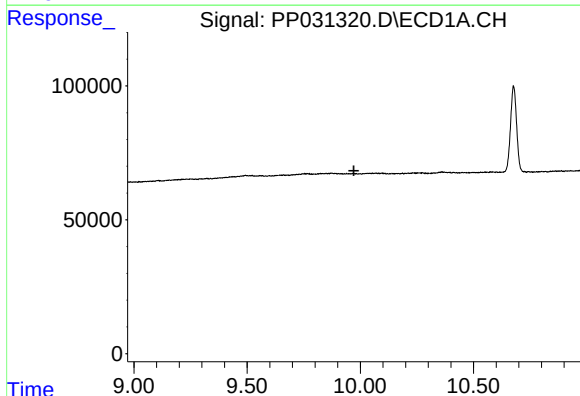

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.972 min
Response: 0
Conc: N.D.

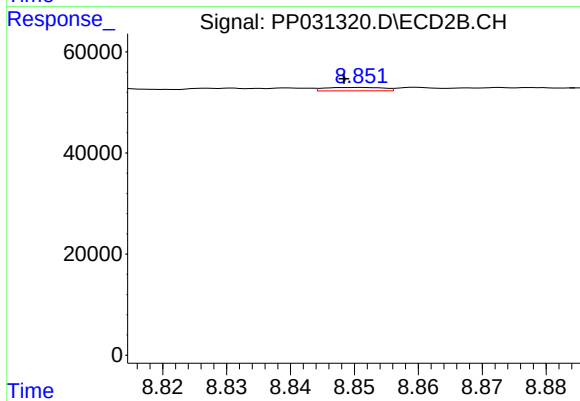

#44 AR-1268-4

R.T.: 8.851 min
Delta R.T.: 0.003 min
Response: 4273
Conc: 2.56 ng/ml