

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031313.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 20:35
 Operator : DD\AJ
 Sample : L4734-01
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 BARNUM-STREET-TEST-PIT-1

Manual Integrations
 APPROVED

Ankita
 11/18/2020 9:02:21 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:44:22 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.796	4.070	996937	951777	24.471	22.765
2) SA Decachlor...	10.675	9.384	665623	718933	21.672	21.470
Target Compounds						
31) L7 AR-1260-1	7.779	6.916	62677	64661	44.878m	38.698
32) L7 AR-1260-2	8.042	7.114	196469	90857	118.067m	44.646 #
33) L7 AR-1260-3	8.411	7.268	35585	62097	27.855m	32.184
34) L7 AR-1260-4	8.639	7.752	48569	43614	31.770m	27.044
35) L7 AR-1260-5	8.954	7.998	74303	100397	23.576	25.412

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031313.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 20:35
Operator : DD\AJ
Sample : L4734-01
Misc :
ALS Vial : 27 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
BARNUM-STREET-TEST-PIT-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:21 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:44:22 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

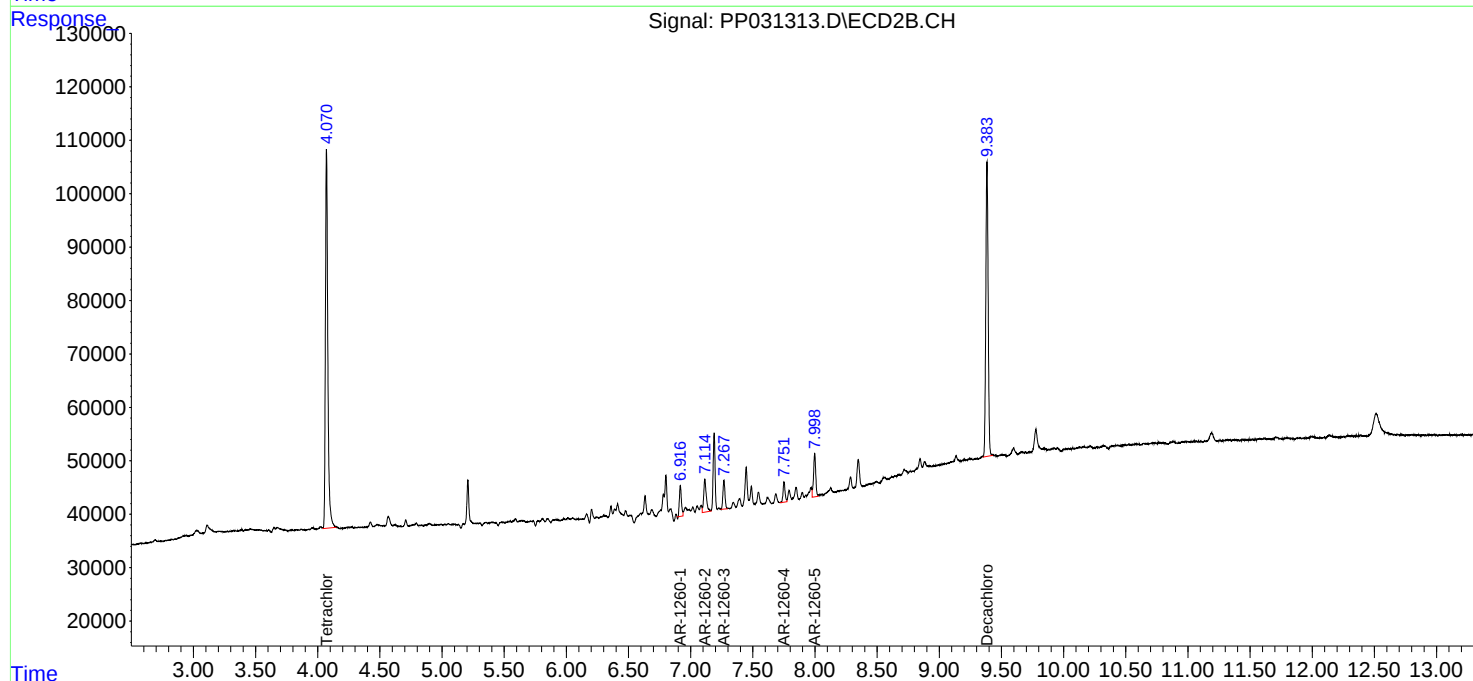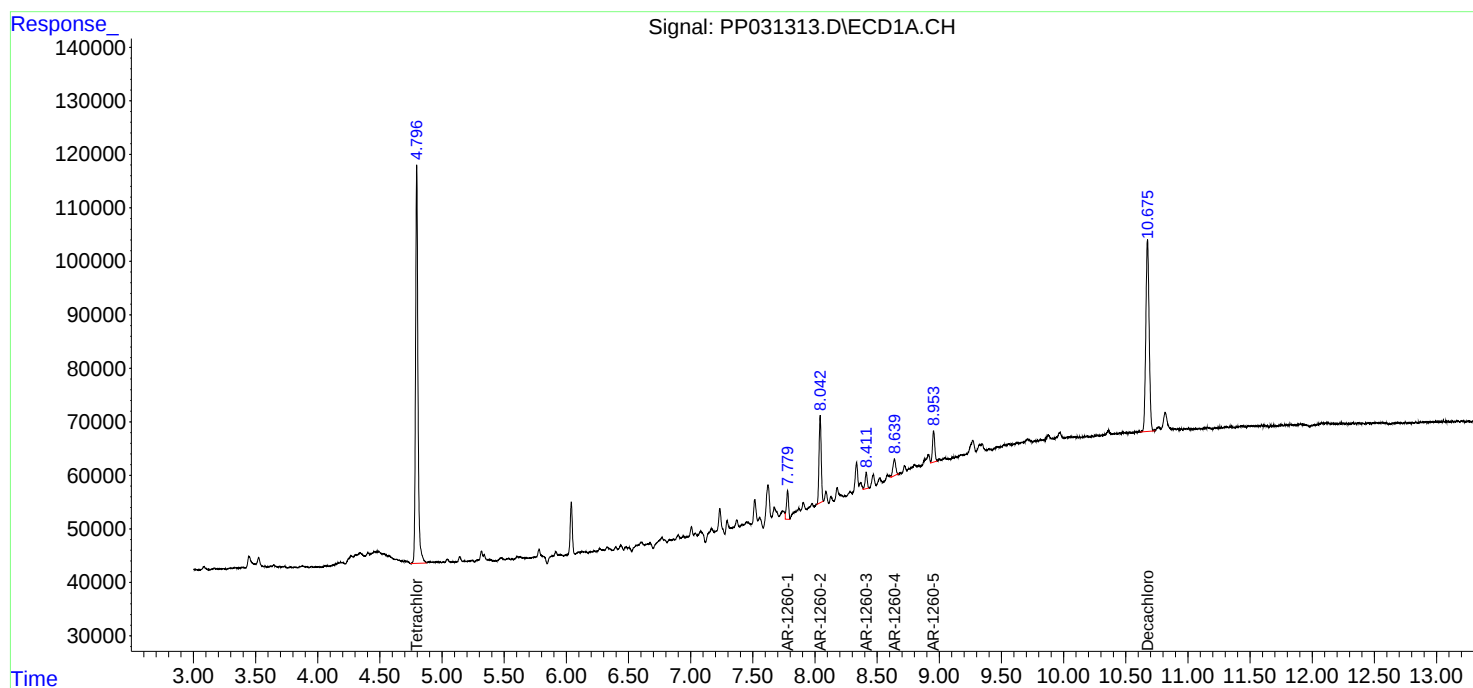

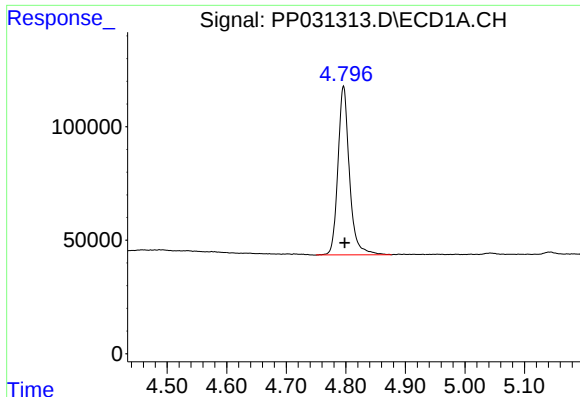


#1 Tetrachloro-m-xylene

R.T.: 4.796 min
Delta R.T.: -0.002 min
Response: 996937
Conc: 24.47 ng/ml

Instrument :
ECD_P
ClientSampleId :
BARNUM-STREET-TEST-PIT-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:21 AM

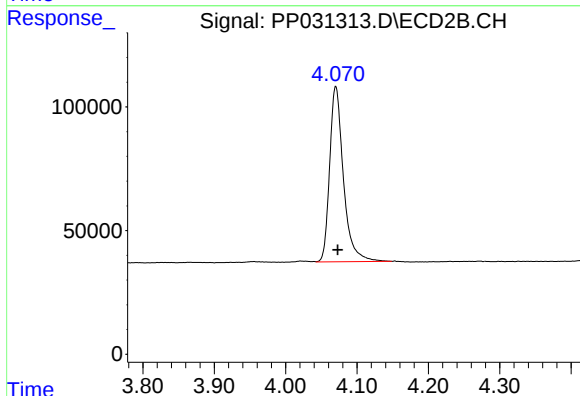


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.003 min
Response: 951777
Conc: 22.77 ng/ml

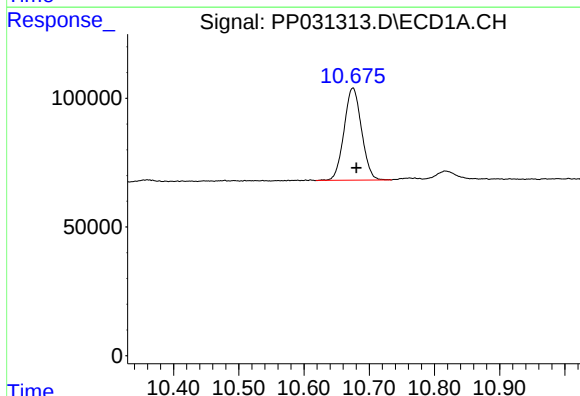


#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: -0.005 min
Response: 665623
Conc: 21.67 ng/ml

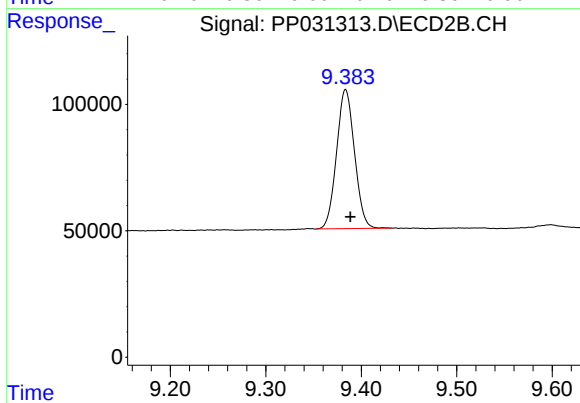

#2 Decachlorobiphenyl

R.T.: 9.384 min
Delta R.T.: -0.005 min
Response: 718933
Conc: 21.47 ng/ml

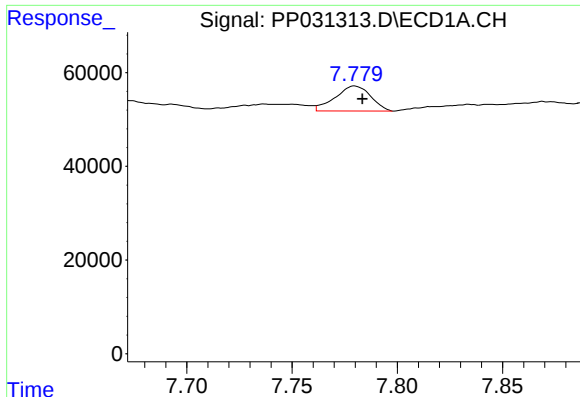


#31 AR-1260-1

R.T.: 7.779 min
Delta R.T.: -0.004 min
Response: 62677
Conc: 44.88 ng/ml m

Instrument :
ECD_P
ClientSampleId :
BARNUM-STREET-TEST-PIT-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:21 AM

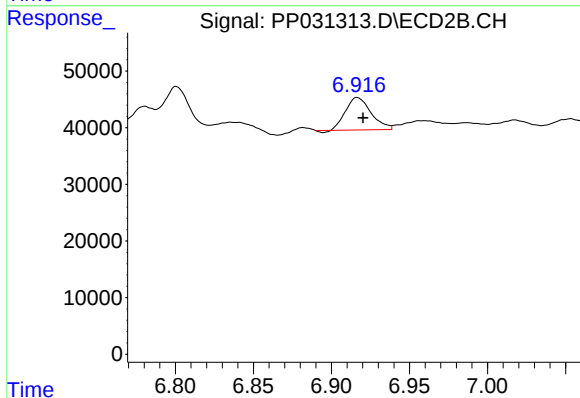


#31 AR-1260-1

R.T.: 6.916 min
Delta R.T.: -0.004 min
Response: 64661
Conc: 38.70 ng/ml

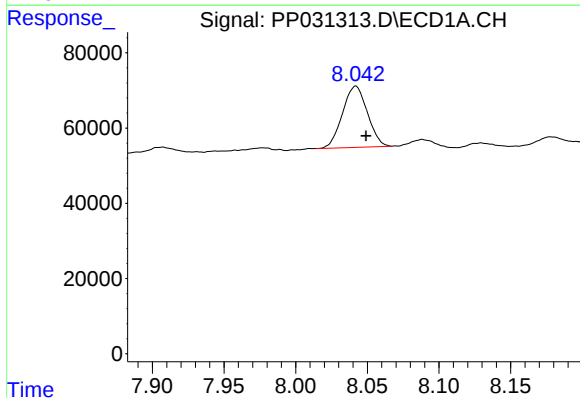


#32 AR-1260-2

R.T.: 8.042 min
Delta R.T.: -0.008 min
Response: 196469
Conc: 118.07 ng/ml m

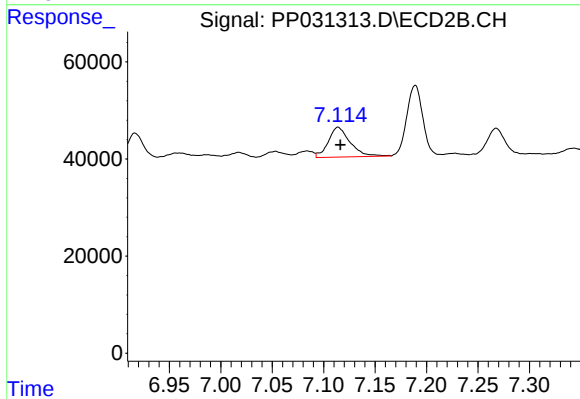

#32 AR-1260-2

R.T.: 7.114 min
Delta R.T.: -0.002 min
Response: 90857
Conc: 44.65 ng/ml

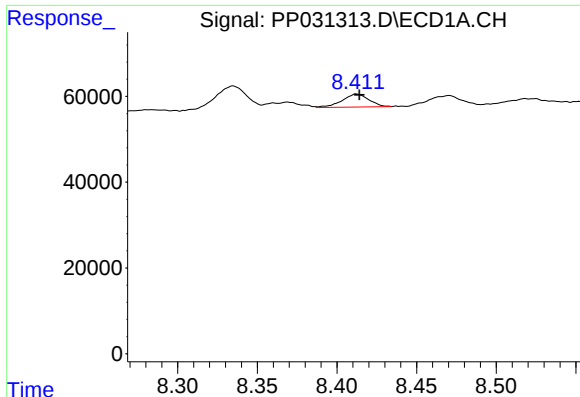


#33 AR-1260-3

R.T.: 8.411 min
Delta R.T.: -0.003 min
Response: 35585
Conc: 27.86 ng/ml m

Instrument :
ECD_P
ClientSampleId :
BARNUM-STREET-TEST-PIT-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:21 AM

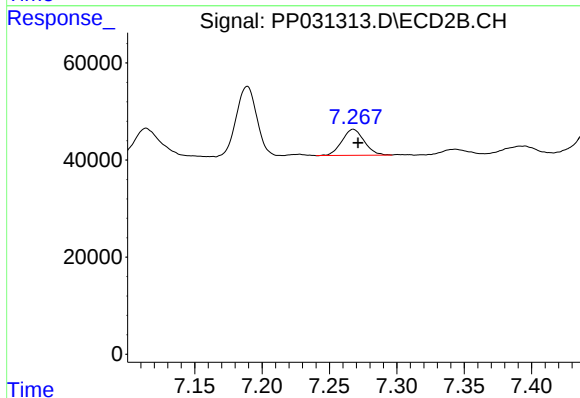


#33 AR-1260-3

R.T.: 7.268 min
Delta R.T.: -0.004 min
Response: 62097
Conc: 32.18 ng/ml

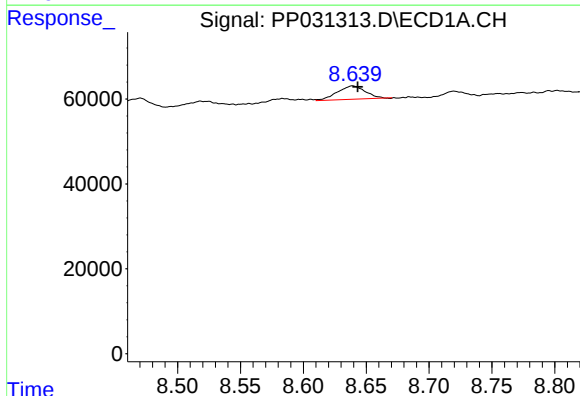


#34 AR-1260-4

R.T.: 8.639 min
Delta R.T.: -0.004 min
Response: 48569
Conc: 31.77 ng/ml m

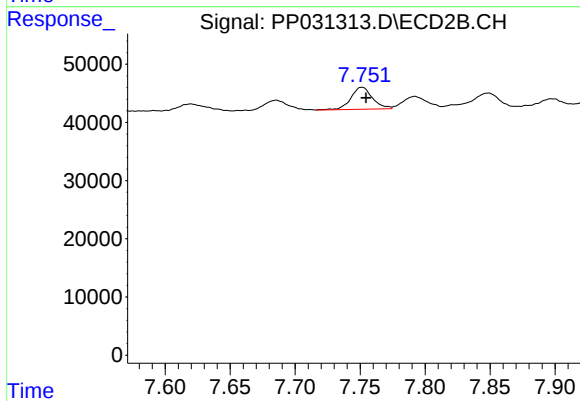

#34 AR-1260-4

R.T.: 7.752 min
Delta R.T.: -0.003 min
Response: 43614
Conc: 27.04 ng/ml

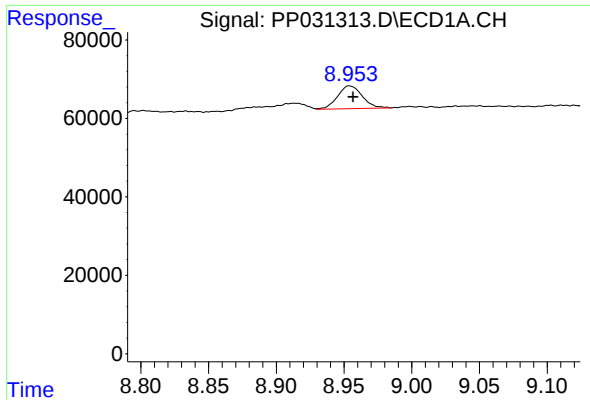


#35 AR-1260-5

R.T.: 8.954 min
Delta R.T.: -0.003 min
Response: 74303
Conc: 23.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
BARNUM-STREET-TEST-PIT-1

Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:21 AM

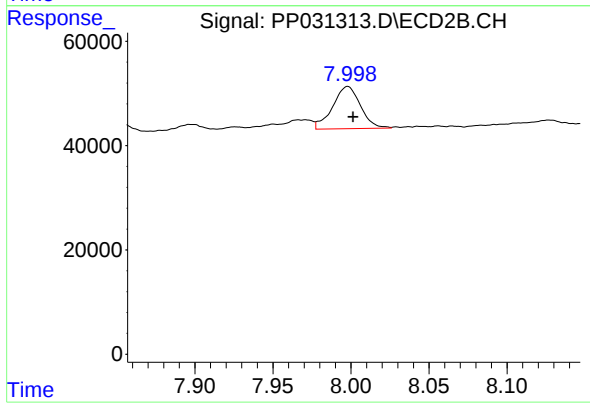

#35 AR-1260-5

R.T.: 7.998 min
Delta R.T.: -0.003 min
Response: 100397
Conc: 25.41 ng/ml