

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031316.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Nov 2020 21:25
 Operator : DD\AJ
 Sample : L4770-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FJ-BH-02-0-1

Manual Integrations
 APPROVED

Ankita
 11/18/2020 9:02:23 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:45:38 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.796	4.071	1074924	1029210	26.386	24.617
2) SA Decachlor...	10.675	9.384	801581	826942	26.098m	24.696

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031316.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Nov 2020 21:25
Operator : DD\AJ
Sample : L4770-07
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
FJ-BH-02-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:23 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:45:38 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

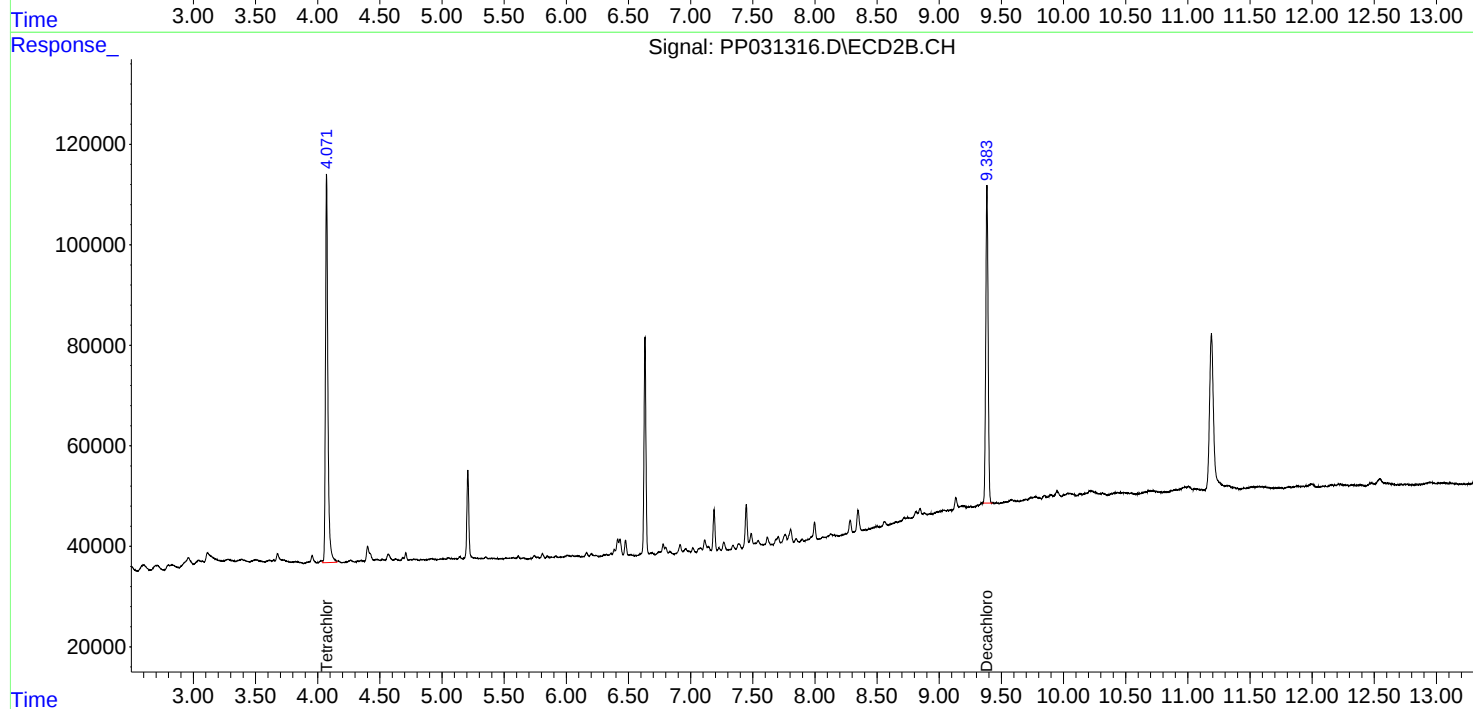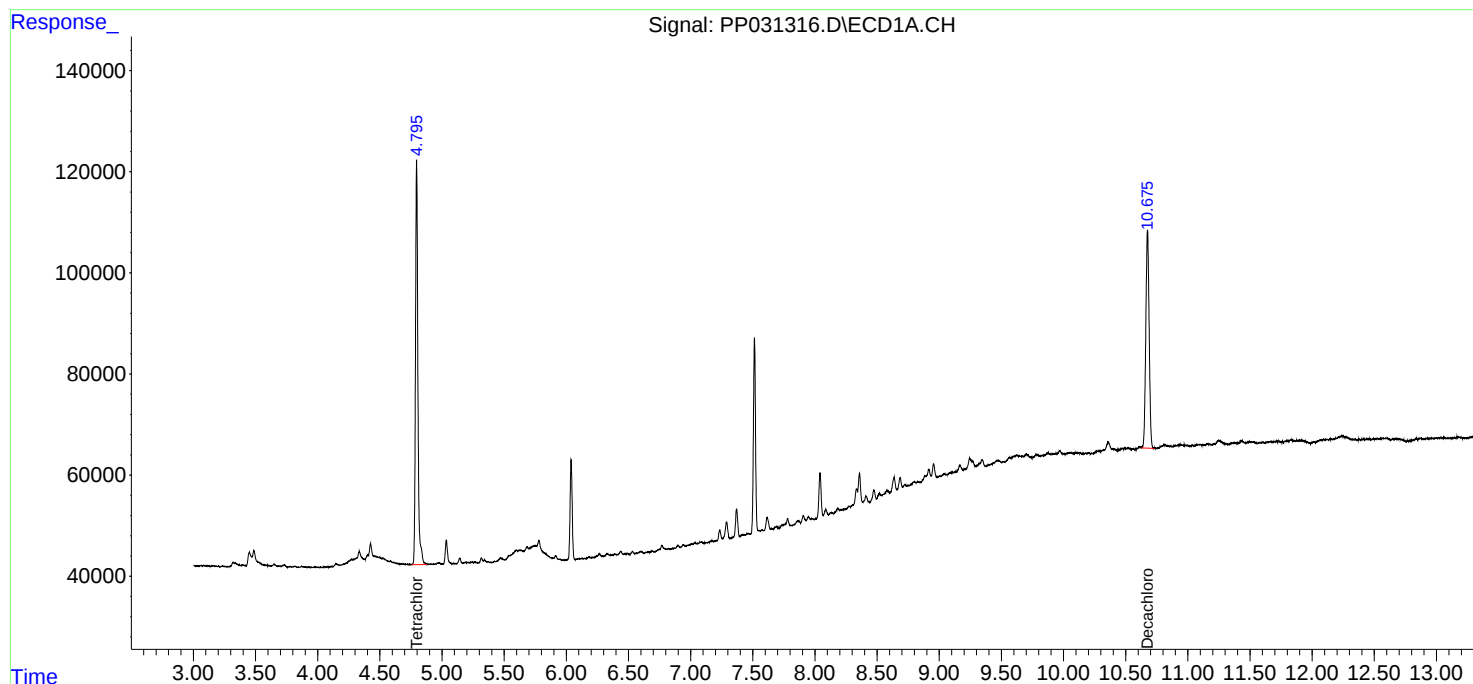

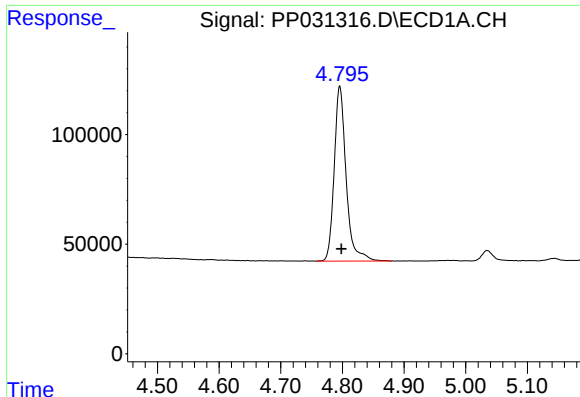


#1 Tetrachloro-m-xylene

R.T.: 4.796 min
Delta R.T.: -0.002 min
Response: 1074924
Conc: 26.39 ng/ml

Instrument :
ECD_P
ClientSampleId :
FJ-BH-02-0-1


Manual Integrations
APPROVED

Ankita
11/18/2020 9:02:23 AM

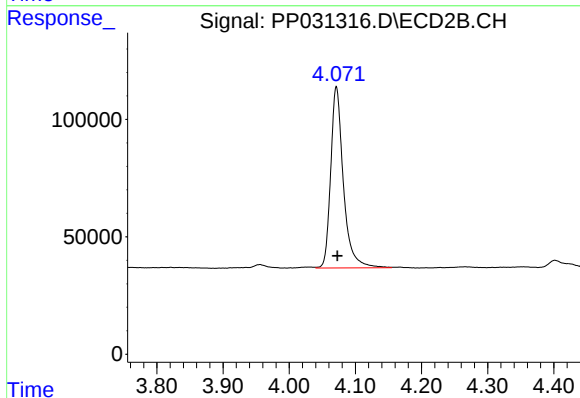


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.002 min
Response: 1029210
Conc: 24.62 ng/ml

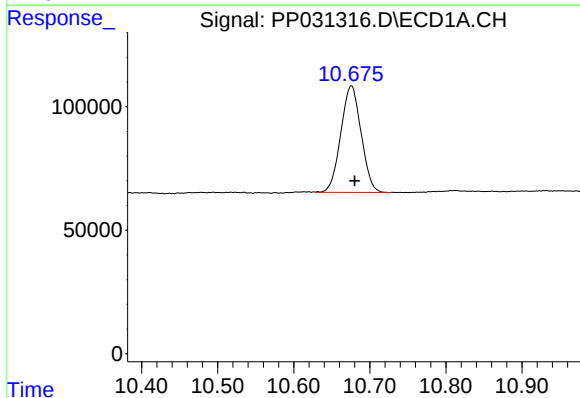

#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: -0.005 min
Response: 801581
Conc: 26.10 ng/ml m

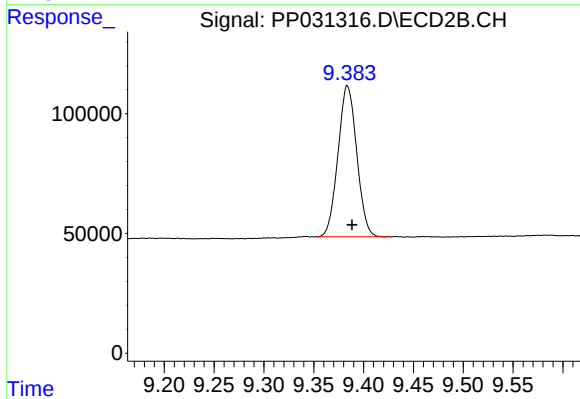

#2 Decachlorobiphenyl

R.T.: 9.384 min
Delta R.T.: -0.005 min
Response: 826942
Conc: 24.70 ng/ml