

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
 Data File : PP031335.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 2:58
 Operator : DD\AJ
 Sample : PB133058BL
 Misc :
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB133058BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 04:54:28 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.796	4.072	894387	871954	21.954	20.856
2) SA Decachlor...	10.673	9.383	684299	749249	22.280	22.376

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111720\
Data File : PP031335.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 2:58
Operator : DD\AJ
Sample : PB133058BL
Misc :
ALS Vial : 47 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB133058BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 04:54:28 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

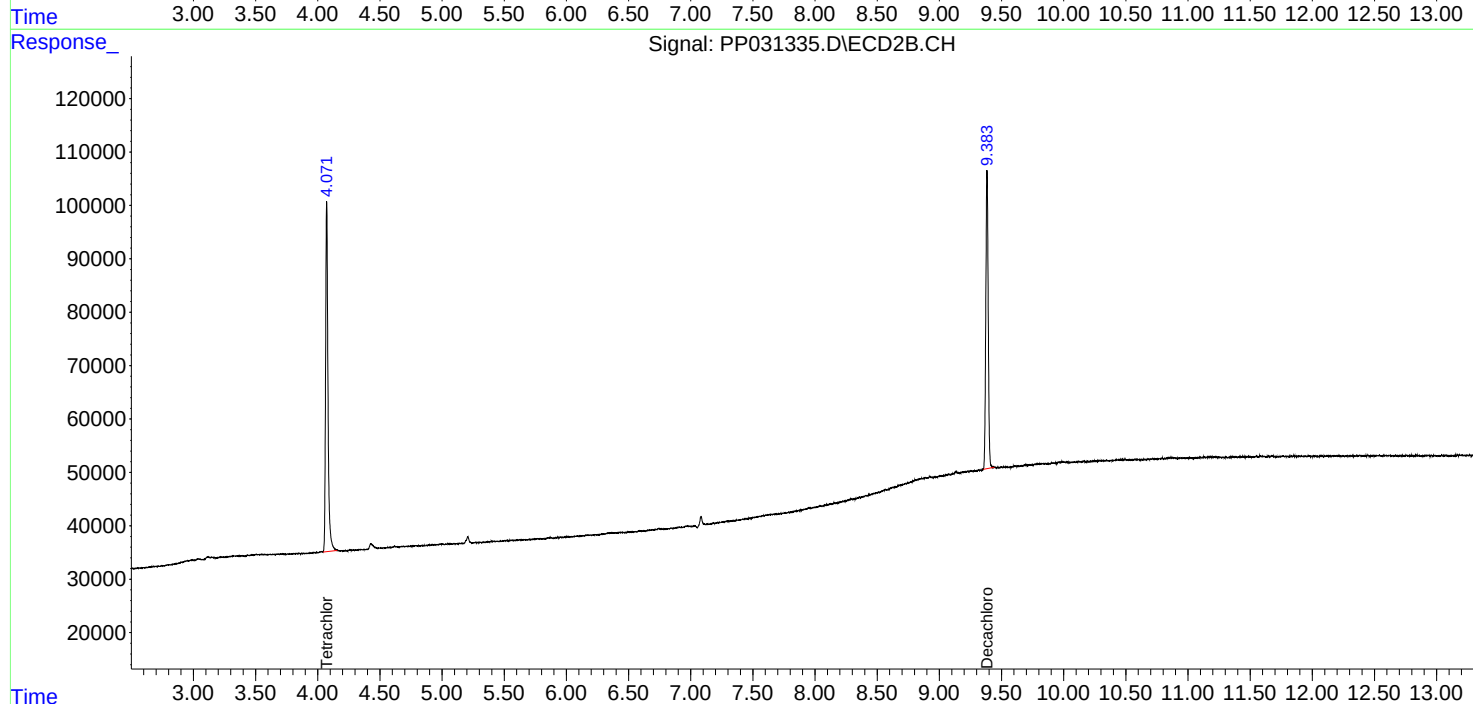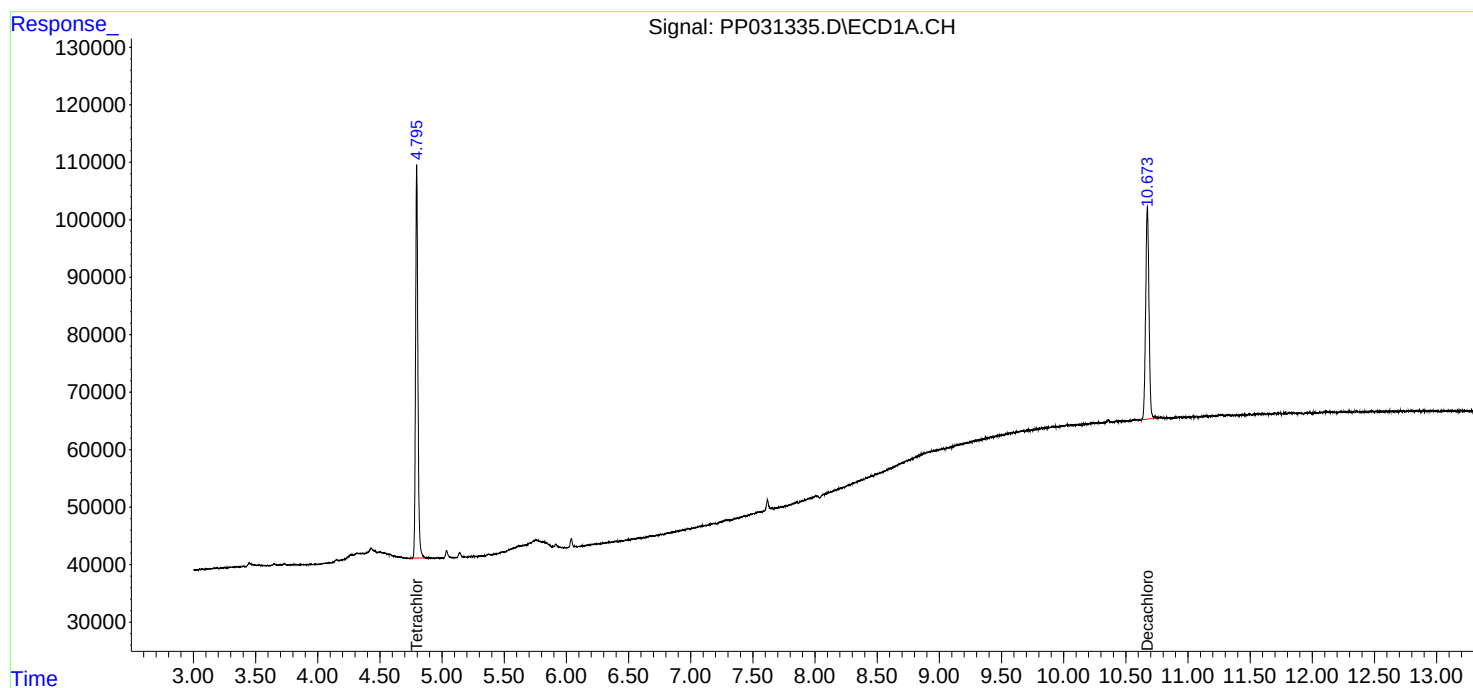


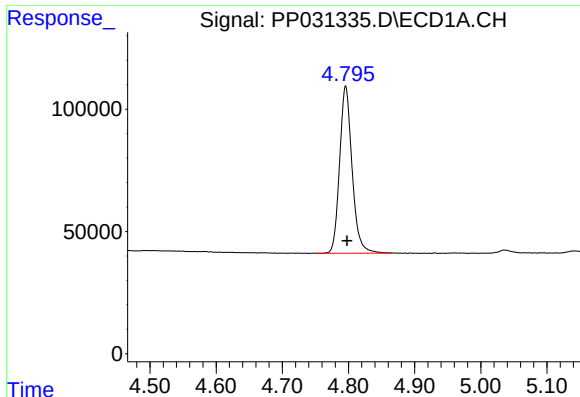

#1 Tetrachloro-m-xylene


R.T.: 4.796 min
Delta R.T.: -0.002 min
Response: 894387
Conc: 21.95 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB133058BL

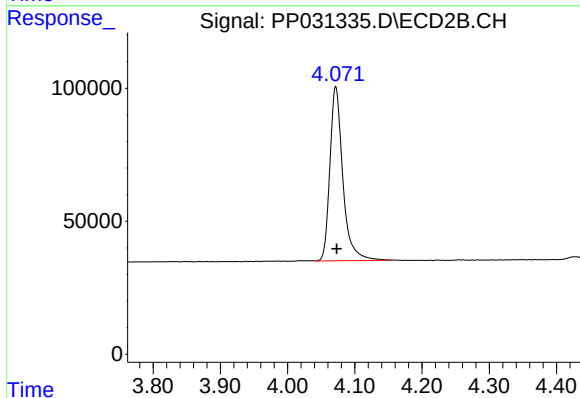


#1 Tetrachloro-m-xylene

R.T.: 4.072 min
Delta R.T.: -0.001 min
Response: 871954
Conc: 20.86 ng/ml

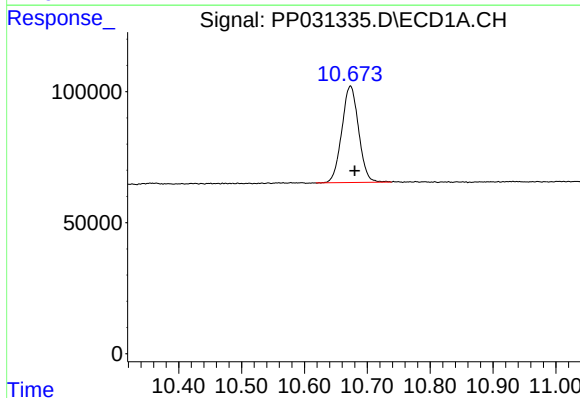

#2 Decachlorobiphenyl

R.T.: 10.673 min
Delta R.T.: -0.007 min
Response: 684299
Conc: 22.28 ng/ml

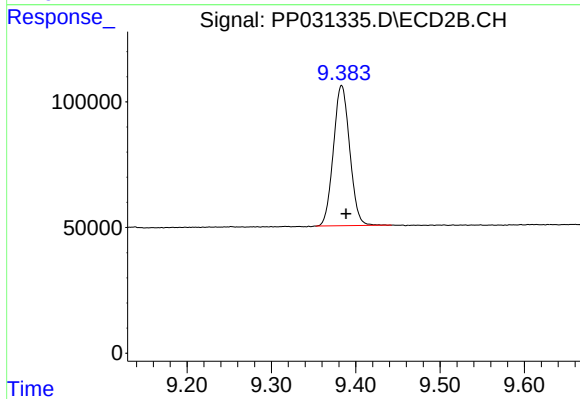

#2 Decachlorobiphenyl

R.T.: 9.383 min
Delta R.T.: -0.005 min
Response: 749249
Conc: 22.38 ng/ml