

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111723\
 Data File : PP061708.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2023 11:05
 Operator : YP\AJ
 Sample : 05434-07
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-4

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/20/2023
 Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 00:20:51 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111523.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Thu Nov 16 04:03:35 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.453	3.728	26558148	39973710	20.154	19.000
2) SA Decachlor...	10.244	8.861	22866401	32152958	22.650	19.700m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111723\
Data File : PP061708.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2023 11:05
Operator : YP\AJ
Sample : 05434-07
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 00:20:51 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111523.M
Quant Title : GC EXTRACTABLES
QLast Update : Thu Nov 16 04:03:35 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

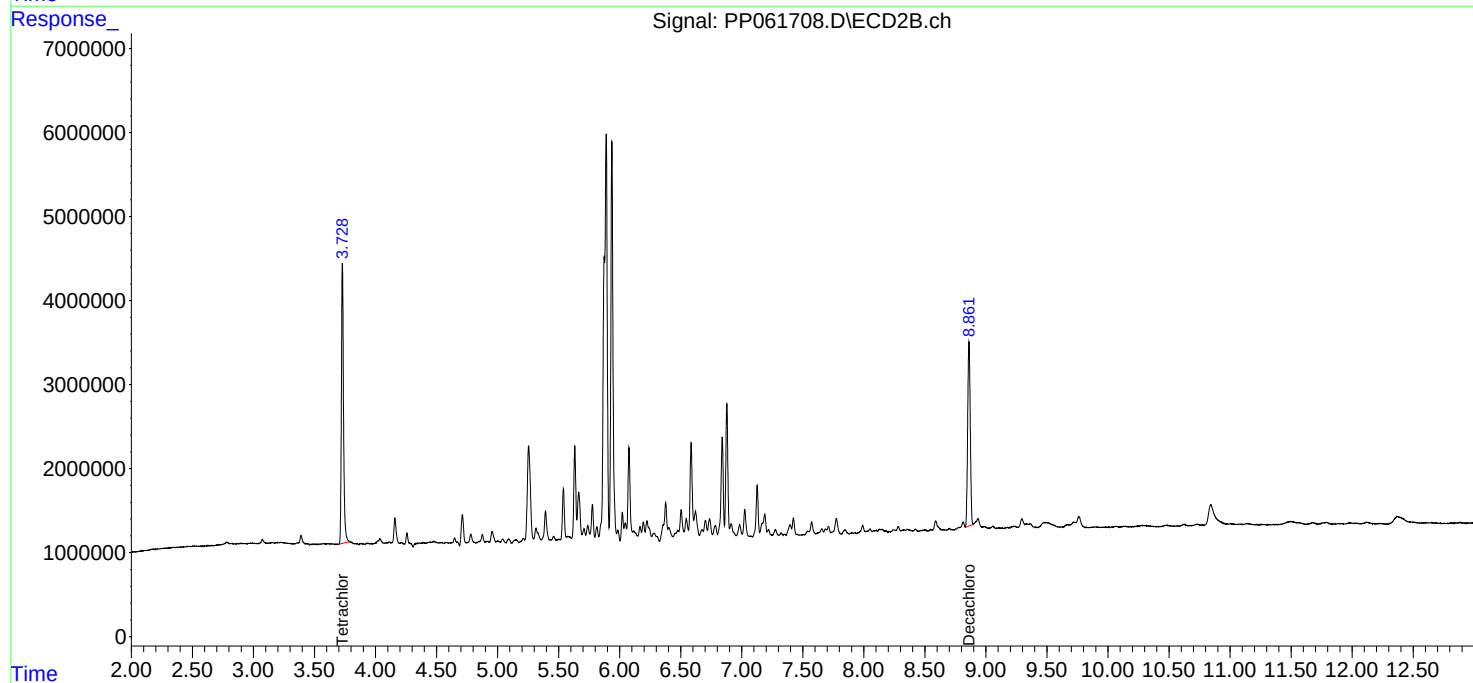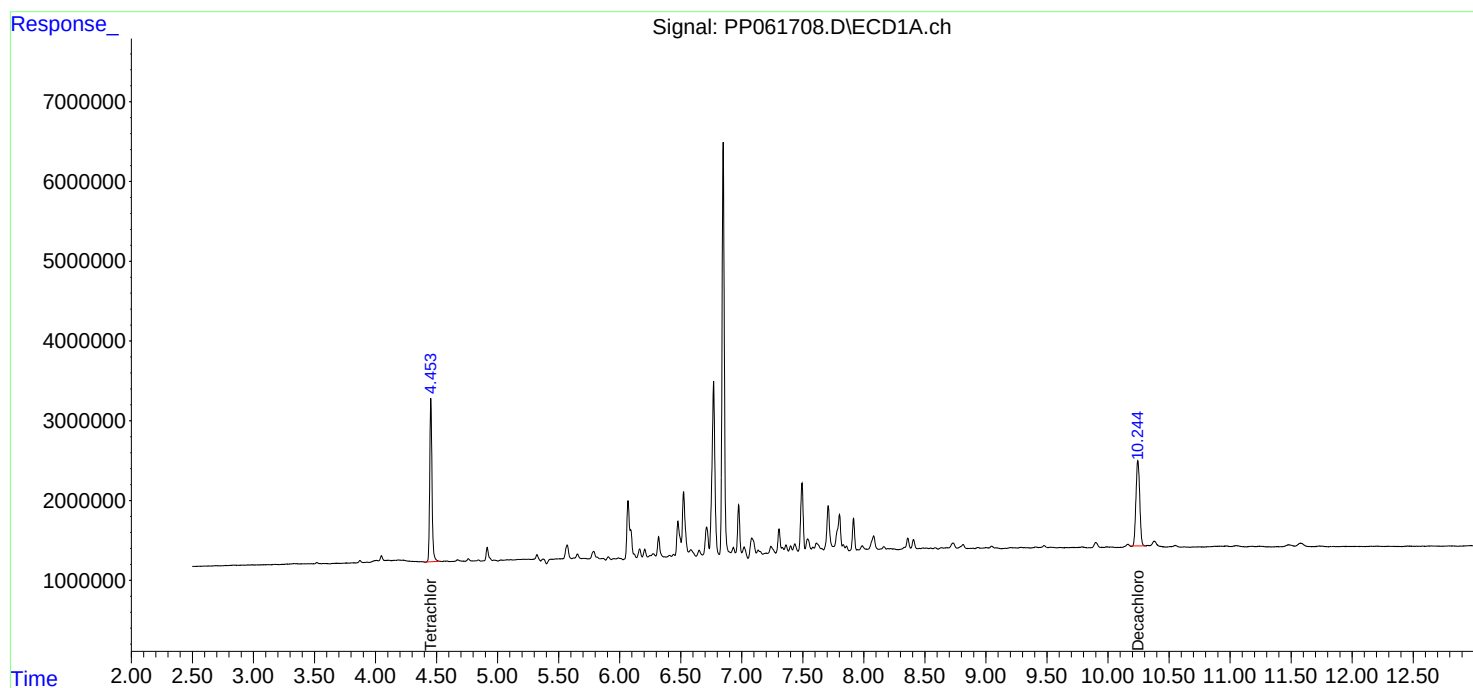

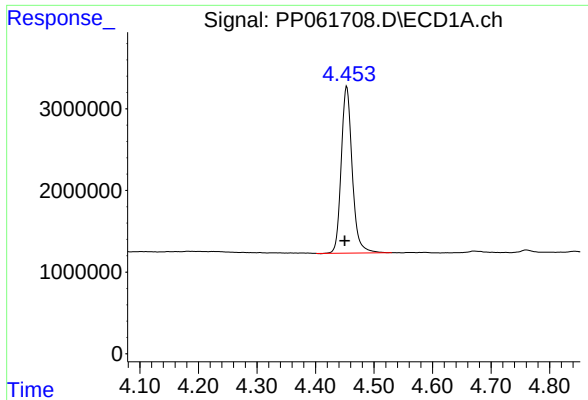


#1 Tetrachloro-m-xylene

R.T.: 4.453 min
Delta R.T.: 0.003 min
Response: 26558148
Conc: 20.15 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-4


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/20/2023
Supervised By :Ankita Jodhani 11/20/2023

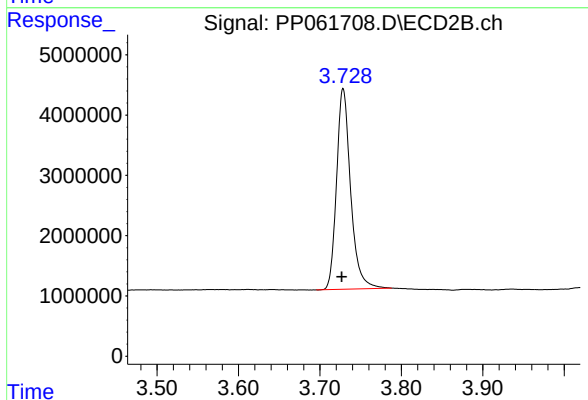


#1 Tetrachloro-m-xylene

R.T.: 3.728 min
Delta R.T.: 0.002 min
Response: 39973710
Conc: 19.00 ng/ml

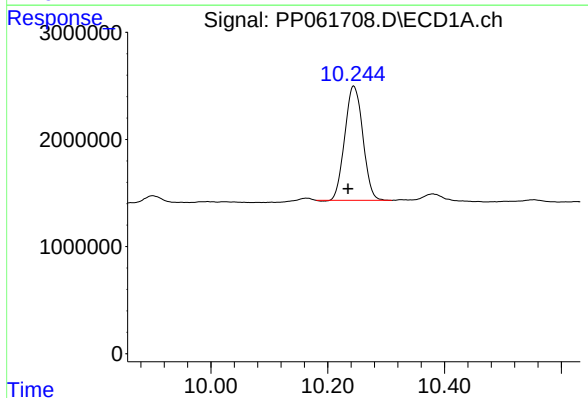

#2 Decachlorobiphenyl

R.T.: 10.244 min
Delta R.T.: 0.009 min
Response: 22866401
Conc: 22.65 ng/ml

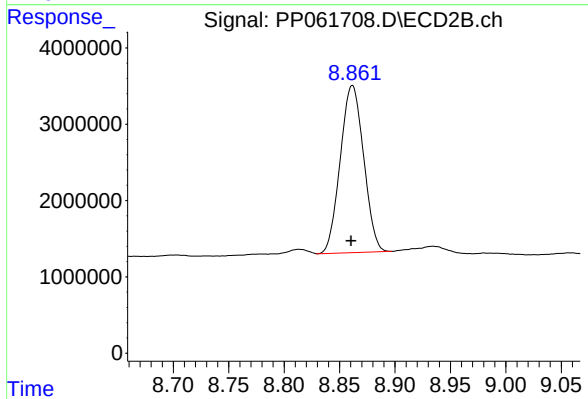

#2 Decachlorobiphenyl

R.T.: 8.861 min
Delta R.T.: 0.000 min
Response: 32152958
Conc: 19.70 ng/ml m