

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
 Data File : PP076529.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 11:25
 Operator : YP\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 11/18/2025
 Supervised By :Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 12:55:23 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.637	3.776	34707592	145.5E6	24.286m	21.982
2) SA Decachlor...	10.412	8.771	25330540	174.7E6	23.530	21.240

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
Data File : PP076529.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 11:25
Operator : YP\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
I.BLK


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2025
Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 12:55:23 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

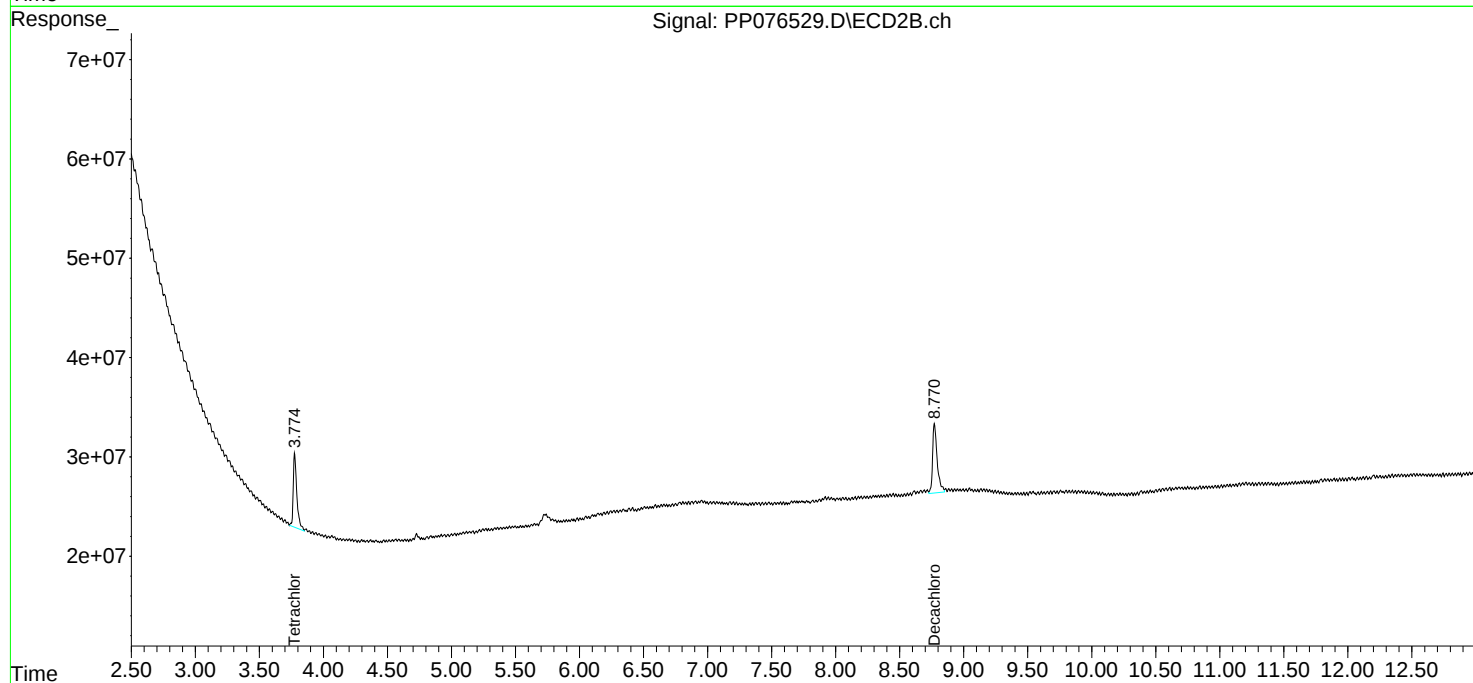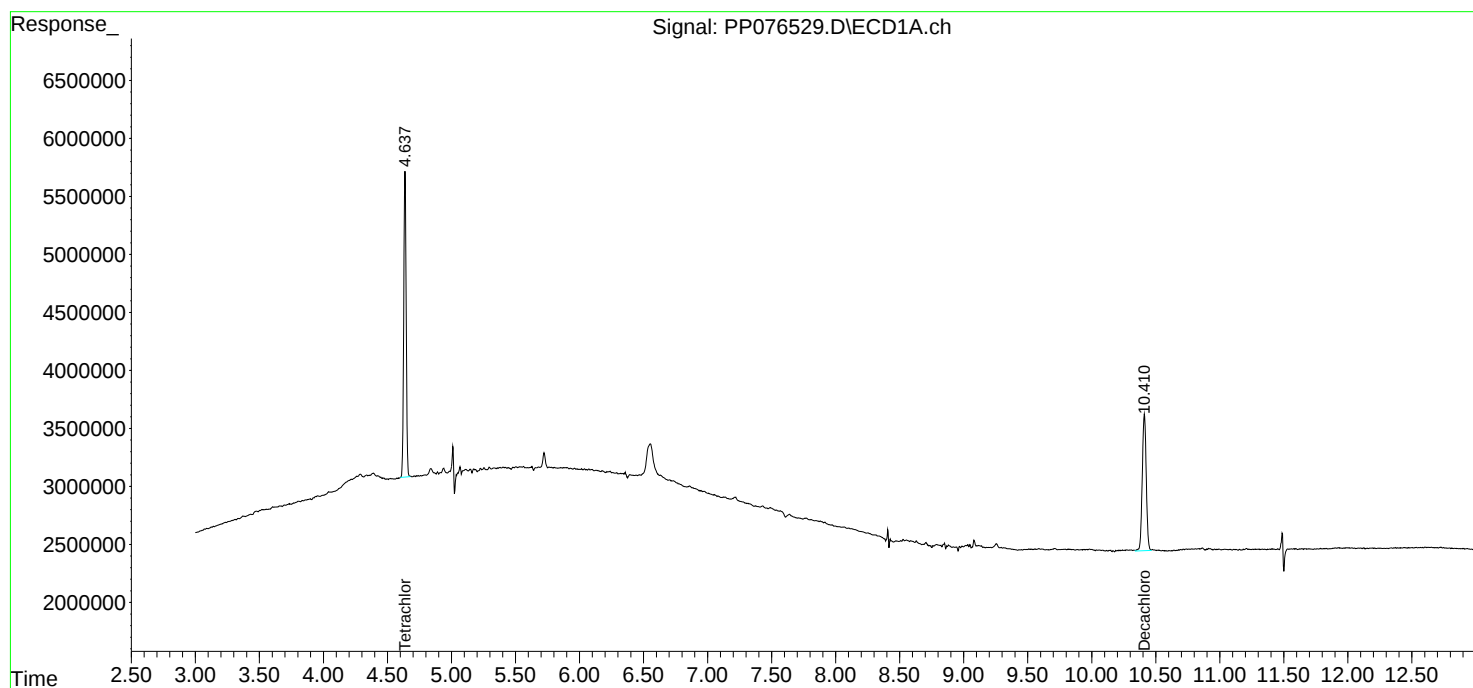

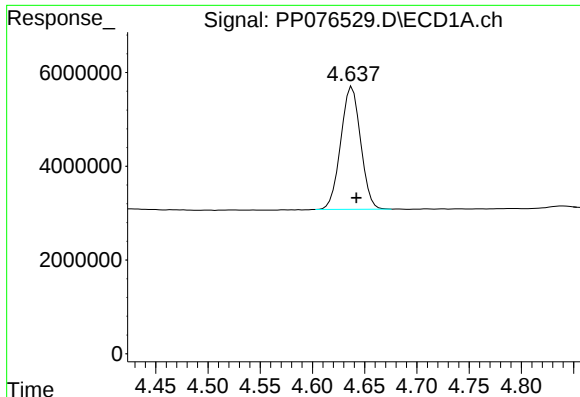

#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.005 min
Response: 34707592
Conc: 24.29 ng/ml

Instrument :

ECD_P


ClientSampleId :

I.BLK

Manual Integrations


APPROVED

Reviewed By :Abdul Mirza 11/18/2025
Supervised By :Sohil Jodhani 11/19/2025

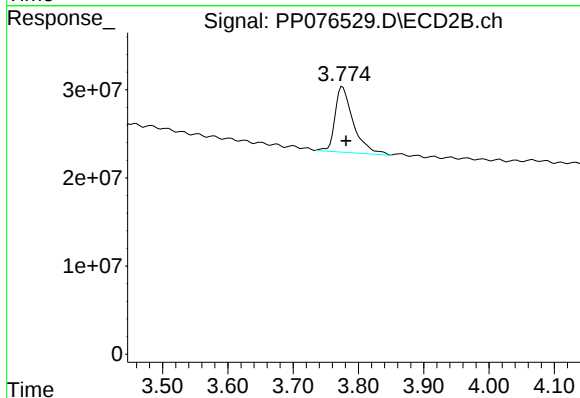


#1 Tetrachloro-m-xylene

R.T.: 3.776 min
Delta R.T.: -0.006 min
Response: 145484533
Conc: 21.98 ng/ml

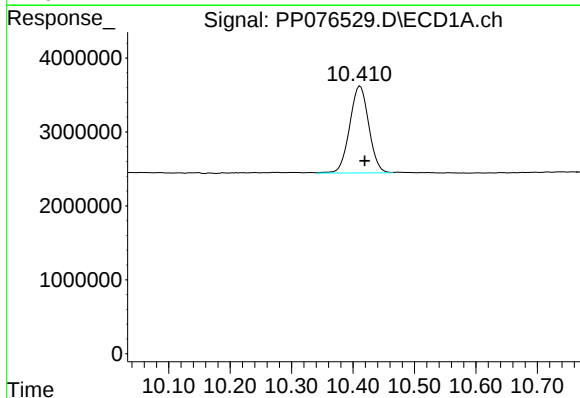

#2 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.007 min
Response: 25330540
Conc: 23.53 ng/ml

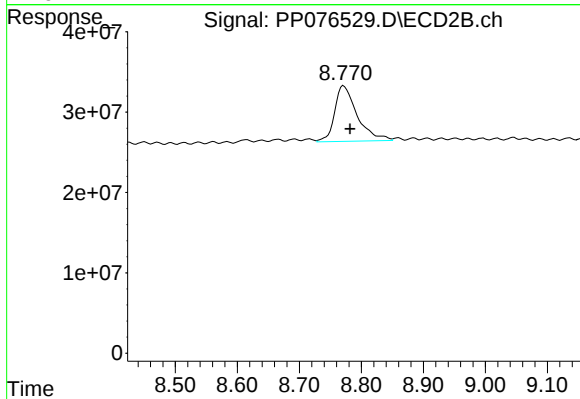

#2 Decachlorobiphenyl

R.T.: 8.771 min
Delta R.T.: -0.011 min
Response: 174656885
Conc: 21.24 ng/ml