

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
 Data File : PP076530.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 11:59
 Operator : YP\AJ
 Sample : PB170572BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 PB170572BL

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2025
 Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 12:56:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.647	3.777	41714358	181.2E6	29.189m	27.382
2) SA Decachlor...	10.435	8.779	31357441	196.5E6	29.128	23.898

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
Data File : PP076530.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 11:59
Operator : YP\AJ
Sample : PB170572BL
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
PB170572BL


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2025
Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 12:56:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

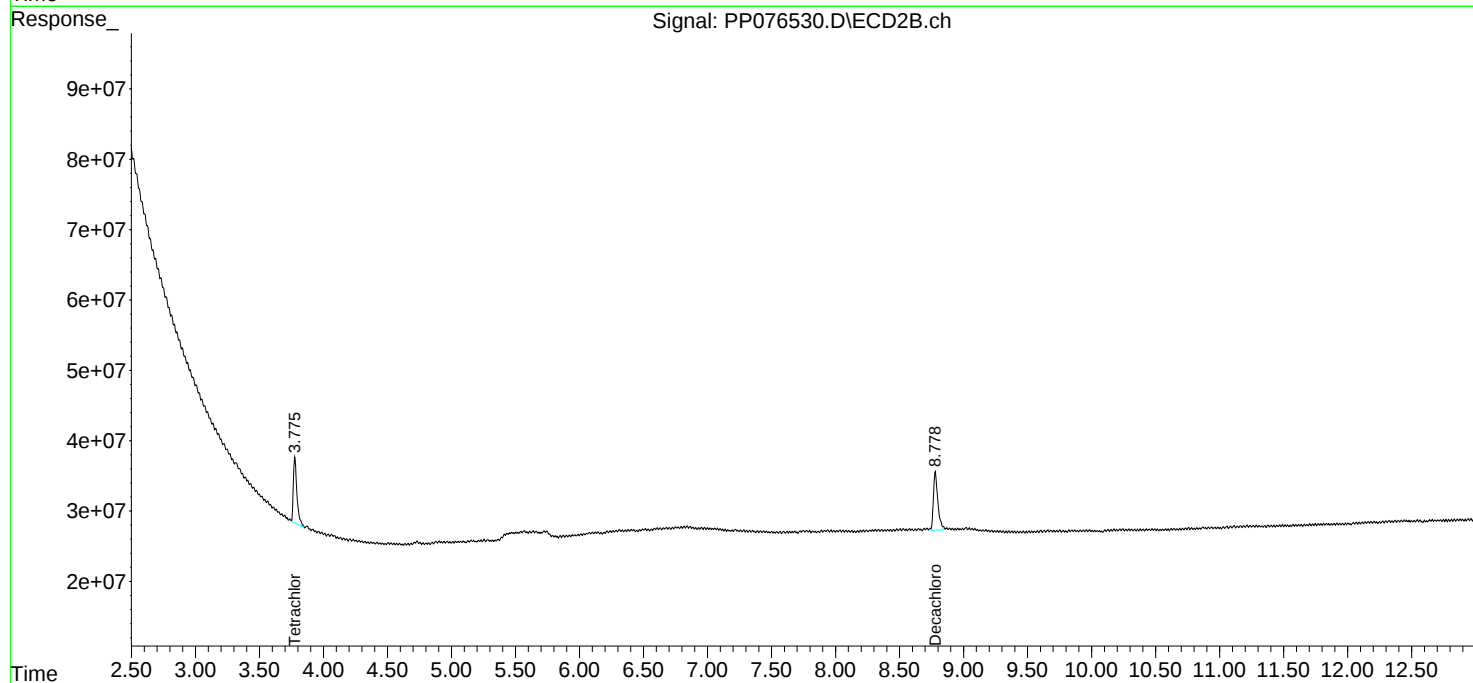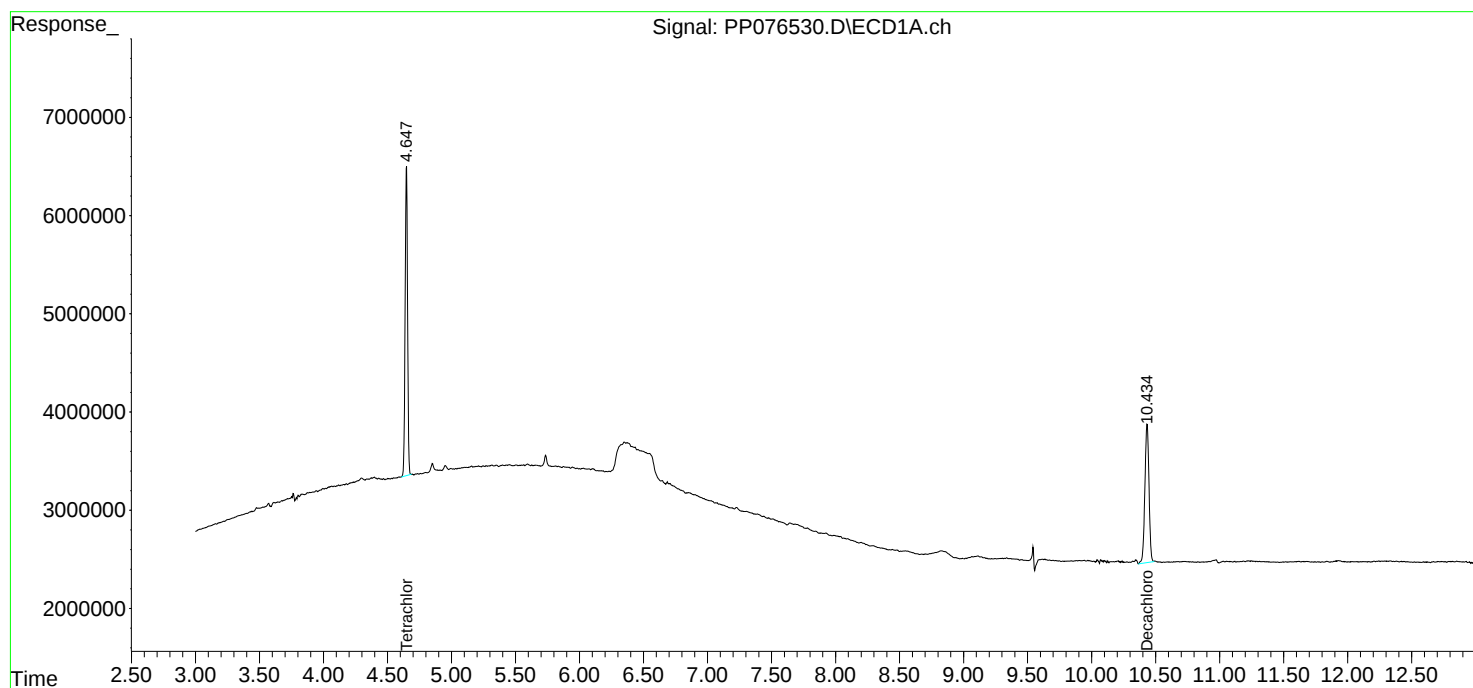

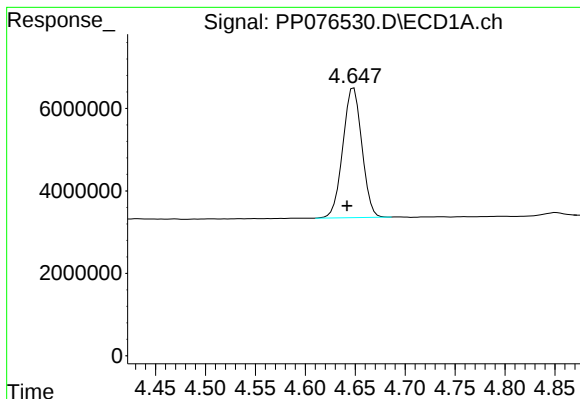


#1 Tetrachloro-m-xylene

R.T.: 4.647 min
Delta R.T.: 0.005 min
Response: 41714358
Conc: 29.19 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB170572BL


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/18/2025
Supervised By :Sohil Jodhani 11/19/2025

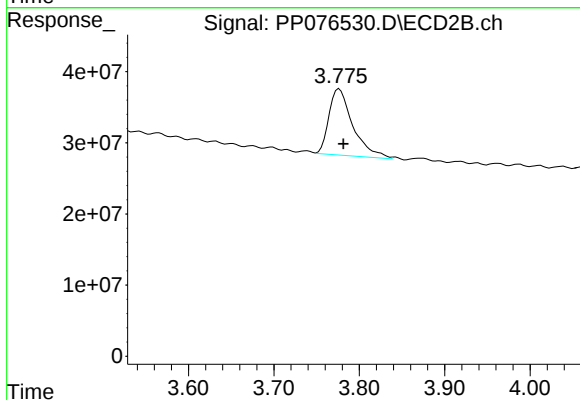


#1 Tetrachloro-m-xylene

R.T.: 3.777 min
Delta R.T.: -0.005 min
Response: 181222975
Conc: 27.38 ng/ml

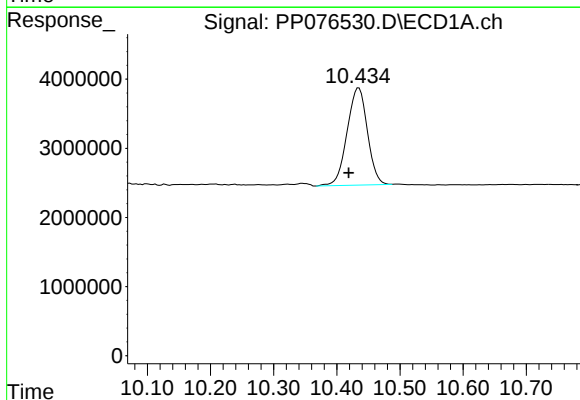

#2 Decachlorobiphenyl

R.T.: 10.435 min
Delta R.T.: 0.016 min
Response: 31357441
Conc: 29.13 ng/ml

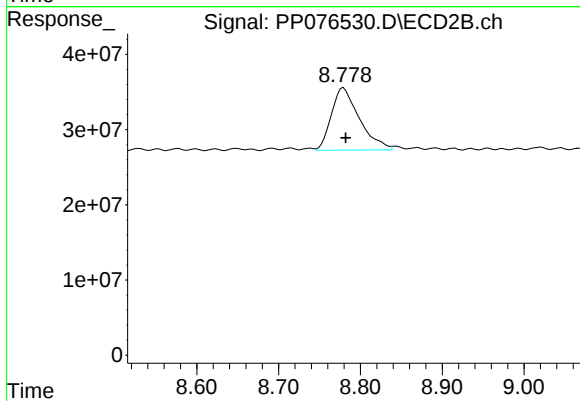

#2 Decachlorobiphenyl

R.T.: 8.779 min
Delta R.T.: -0.003 min
Response: 196514892
Conc: 23.90 ng/ml