

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
 Data File : PP076536.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 13:40
 Operator : YP\AJ
 Sample : Q3620-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1010-B

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2025
 Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 17 13:54:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.637	3.773	30098567	173.8E6	21.061m	26.253
2) SA Decachlor...	10.412	8.773	20695910	136.8E6	19.225	16.633

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
Data File : PP076536.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 13:40
Operator : YP\AJ
Sample : Q3620-02
Misc :
ALS Vial : 13 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1010-B


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2025
Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 17 13:54:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

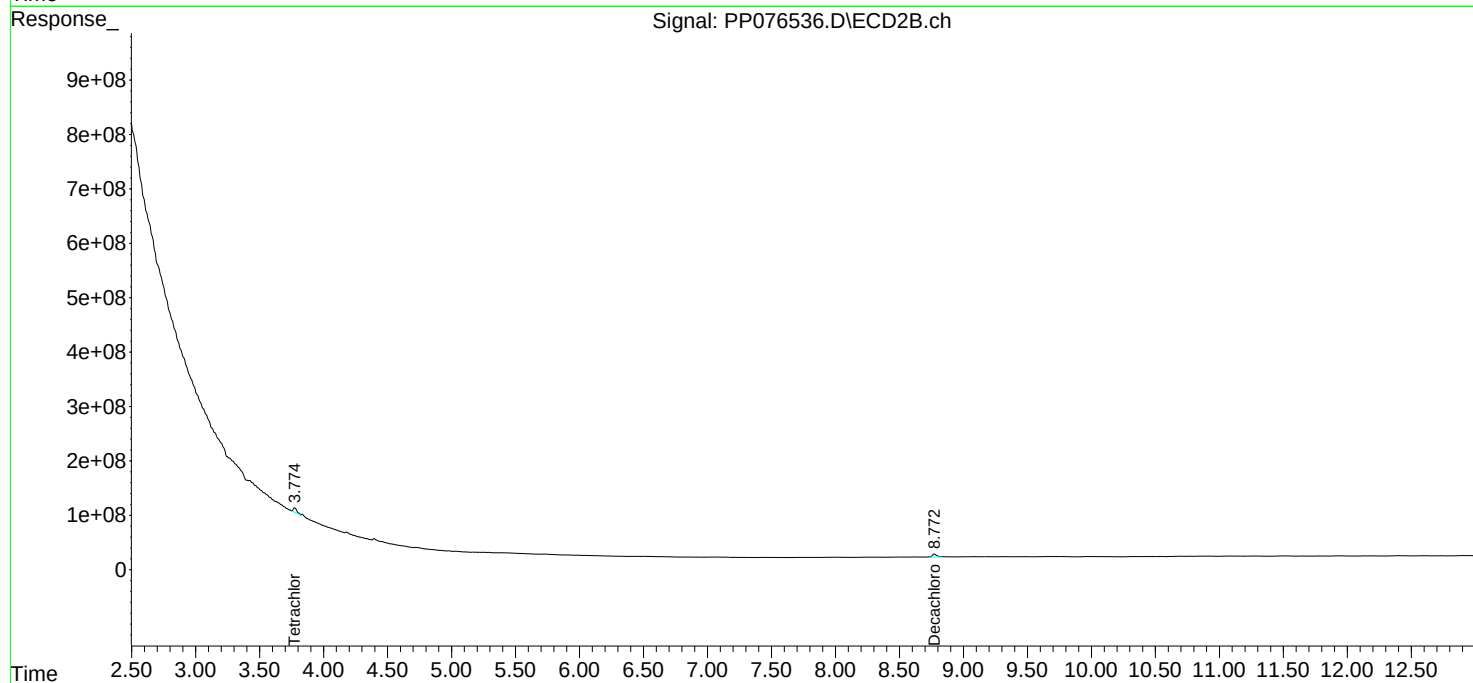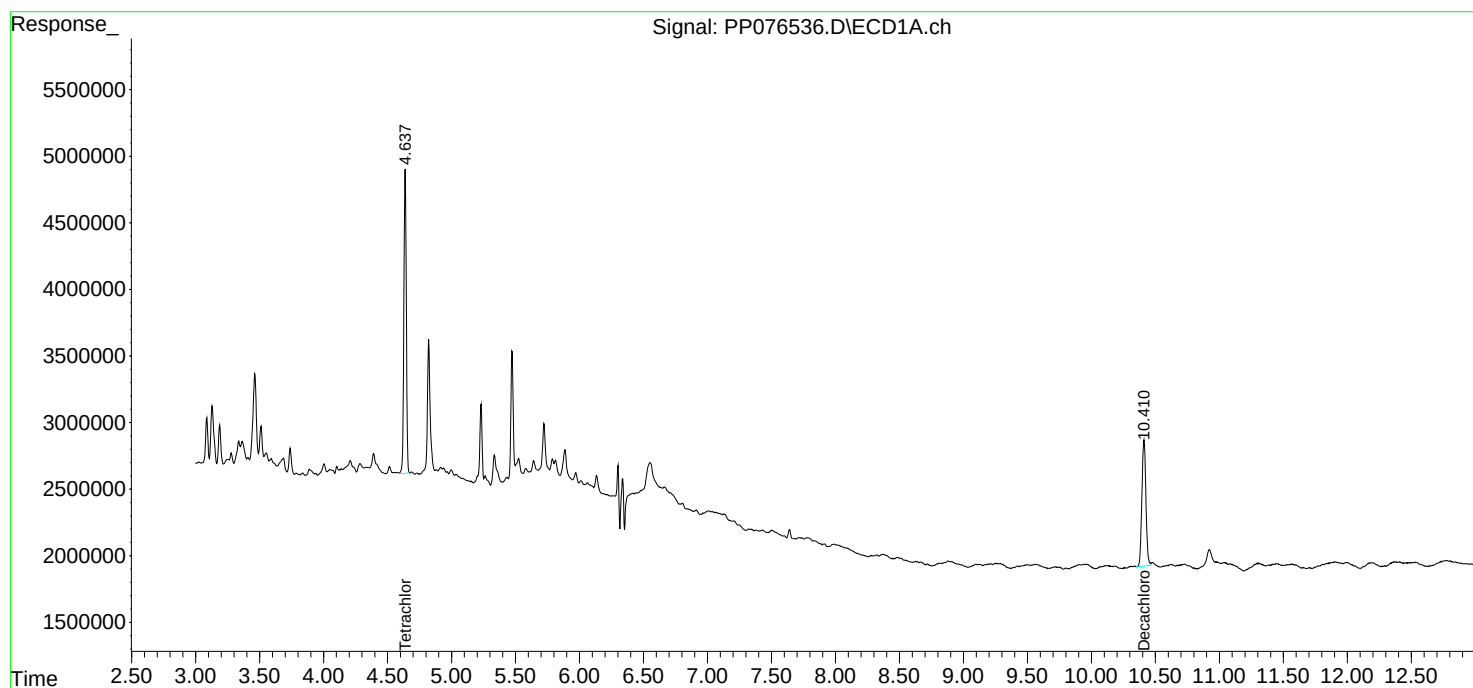

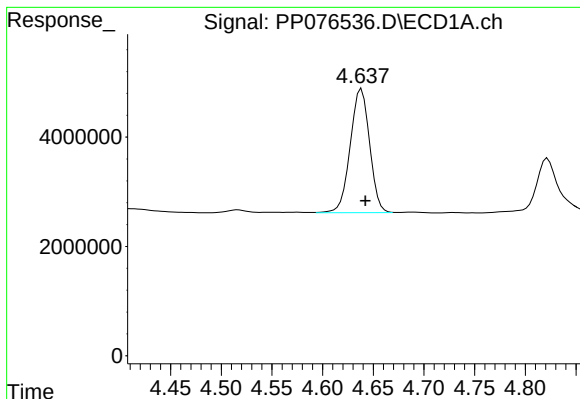


#1 Tetrachloro-m-xylene

R.T.: 4.637 min
Delta R.T.: -0.005 min
Response: 30098567
Conc: 21.06 ng/ml

Instrument :
ECD_P
ClientSampleId :
1010-B


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 11/18/2025
Supervised By :Sohil Jodhani 11/19/2025

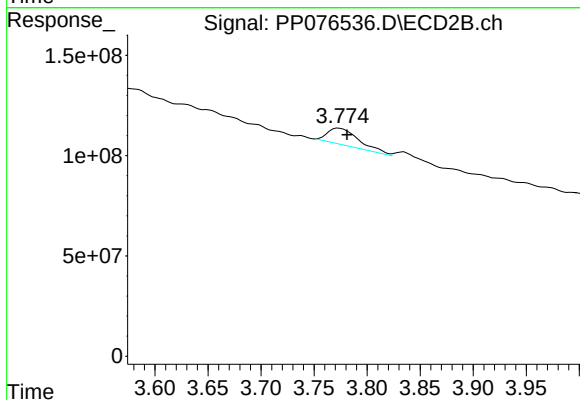


#1 Tetrachloro-m-xylene

R.T.: 3.773 min
Delta R.T.: -0.008 min
Response: 173752131
Conc: 26.25 ng/ml

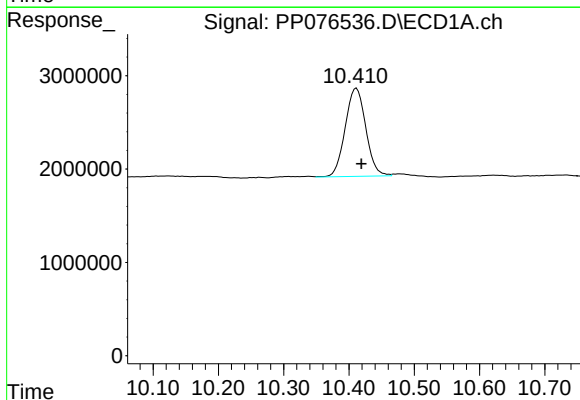

#2 Decachlorobiphenyl

R.T.: 10.412 min
Delta R.T.: -0.007 min
Response: 20695910
Conc: 19.22 ng/ml

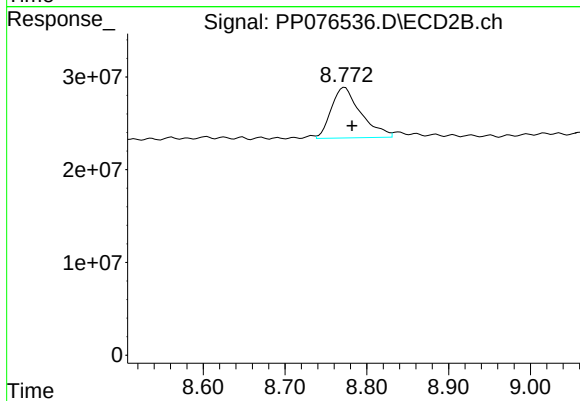

#2 Decachlorobiphenyl

R.T.: 8.773 min
Delta R.T.: -0.009 min
Response: 136769713
Conc: 16.63 ng/ml