

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
 Data File : PP076538.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Nov 2025 14:12
 Operator : YP\AJ
 Sample : Q3640-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 LAW-25-0183

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 11/18/2025
 Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 18 01:10:46 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Oct 24 15:40:32 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.642	3.779	28817958	93778268	20.165	14.170m#
2) SA Decachlor...	10.414	8.772	6856894	63126676	6.369m	7.677m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111725\
Data File : PP076538.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Nov 2025 14:12
Operator : YP\AJ
Sample : Q3640-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
LAW-25-0183


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 11/18/2025
Supervised By : Sohil Jodhani 11/19/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 18 01:10:46 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP102125.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Oct 24 15:40:32 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

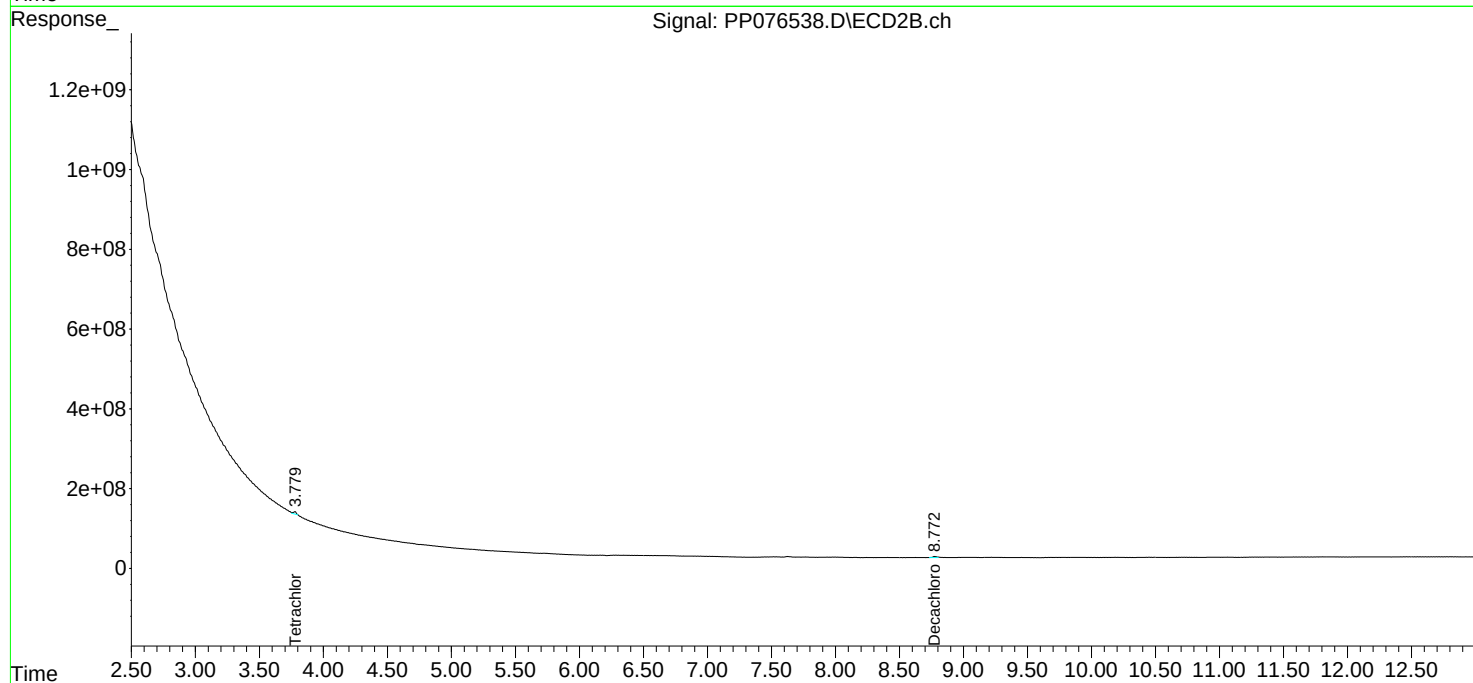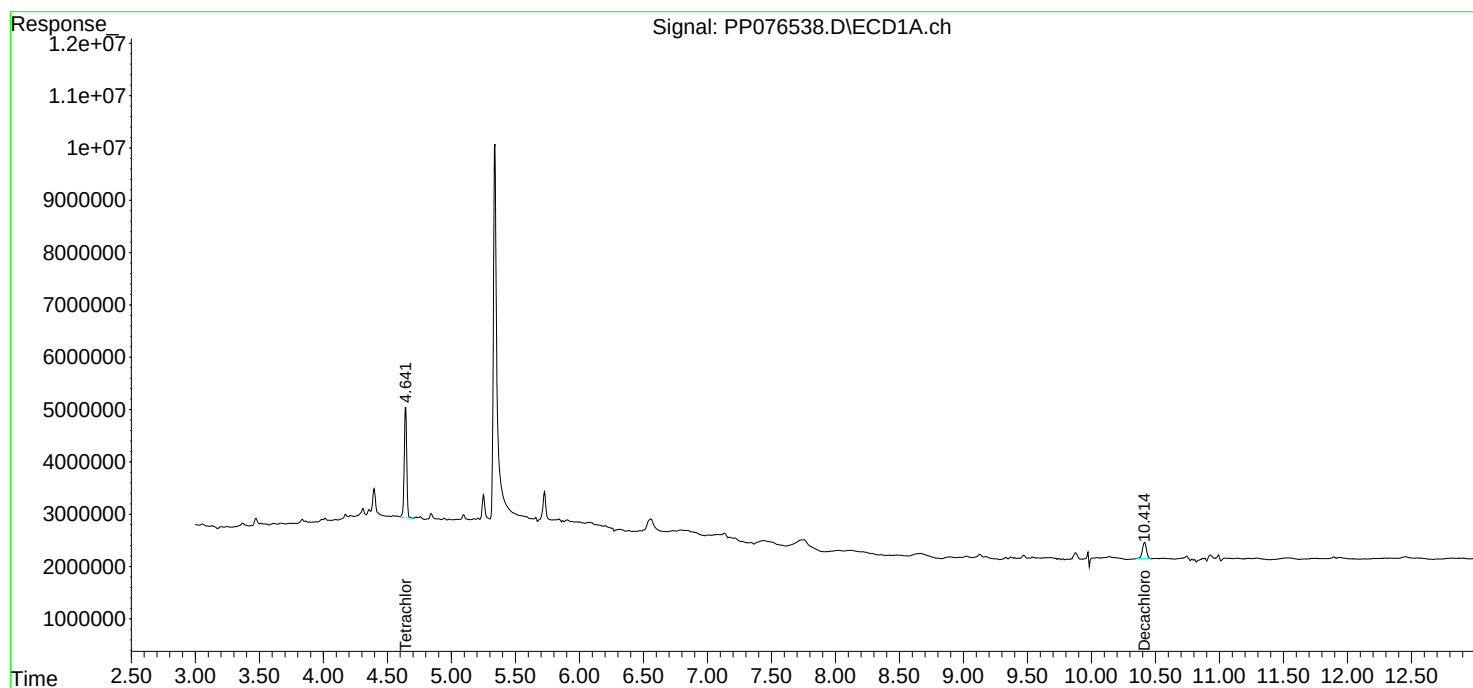

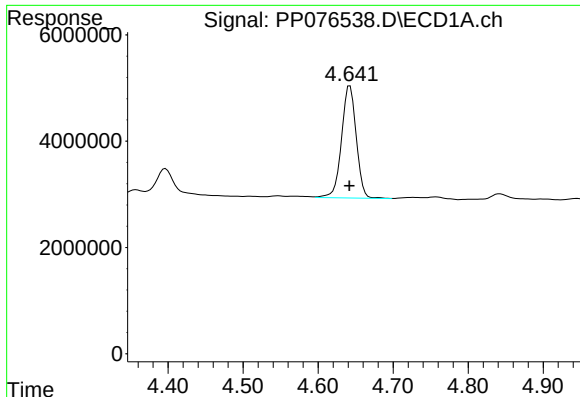

#1 Tetrachloro-m-xylene

R.T.: 4.642 min
Delta R.T.: 0.000 min
Response: 28817958
Conc: 20.17 ng/ml

Instrument :

ECD_P

ClientSampleId :


LAW-25-0183

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 11/18/2025

Supervised By :Sohil Jodhani 11/19/2025

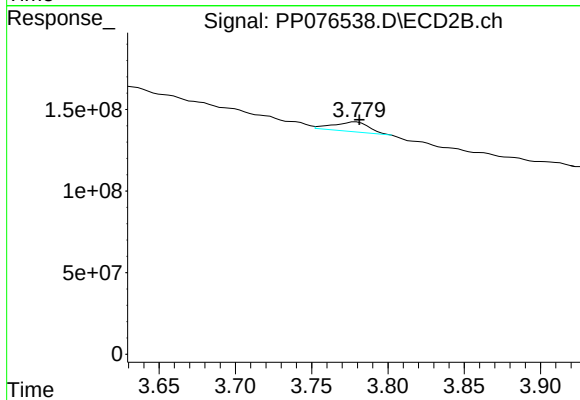


#1 Tetrachloro-m-xylene

R.T.: 3.779 min
Delta R.T.: -0.002 min
Response: 93778268
Conc: 14.17 ng/ml m

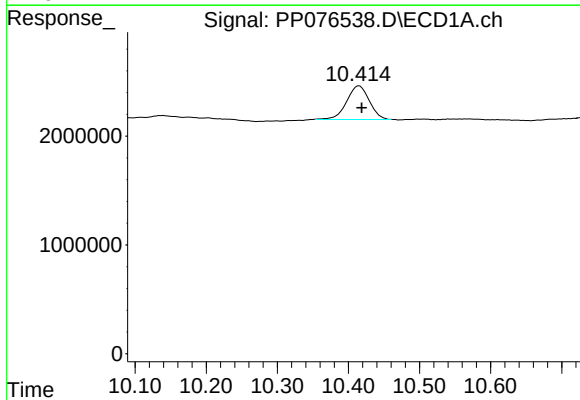

#2 Decachlorobiphenyl

R.T.: 10.414 min
Delta R.T.: -0.005 min
Response: 6856894
Conc: 6.37 ng/ml m

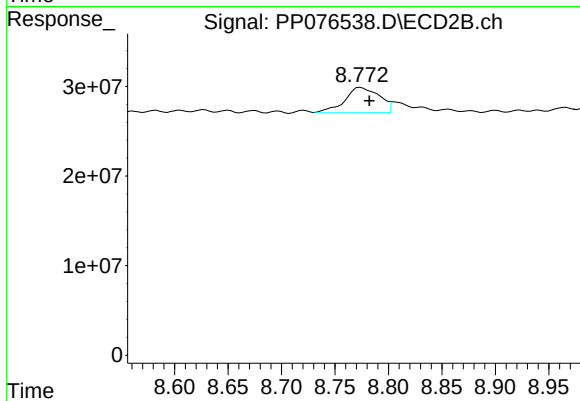

#2 Decachlorobiphenyl

R.T.: 8.772 min
Delta R.T.: -0.010 min
Response: 63126676
Conc: 7.68 ng/ml m