

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031341.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 9:10
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:37:15 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.804	4.069	1021301	998061	25.069	23.872
2)	SA Decachlor...	10.679	9.383	765968	863948	24.939	25.801
Target Compounds							
9)	L2 AR-1221-2	0.000	4.422	0	11403	N.D.	32.292 #
20)	L4 AR-1242-5	0.000	6.224f	0	5966	N.D.	6.750 #
25)	L5 AR-1248-5	0.000	6.224f	0	5966	N.D.	4.750 #
26)	L6 AR-1254-1	0.000	6.224f	0	5966	N.D.	3.135 #
28)	L6 AR-1254-3	0.000	6.767	0	902	N.D.	0.330 #
32)	L7 AR-1260-2	0.000	7.113	0	1881	N.D.	0.924 #
35)	L7 AR-1260-5	0.000	7.999	0	4176	N.D.	1.057 #
37)	L8 AR-1262-2	0.000	7.999	0	4176	N.D.	1.015 #
38)	L8 AR-1262-3	0.000	8.282	0	8598	N.D.	5.394 #
39)	L8 AR-1262-4	0.000	8.355	0	1726	N.D.	0.551 #
40)	L8 AR-1262-5	0.000	8.854	0	4387	N.D.	3.109 #
41)	L9 AR-1268-1	0.000	8.282	0	8598	N.D.	1.747 #
42)	L9 AR-1268-2	0.000	8.355	0	1726	N.D.	0.355 #
43)	L9 AR-1268-3	0.000	8.557	0	1638	N.D.	0.393 #
44)	L9 AR-1268-4	0.000	8.854	0	4387	N.D.	2.632 #
45)	L9 AR-1268-5	0.000	9.134	0	6814	N.D.	0.522 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031341.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 9:10
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampled :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:37:15 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

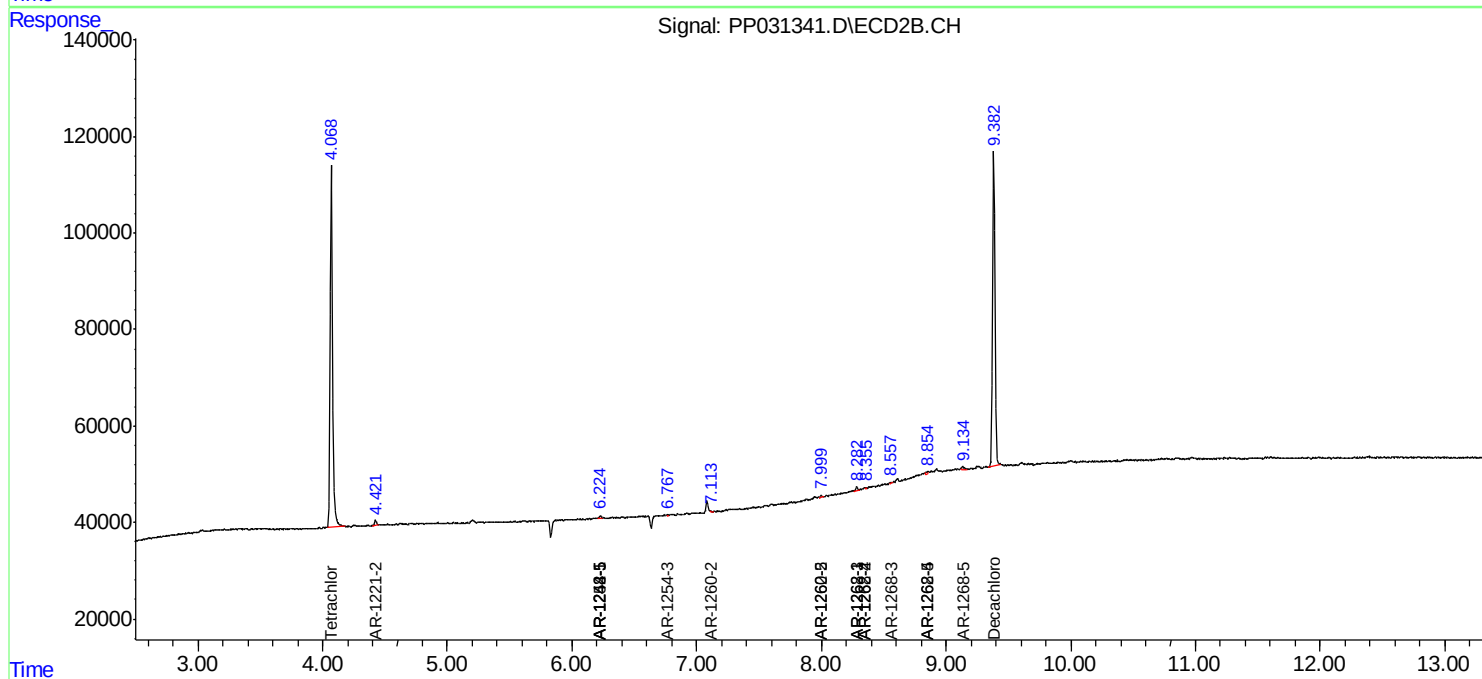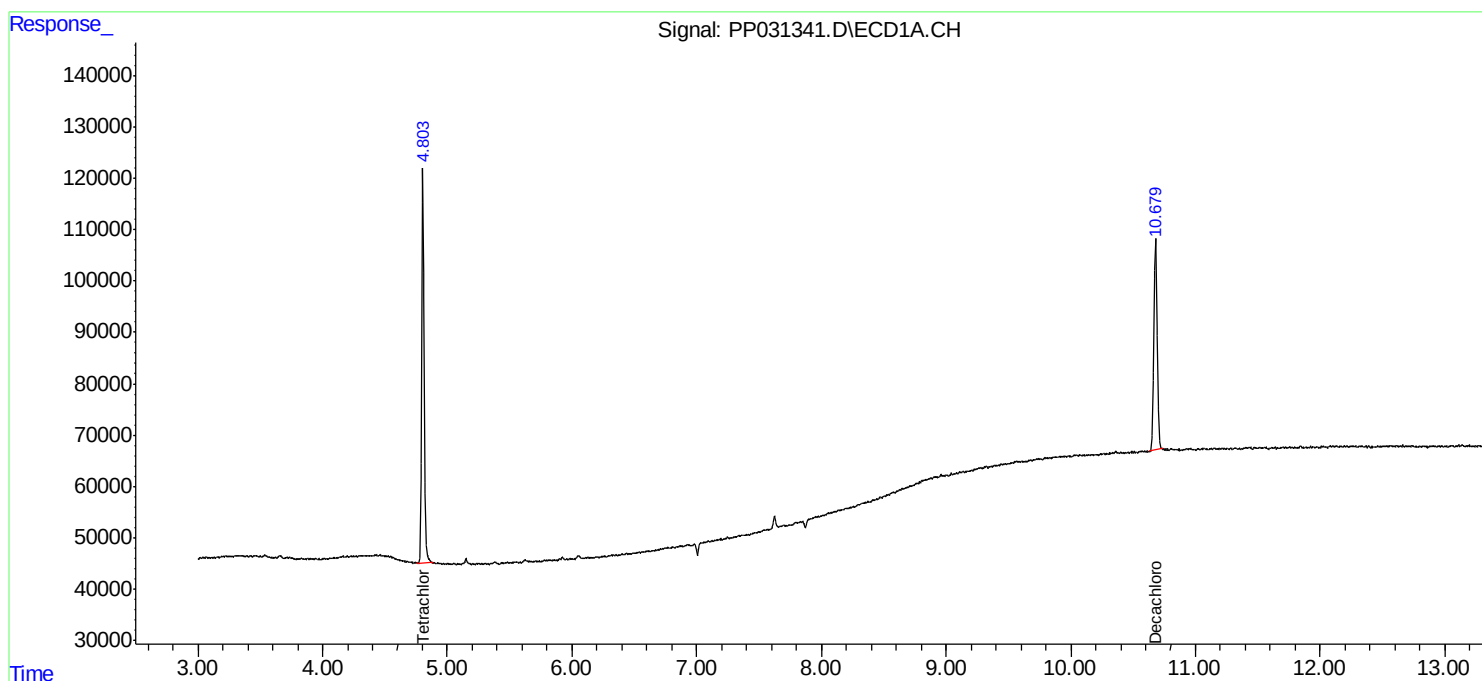


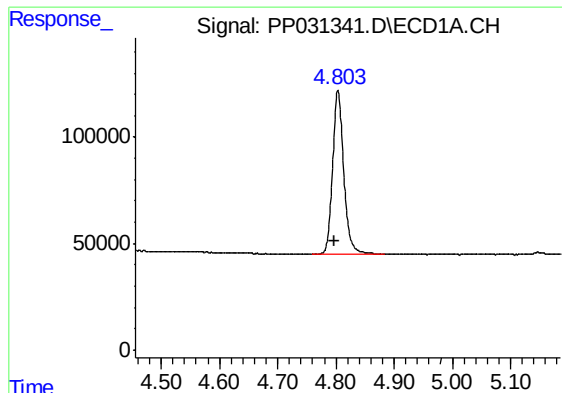

#1 Tetrachloro-m-xylene


R.T.: 4.804 min
Delta R.T.: 0.006 min
Response: 1021301
Conc: 25.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

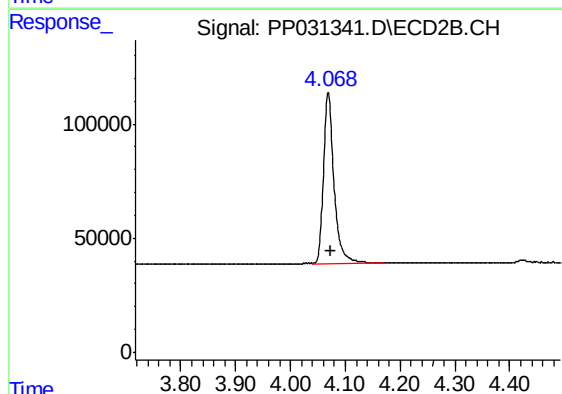


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.004 min
Response: 998061
Conc: 23.87 ng/ml

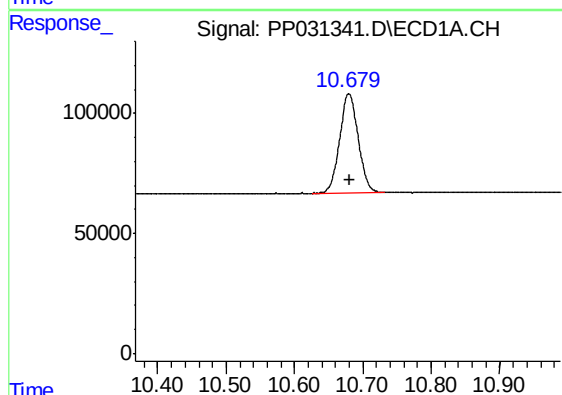


#2 Decachlorobiphenyl

R.T.: 10.679 min
Delta R.T.: 0.000 min
Response: 765968
Conc: 24.94 ng/ml

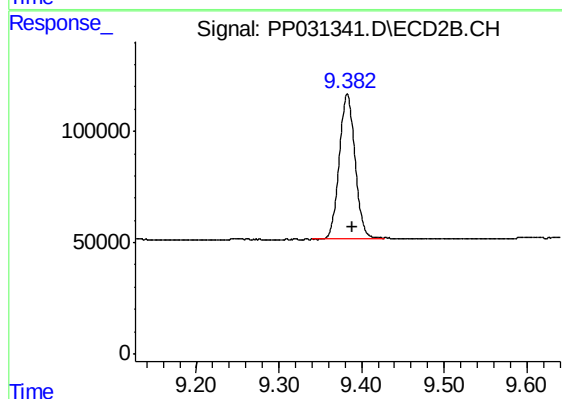

#2 Decachlorobiphenyl


R.T.: 9.383 min
Delta R.T.: -0.006 min
Response: 863948
Conc: 25.80 ng/ml

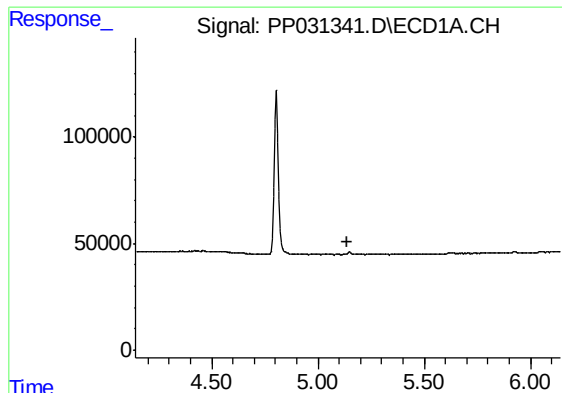

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

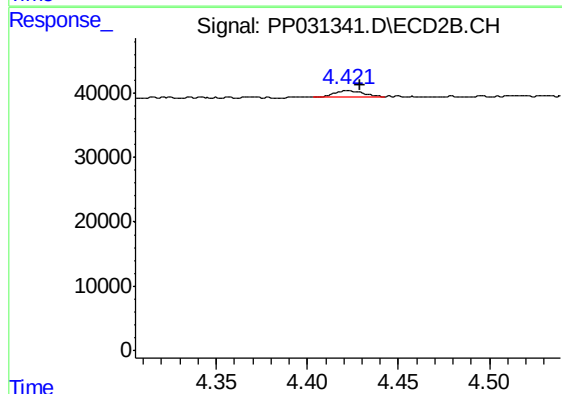


#9 AR-1221-2

R.T.: 4.422 min
Delta R.T.: -0.007 min
Response: 11403
Conc: 32.29 ng/ml

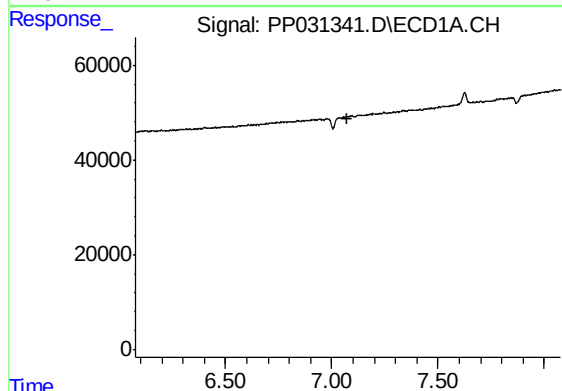


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

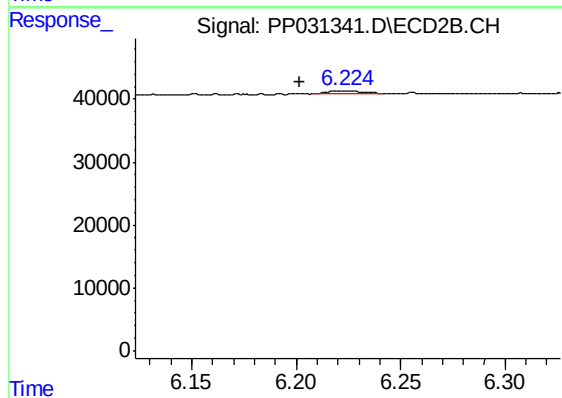

#20 AR-1242-5


R.T.: 6.224 min
Delta R.T.: 0.022 min
Response: 5966
Conc: 6.75 ng/ml

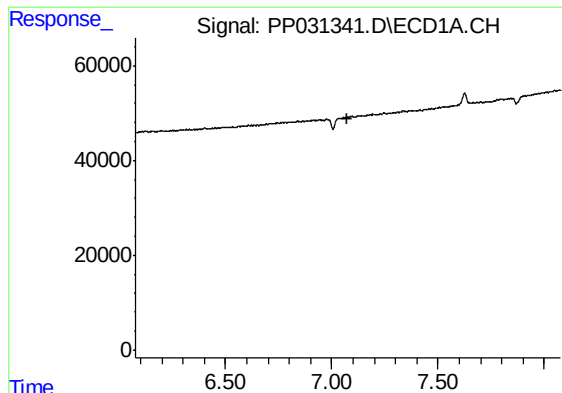

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

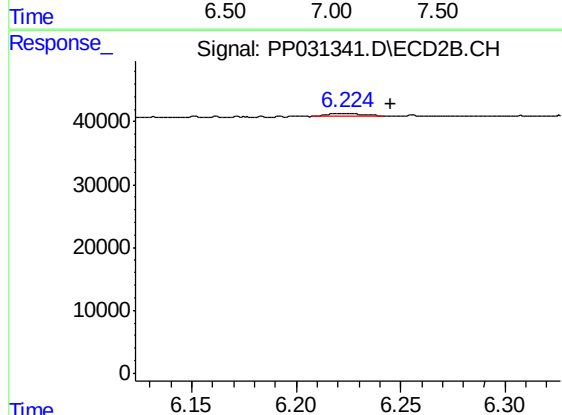


#25 AR-1248-5

R.T.: 6.224 min
Delta R.T.: -0.021 min
Response: 5966
Conc: 4.75 ng/ml

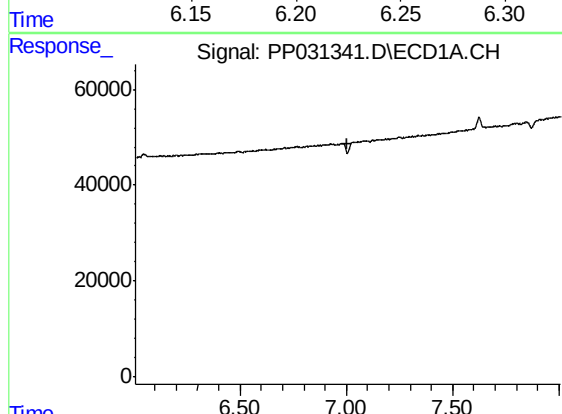


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

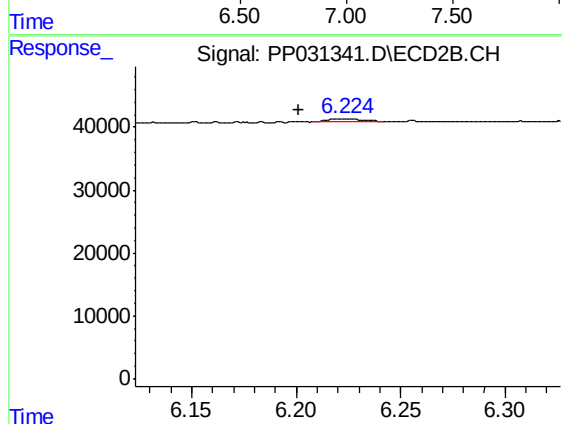

#26 AR-1254-1


R.T.: 6.224 min
Delta R.T.: 0.023 min
Response: 5966
Conc: 3.14 ng/ml

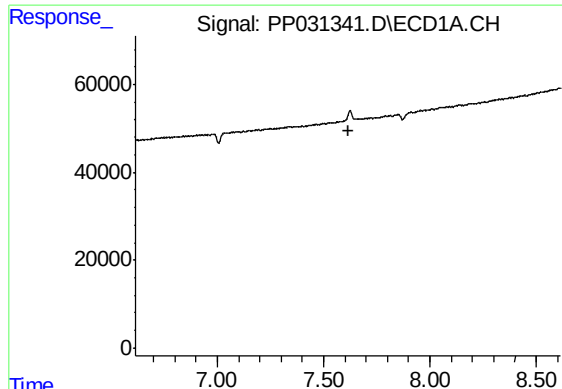

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

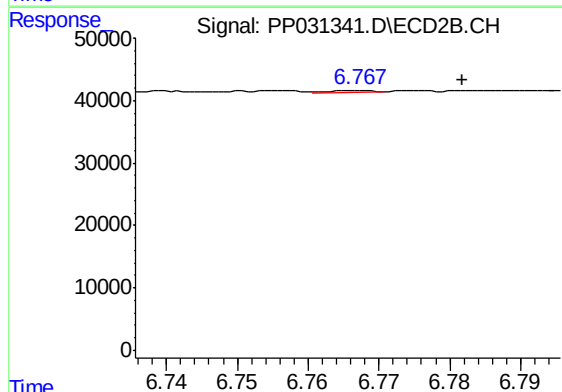


#28 AR-1254-3

R.T.: 6.767 min
Delta R.T.: -0.015 min
Response: 902
Conc: 0.33 ng/ml

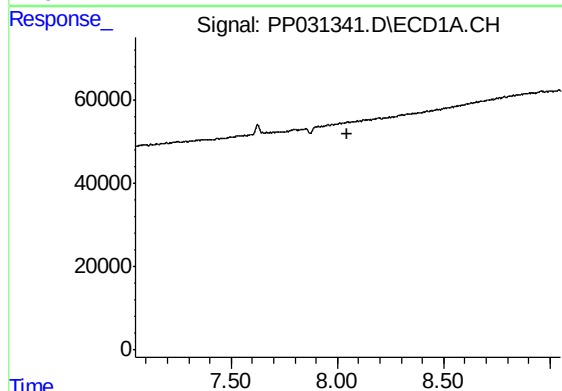


#32 AR-1260-2

R.T.: 0.000 min
Exp R.T. : 8.049 min
Response: 0
Conc: N.D.

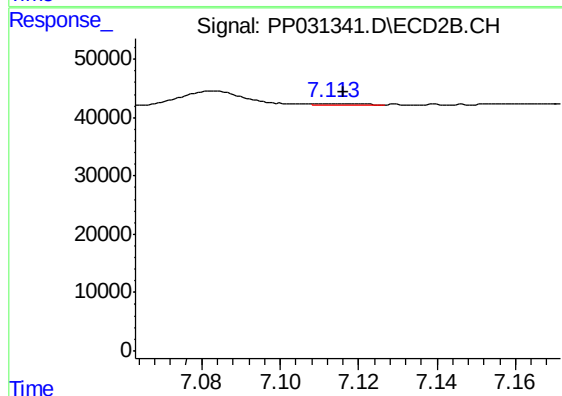

#32 AR-1260-2


R.T.: 7.113 min
Delta R.T.: -0.003 min
Response: 1881
Conc: 0.92 ng/ml

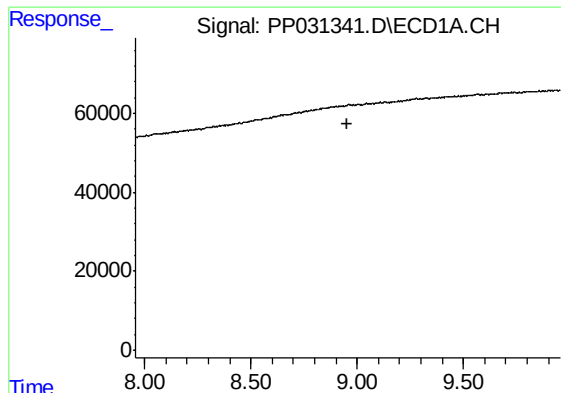

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

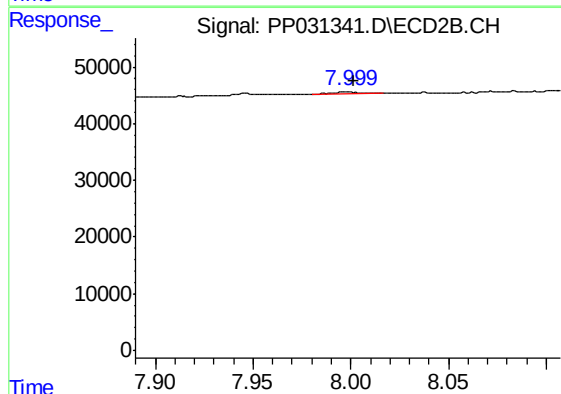


#35 AR-1260-5

R.T.: 7.999 min
Delta R.T.: -0.002 min
Response: 4176
Conc: 1.06 ng/ml

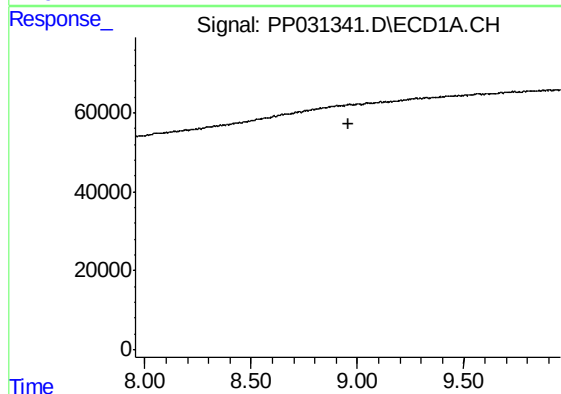


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.956 min
Response: 0
Conc: N.D.

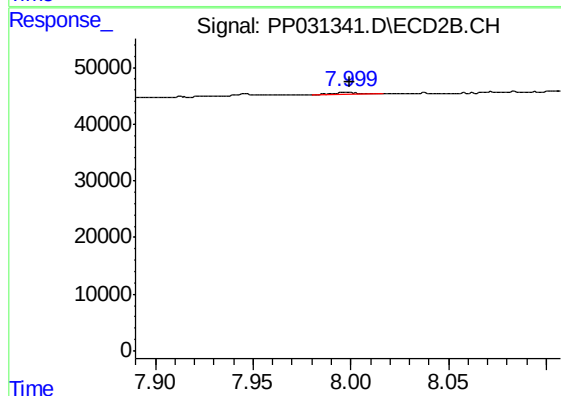

#37 AR-1262-2


R.T.: 7.999 min
Delta R.T.: 0.000 min
Response: 4176
Conc: 1.02 ng/ml

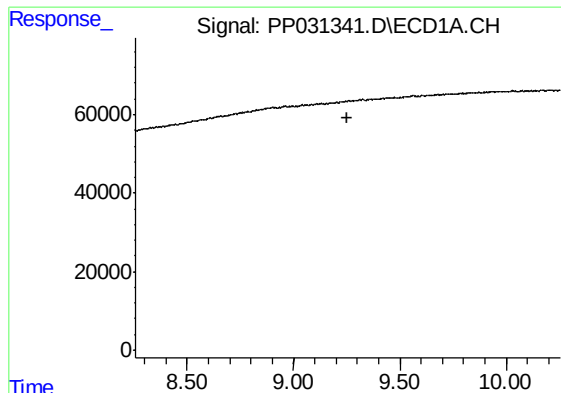

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

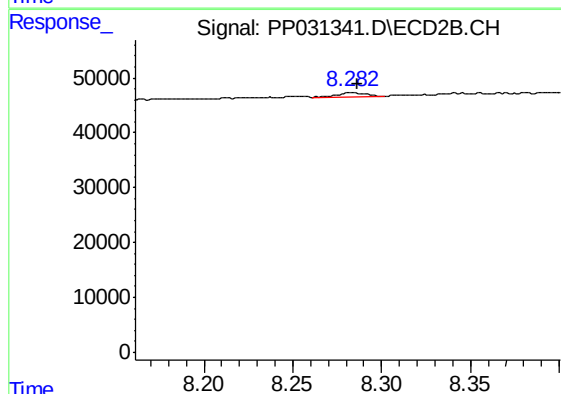


#38 AR-1262-3

R.T.: 8.282 min
Delta R.T.: -0.004 min
Response: 8598
Conc: 5.39 ng/ml

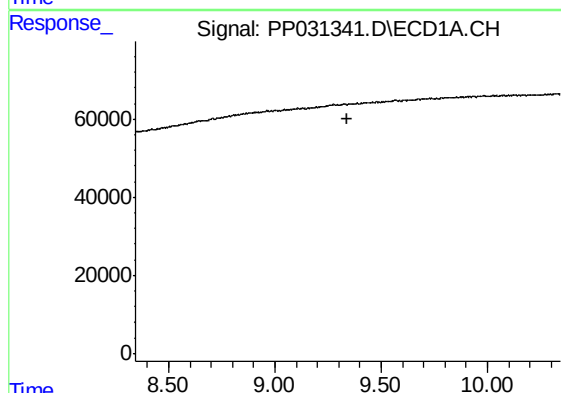


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.343 min
Response: 0
Conc: N.D.

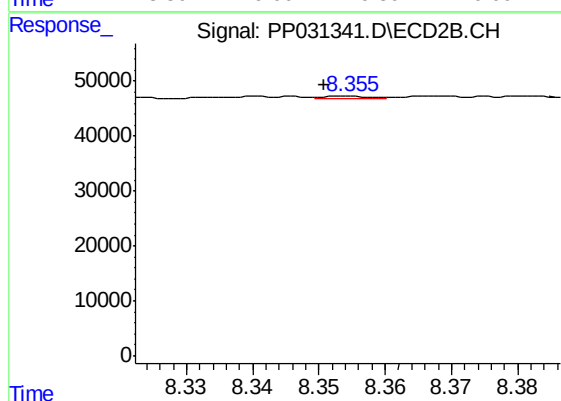

#39 AR-1262-4


R.T.: 8.355 min
Delta R.T.: 0.004 min
Response: 1726
Conc: 0.55 ng/ml

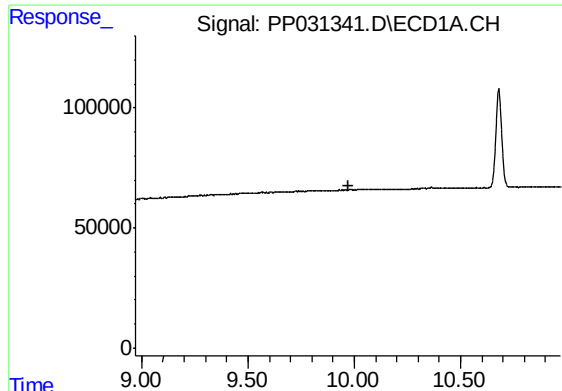

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

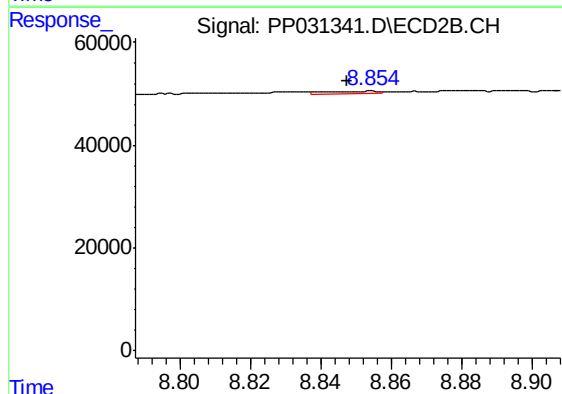


#40 AR-1262-5

R.T.: 8.854 min
Delta R.T.: 0.007 min
Response: 4387
Conc: 3.11 ng/ml

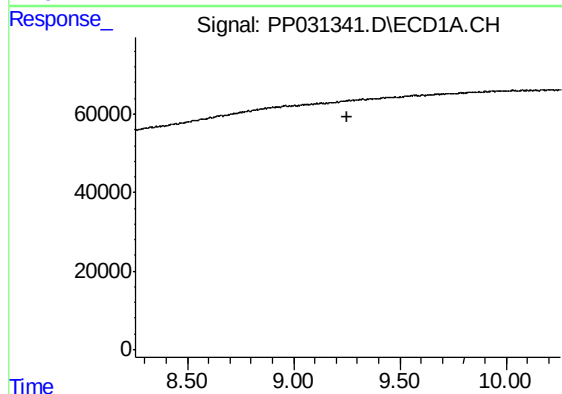


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.255 min
Response: 0
Conc: N.D.

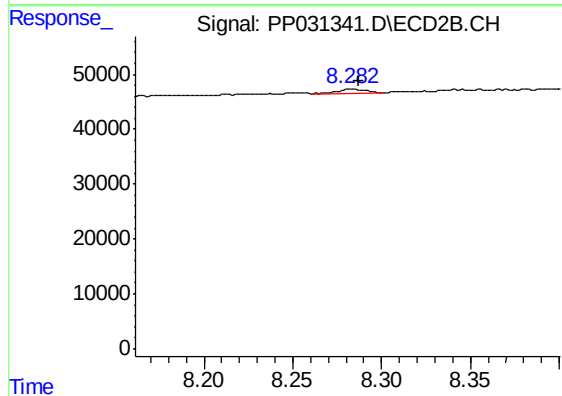

#41 AR-1268-1


R.T.: 8.282 min
Delta R.T.: -0.005 min
Response: 8598
Conc: 1.75 ng/ml

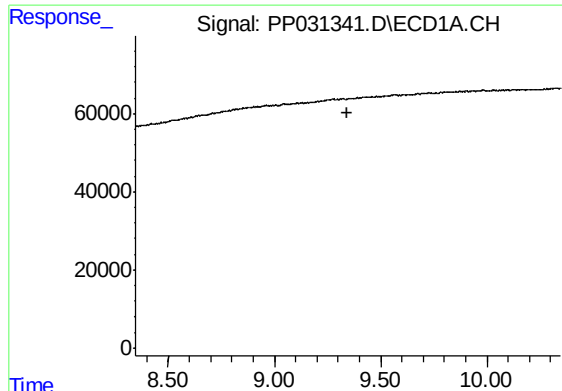

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

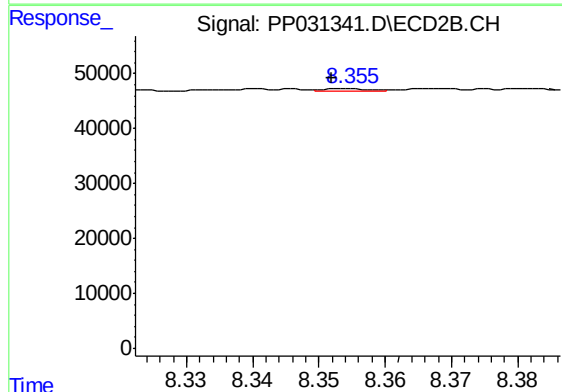


#42 AR-1268-2

R.T.: 8.355 min
Delta R.T.: 0.003 min
Response: 1726
Conc: 0.36 ng/ml

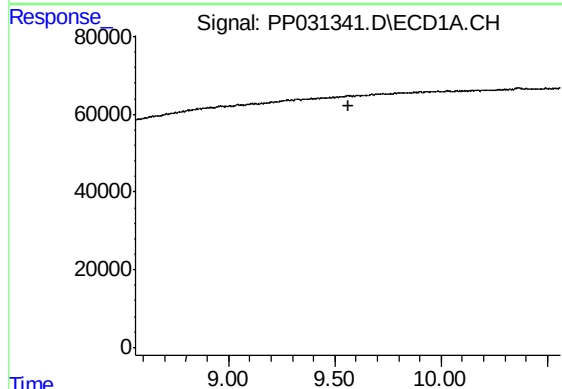


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.562 min
Response: 0
Conc: N.D.

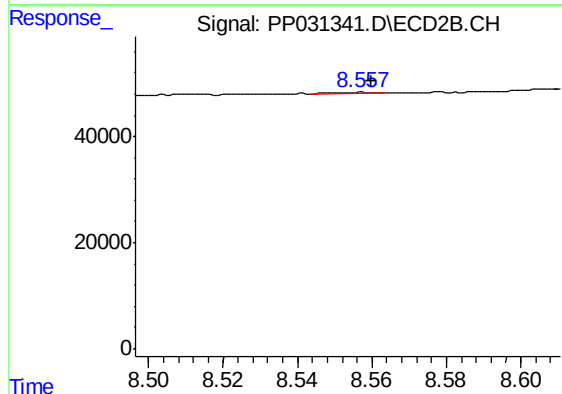

#43 AR-1268-3


R.T.: 8.557 min
Delta R.T.: -0.003 min
Response: 1638
Conc: 0.39 ng/ml

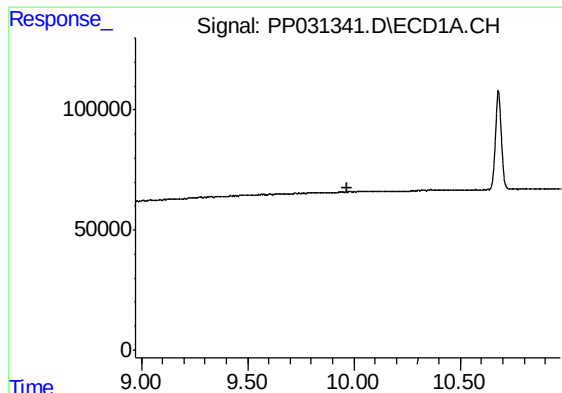

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

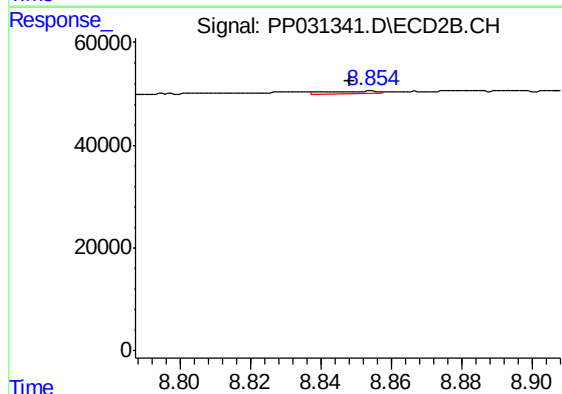


#44 AR-1268-4

R.T.: 8.854 min
Delta R.T.: 0.006 min
Response: 4387
Conc: 2.63 ng/ml

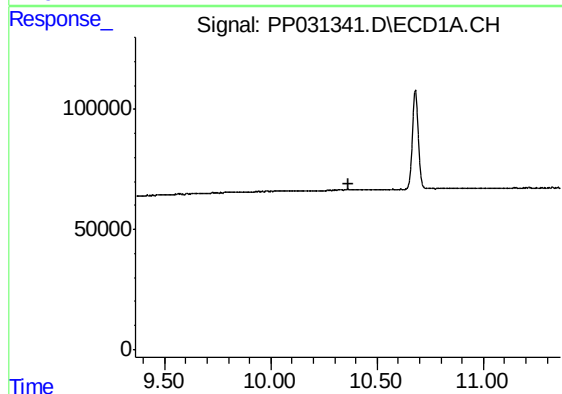

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.363 min
Response: 0
Conc: N.D.

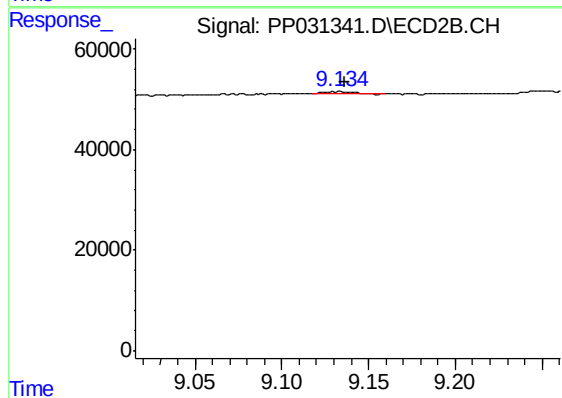

#45 AR-1268-5

R.T.: 9.134 min
Delta R.T.: -0.002 min
Response: 6814
Conc: 0.52 ng/ml