

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031365.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 16:28
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:53:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.798	4.069	1040518	1017650	25.541	24.341
2)	SA Decachlor...	10.674	9.380	713755	826746	23.239	24.690
Target Compounds							
9)	L2 AR-1221-2	0.000	4.423	0	14141	N.D.	40.045 #
20)	L4 AR-1242-5	0.000	6.224f	0	9478	N.D.	10.724 #
25)	L5 AR-1248-5	0.000	6.224f	0	9478	N.D.	7.546 #
26)	L6 AR-1254-1	0.000	6.224f	0	9478	N.D.	4.980 #
28)	L6 AR-1254-3	0.000	6.766f	0	270	N.D.	0.099 #
30)	L6 AR-1254-5	0.000	7.445	0	2633	N.D.	1.089 #
32)	L7 AR-1260-2	0.000	7.107	0	448	N.D.	0.220 #
33)	L7 AR-1260-3	0.000	7.260	0	843	N.D.	0.437 #
35)	L7 AR-1260-5	0.000	8.004	0	783	N.D.	0.198 #
37)	L8 AR-1262-2	0.000	7.997	0	5470	N.D.	1.330 #
39)	L8 AR-1262-4	0.000	8.350	0	1904	N.D.	0.608 #
40)	L8 AR-1262-5	0.000	8.845	0	1929	N.D.	1.367 #
42)	L9 AR-1268-2	0.000	8.350	0	1904	N.D.	0.392 #
43)	L9 AR-1268-3	0.000	8.576f	0	797	N.D.	0.191 #
44)	L9 AR-1268-4	0.000	8.845	0	1929	N.D.	1.157 #
45)	L9 AR-1268-5	0.000	9.131	0	1890	N.D.	0.145 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031365.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 16:28
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:53:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

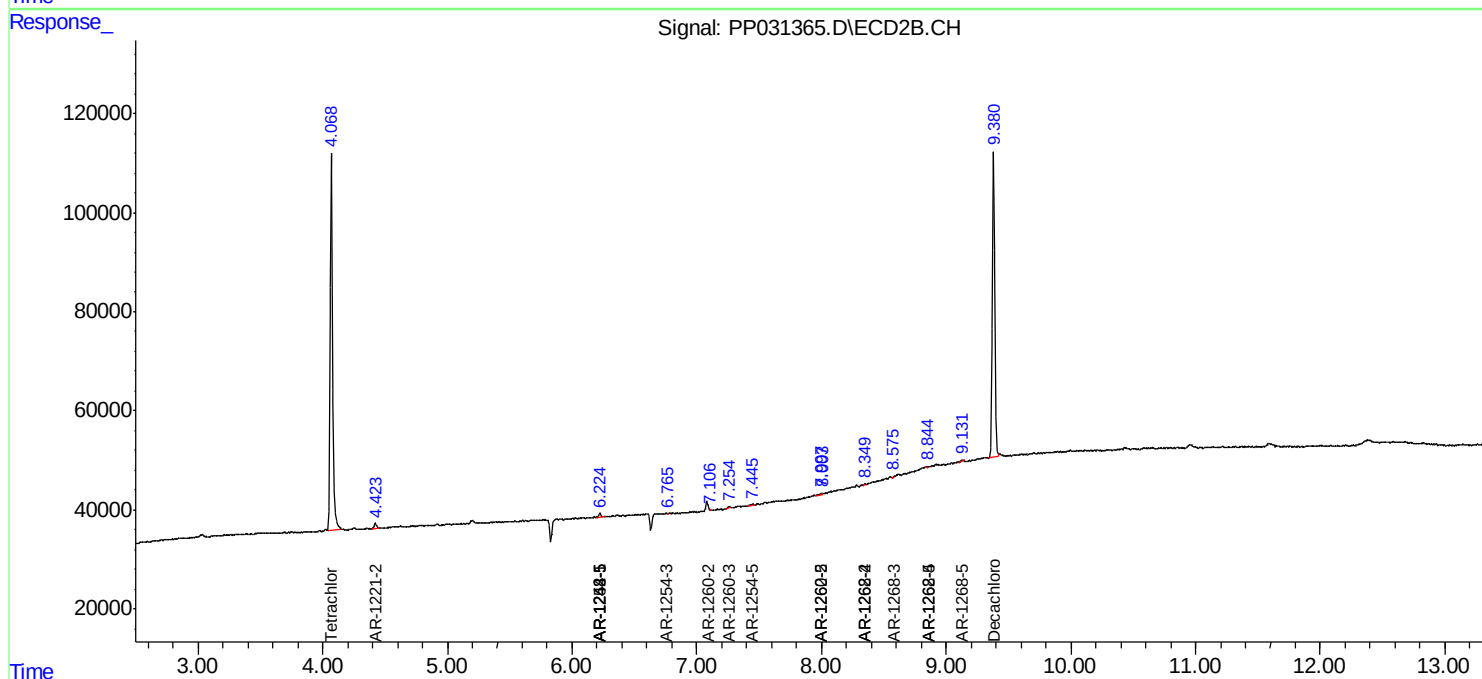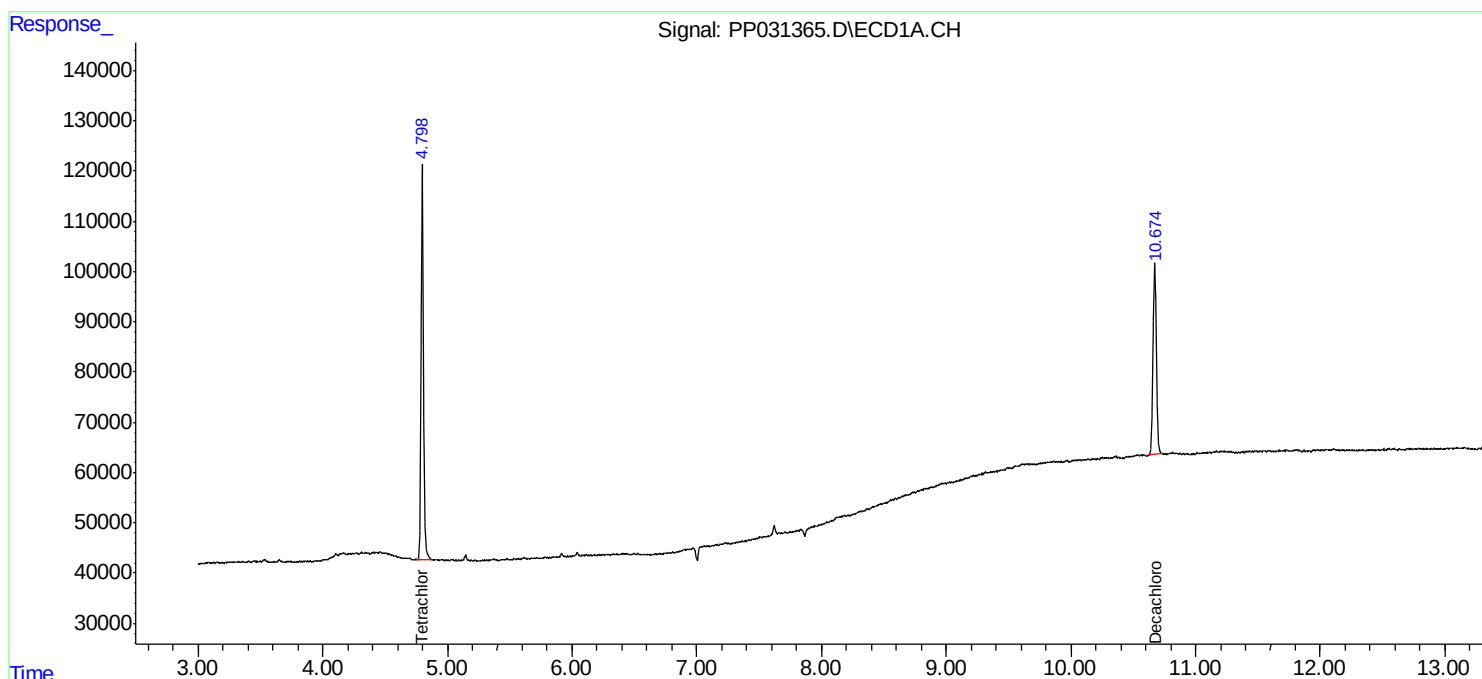


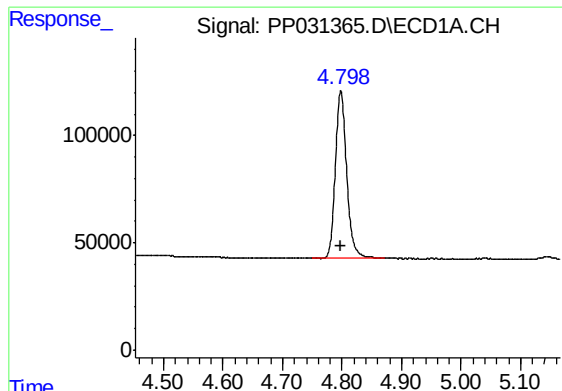

#1 Tetrachloro-m-xylene


R.T.: 4.798 min
Delta R.T.: 0.000 min
Response: 1040518
Conc: 25.54 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

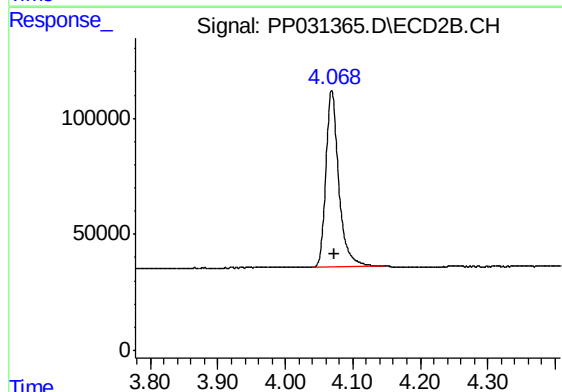


#1 Tetrachloro-m-xylene

R.T.: 4.069 min
Delta R.T.: -0.004 min
Response: 1017650
Conc: 24.34 ng/ml

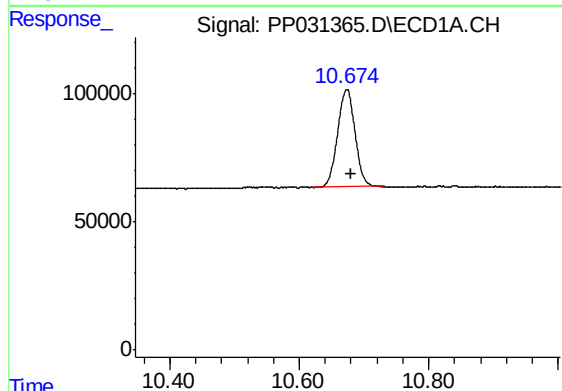


#2 Decachlorobiphenyl

R.T.: 10.674 min
Delta R.T.: -0.006 min
Response: 713755
Conc: 23.24 ng/ml

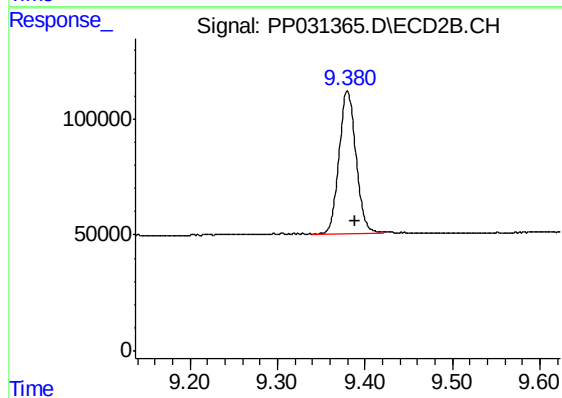

#2 Decachlorobiphenyl


R.T.: 9.380 min
Delta R.T.: -0.008 min
Response: 826746
Conc: 24.69 ng/ml

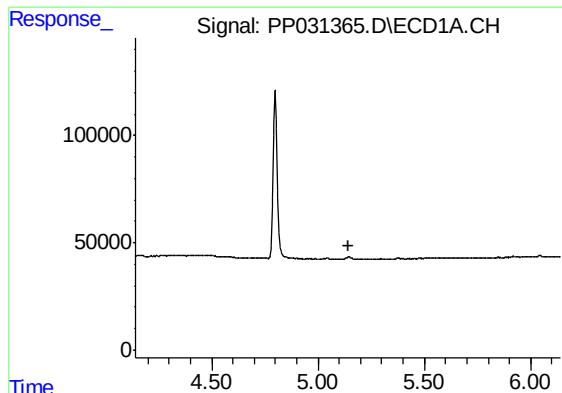

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

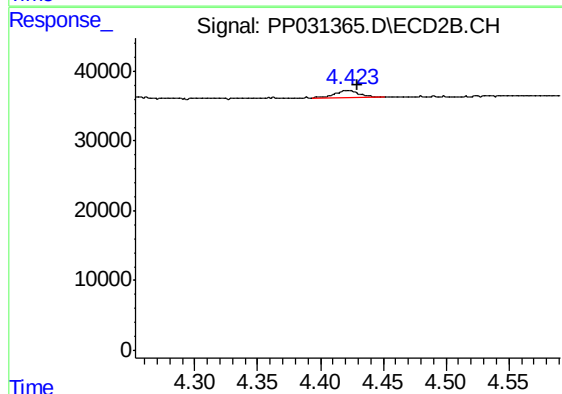


#9 AR-1221-2

R.T.: 4.423 min
Delta R.T.: -0.006 min
Response: 14141
Conc: 40.04 ng/ml

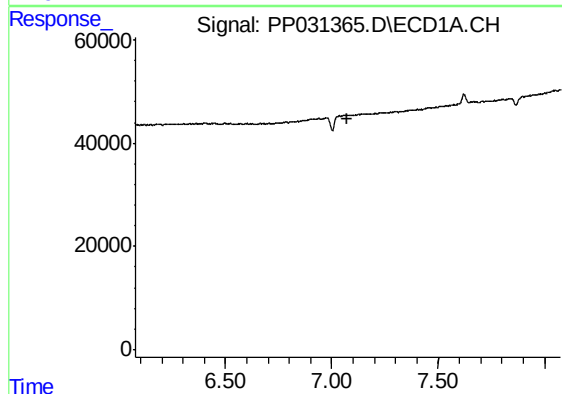


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

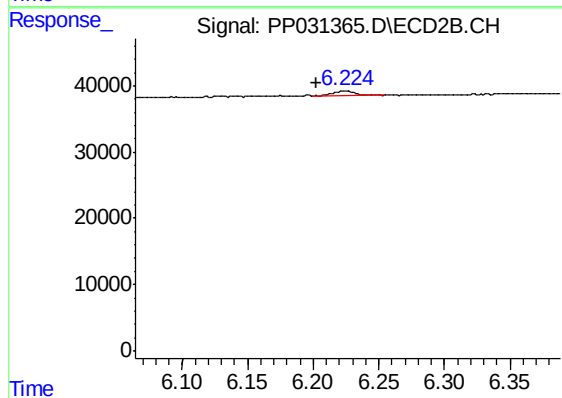

#20 AR-1242-5


R.T.: 6.224 min
Delta R.T.: 0.022 min
Response: 9478
Conc: 10.72 ng/ml

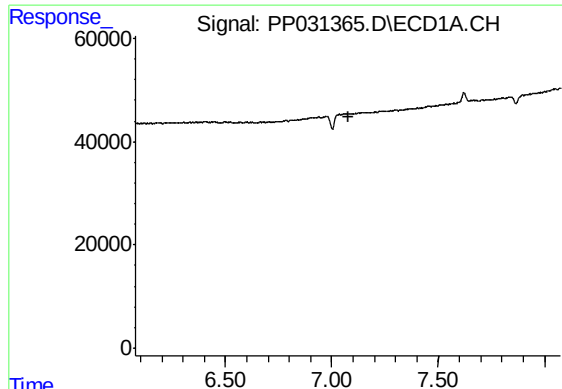

#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

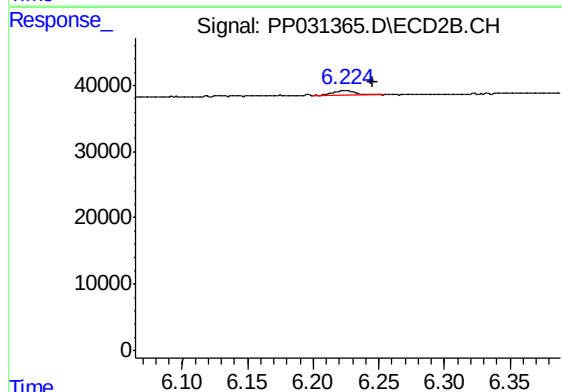


#25 AR-1248-5

R.T.: 6.224 min
Delta R.T.: -0.021 min
Response: 9478
Conc: 7.55 ng/ml

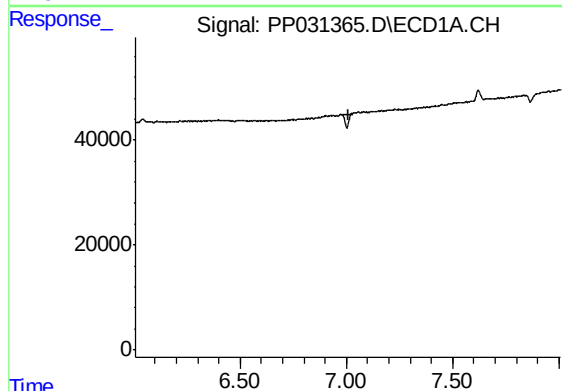


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

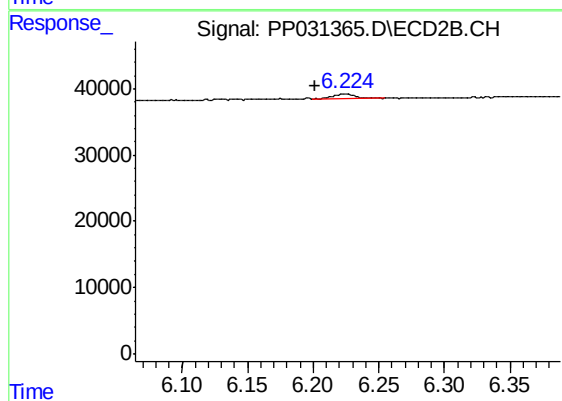

#26 AR-1254-1


R.T.: 6.224 min
Delta R.T.: 0.023 min
Response: 9478
Conc: 4.98 ng/ml

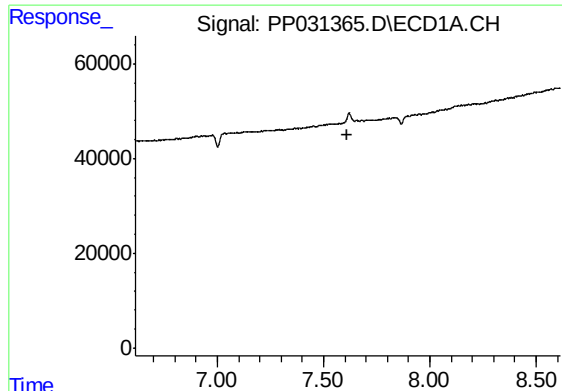

#28 AR-1254-3


R.T.: 0.000 min
Exp R.T. : 7.615 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

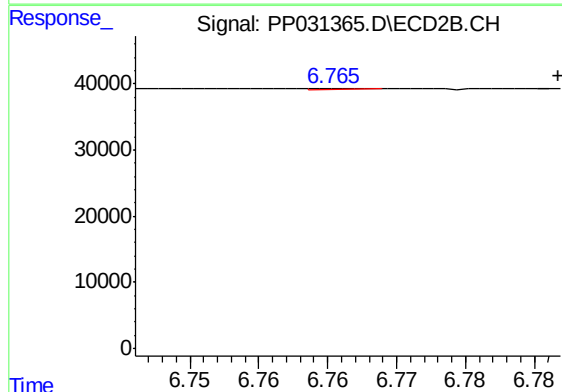


#28 AR-1254-3

R.T.: 6.766 min
Delta R.T.: -0.016 min
Response: 270
Conc: 0.10 ng/ml

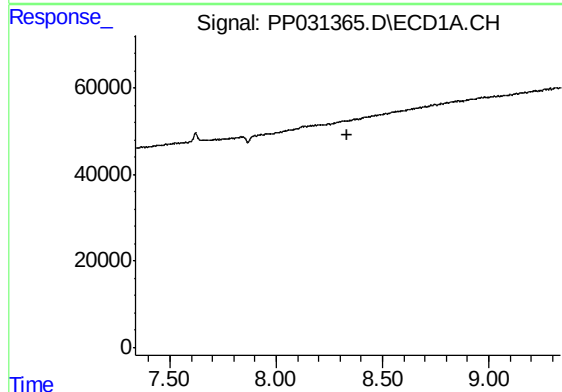


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.337 min
Response: 0
Conc: N.D.

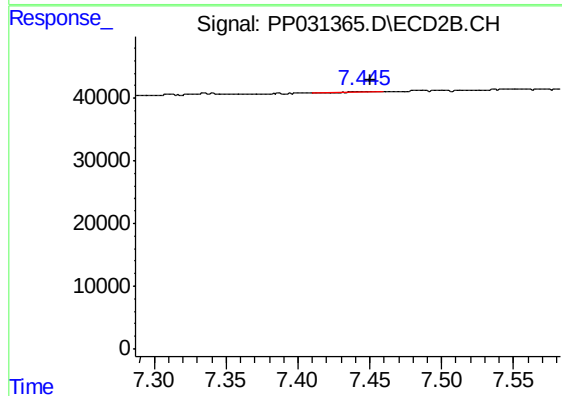

#30 AR-1254-5


R.T.: 7.445 min
Delta R.T.: -0.005 min
Response: 2633
Conc: 1.09 ng/ml

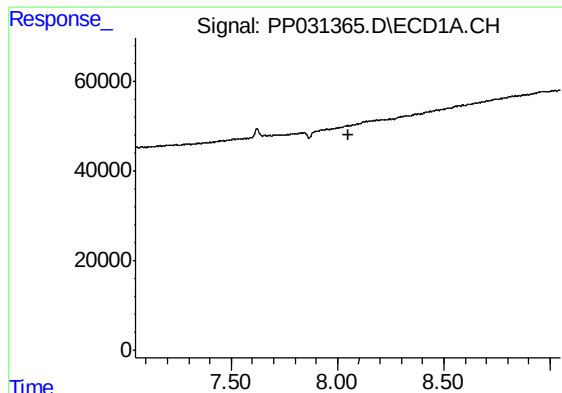

#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

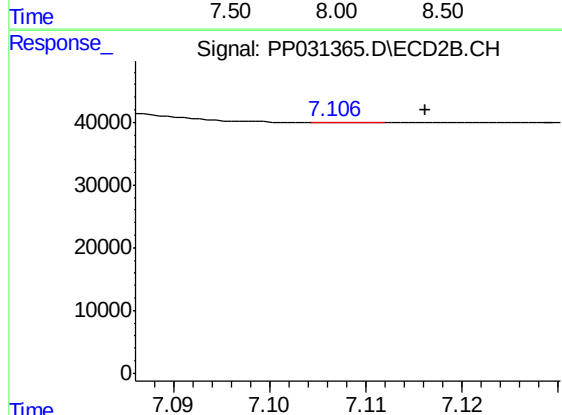


#32 AR-1260-2

R.T.: 7.107 min
Delta R.T.: -0.009 min
Response: 448
Conc: 0.22 ng/ml

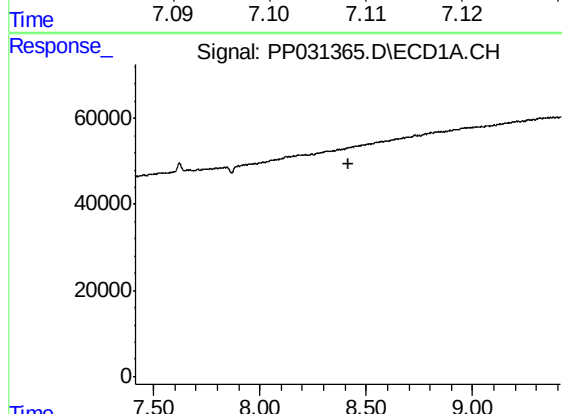


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.414 min
Response: 0
Conc: N.D.

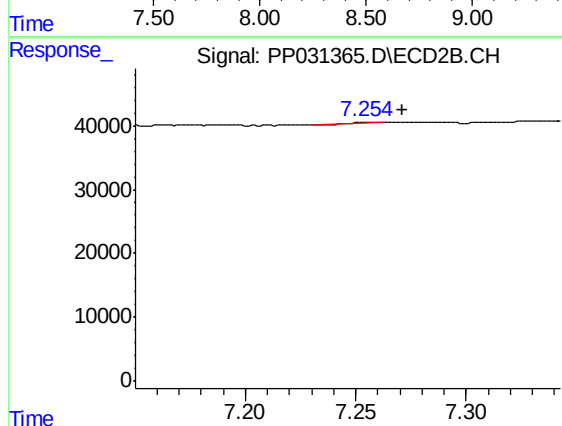

#33 AR-1260-3


R.T.: 7.260 min
Delta R.T.: -0.012 min
Response: 843
Conc: 0.44 ng/ml

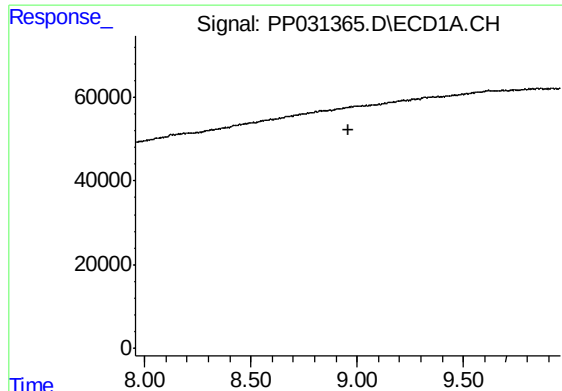

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

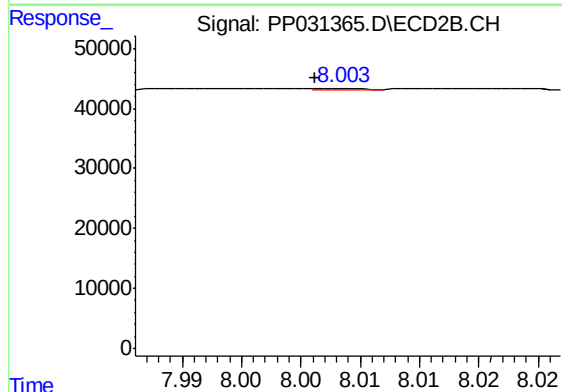


#35 AR-1260-5

R.T.: 8.004 min
Delta R.T.: 0.002 min
Response: 783
Conc: 0.20 ng/ml

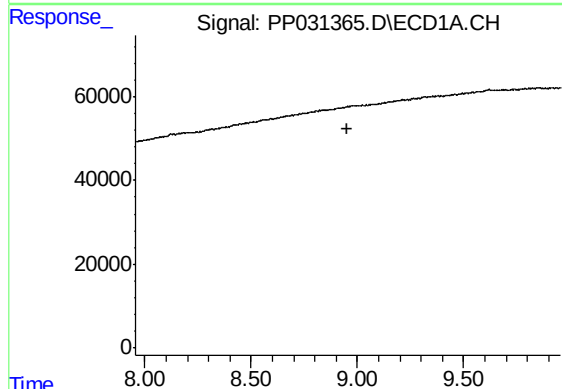


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.956 min
Response: 0
Conc: N.D.

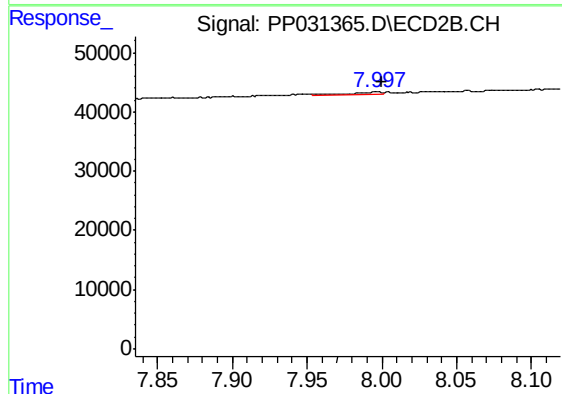

#37 AR-1262-2


R.T.: 7.997 min
Delta R.T.: -0.002 min
Response: 5470
Conc: 1.33 ng/ml

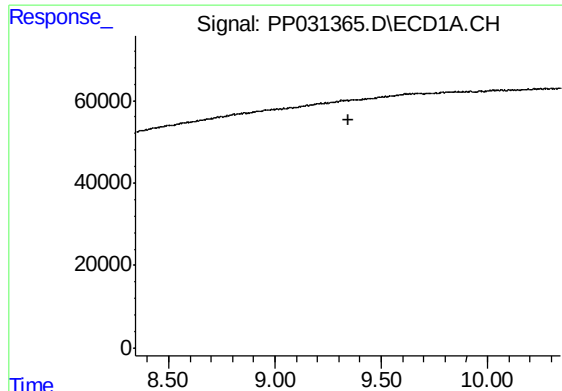

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

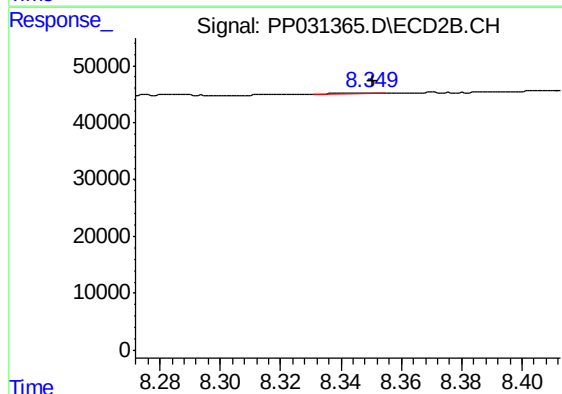


#39 AR-1262-4

R.T.: 8.350 min
Delta R.T.: -0.001 min
Response: 1904
Conc: 0.61 ng/ml

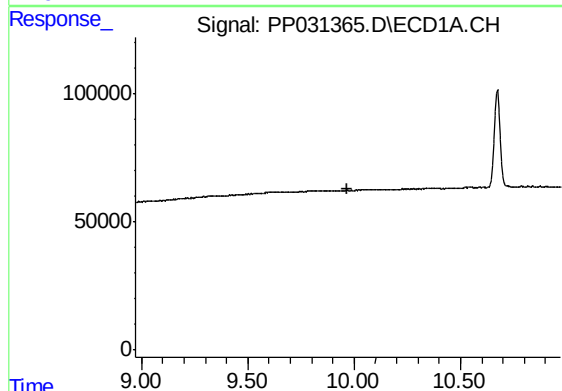


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

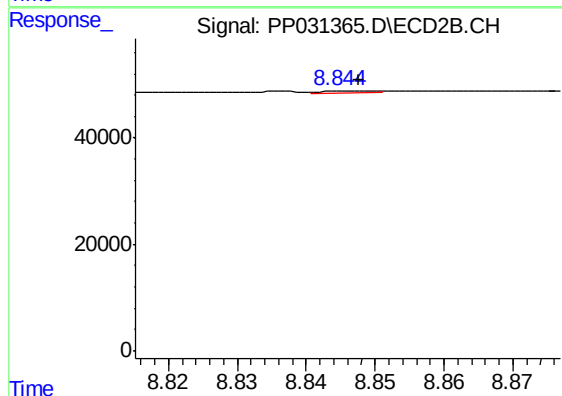

#40 AR-1262-5


R.T.: 8.845 min
Delta R.T.: -0.002 min
Response: 1929
Conc: 1.37 ng/ml

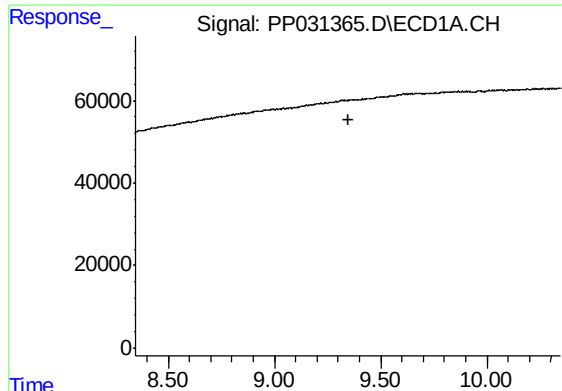

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

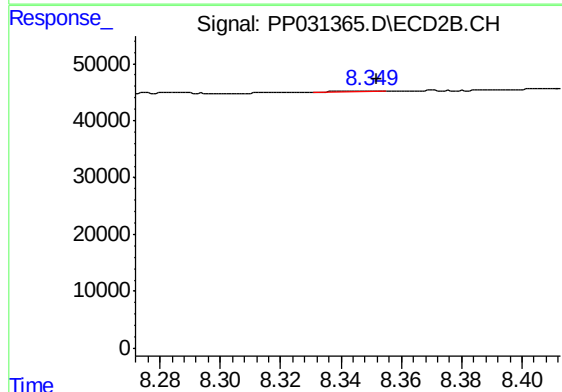


#42 AR-1268-2

R.T.: 8.350 min
Delta R.T.: -0.002 min
Response: 1904
Conc: 0.39 ng/ml

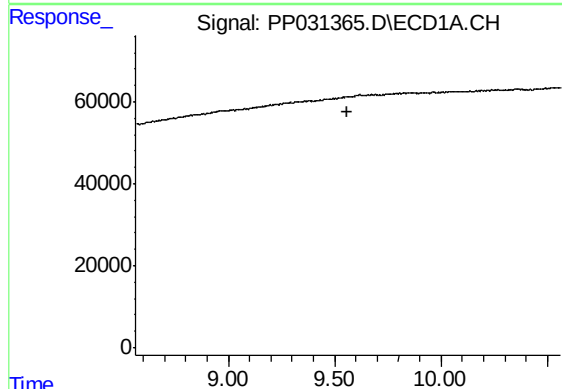


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.562 min
Response: 0
Conc: N.D.

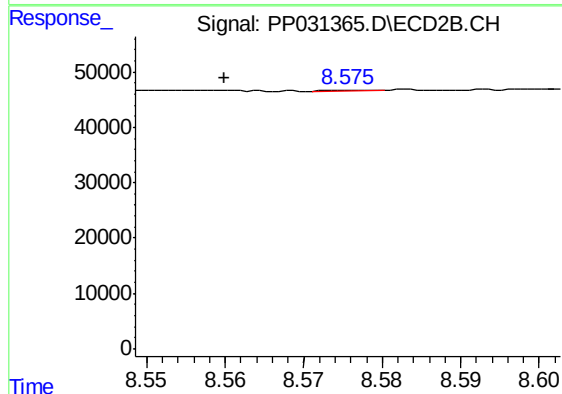

#43 AR-1268-3


R.T.: 8.576 min
Delta R.T.: 0.016 min
Response: 797
Conc: 0.19 ng/ml

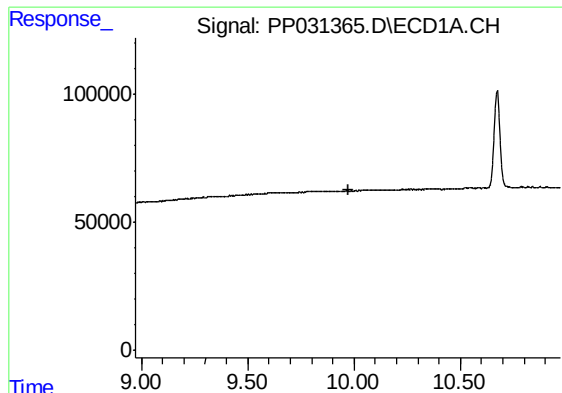

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

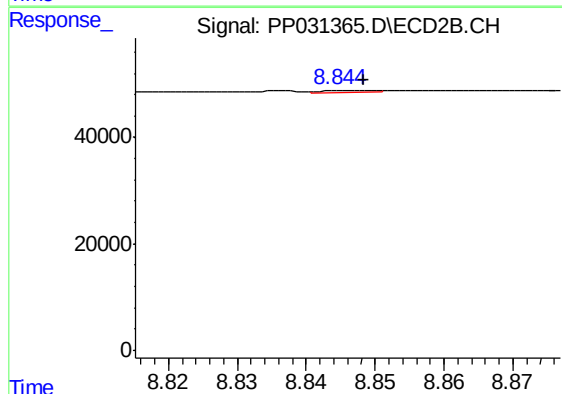


#44 AR-1268-4

R.T.: 8.845 min
Delta R.T.: -0.003 min
Response: 1929
Conc: 1.16 ng/ml

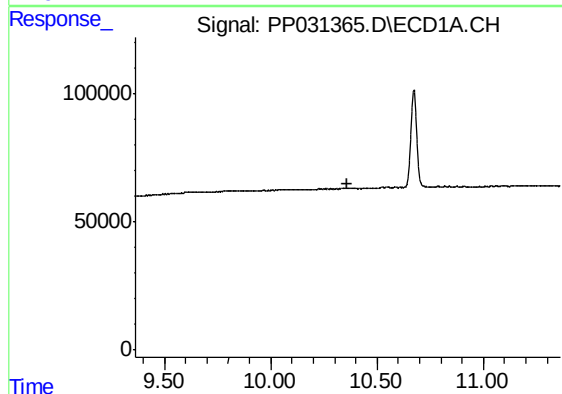

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.363 min
Response: 0
Conc: N.D.

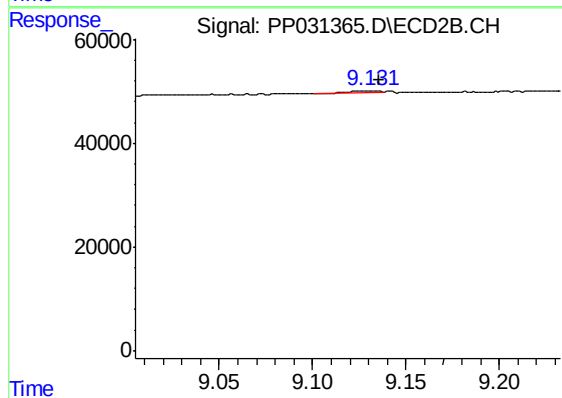

#45 AR-1268-5

R.T.: 9.131 min
Delta R.T.: -0.005 min
Response: 1890
Conc: 0.14 ng/ml