

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031366.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 16:45
 Operator : DD\AJ
 Sample : L4784-01
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SIMW-02-20201117

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:53:27 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.797	4.071	892412	868003	21.906	20.762
2)	SA Decachlor...	10.669	9.380	497773	569298	16.207	17.002
Target Compounds							
9)	L2 AR-1221-2	0.000	4.422	0	20885	N.D.	59.142 #
33)	L7 AR-1260-3	0.000	7.277	0	6108	N.D.	3.166 #
35)	L7 AR-1260-5	0.000	7.979f	0	1054	N.D.	0.267 #
37)	L8 AR-1262-2	0.000	7.979f	0	1054	N.D.	0.256 #
38)	L8 AR-1262-3	0.000	8.285	0	2923	N.D.	1.834 #
40)	L8 AR-1262-5	0.000	8.837	0	1825	N.D.	1.293 #
41)	L9 AR-1268-1	0.000	8.285	0	2923	N.D.	0.594 #
44)	L9 AR-1268-4	0.000	8.859	0	1208	N.D.	0.725 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031366.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 16:45
Operator : DD\AJ
Sample : L4784-01
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:53:27 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

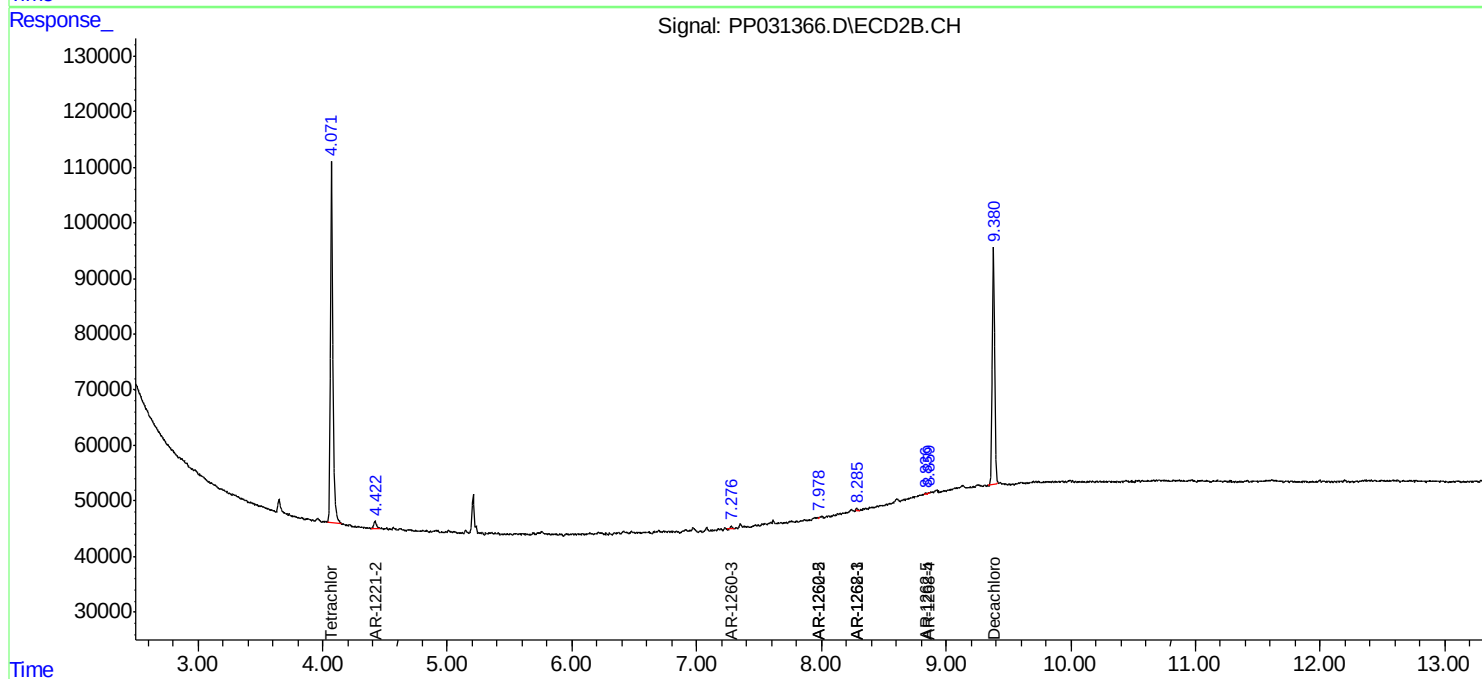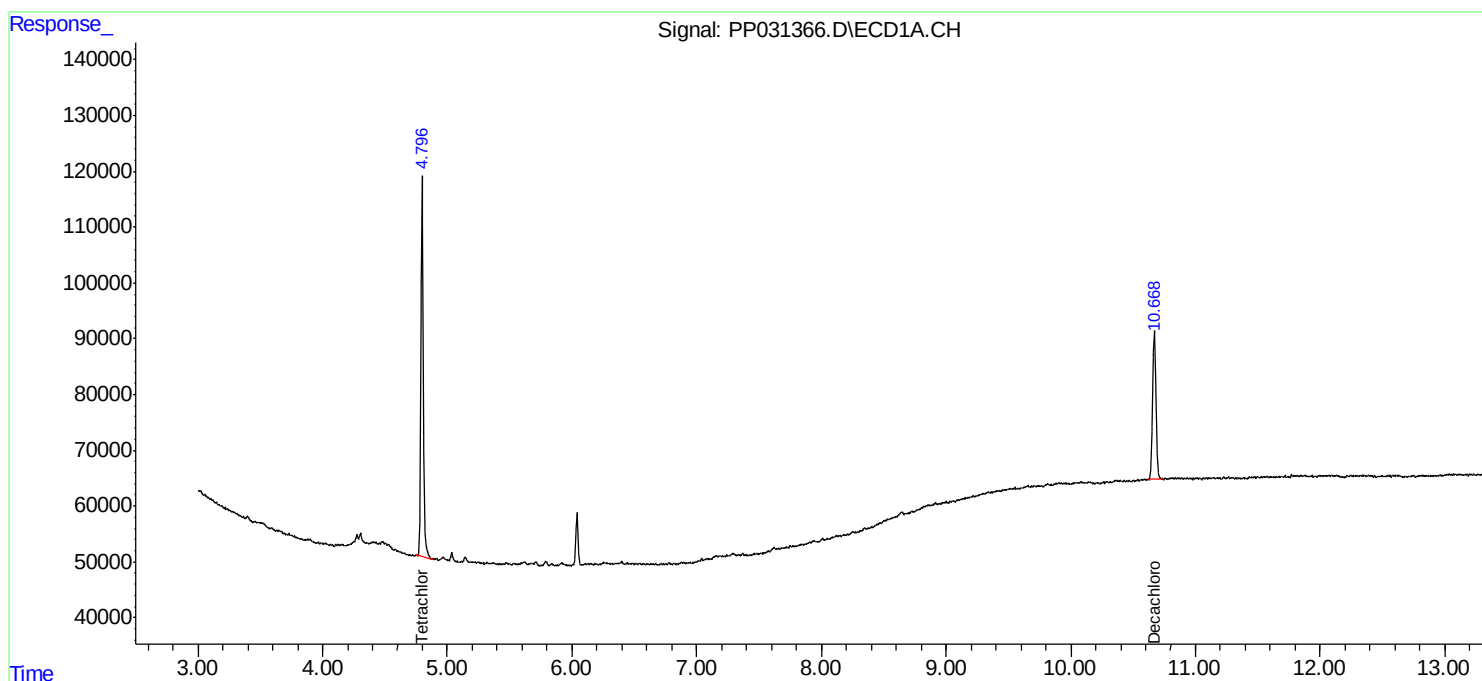


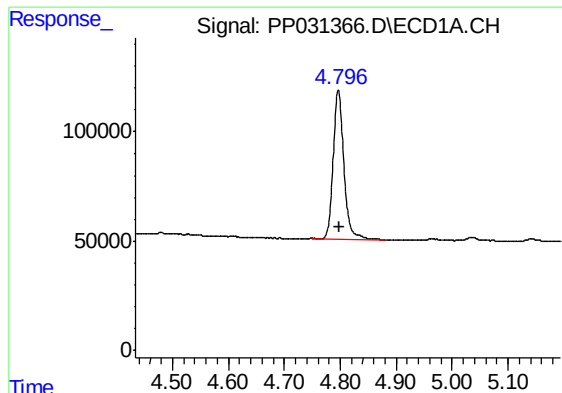

#1 Tetrachloro-m-xylene


R.T.: 4.797 min
Delta R.T.: -0.001 min
Response: 892412
Conc: 21.91 ng/ml

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

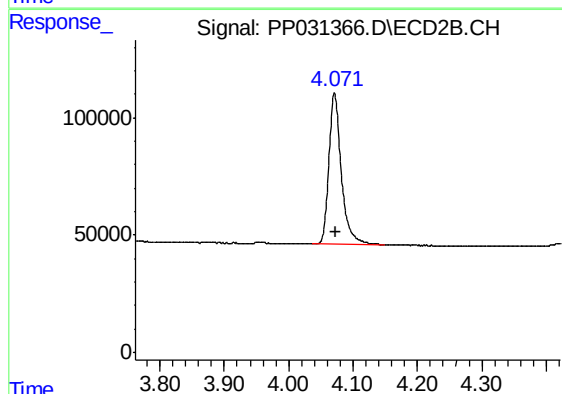


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.002 min
Response: 868003
Conc: 20.76 ng/ml

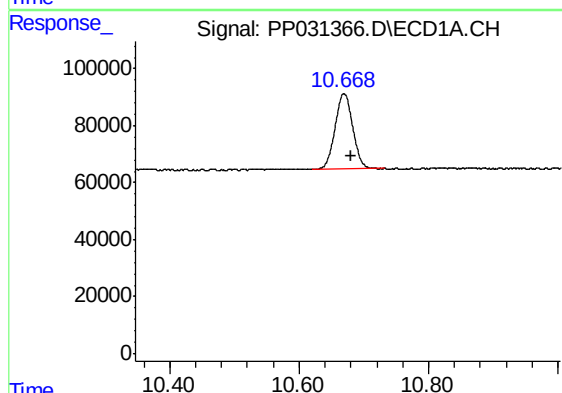


#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.011 min
Response: 497773
Conc: 16.21 ng/ml

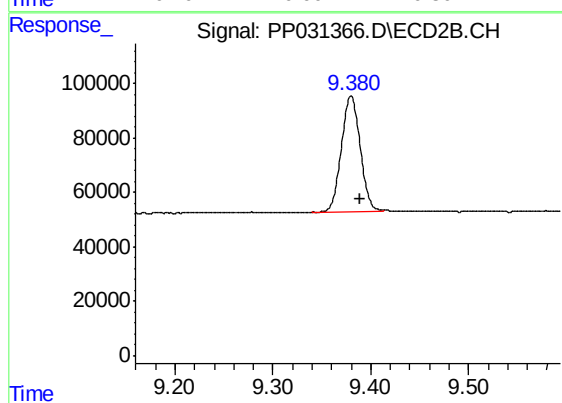

#2 Decachlorobiphenyl


R.T.: 9.380 min
Delta R.T.: -0.009 min
Response: 569298
Conc: 17.00 ng/ml

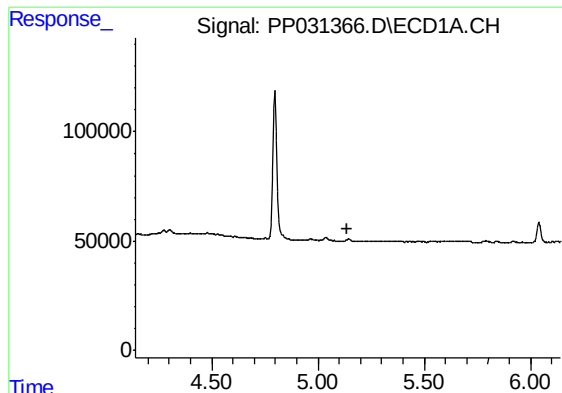

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

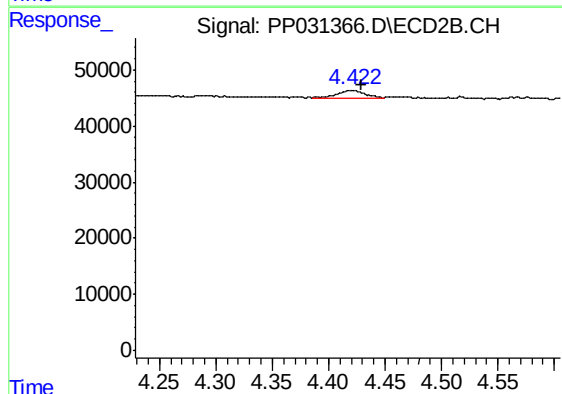


#9 AR-1221-2

R.T.: 4.422 min
Delta R.T.: -0.007 min
Response: 20885
Conc: 59.14 ng/ml

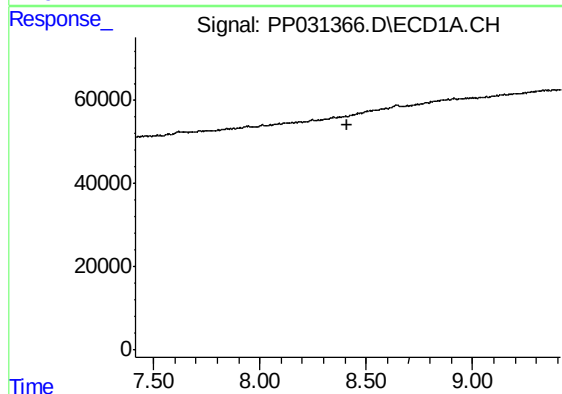


#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.414 min
Response: 0
Conc: N.D.

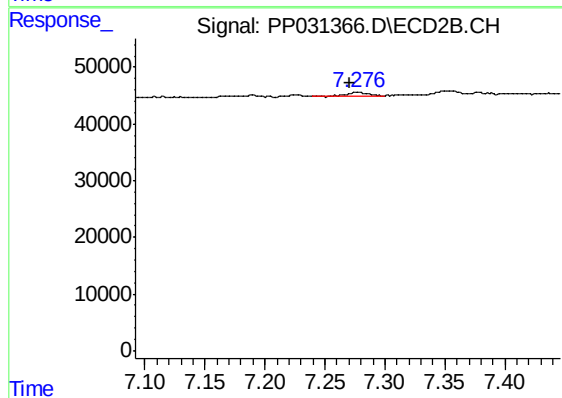

#33 AR-1260-3


R.T.: 7.277 min
Delta R.T.: 0.005 min
Response: 6108
Conc: 3.17 ng/ml

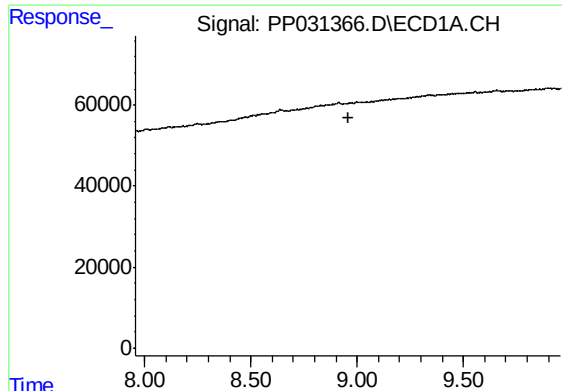

#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

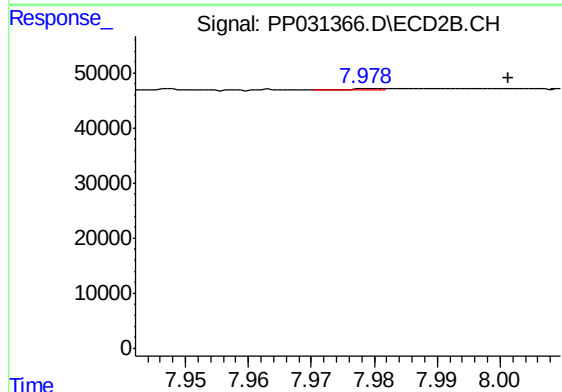


#35 AR-1260-5

R.T.: 7.979 min
Delta R.T.: -0.022 min
Response: 1054
Conc: 0.27 ng/ml

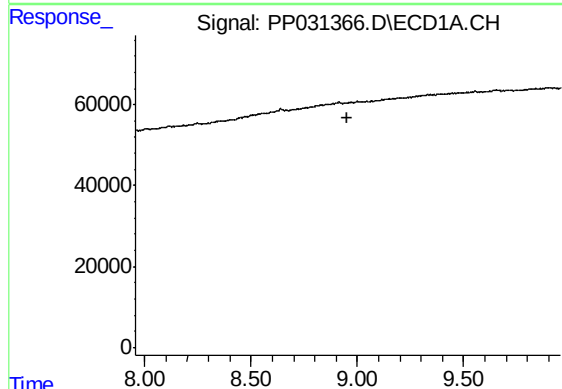


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.956 min
Response: 0
Conc: N.D.

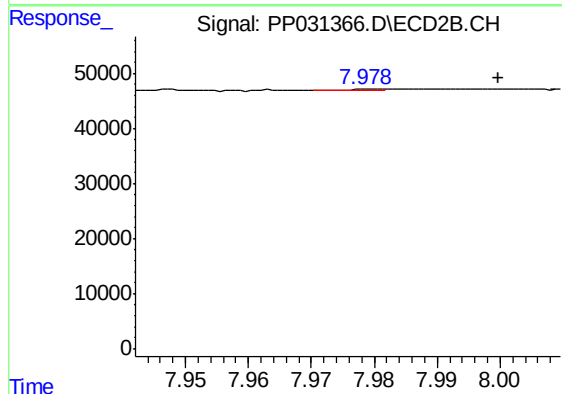

#37 AR-1262-2


R.T.: 7.979 min
Delta R.T.: -0.021 min
Response: 1054
Conc: 0.26 ng/ml

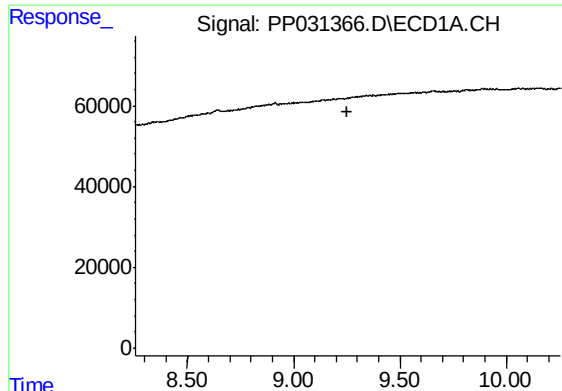

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

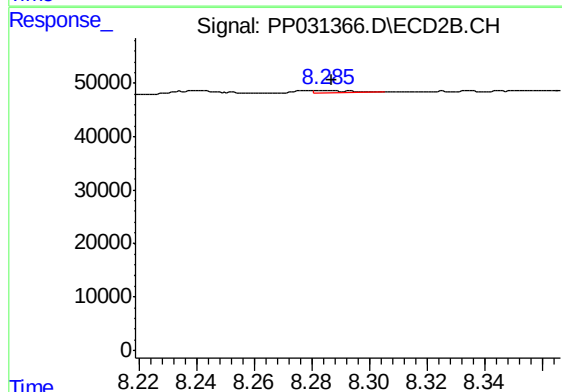


#38 AR-1262-3

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 2923
Conc: 1.83 ng/ml

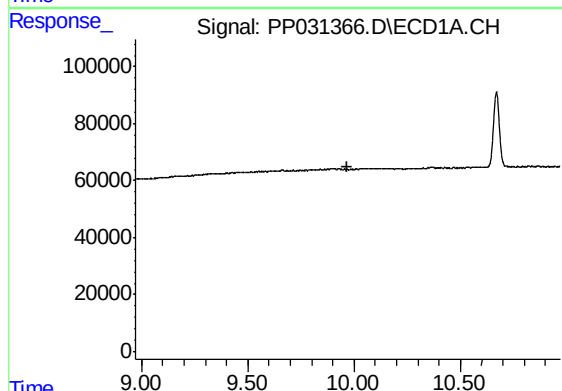


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

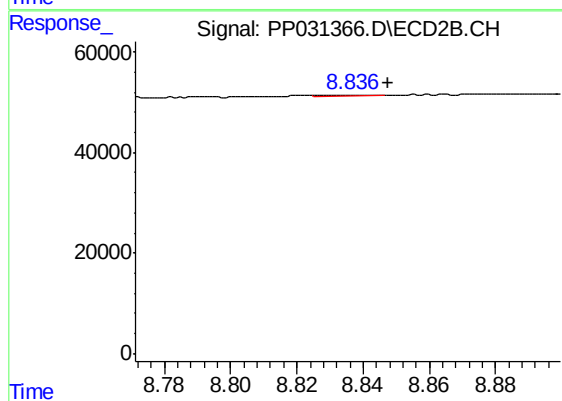

#40 AR-1262-5


R.T.: 8.837 min
Delta R.T.: -0.011 min
Response: 1825
Conc: 1.29 ng/ml

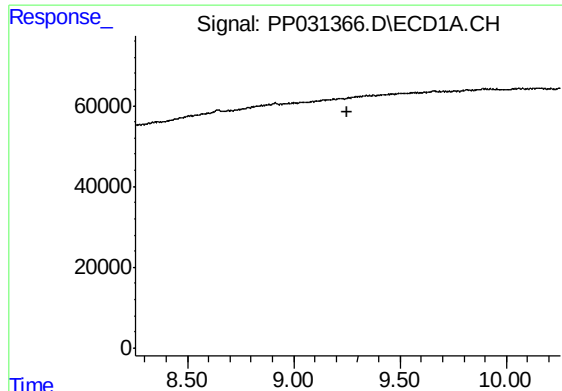

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T. : 9.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
SIMW-02-20201117

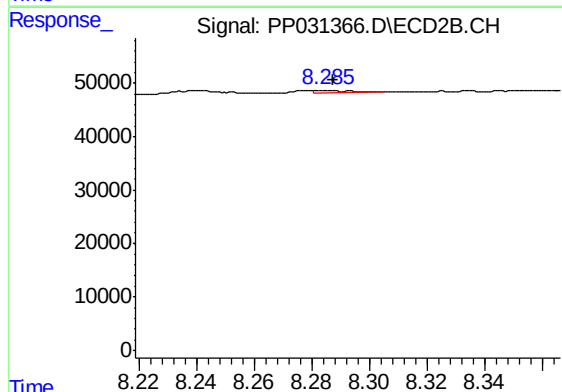


#41 AR-1268-1

R.T.: 8.285 min
Delta R.T.: -0.002 min
Response: 2923
Conc: 0.59 ng/ml

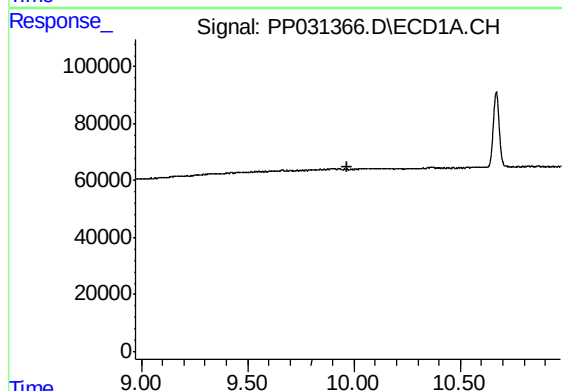

#44 AR-1268-4

R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

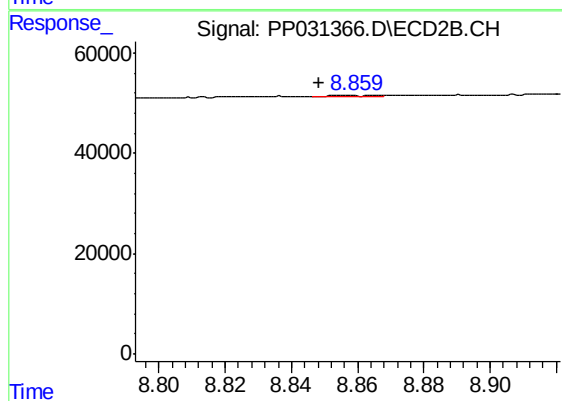

#44 AR-1268-4

R.T.: 8.859 min
Delta R.T.: 0.011 min
Response: 1208
Conc: 0.73 ng/ml