

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031377.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 20:04
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:59:10 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.794	4.067	1042129	1022721	25.581	24.462
2)	SA Decachlor...	10.666	9.377	762410	882385	24.823	26.352
Target Compounds							
9)	L2 AR-1221-2	0.000	4.420	0	12023	N.D.	34.048 #
20)	L4 AR-1242-5	0.000	6.222f	0	6954	N.D.	7.869 #
25)	L5 AR-1248-5	0.000	6.222f	0	6954	N.D.	5.537 #
26)	L6 AR-1254-1	0.000	6.222f	0	6954	N.D.	3.654 #
28)	L6 AR-1254-3	7.615	6.784	47080	741	21.718	0.271 #
30)	L6 AR-1254-5	0.000	7.442	0	728	N.D.	0.301 #
32)	L7 AR-1260-2	0.000	7.107	0	2132	N.D.	1.047 #
33)	L7 AR-1260-3	0.000	7.262	0	2032	N.D.	1.053 #
35)	L7 AR-1260-5	0.000	7.992	0	3528	N.D.	0.893 #
37)	L8 AR-1262-2	0.000	7.992	0	3528	N.D.	0.858 #
39)	L8 AR-1262-4	0.000	8.339	0	242	N.D.	0.077 #
40)	L8 AR-1262-5	0.000	8.842	0	2675	N.D.	1.896 #
42)	L9 AR-1268-2	0.000	8.339	0	242	N.D.	0.050 #
43)	L9 AR-1268-3	0.000	8.549	0	1768	N.D.	0.424 #
44)	L9 AR-1268-4	0.000	8.842	0	2675	N.D.	1.605 #
45)	L9 AR-1268-5	0.000	9.133	0	1923	N.D.	0.147 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031377.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 20:04
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:59:10 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

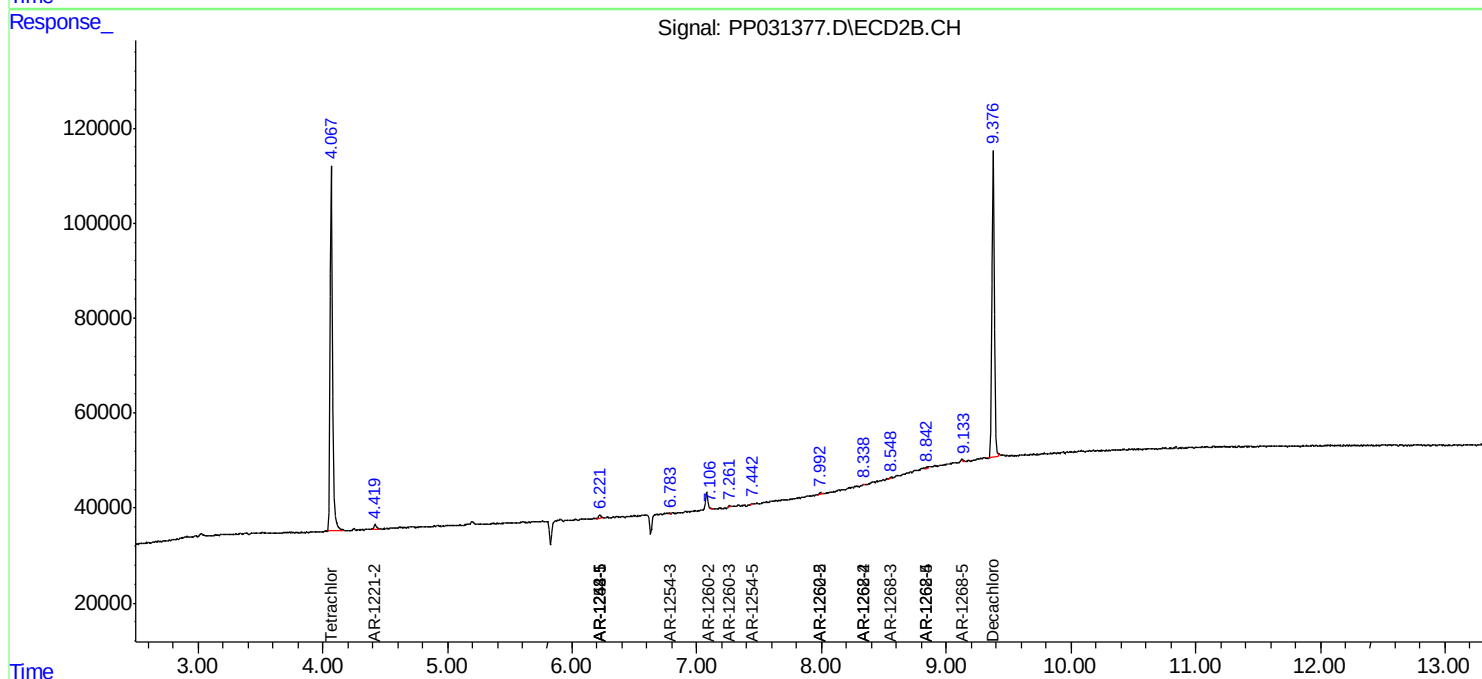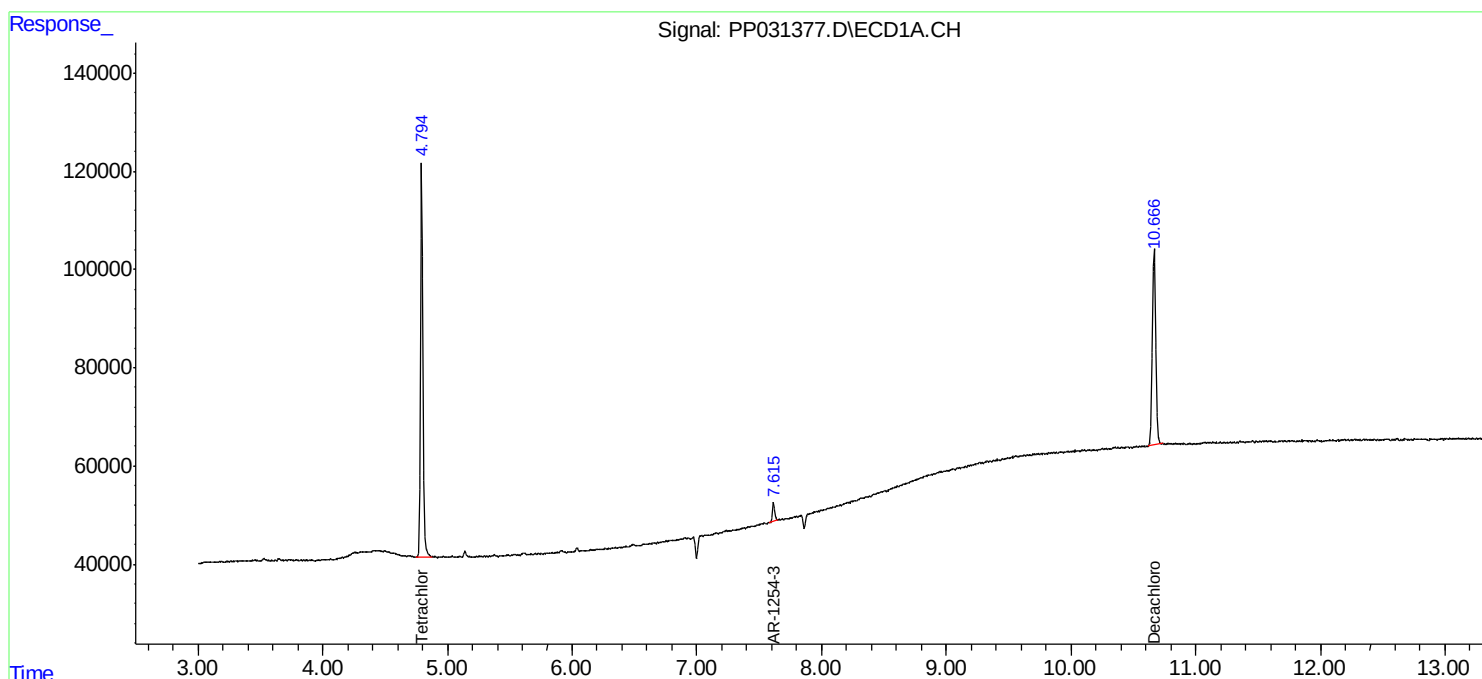




#1 Tetrachloro-m-xylene


R.T.: 4.794 min
Delta R.T.: -0.004 min
Response: 1042129
Conc: 25.58 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

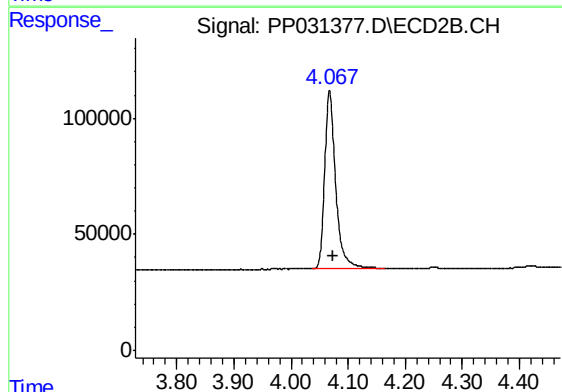


#1 Tetrachloro-m-xylene

R.T.: 4.067 min
Delta R.T.: -0.005 min
Response: 1022721
Conc: 24.46 ng/ml




#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.014 min
Response: 762410
Conc: 24.82 ng/ml

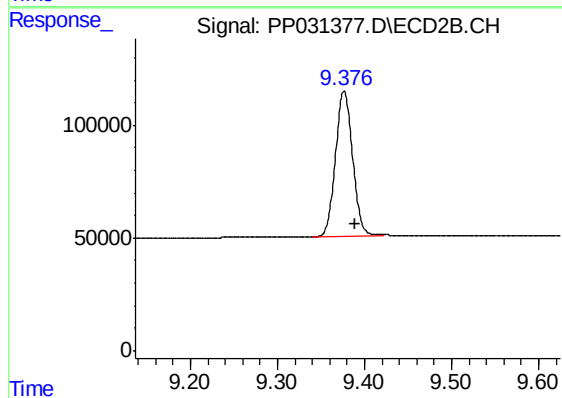

#2 Decachlorobiphenyl


R.T.: 9.377 min
Delta R.T.: -0.012 min
Response: 882385
Conc: 26.35 ng/ml

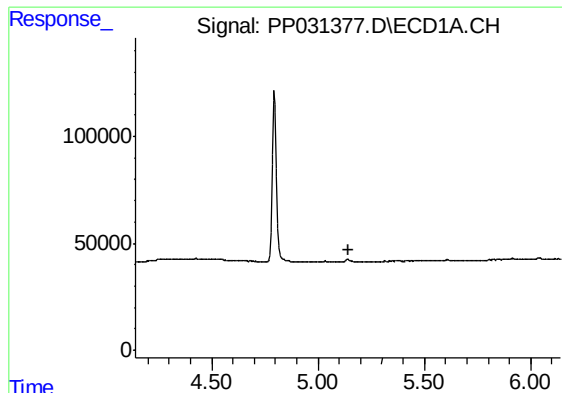

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

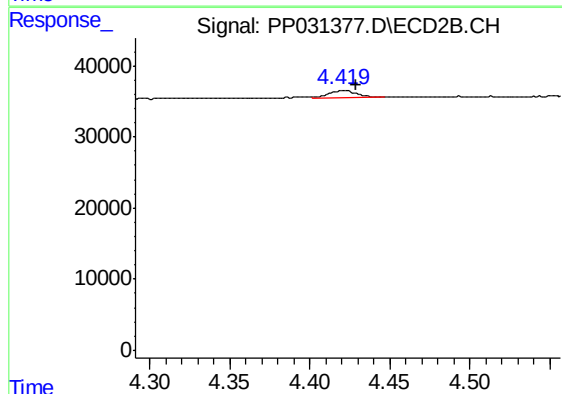


#9 AR-1221-2

R.T.: 4.420 min
Delta R.T.: -0.009 min
Response: 12023
Conc: 34.05 ng/ml

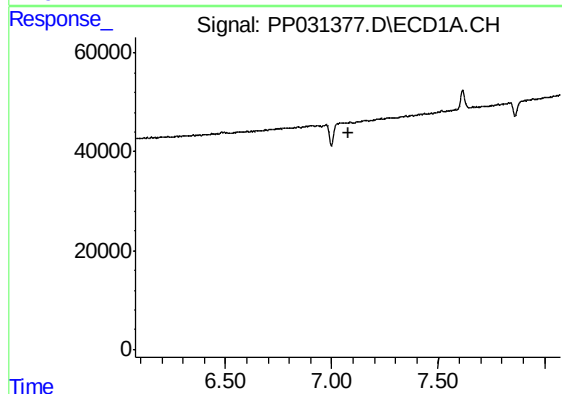


#20 AR-1242-5

R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

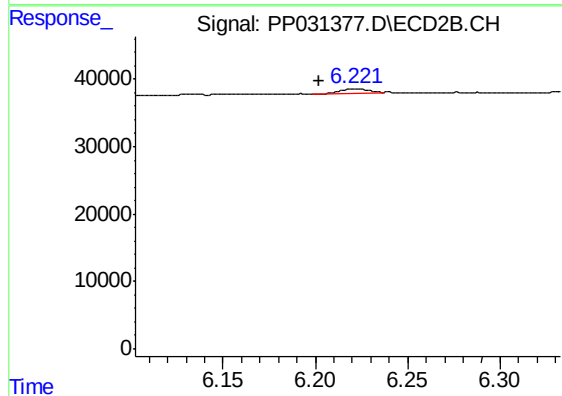

#20 AR-1242-5


R.T.: 6.222 min
Delta R.T.: 0.020 min
Response: 6954
Conc: 7.87 ng/ml



#25 AR-1248-5


R.T.: 0.000 min
Exp R.T. : 7.076 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

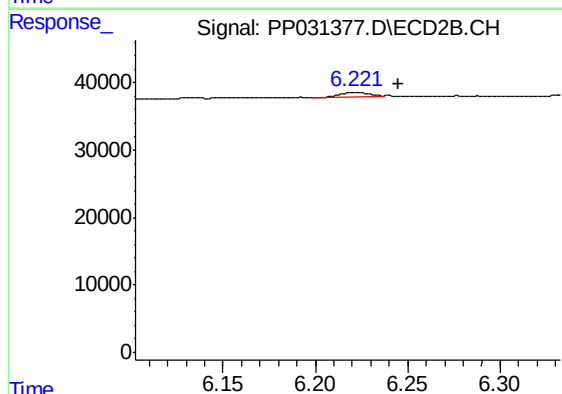


#25 AR-1248-5

R.T.: 6.222 min
Delta R.T.: -0.023 min
Response: 6954
Conc: 5.54 ng/ml

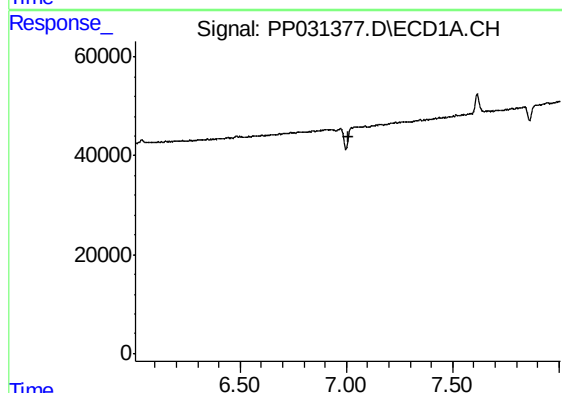


#26 AR-1254-1

R.T.: 0.000 min
Exp R.T. : 7.008 min
Response: 0
Conc: N.D.

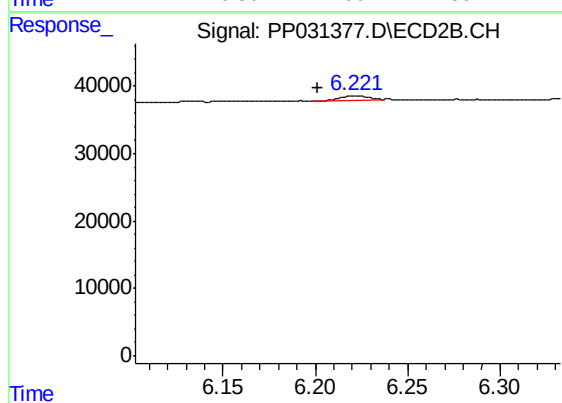

#26 AR-1254-1


R.T.: 6.222 min
Delta R.T.: 0.021 min
Response: 6954
Conc: 3.65 ng/ml

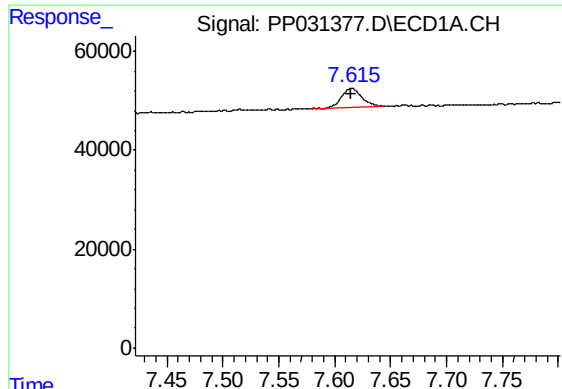

#28 AR-1254-3


R.T.: 7.615 min
Delta R.T.: 0.000 min
Response: 47080
Conc: 21.72 ng/ml

Instrument :
ECD_P
ClientSampleId :
I.BLK

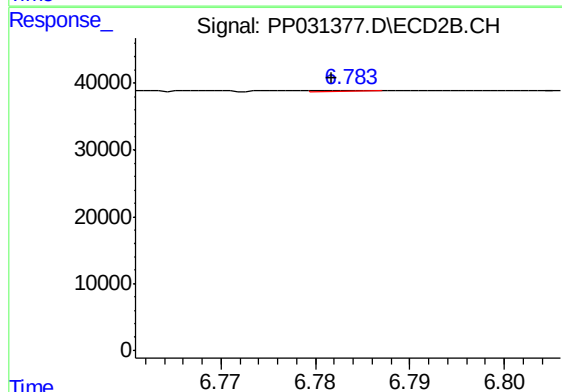


#28 AR-1254-3

R.T.: 6.784 min
Delta R.T.: 0.002 min
Response: 741
Conc: 0.27 ng/ml




#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.337 min
Response: 0
Conc: N.D.

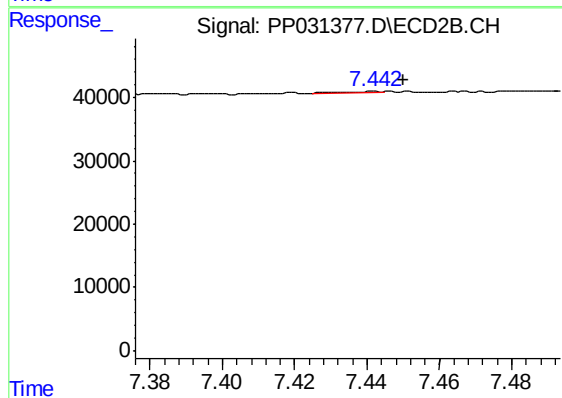

#30 AR-1254-5


R.T.: 7.442 min
Delta R.T.: -0.008 min
Response: 728
Conc: 0.30 ng/ml



#32 AR-1260-2


R.T.: 0.000 min
Exp R.T. : 8.049 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

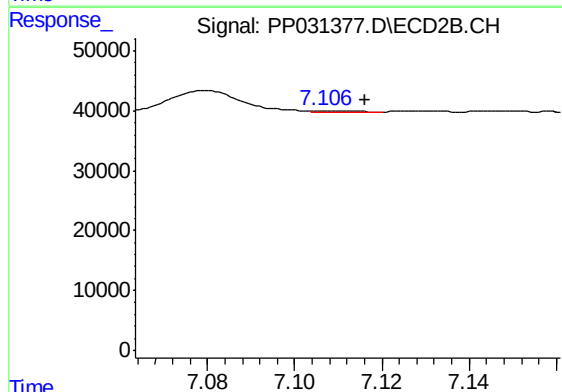


#32 AR-1260-2

R.T.: 7.107 min
Delta R.T.: -0.009 min
Response: 2132
Conc: 1.05 ng/ml




#33 AR-1260-3

R.T.: 0.000 min
Exp R.T. : 8.414 min
Response: 0
Conc: N.D.

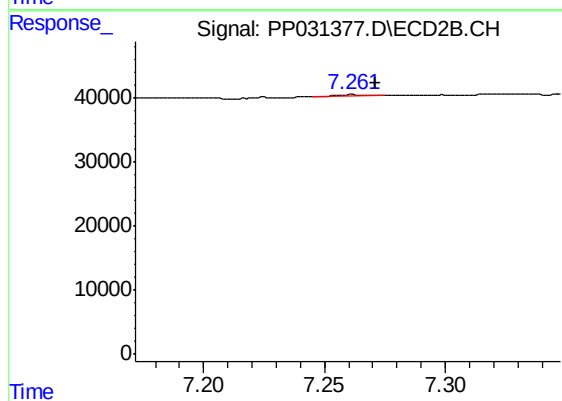

#33 AR-1260-3


R.T.: 7.262 min
Delta R.T.: -0.010 min
Response: 2032
Conc: 1.05 ng/ml



#35 AR-1260-5


R.T.: 0.000 min
Exp R.T. : 8.957 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

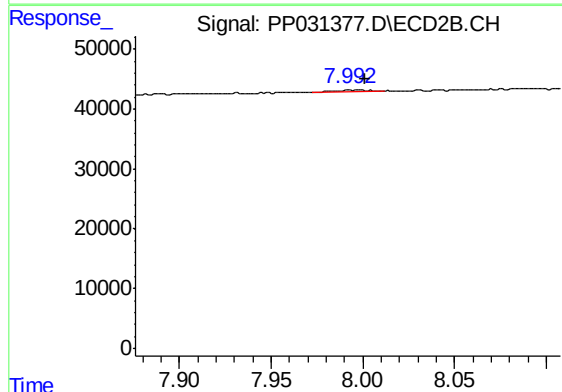


#35 AR-1260-5

R.T.: 7.992 min
Delta R.T.: -0.009 min
Response: 3528
Conc: 0.89 ng/ml

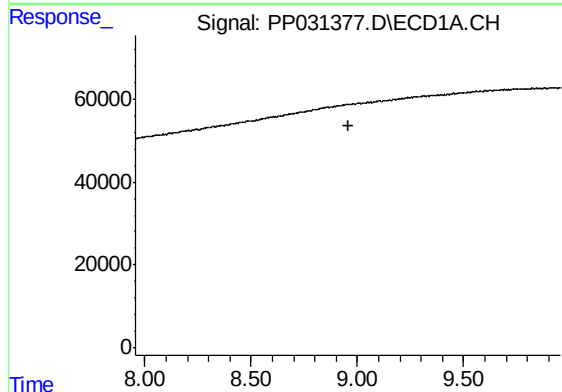


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.956 min
Response: 0
Conc: N.D.

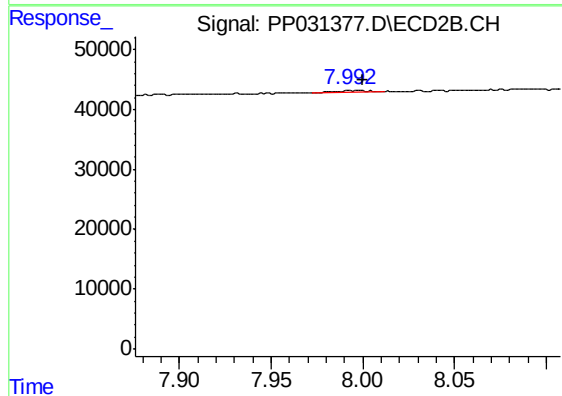

#37 AR-1262-2


R.T.: 7.992 min
Delta R.T.: -0.008 min
Response: 3528
Conc: 0.86 ng/ml



#39 AR-1262-4


R.T.: 0.000 min
Exp R.T. : 9.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

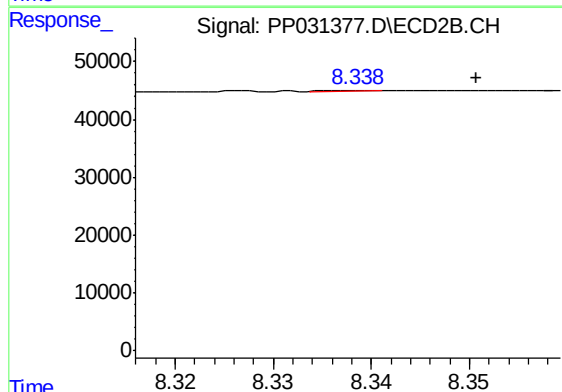


#39 AR-1262-4

R.T.: 8.339 min
Delta R.T.: -0.012 min
Response: 242
Conc: 0.08 ng/ml




#40 AR-1262-5

R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

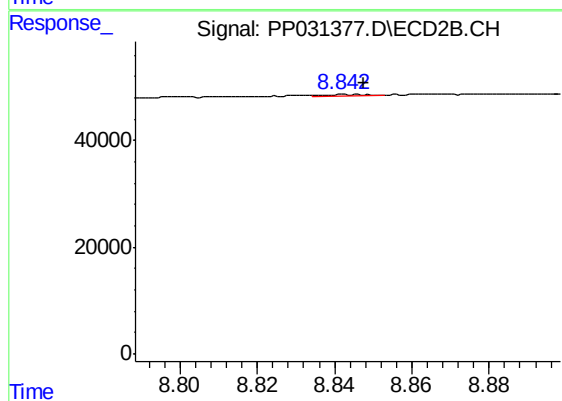

#40 AR-1262-5


R.T.: 8.842 min
Delta R.T.: -0.005 min
Response: 2675
Conc: 1.90 ng/ml

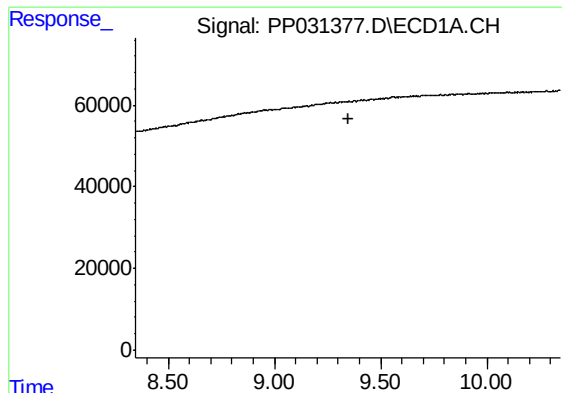

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T. : 9.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

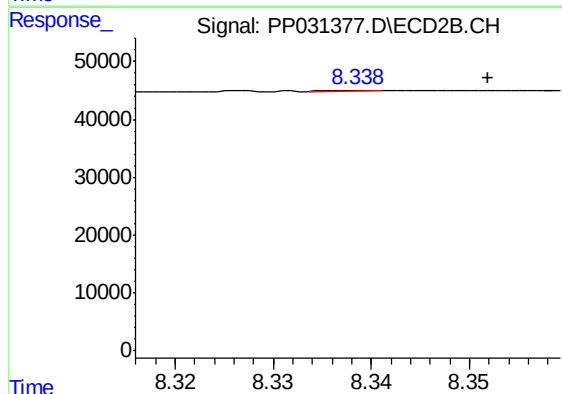


#42 AR-1268-2

R.T.: 8.339 min
Delta R.T.: -0.013 min
Response: 242
Conc: 0.05 ng/ml




#43 AR-1268-3

R.T.: 0.000 min
Exp R.T. : 9.562 min
Response: 0
Conc: N.D.

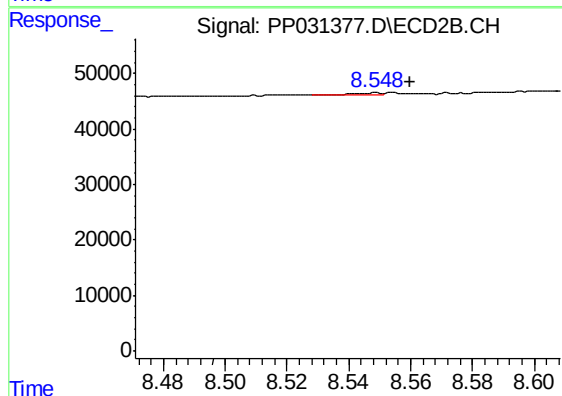

#43 AR-1268-3


R.T.: 8.549 min
Delta R.T.: -0.011 min
Response: 1768
Conc: 0.42 ng/ml

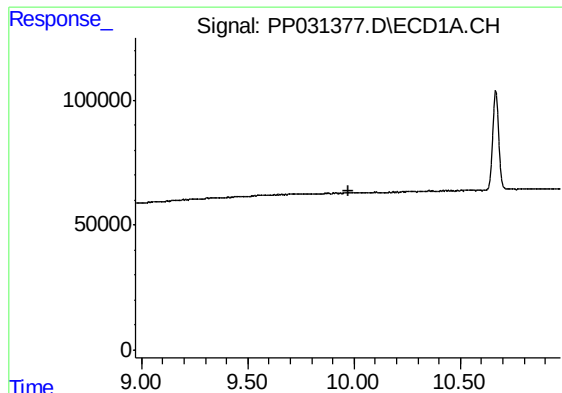

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
I.BLK

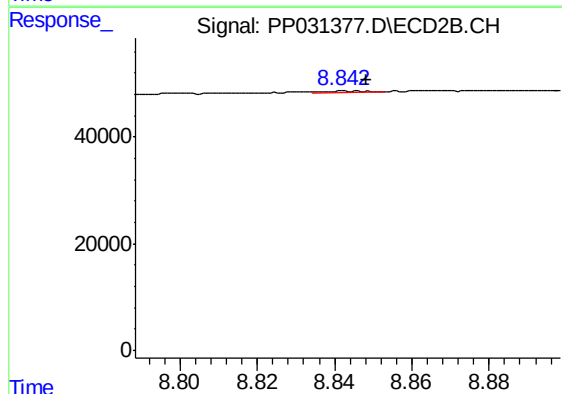


#44 AR-1268-4

R.T.: 8.842 min
Delta R.T.: -0.006 min
Response: 2675
Conc: 1.61 ng/ml

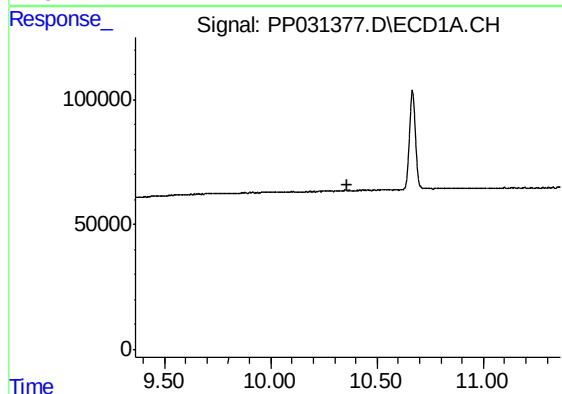

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.363 min
Response: 0
Conc: N.D.

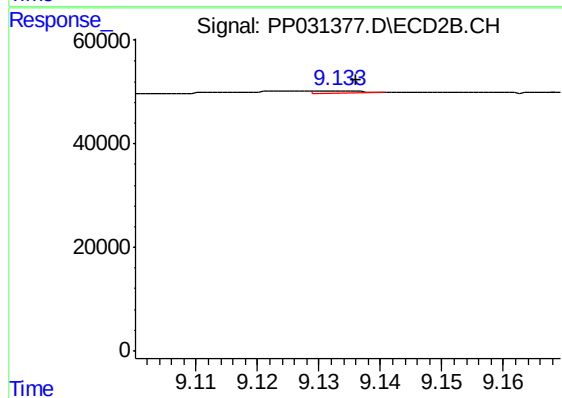

#45 AR-1268-5

R.T.: 9.133 min
Delta R.T.: -0.003 min
Response: 1923
Conc: 0.15 ng/ml