

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031345.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 10:16
 Operator : DD\AJ
 Sample : L4741-02 5X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 11-13-B

Manual Integrations
 APPROVED

Ankita
 11/19/2020 1:16:15 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:39:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.795	4.070	377443	559241	9.265	13.376m#
2) SA Decachlor...	10.669	9.375	107521	425669	3.501	12.712m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031345.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 10:16
Operator : DD\AJ
Sample : L4741-02 5X
Misc :
ALS Vial : 7 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
11-13-B


Manual Integrations
APPROVED

Ankita
11/19/2020 1:16:15 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:39:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

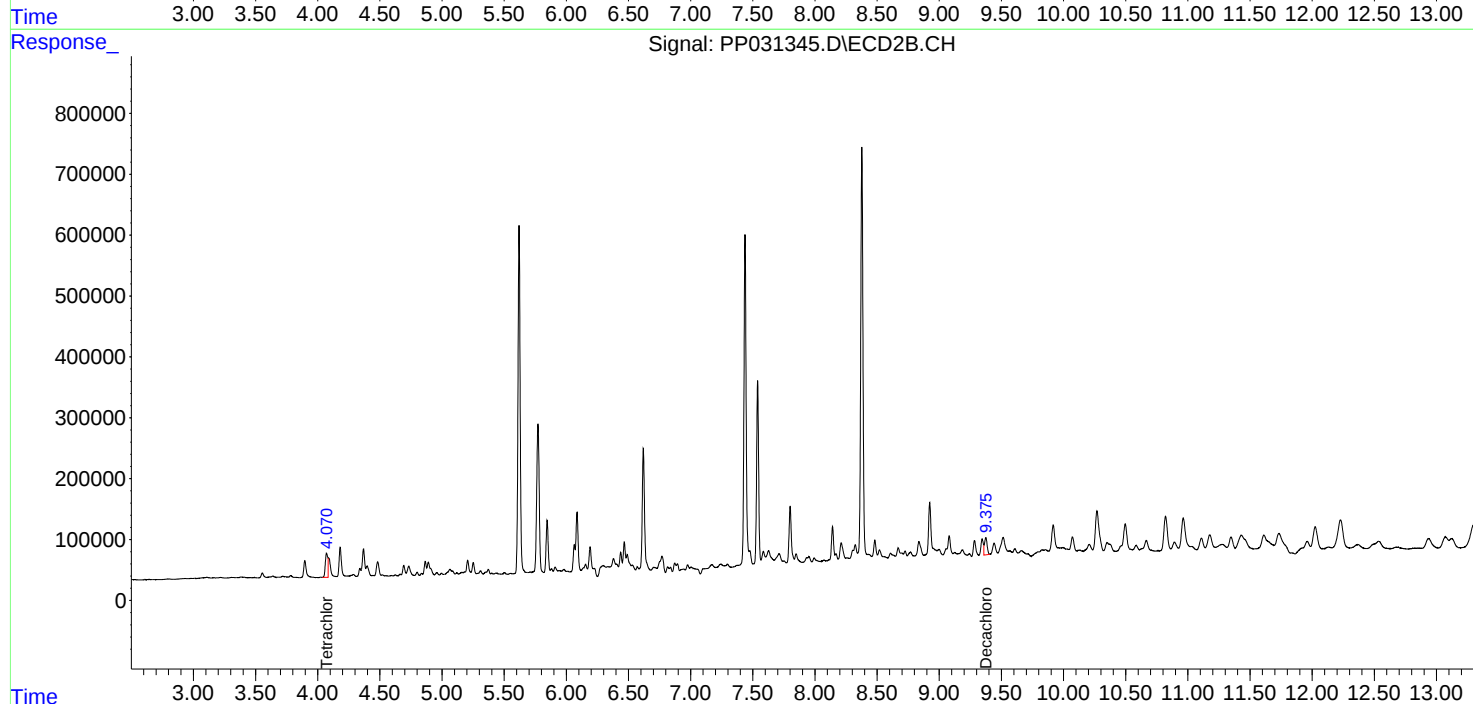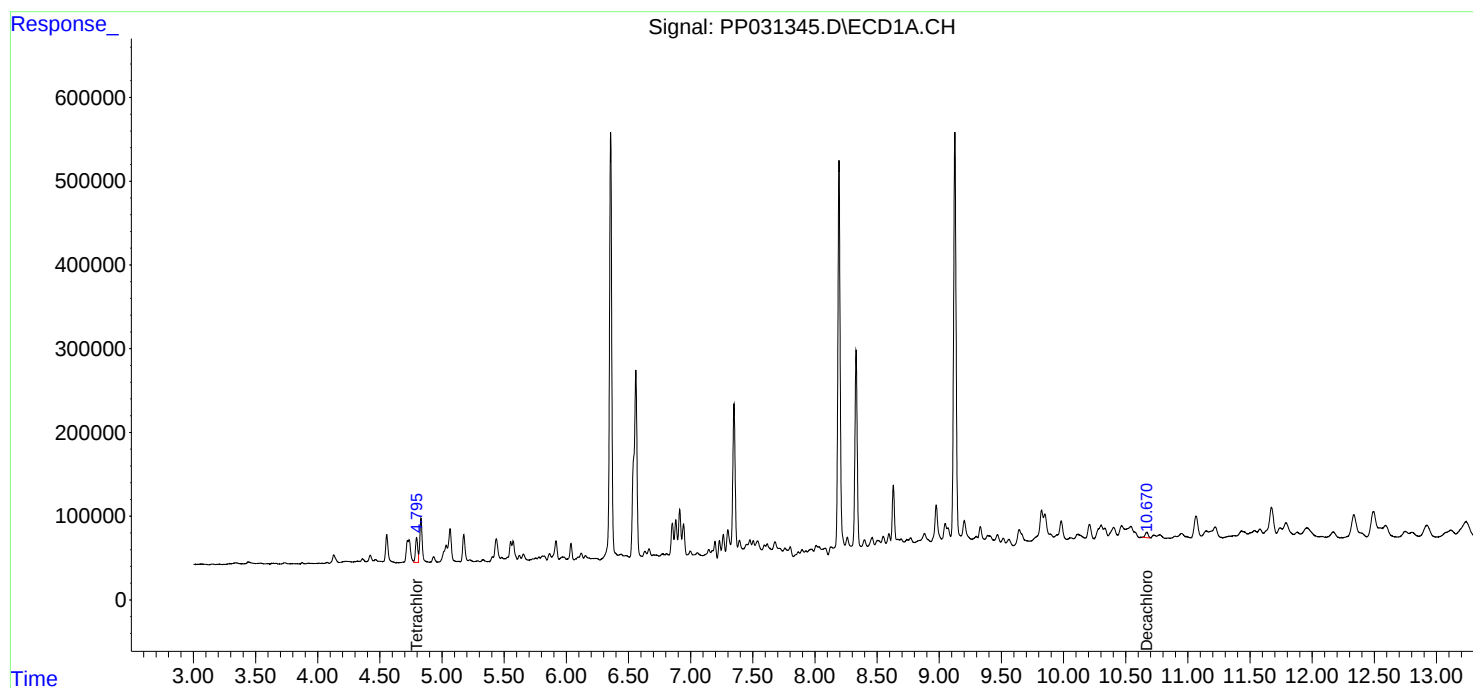

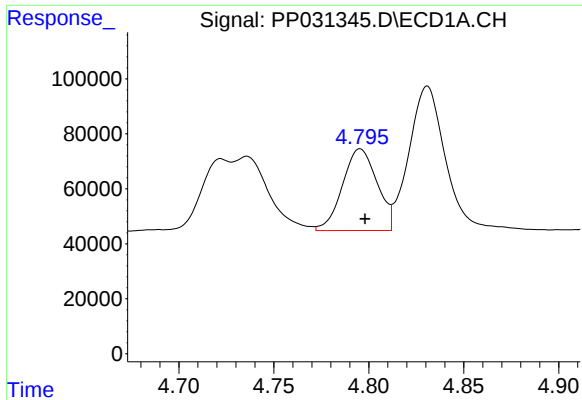


#1 Tetrachloro-m-xylene

R.T.: 4.795 min
Delta R.T.: -0.003 min
Response: 377443
Conc: 9.26 ng/ml

Instrument :
ECD_P
ClientSampleId :
11-13-B


Manual Integrations
APPROVED

Ankita
11/19/2020 1:16:15 PM

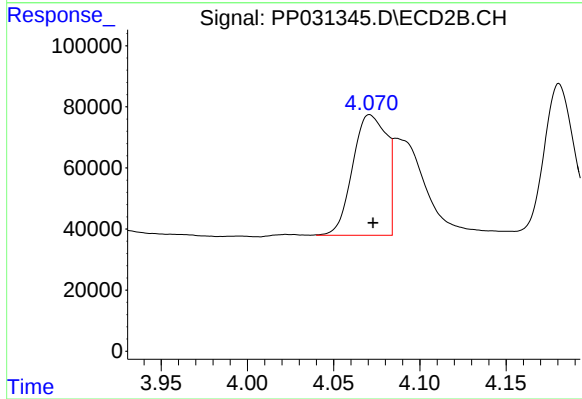


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.003 min
Response: 559241
Conc: 13.38 ng/ml m

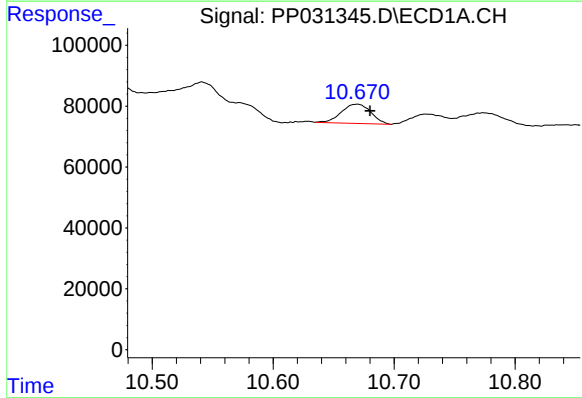

#2 Decachlorobiphenyl

R.T.: 10.669 min
Delta R.T.: -0.011 min
Response: 107521
Conc: 3.50 ng/ml

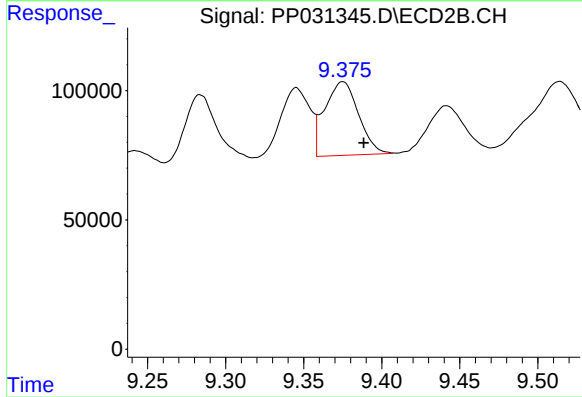

#2 Decachlorobiphenyl

R.T.: 9.375 min
Delta R.T.: -0.014 min
Response: 425669
Conc: 12.71 ng/ml m