

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031355.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 13:40
 Operator : DD\AJ
 Sample : L4778-04
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1811

Manual Integrations
 APPROVED

Ankita
 11/19/2020 1:16:25 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:45:55 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.796	4.070	1061484	1054871	26.056m	25.231
2) SA Decachlor...	10.672	9.381	804982	912245	26.209	27.243

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031355.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 13:40
Operator : DD\AJ
Sample : L4778-04
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1811


Manual Integrations
APPROVED

Ankita
11/19/2020 1:16:25 PM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:45:55 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

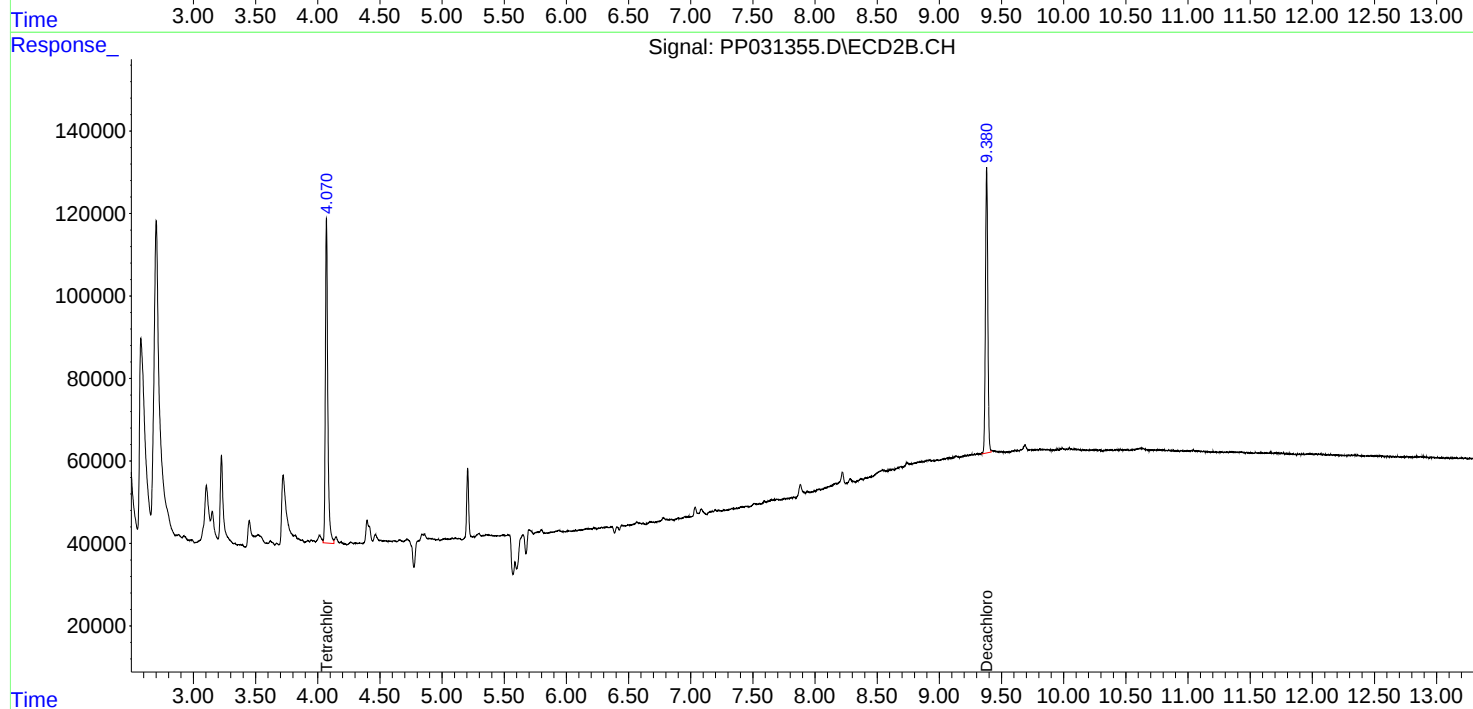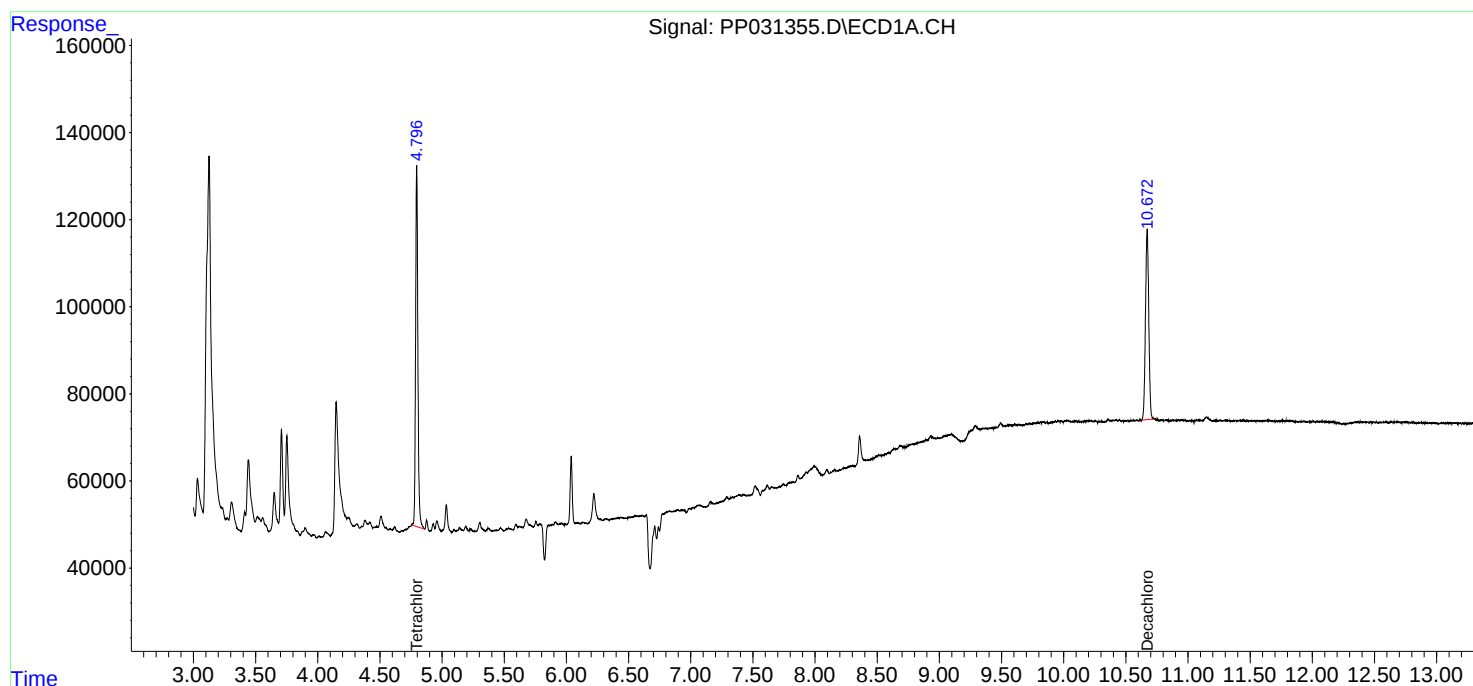

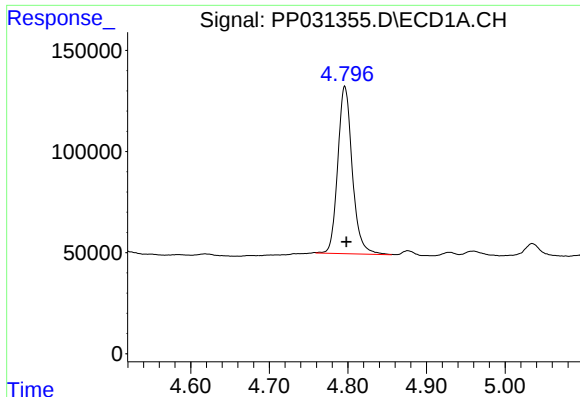


#1 Tetrachloro-m-xylene

R.T.: 4.796 min
Delta R.T.: -0.002 min
Response: 1061484
Conc: 26.06 ng/ml m

Instrument :
ECD_P
ClientSampleId :
1811


Manual Integrations
APPROVED

Ankita
11/19/2020 1:16:25 PM

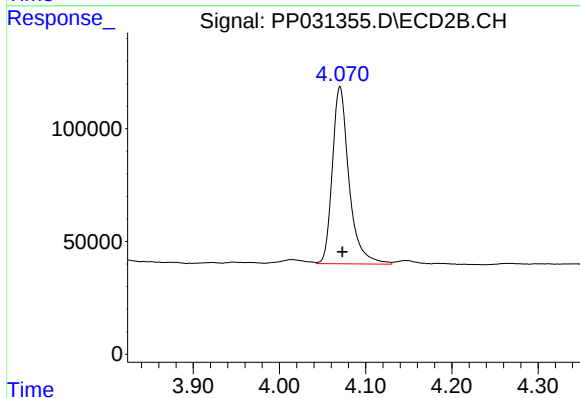


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.003 min
Response: 1054871
Conc: 25.23 ng/ml

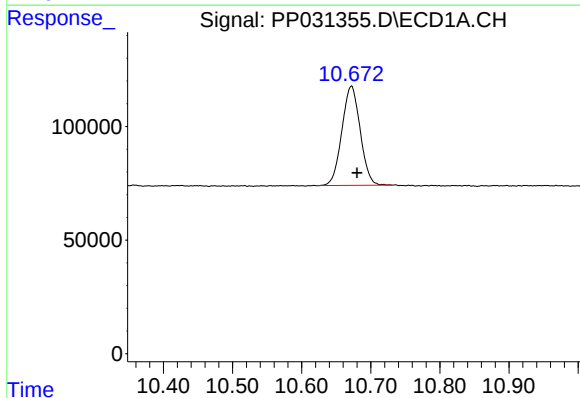

#2 Decachlorobiphenyl

R.T.: 10.672 min
Delta R.T.: -0.008 min
Response: 804982
Conc: 26.21 ng/ml

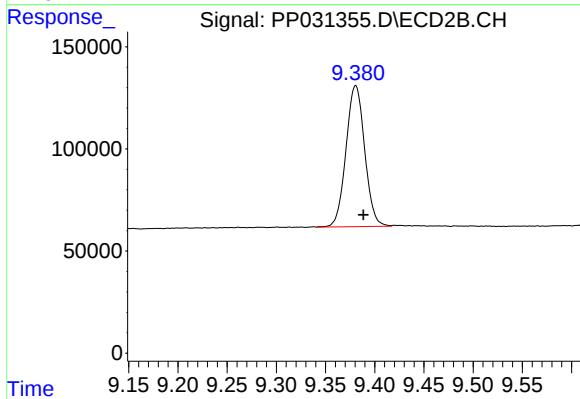

#2 Decachlorobiphenyl

R.T.: 9.381 min
Delta R.T.: -0.008 min
Response: 912245
Conc: 27.24 ng/ml