

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
 Data File : PP031373.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2020 18:41
 Operator : DD\AJ
 Sample : L4784-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 CSIMW-1-20201117

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:56:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.795	4.071	888505	869165	21.810	20.789
2) SA Decachlor...	10.667	9.378	568083	651979	18.496	19.471

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031373.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2020 18:41
Operator : DD\AJ
Sample : L4784-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
CSIMW-1-20201117

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:56:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

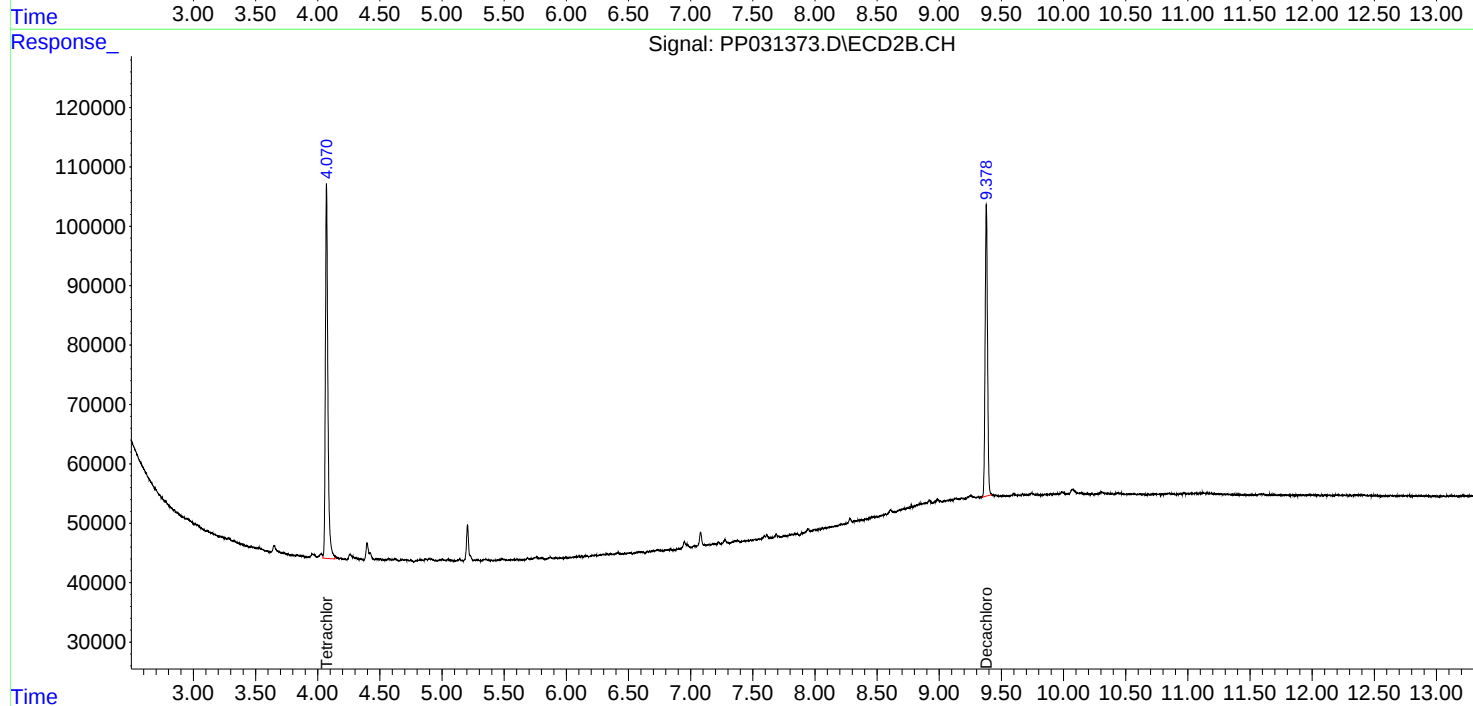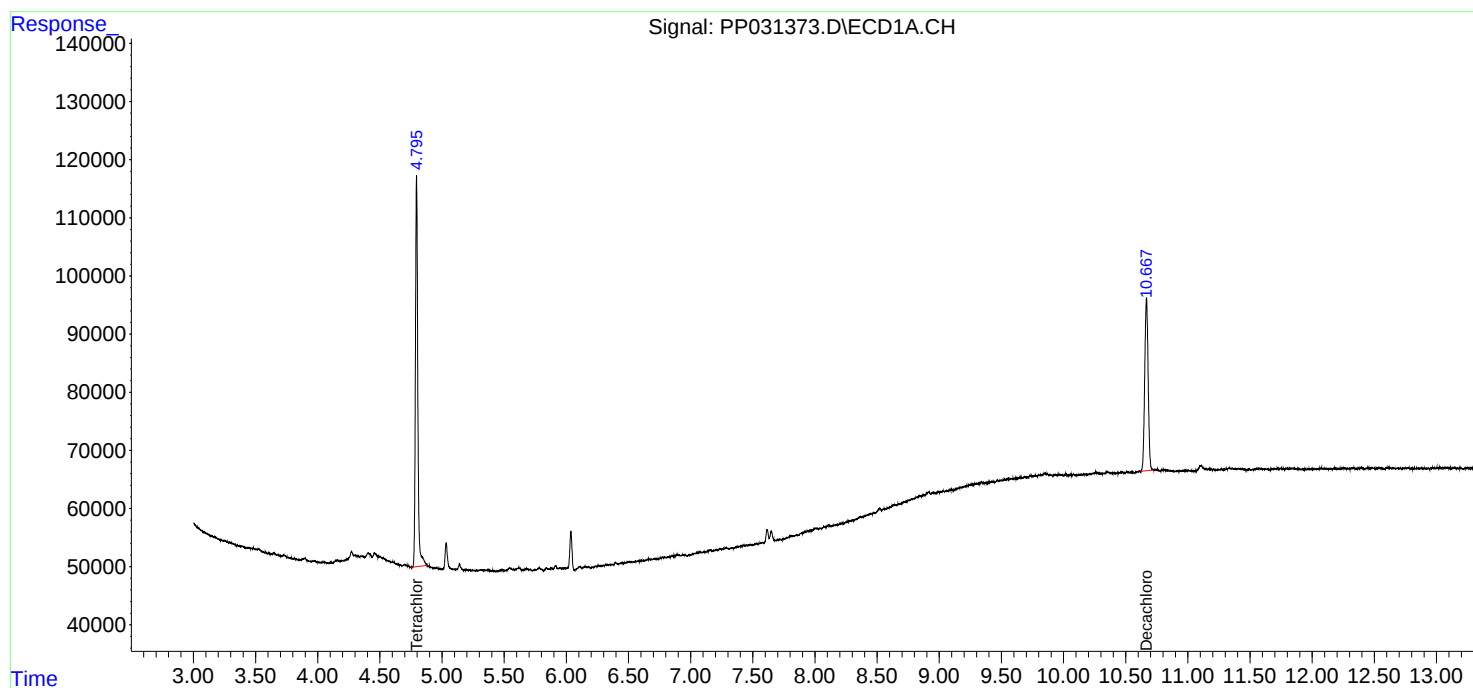


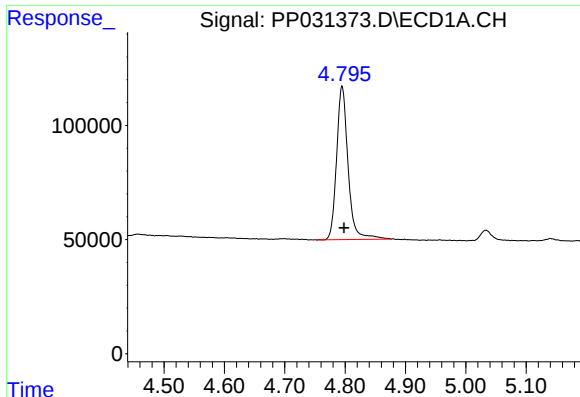

#1 Tetrachloro-m-xylene


R.T.: 4.795 min
Delta R.T.: -0.003 min
Response: 888505
Conc: 21.81 ng/ml

Instrument :
ECD_P
ClientSampleId :
CSIMW-1-20201117

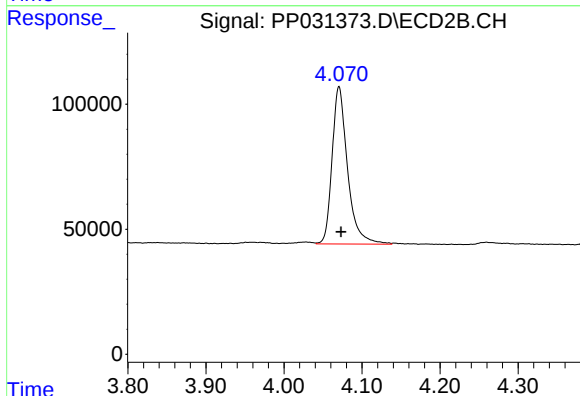


#1 Tetrachloro-m-xylene

R.T.: 4.071 min
Delta R.T.: -0.002 min
Response: 869165
Conc: 20.79 ng/ml

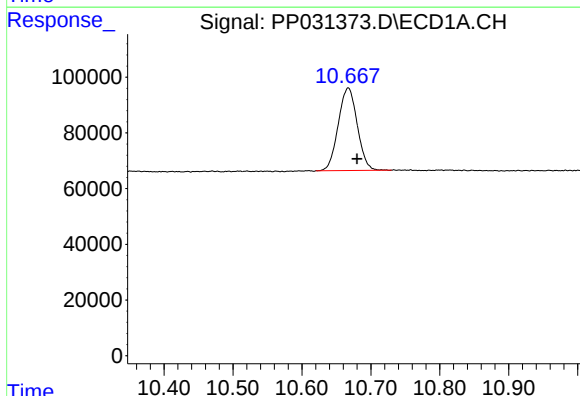

#2 Decachlorobiphenyl

R.T.: 10.667 min
Delta R.T.: -0.013 min
Response: 568083
Conc: 18.50 ng/ml

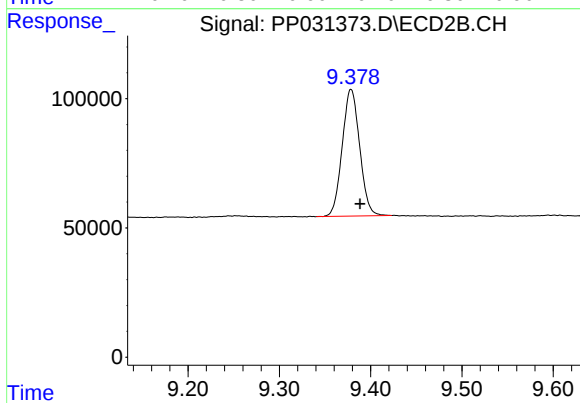

#2 Decachlorobiphenyl

R.T.: 9.378 min
Delta R.T.: -0.010 min
Response: 651979
Conc: 19.47 ng/ml