

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031392.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 00:31
Operator : DD\AJ
Sample : L4779-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
1641

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:08:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.795	4.070	205385	123747	5.041	2.960 #
2) SA Decachlor...	10.666	9.377	107377	191784	3.496	5.727 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111820\
Data File : PP031392.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 00:31
Operator : DD\AJ
Sample : L4779-02
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
1641

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:08:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

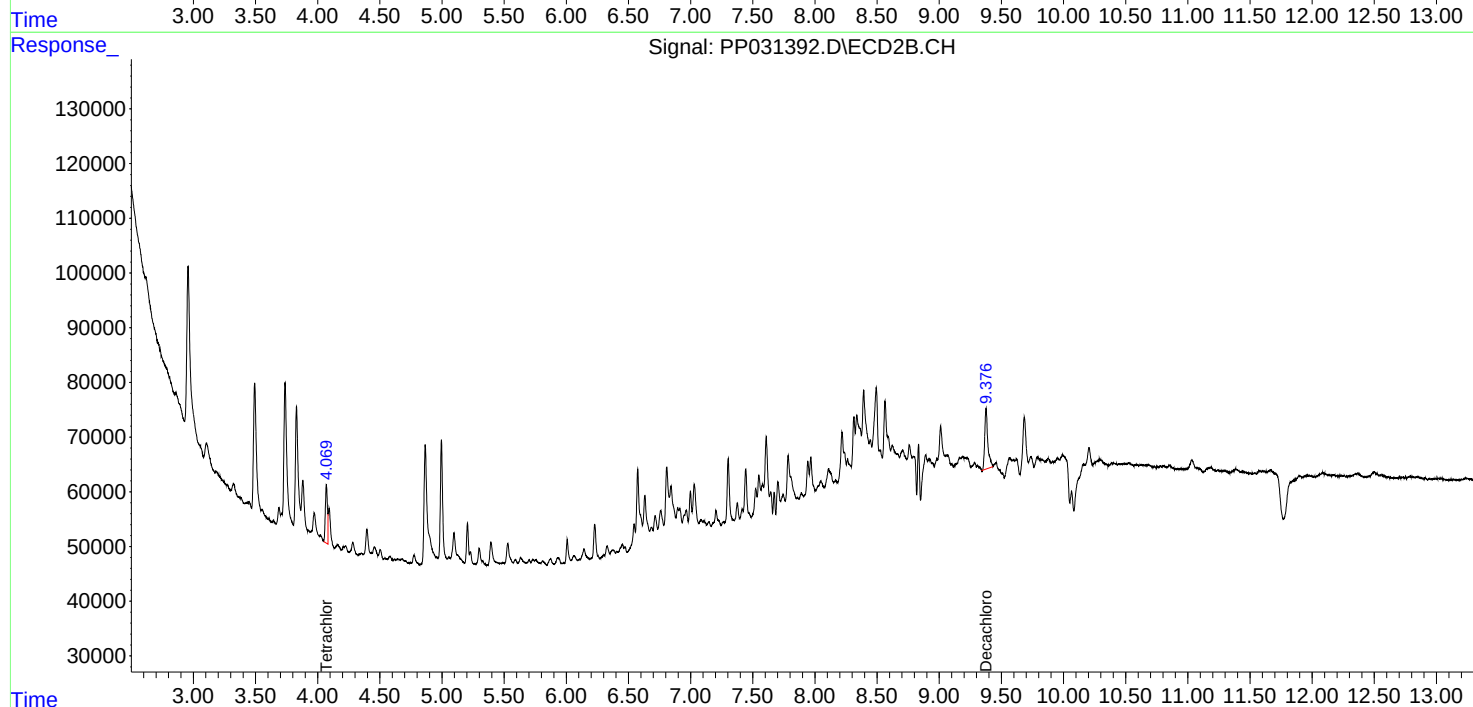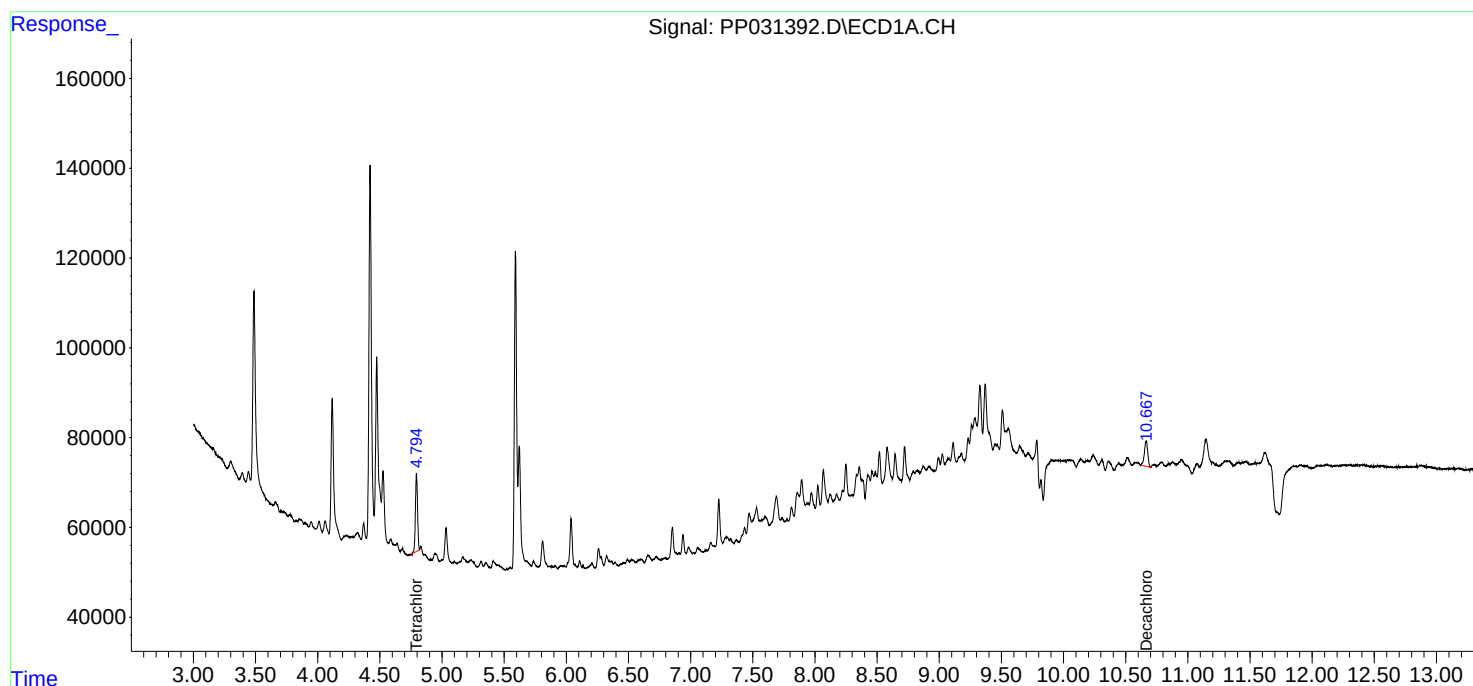


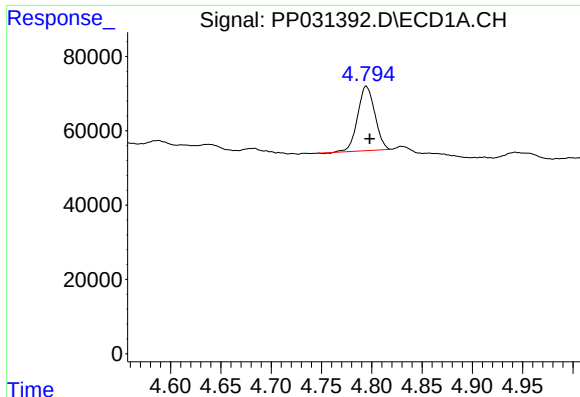

#1 Tetrachloro-m-xylene


R.T.: 4.795 min
Delta R.T.: -0.003 min
Response: 205385
Conc: 5.04 ng/ml

Instrument :
ECD_P
ClientSampleId :
1641

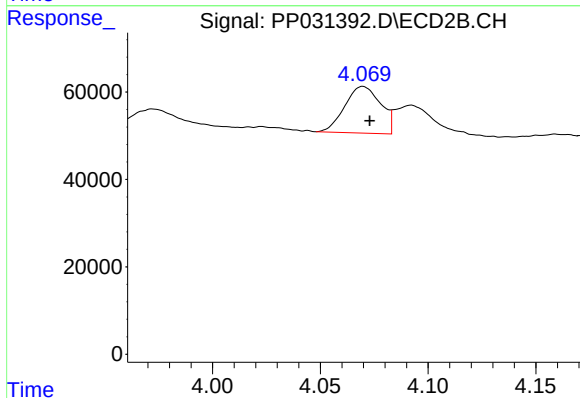


#1 Tetrachloro-m-xylene

R.T.: 4.070 min
Delta R.T.: -0.003 min
Response: 123747
Conc: 2.96 ng/ml

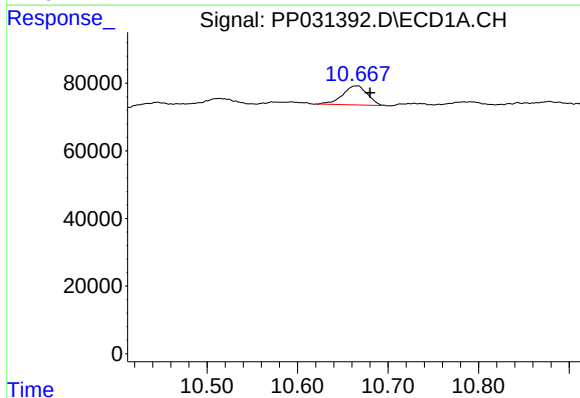

#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.014 min
Response: 107377
Conc: 3.50 ng/ml

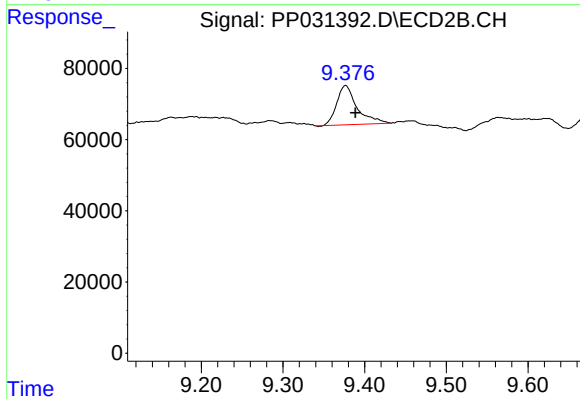

#2 Decachlorobiphenyl

R.T.: 9.377 min
Delta R.T.: -0.012 min
Response: 191784
Conc: 5.73 ng/ml