

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111821\
 Data File : PP041052.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 14:48
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 02:52:35 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.758	3.762	420852	610026	19.956	21.951
2) SA Decachlor...	10.660	9.025	460988	300937	21.104	20.993
Target Compounds						
9) L2 AR-1221-2	0.000	4.111	0	7755	N.D.	30.585 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111821\
Data File : PP041052.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 14:48
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 02:52:35 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

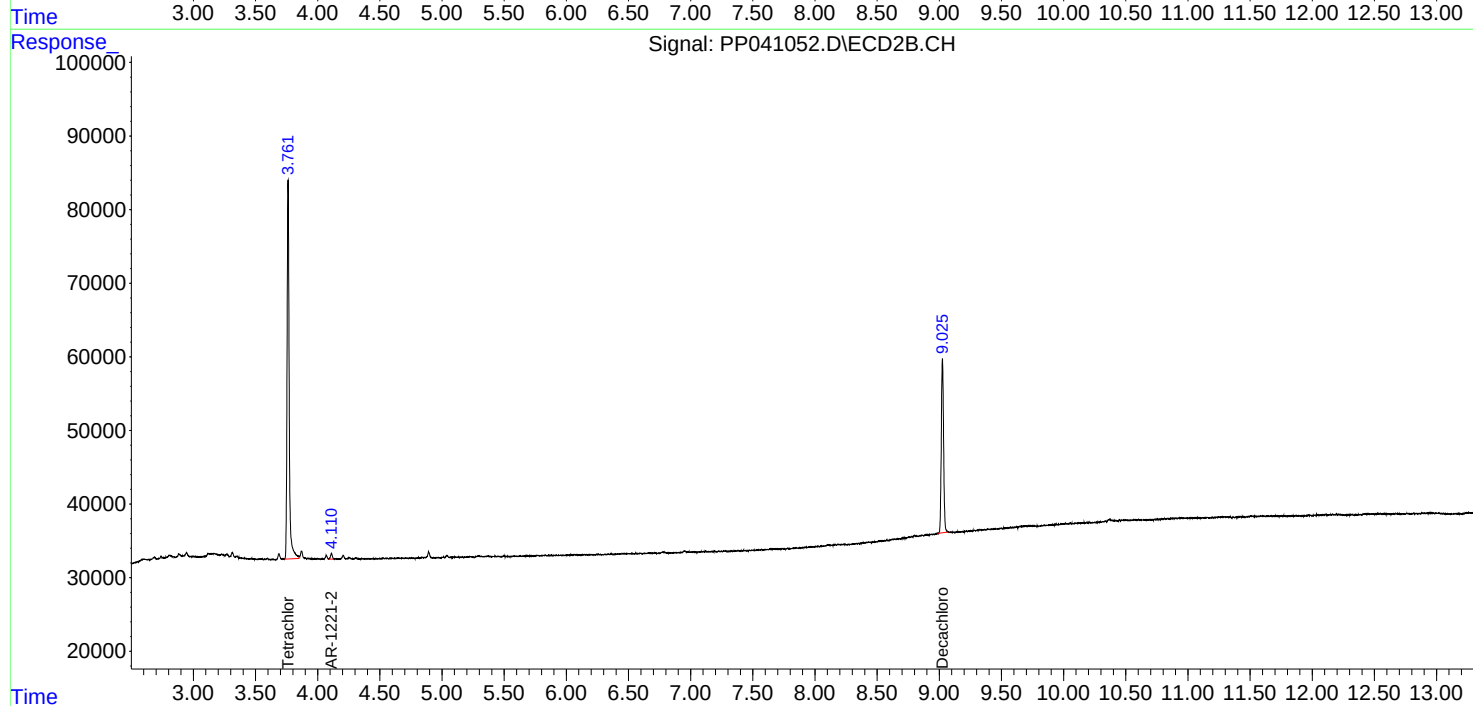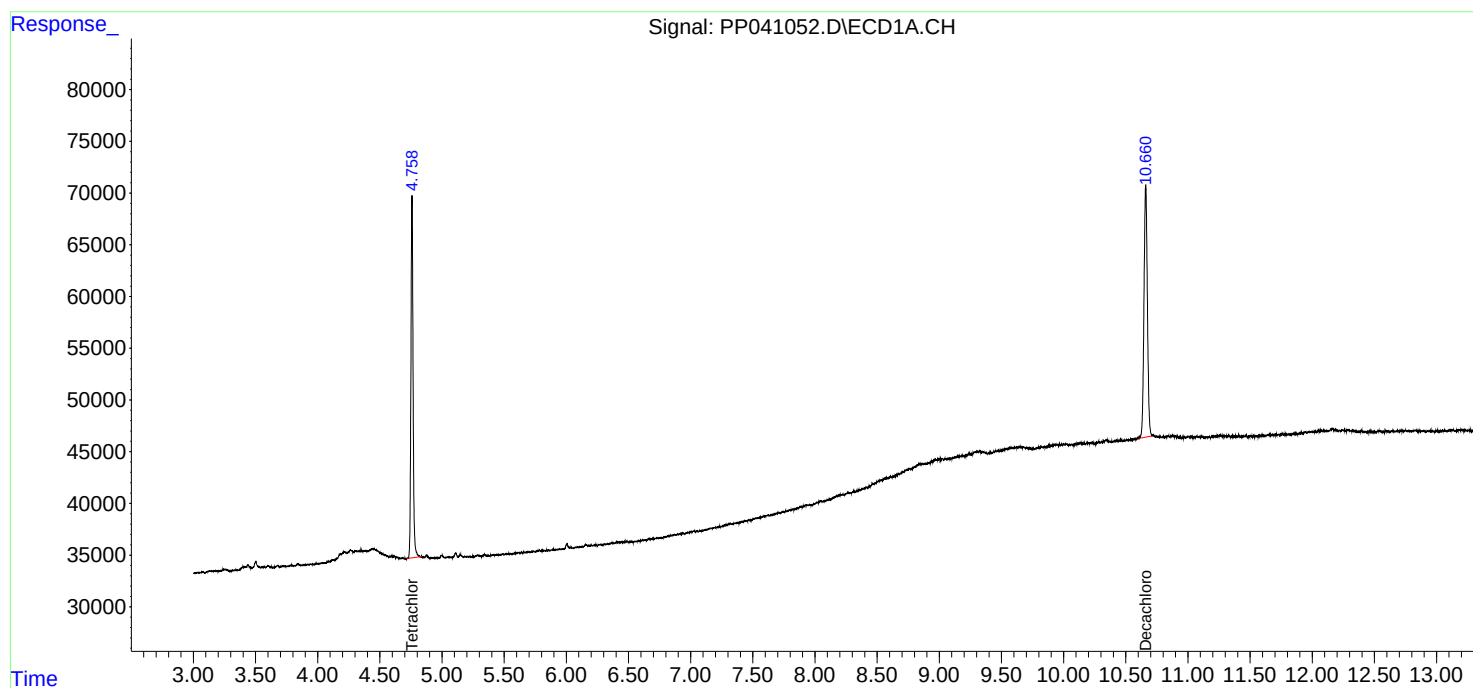


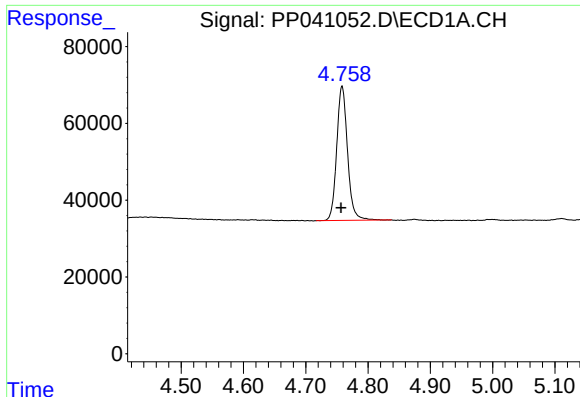

#1 Tetrachloro-m-xylene


R.T.: 4.758 min
Delta R.T.: 0.001 min
Response: 420852
Conc: 19.96 ng/ml

Instrument :
ECD_P
ClientSampleId :

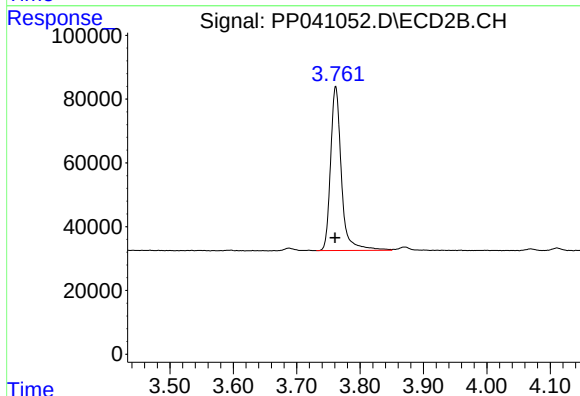


#1 Tetrachloro-m-xylene

R.T.: 3.762 min
Delta R.T.: 0.001 min
Response: 610026
Conc: 21.95 ng/ml

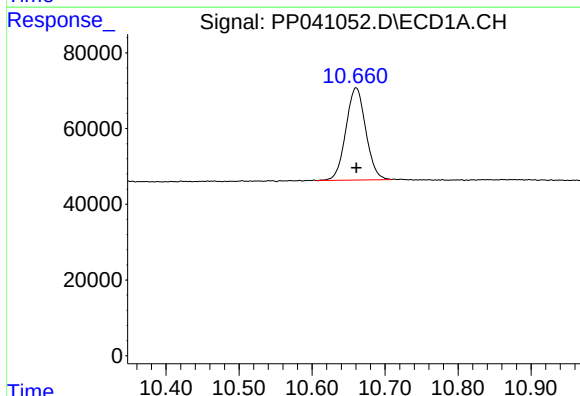


#2 Decachlorobiphenyl

R.T.: 10.660 min
Delta R.T.: 0.000 min
Response: 460988
Conc: 21.10 ng/ml

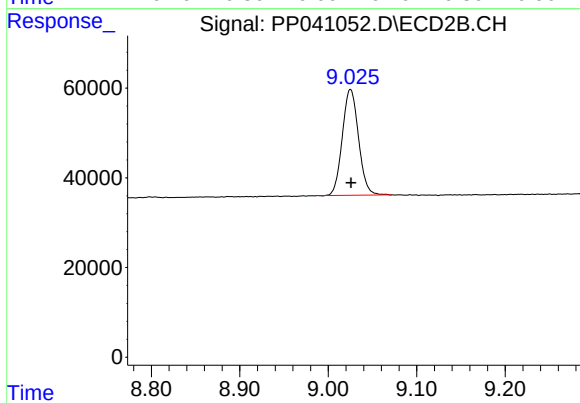

#2 Decachlorobiphenyl


R.T.: 9.025 min
Delta R.T.: 0.000 min
Response: 300937
Conc: 20.99 ng/ml

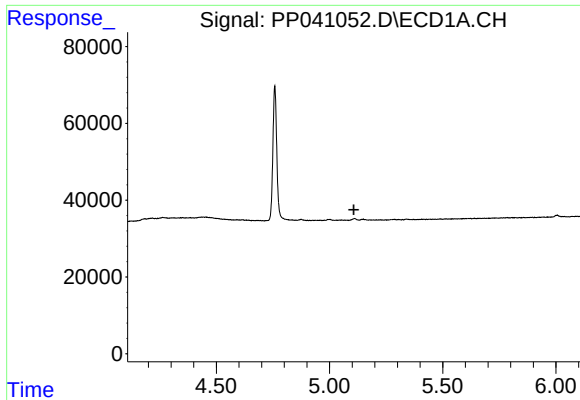

#9 AR-1221-2

R.T.: 0.000 min
Exp R.T.: 5.108 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :

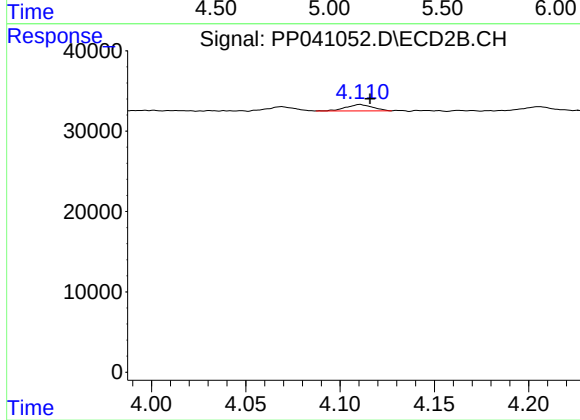

#9 AR-1221-2

R.T.: 4.111 min
Delta R.T.: -0.005 min
Response: 7755
Conc: 30.58 ng/ml