

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111821\
 Data File : PP041083.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Nov 2021 23:54
 Operator : AJ\MA
 Sample : M4737-05
 Misc :
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 COMP-2A-20916-21

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:03:31 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Tue Nov 16 04:45:00 2021
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.757	3.760	272781	408984	12.935m	14.717m
2)	SA Decachlor...	10.658	9.022	228591	204543	10.465m	14.269 #

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111821\
Data File : PP041083.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Nov 2021 23:54
Operator : AJ\MA
Sample : M4737-05
Misc :
ALS Vial : 27 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
COMP-2A-20916-21

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:03:31 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111521.M
Quant Title : GC EXTRACTABLES
QLast Update : Tue Nov 16 04:45:00 2021
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

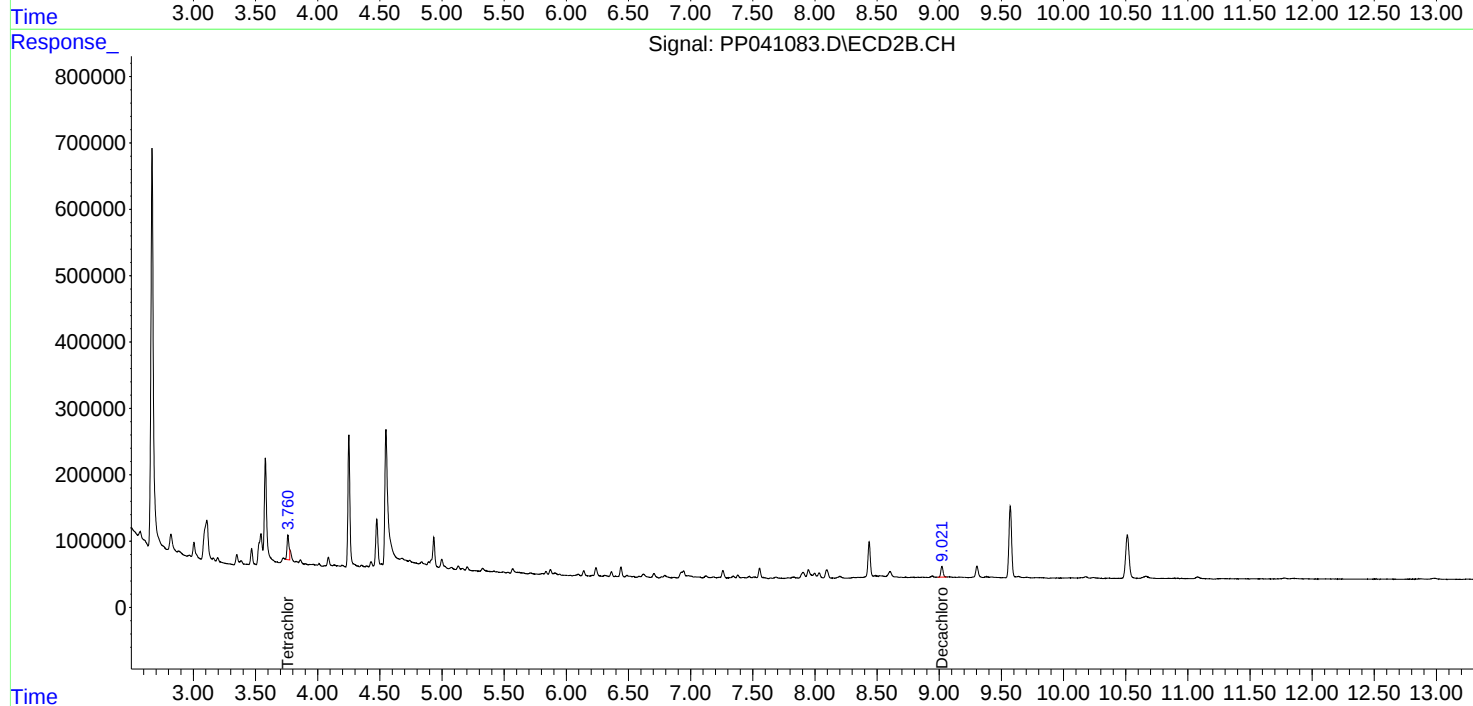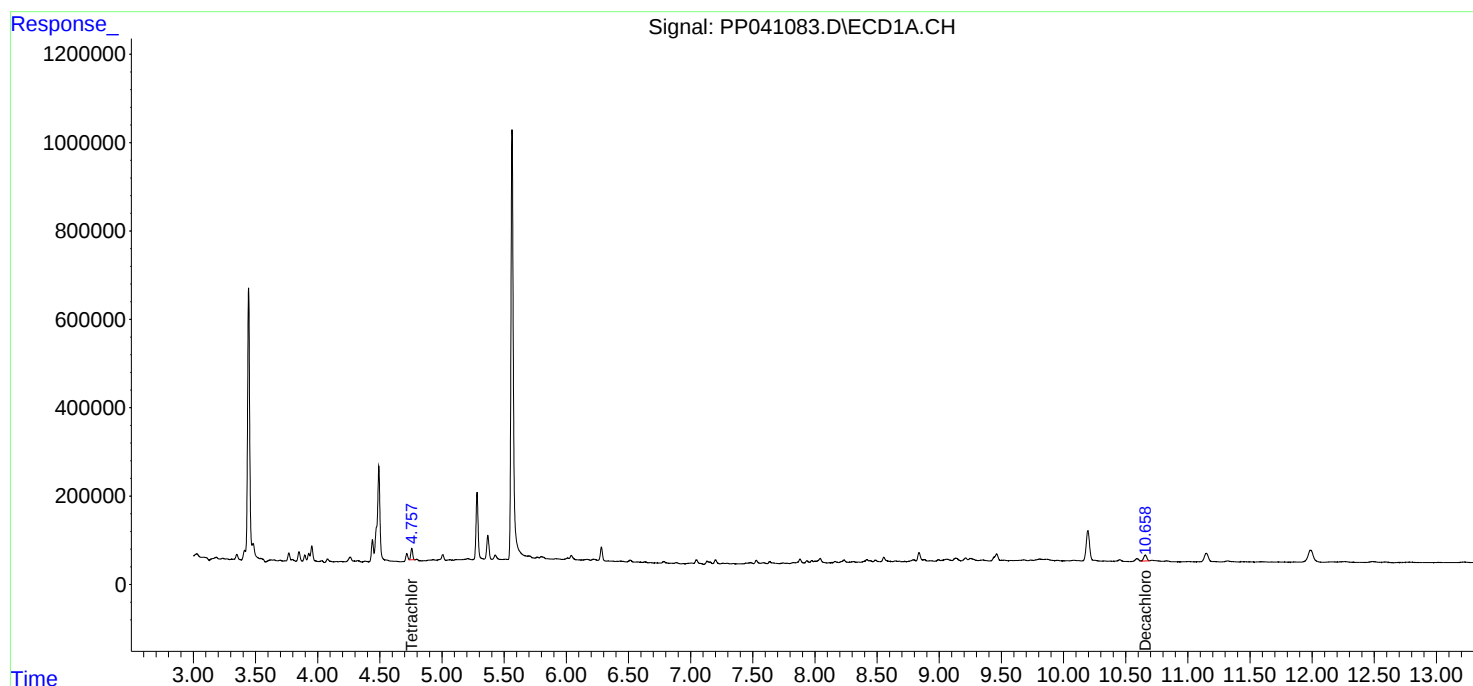


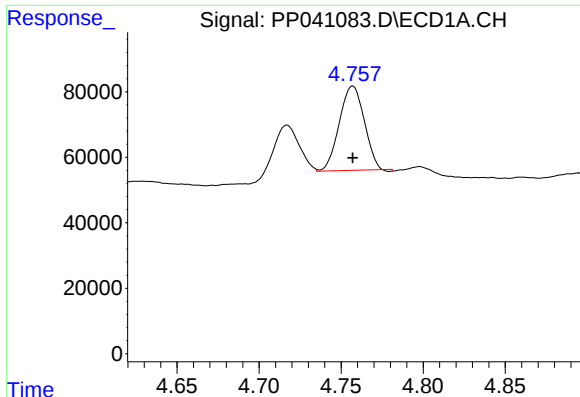

#1 Tetrachloro-m-xylene


R.T.: 4.757 min
Delta R.T.: 0.000 min
Response: 272781
Conc: 12.93 ng/ml

Instrument :
ECD_P
ClientSampleId :
COMP-2A-20916-21

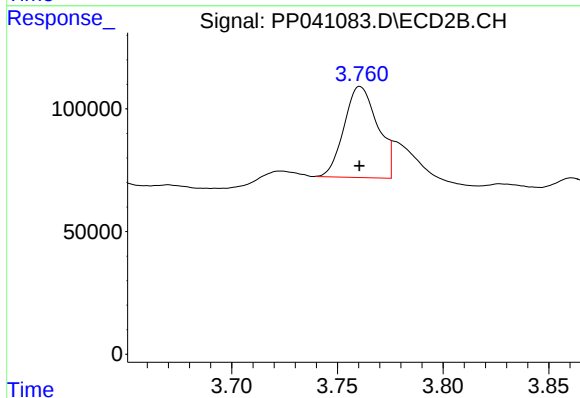


#1 Tetrachloro-m-xylene

R.T.: 3.760 min
Delta R.T.: 0.000 min
Response: 408984
Conc: 14.72 ng/ml m

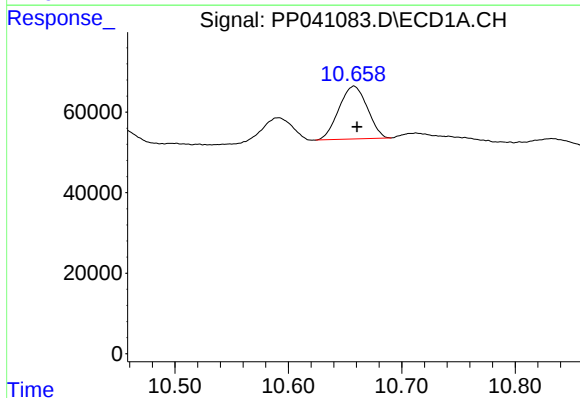

#2 Decachlorobiphenyl

R.T.: 10.658 min
Delta R.T.: -0.003 min
Response: 228591
Conc: 10.46 ng/ml m

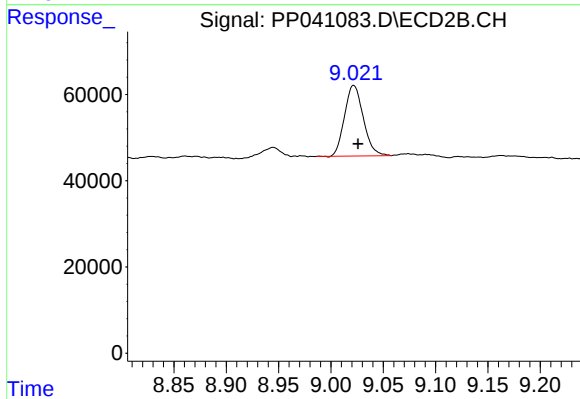

#2 Decachlorobiphenyl

R.T.: 9.022 min
Delta R.T.: -0.004 min
Response: 204543
Conc: 14.27 ng/ml