

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111822\
 Data File : PP053379.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 16:27
 Operator : YP\AJ
 Sample : N5670-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 1-DRUM

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2022
 Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 00:52:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.400	3.645	10565439	10398515	5.496m	6.913m#
2) SA Decachlor...	10.202	8.726	25711765	30543447	18.962	16.295

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111822\
Data File : PP053379.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 16:27
Operator : YP\AJ
Sample : N5670-01
Misc :
ALS Vial : 15 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
1-DRUM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 00:52:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

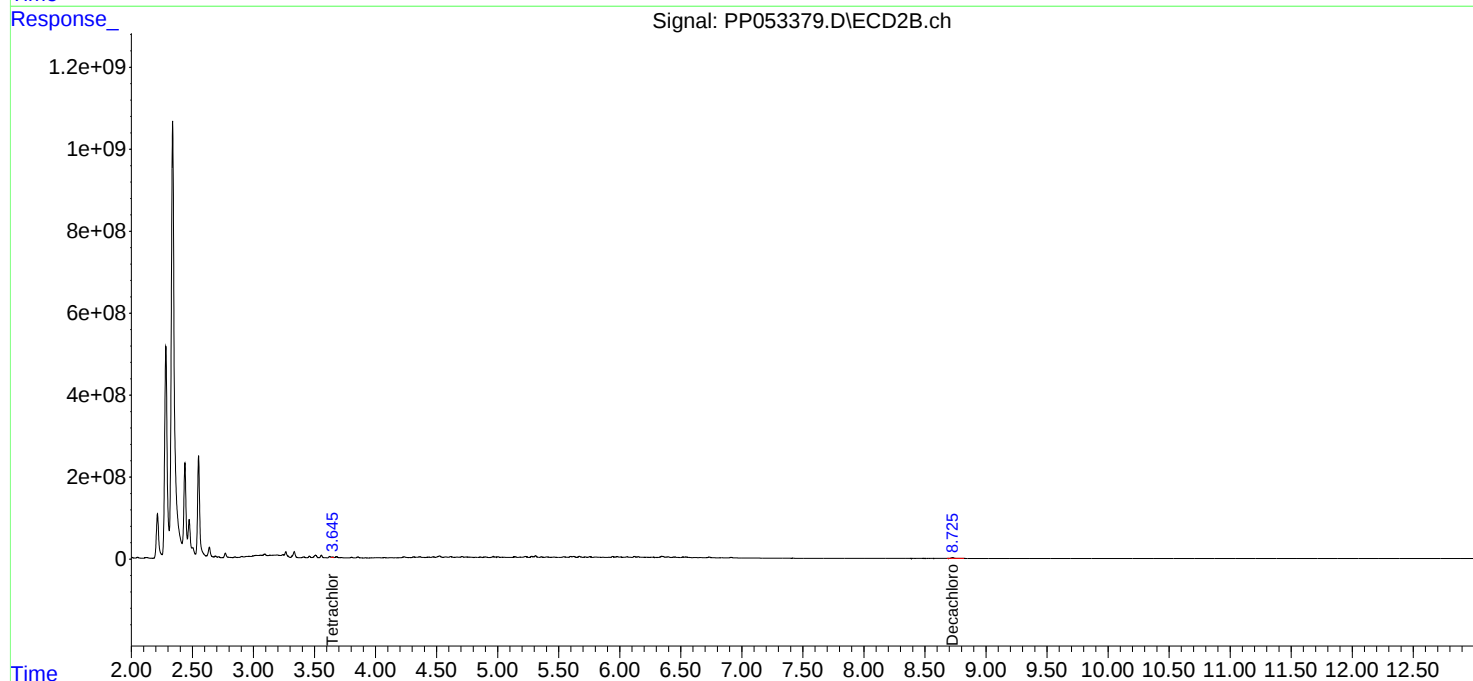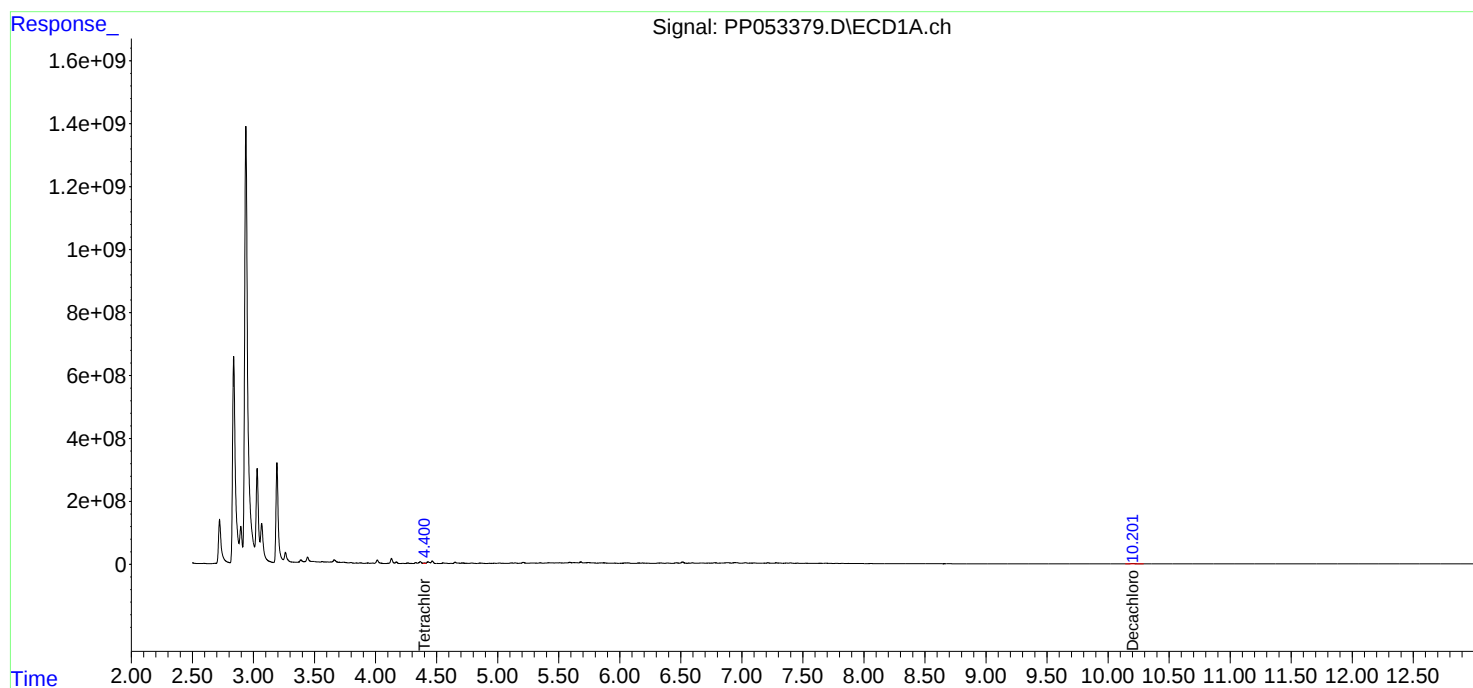

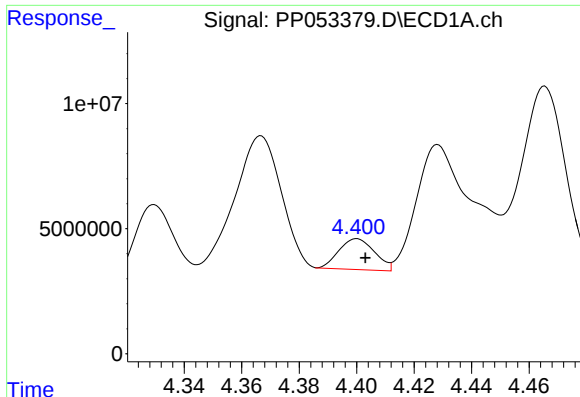


#1 Tetrachloro-m-xylene

R.T.: 4.400 min
Delta R.T.: -0.003 min
Response: 10565439
Conc: 5.50 ng/ml

Instrument :
ECD_P
ClientSampleId :
1-DRUM


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

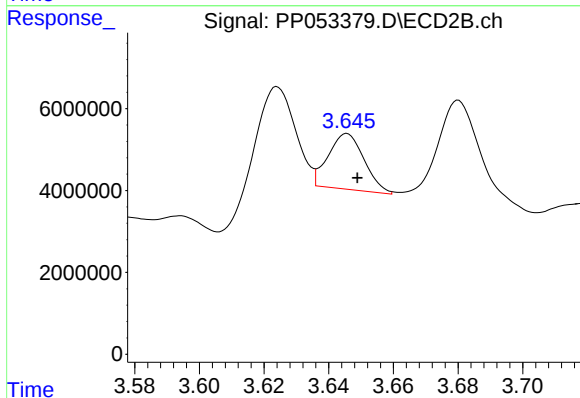


#1 Tetrachloro-m-xylene

R.T.: 3.645 min
Delta R.T.: -0.004 min
Response: 10398515
Conc: 6.91 ng/ml m

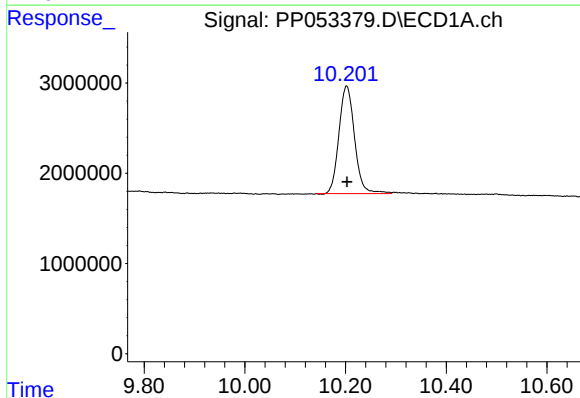

#2 Decachlorobiphenyl

R.T.: 10.202 min
Delta R.T.: 0.000 min
Response: 25711765
Conc: 18.96 ng/ml

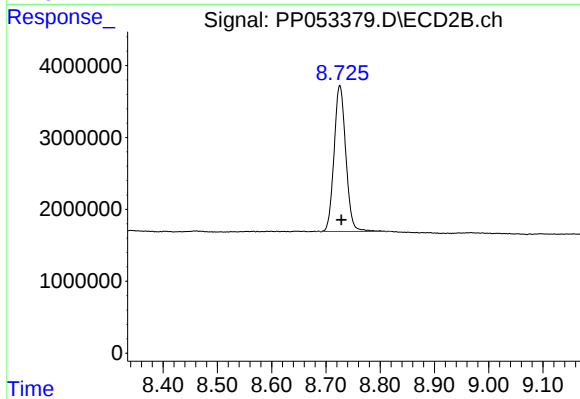

#2 Decachlorobiphenyl

R.T.: 8.726 min
Delta R.T.: -0.003 min
Response: 30543447
Conc: 16.30 ng/ml