

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111822\
 Data File : PP053389.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2022 19:43
 Operator : YP\AJ
 Sample : N5655-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 SEMI-ANNUAL-CONDENSATE

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/21/2022
 Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 01:02:19 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 09 05:50:05 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.399	3.650	20791856	47933197	10.816m	31.865m#
2) SA Decachlor...	10.201	8.723	11791524	20234568	8.696	10.795

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111822\
Data File : PP053389.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2022 19:43
Operator : YP\AJ
Sample : N5655-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 01:02:19 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110822.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 09 05:50:05 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

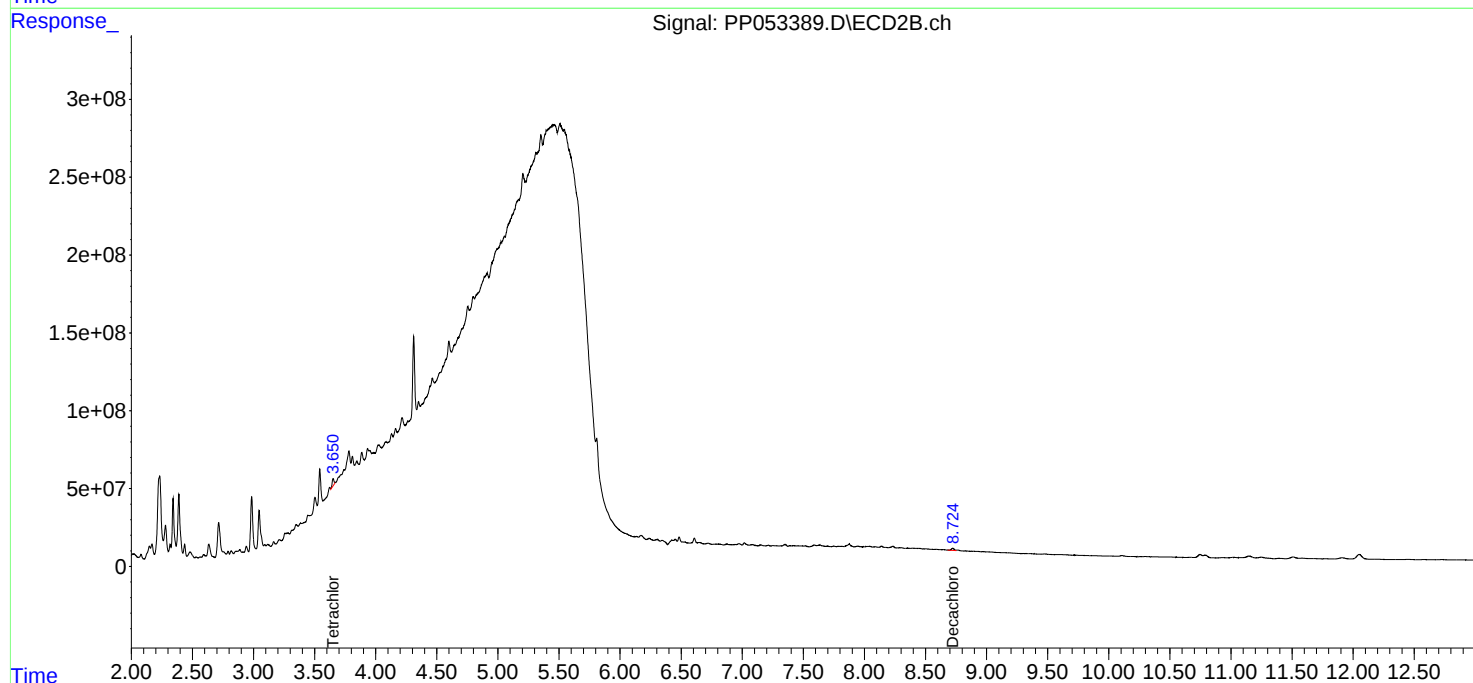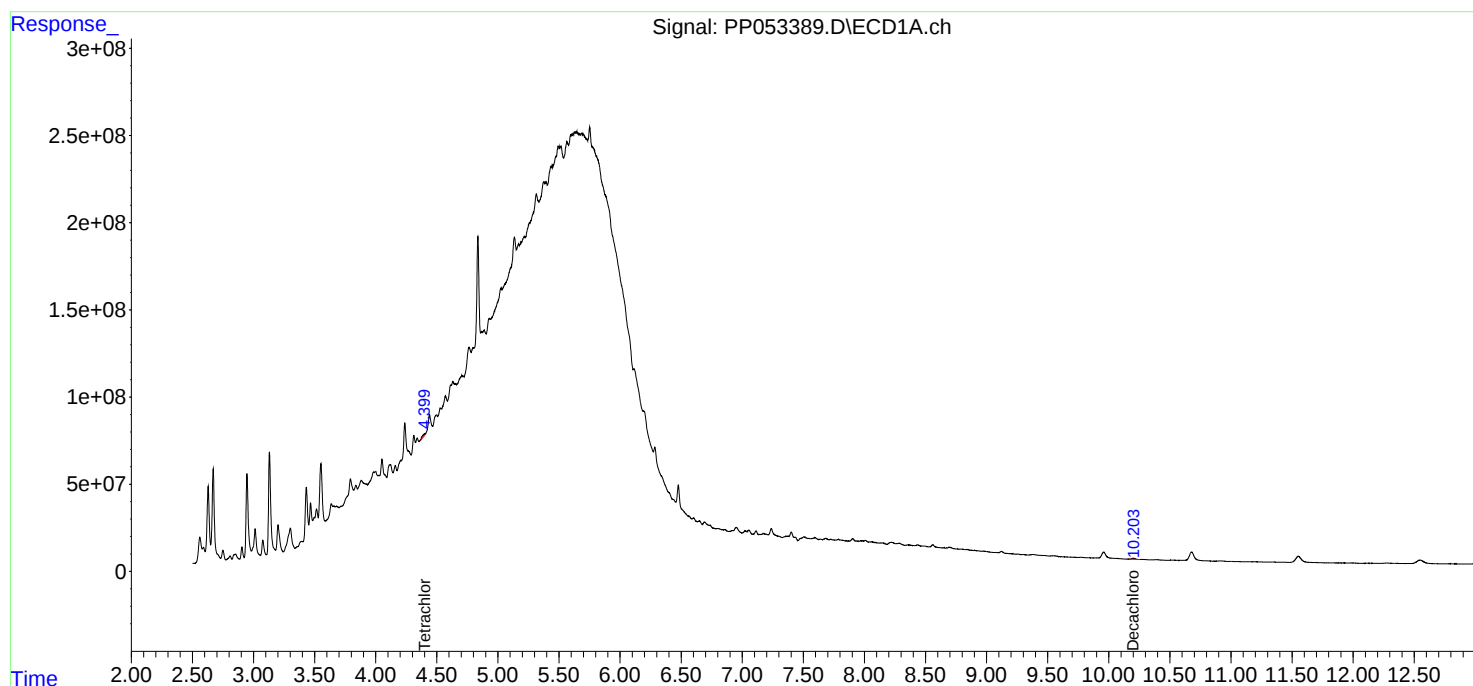

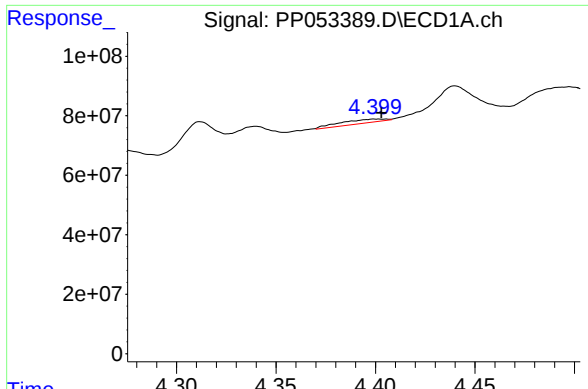


#1 Tetrachloro-m-xylene

R.T.: 4.399 min
Delta R.T.: -0.004 min
Response: 20791856
Conc: 10.82 ng/ml

Instrument :
ECD_P
ClientSampleId :
SEMI-ANNUAL-CONDENSATE


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/21/2022
Supervised By :Ankita Jodhani 11/21/2022

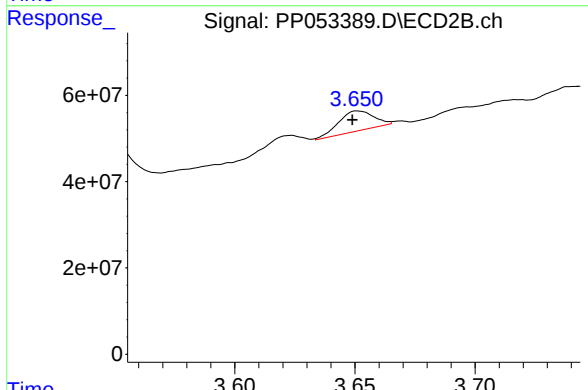


#1 Tetrachloro-m-xylene

R.T.: 3.650 min
Delta R.T.: 0.000 min
Response: 47933197
Conc: 31.87 ng/ml m

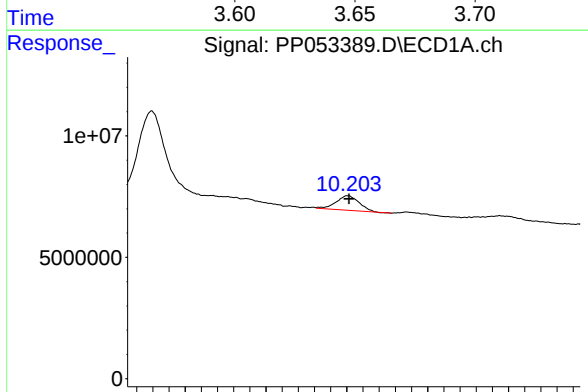

#2 Decachlorobiphenyl

R.T.: 10.201 min
Delta R.T.: -0.002 min
Response: 11791524
Conc: 8.70 ng/ml

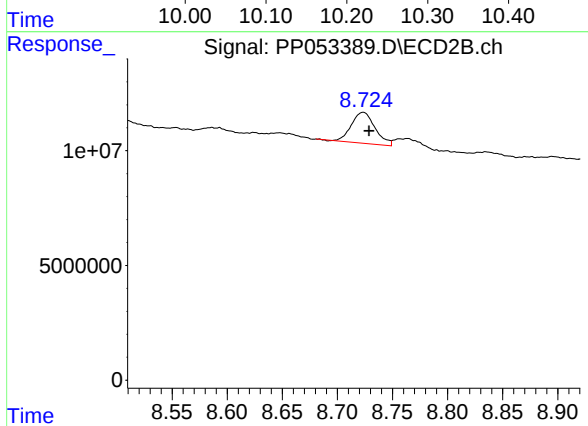

#2 Decachlorobiphenyl

R.T.: 8.723 min
Delta R.T.: -0.005 min
Response: 20234568
Conc: 10.80 ng/ml