

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
 Data File : PP068561.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Nov 2024 18:58
 Operator : YP\AJ
 Sample : P4862-01 10X
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 Y2404-0033-END-1-1

Manual Integrations
 APPROVED

Reviewed By :Yogesh Patel 11/19/2024
 Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 03:38:16 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.759	4.051	1663907	1595248	1.714m	1.647m
2) SA Decachlor...	10.675	9.208	2405195	1938186	1.922m	1.713m

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
Data File : PP068561.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Nov 2024 18:58
Operator : YP\AJ
Sample : P4862-01 10X
Misc :
ALS Vial : 29 Sample Multiplier: 1



Instrument :
ECD_P
ClientSampleId :
Y2404-0033-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 03:38:16 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

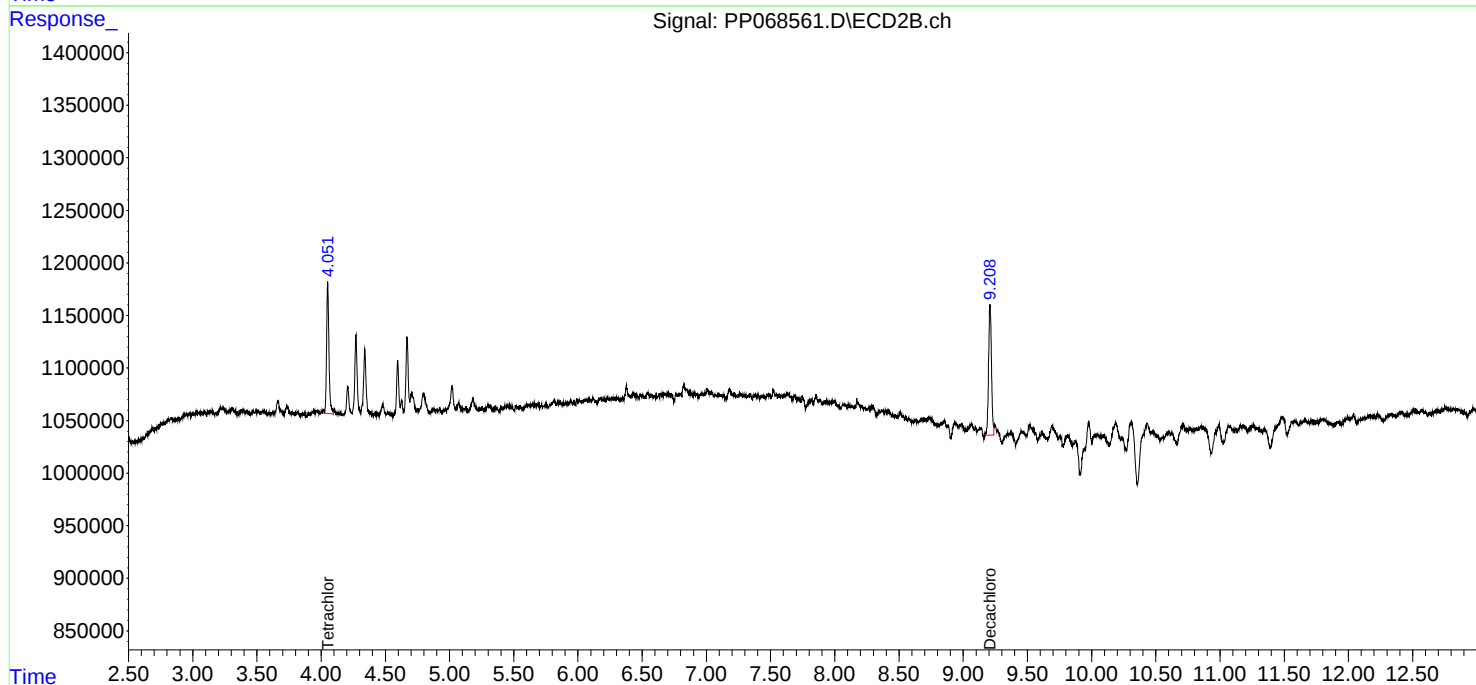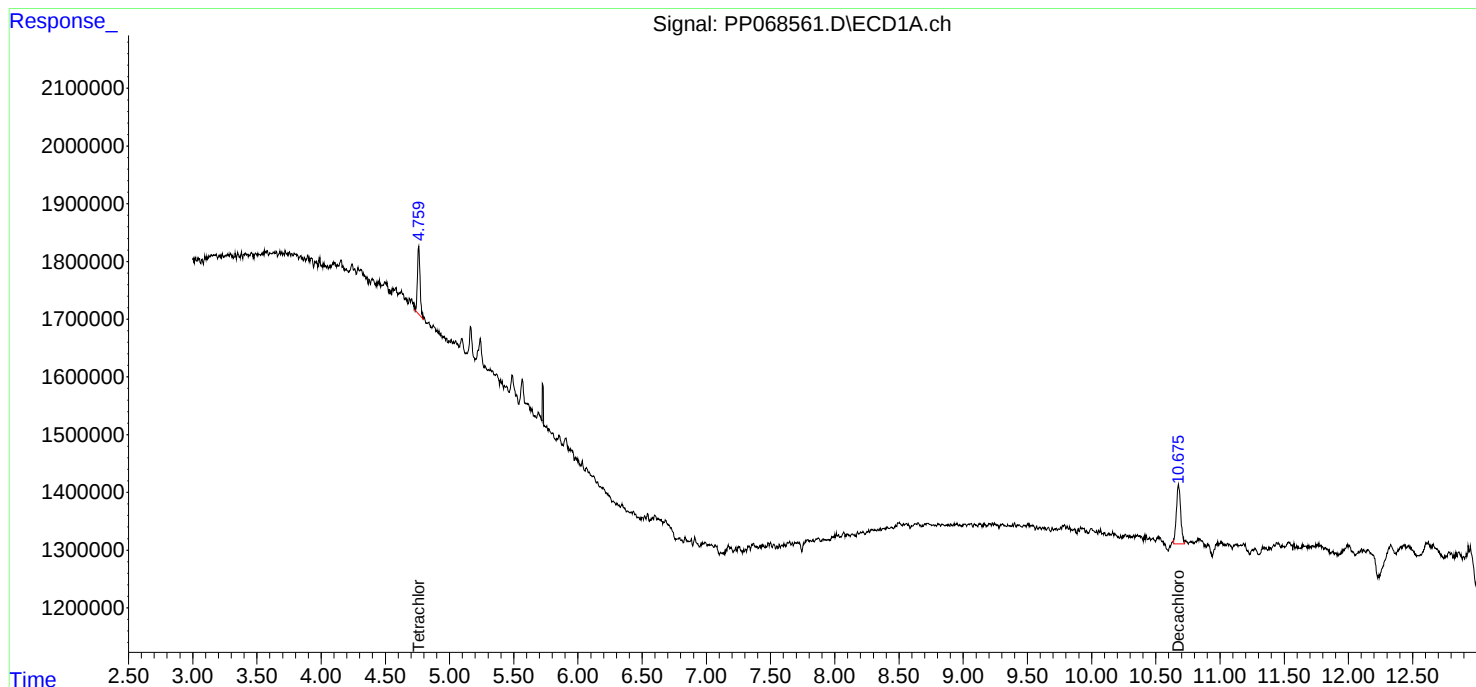

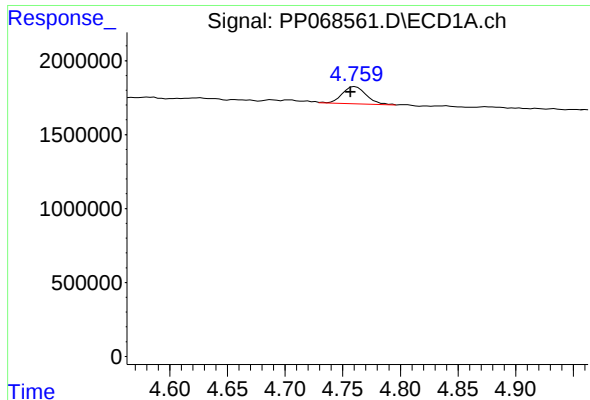


#1 Tetrachloro-m-xylene

R.T.: 4.759 min
Delta R.T.: 0.002 min
Response: 1663907
Conc: 1.71 ng/ml

Instrument : ECD_P
ClientSampleId : Y2404-0033-END-1-1


Manual Integrations
APPROVED

Reviewed By :Yogesh Patel 11/19/2024
Supervised By :Ankita Jodhani 11/19/2024

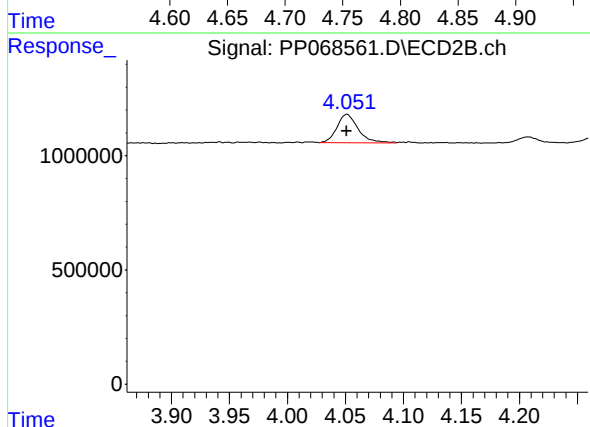


#1 Tetrachloro-m-xylene

R.T.: 4.051 min
Delta R.T.: 0.000 min
Response: 1595248
Conc: 1.65 ng/ml

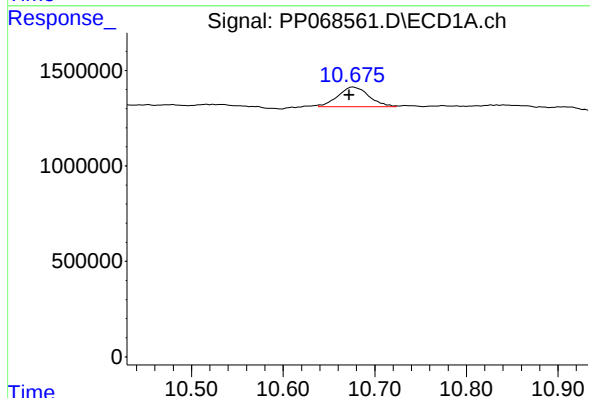

#2 Decachlorobiphenyl

R.T.: 10.675 min
Delta R.T.: 0.003 min
Response: 2405195
Conc: 1.92 ng/ml

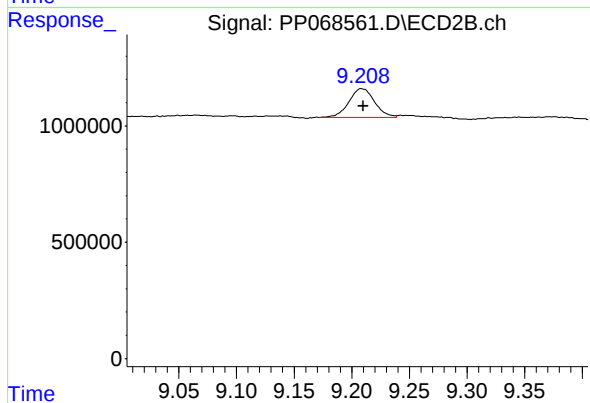

#2 Decachlorobiphenyl

R.T.: 9.208 min
Delta R.T.: -0.002 min
Response: 1938186
Conc: 1.71 ng/ml