

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
Data File : PP068579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 04:24
Operator : YP\AJ
Sample : PB165038BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB165038BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:11:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

1) SA Tetrachlo...	4.757	4.049	17860276	18764666	18.401	19.379
2) SA Decachlor...	10.672	9.206	21773851	20514900	17.398	18.136

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
Data File : PP068579.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 04:24
Operator : YP\AJ
Sample : PB165038BL
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
PB165038BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:11:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

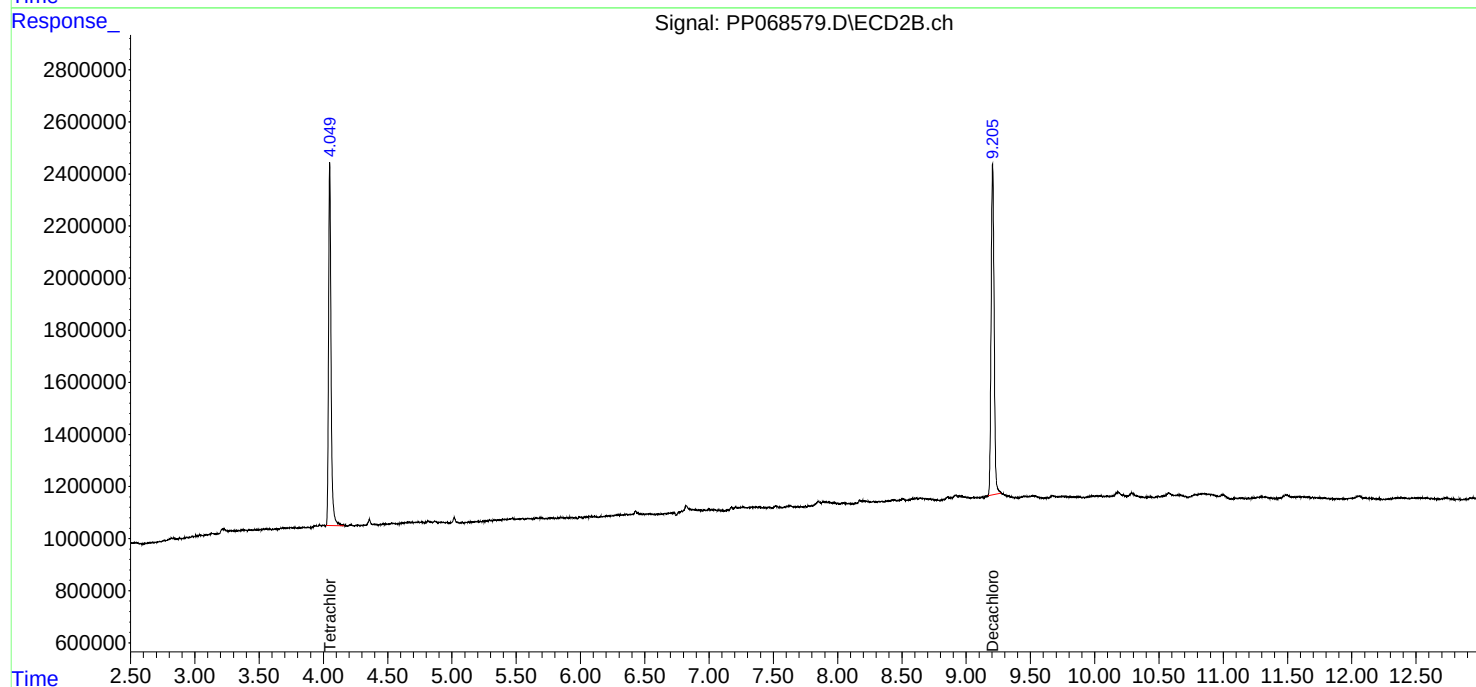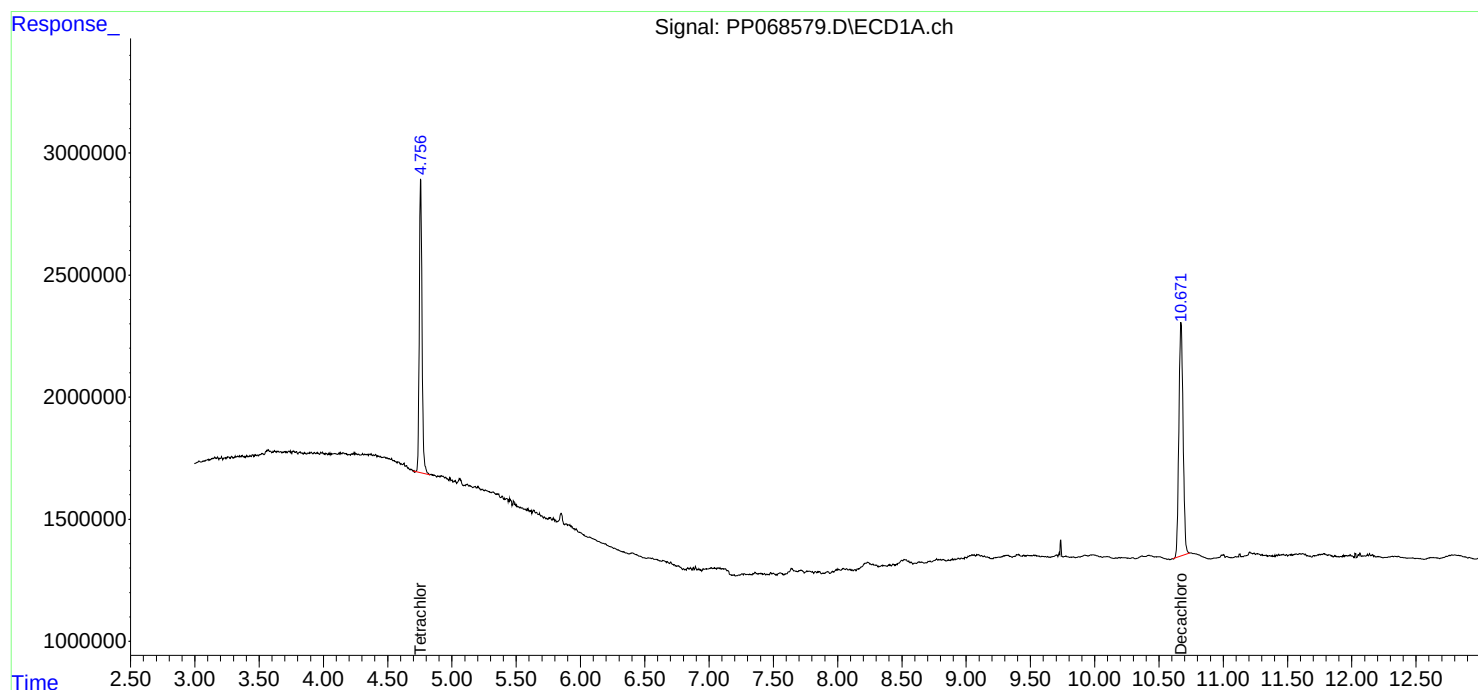


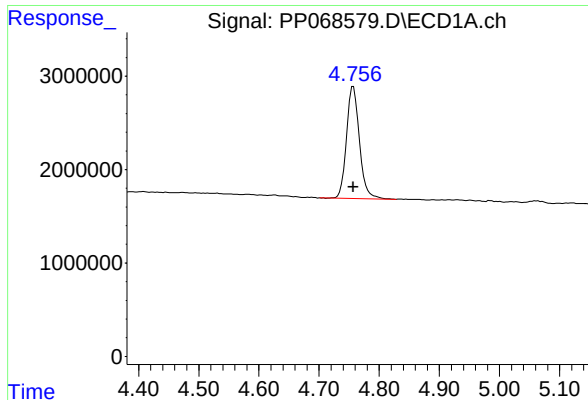

#1 Tetrachloro-m-xylene


R.T.: 4.757 min
Delta R.T.: 0.000 min
Response: 17860276
Conc: 18.40 ng/ml

Instrument :
ECD_P
ClientSampleId :
PB165038BL

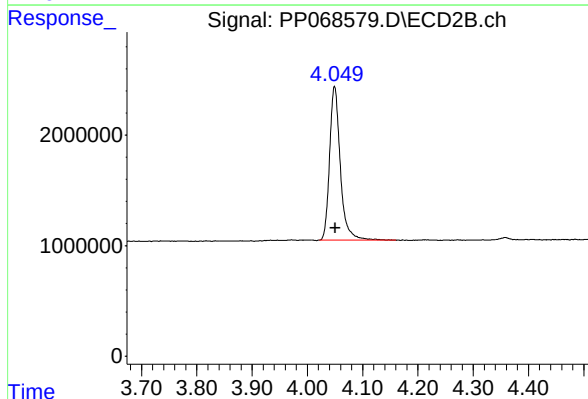


#1 Tetrachloro-m-xylene

R.T.: 4.049 min
Delta R.T.: -0.002 min
Response: 18764666
Conc: 19.38 ng/ml

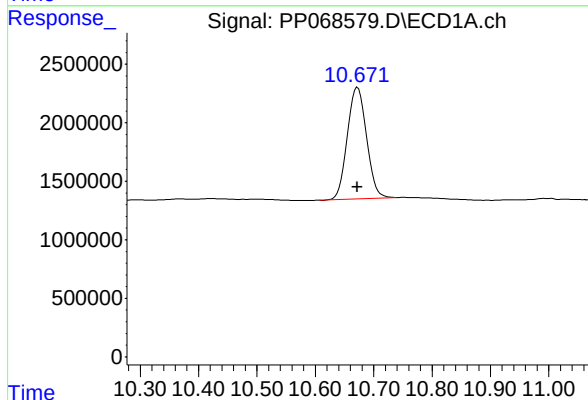

#2 Decachlorobiphenyl

R.T.: 10.672 min
Delta R.T.: 0.000 min
Response: 21773851
Conc: 17.40 ng/ml

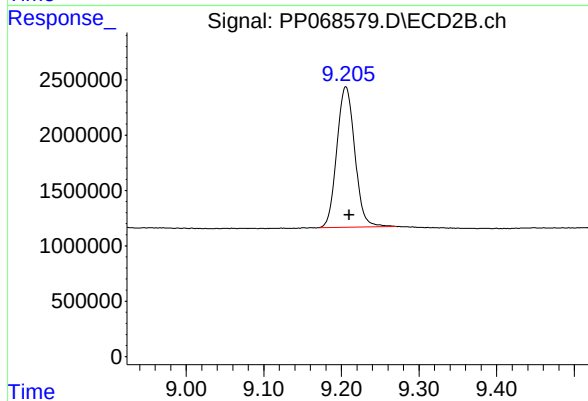

#2 Decachlorobiphenyl

R.T.: 9.206 min
Delta R.T.: -0.004 min
Response: 20514900
Conc: 18.14 ng/ml