

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
 Data File : PP068582.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Nov 2024 05:13
 Operator : YP\AJ
 Sample : P4864-01
 Misc :
 ALS Vial : 45 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 MONTCLAIR-TOTE-2

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 06:12:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Fri Nov 08 11:04:08 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	4.761	4.052	18059693	18832545	18.607	19.449
2) SA Decachlor...	10.677	9.207	22242579	20451569	17.773	18.080

Target Compounds



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111824\
Data File : PP068582.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Nov 2024 05:13
Operator : YP\AJ
Sample : P4864-01
Misc :
ALS Vial : 45 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
MONTCLAIR-TOTE-2

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 06:12:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP110724.M
Quant Title : GC EXTRACTABLES
QLast Update : Fri Nov 08 11:04:08 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µm Signal #2 Info : 30M x 0.32mm x 0.25µm

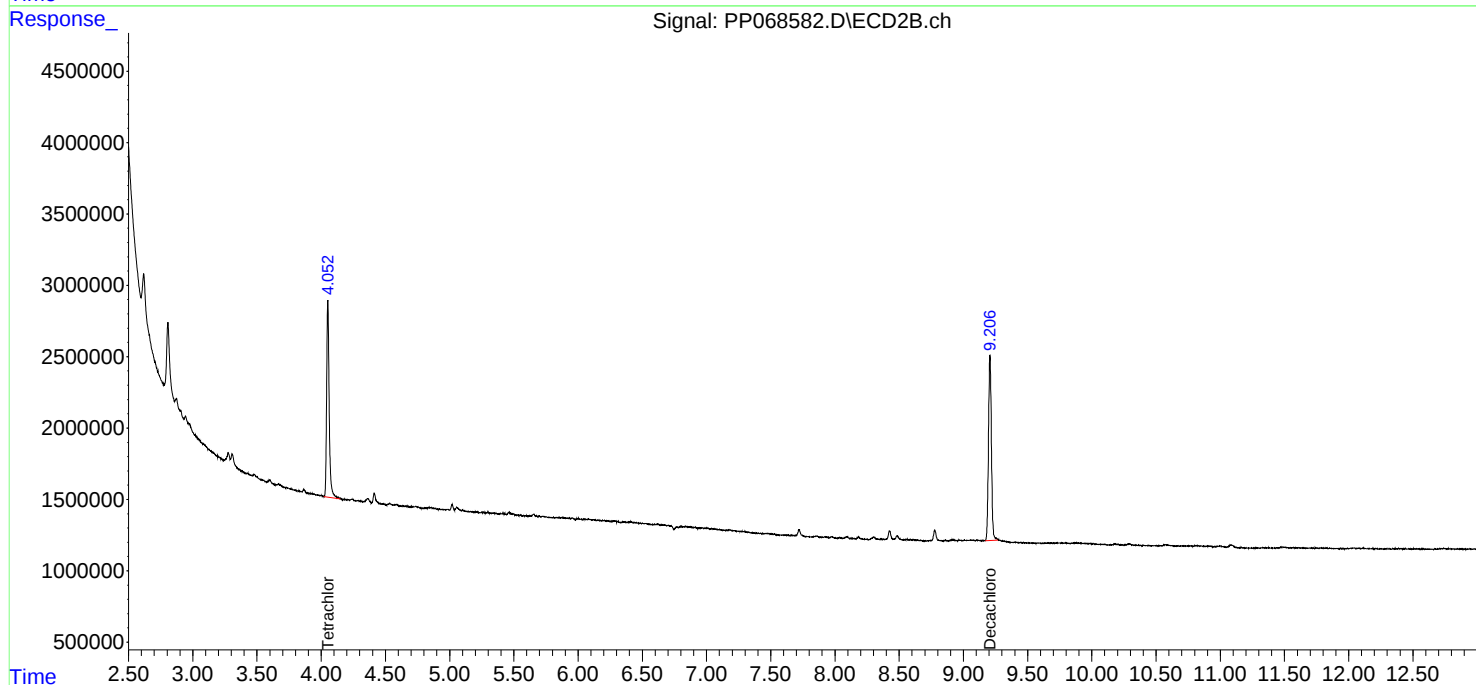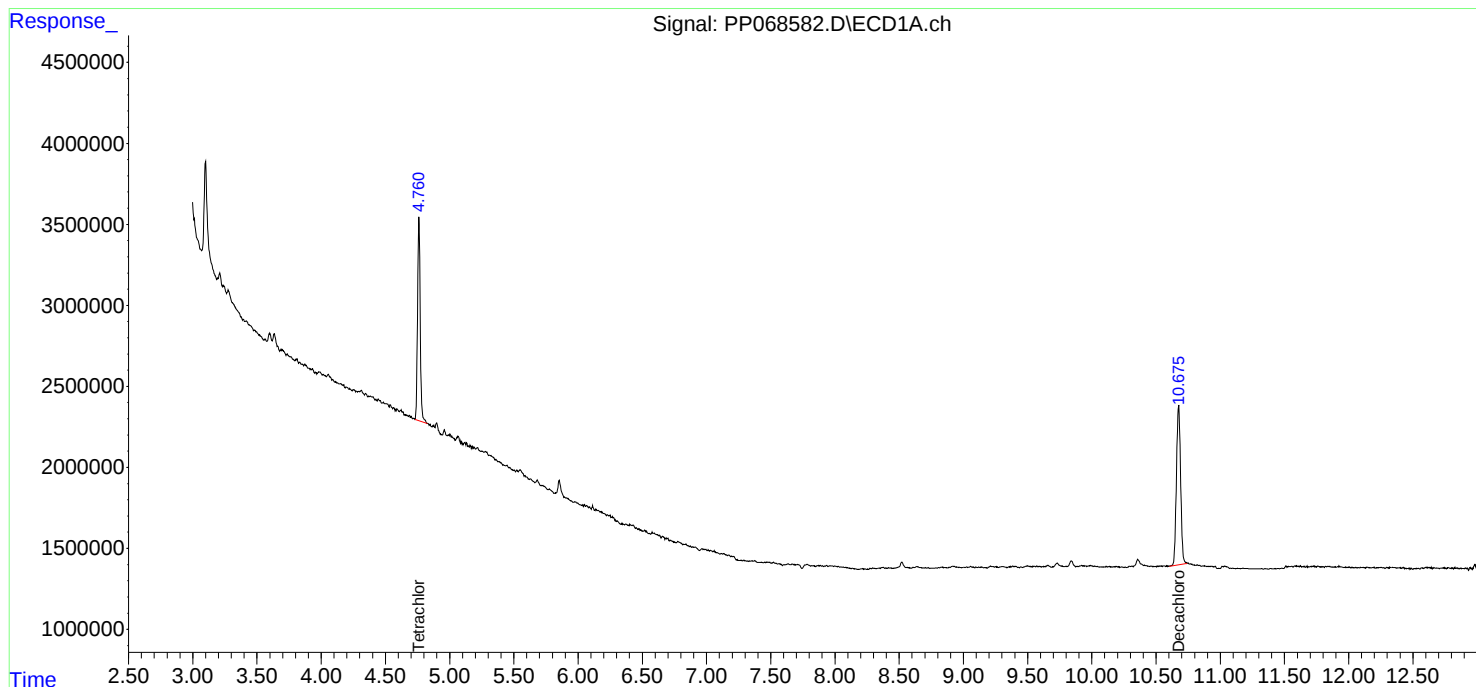


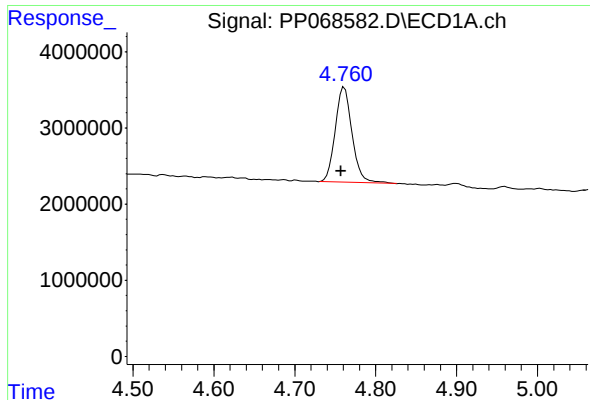

#1 Tetrachloro-m-xylene


R.T.: 4.761 min
Delta R.T.: 0.004 min
Response: 18059693
Conc: 18.61 ng/ml

Instrument :
ECD_P
ClientSampleId :
MONTCLAIR-TOTE-2

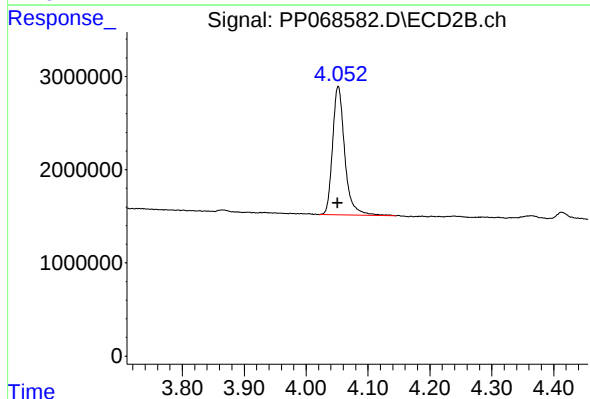


#1 Tetrachloro-m-xylene

R.T.: 4.052 min
Delta R.T.: 0.000 min
Response: 18832545
Conc: 19.45 ng/ml

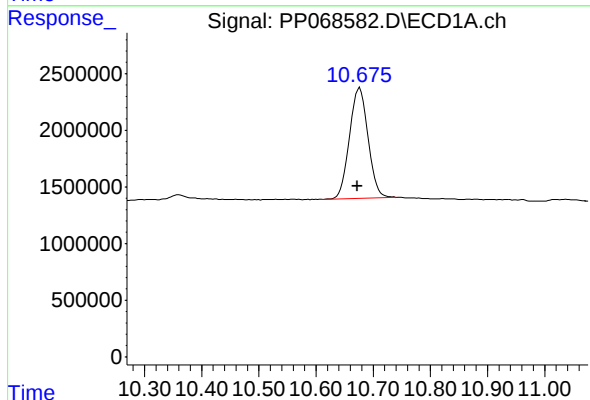

#2 Decachlorobiphenyl

R.T.: 10.677 min
Delta R.T.: 0.005 min
Response: 22242579
Conc: 17.77 ng/ml

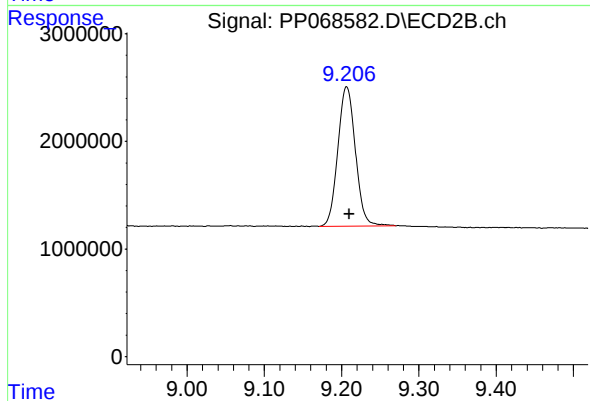

#2 Decachlorobiphenyl

R.T.: 9.207 min
Delta R.T.: -0.003 min
Response: 20451569
Conc: 18.08 ng/ml