

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031418.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 15:05
 Operator : DD\AJ
 Sample : L4804-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-04-012-ABCD

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 17:36:56 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.793	4.066	958534	928781	23.529	22.215
2)	SA Decachlor...	10.666	9.374	617448	709857	20.103	21.199
Target Compounds							
7)	L1 AR-1016-5	0.000	5.802f	0	9617	N.D.	9.894 #
8)	L2 AR-1221-1	5.031	0.000	62449	0	133.024	N.D. #
9)	L2 AR-1221-2	0.000	4.417	0	17645	N.D.	49.968 #
15)	L3 AR-1232-5	0.000	5.802f	0	9617	N.D.	24.164 #
24)	L5 AR-1248-4	0.000	5.802f	0	9617	N.D.	7.519 #
30)	L6 AR-1254-5	0.000	7.454	0	1763	N.D.	0.729 #
34)	L7 AR-1260-4	0.000	7.755	0	4648	N.D.	2.882 #
35)	L7 AR-1260-5	0.000	7.988	0	11041	N.D.	2.795 #
36)	L8 AR-1262-1	0.000	7.490	0	923	N.D.	0.405 #
37)	L8 AR-1262-2	0.000	7.988	0	11041	N.D.	2.684 #
38)	L8 AR-1262-3	0.000	8.283	0	14197	N.D.	8.907 #
39)	L8 AR-1262-4	0.000	8.350	0	6261	N.D.	2.000 #
40)	L8 AR-1262-5	0.000	8.839	0	4604	N.D.	3.263 #
41)	L9 AR-1268-1	0.000	8.283	0	14197	N.D.	2.884 #
42)	L9 AR-1268-2	0.000	8.350	0	6261	N.D.	1.288 #
43)	L9 AR-1268-3	0.000	8.554	0	1320	N.D.	0.317 #
44)	L9 AR-1268-4	0.000	8.839	0	4604	N.D.	2.763 #
45)	L9 AR-1268-5	0.000	9.131	0	241	N.D.	0.019 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031418.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 15:05
Operator : DD\AJ
Sample : L4804-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 17:36:56 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

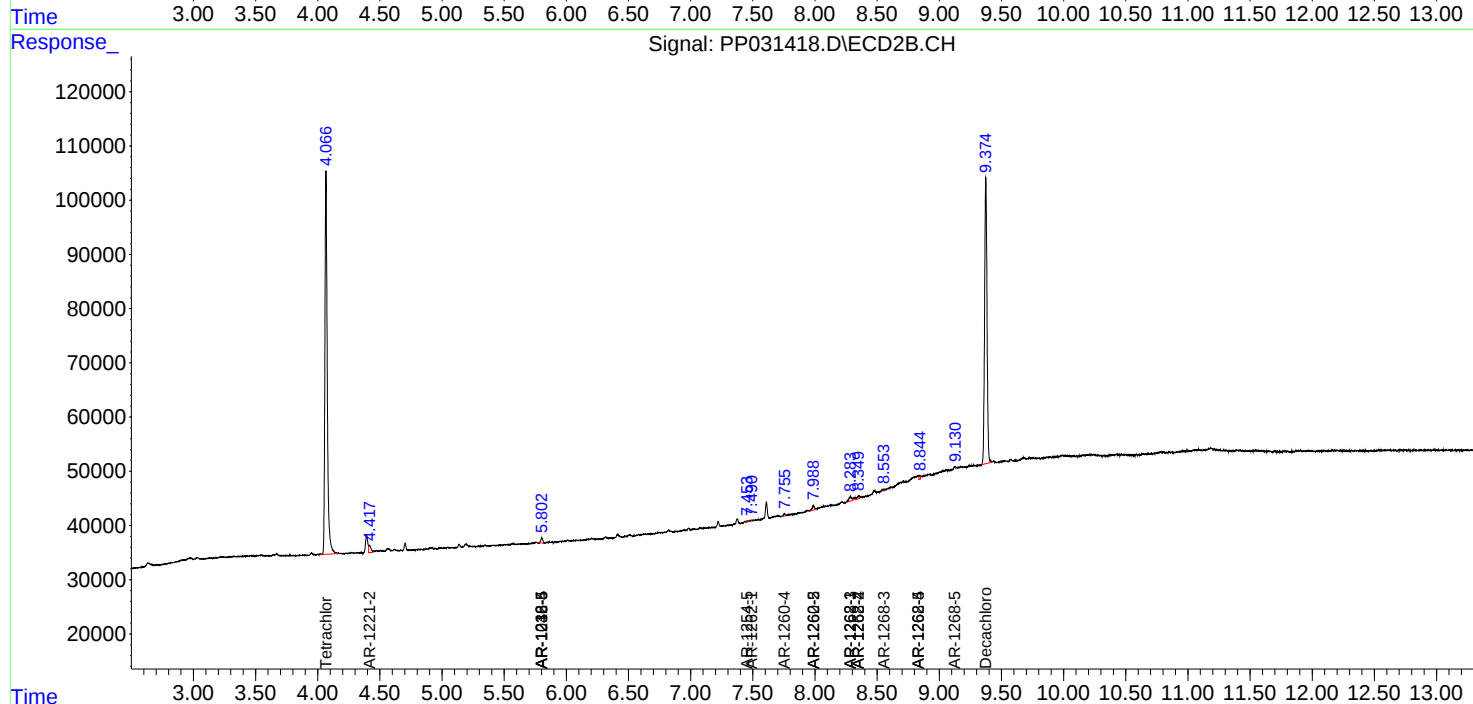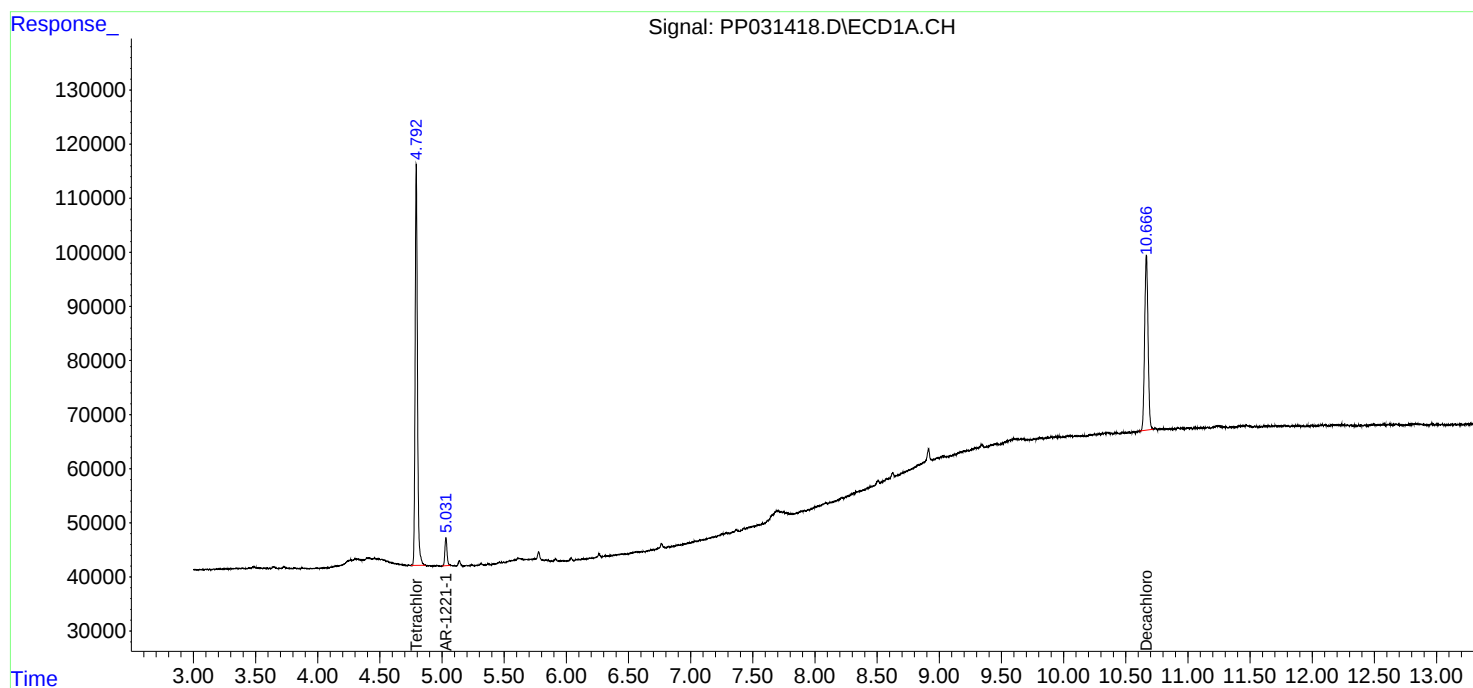


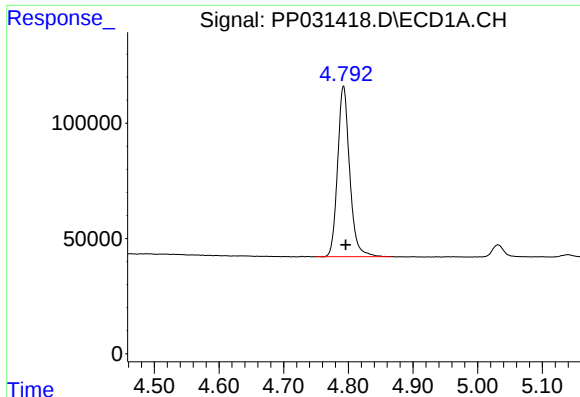

#1 Tetrachloro-m-xylene


R.T.: 4.793 min
Delta R.T.: -0.003 min
Response: 958534
Conc: 23.53 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

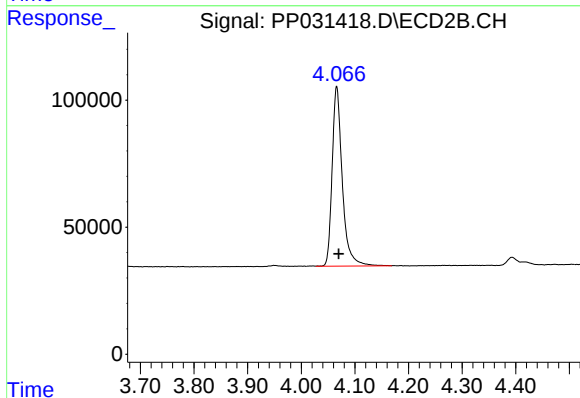


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: -0.004 min
Response: 928781
Conc: 22.22 ng/ml

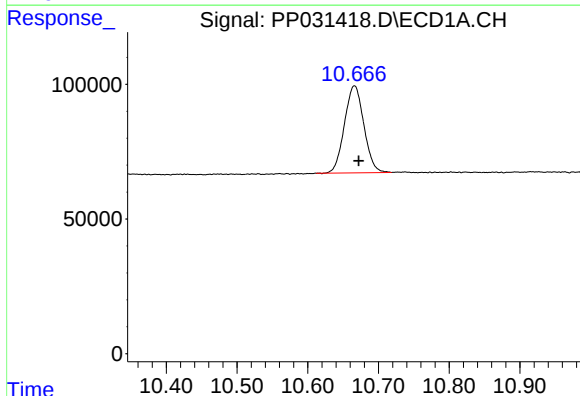


#2 Decachlorobiphenyl

R.T.: 10.666 min
Delta R.T.: -0.006 min
Response: 617448
Conc: 20.10 ng/ml

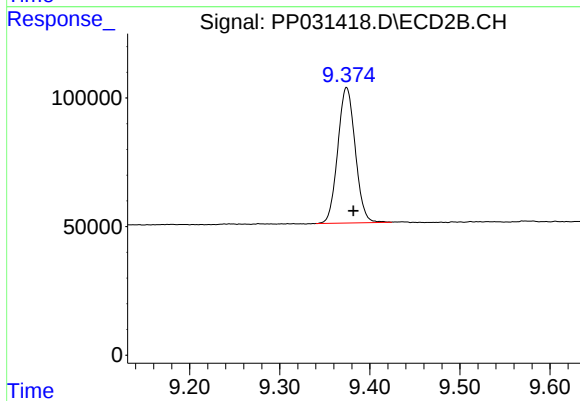

#2 Decachlorobiphenyl


R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 709857
Conc: 21.20 ng/ml

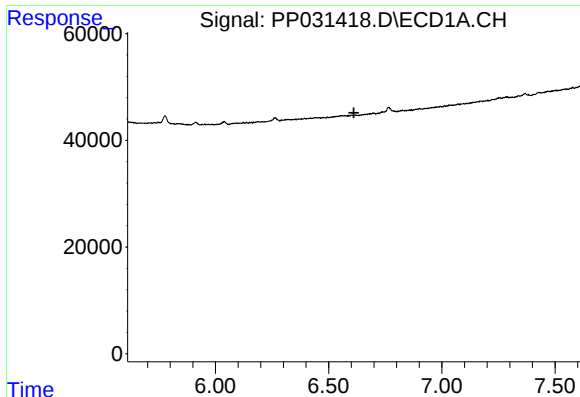

#7 AR-1016-5


R.T.: 0.000 min
Exp R.T.: 6.611 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

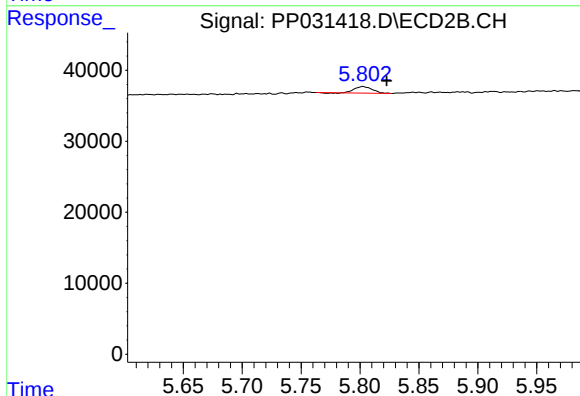


#7 AR-1016-5

R.T.: 5.802 min
Delta R.T.: -0.020 min
Response: 9617
Conc: 9.89 ng/ml

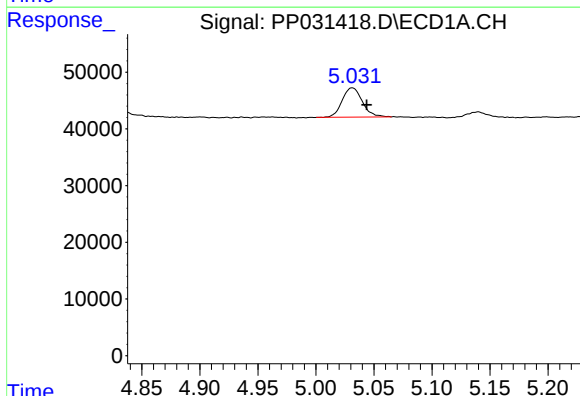


#8 AR-1221-1

R.T.: 5.031 min
Delta R.T.: -0.012 min
Response: 62449
Conc: 133.02 ng/ml

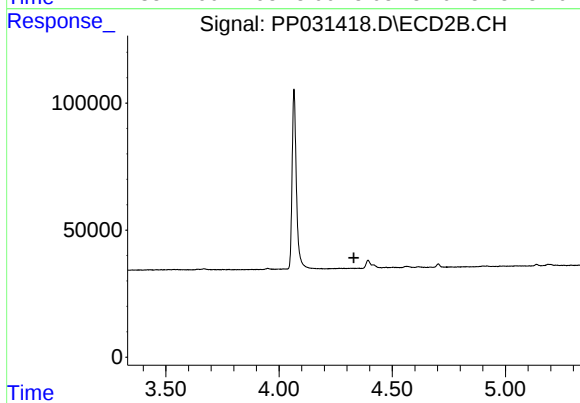

#8 AR-1221-1


R.T.: 0.000 min
Exp R.T.: 4.330 min
Response: 0
Conc: N.D.

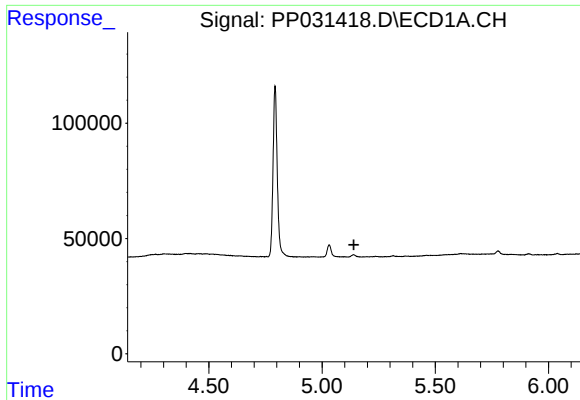

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T. : 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

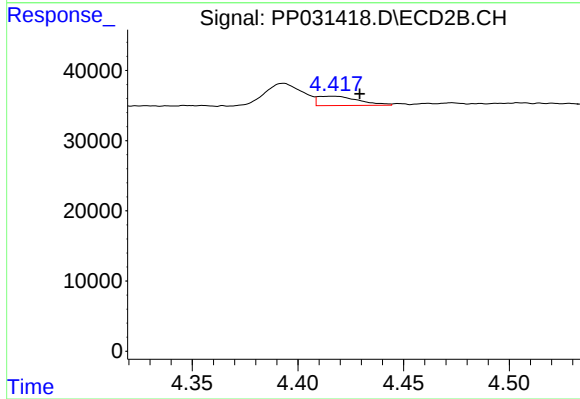


#9 AR-1221-2

R.T.: 4.417 min
Delta R.T.: -0.012 min
Response: 17645
Conc: 49.97 ng/ml

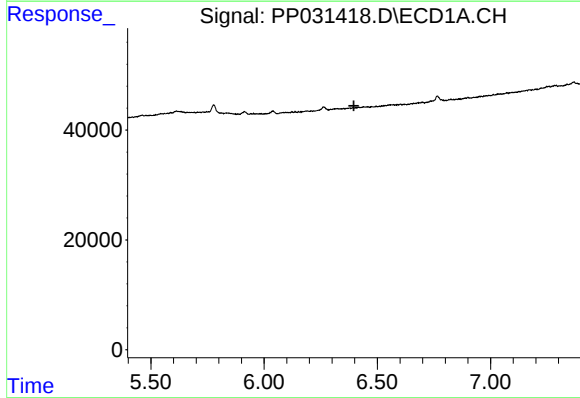


#15 AR-1232-5

R.T.: 0.000 min
Exp R.T. : 6.396 min
Response: 0
Conc: N.D.

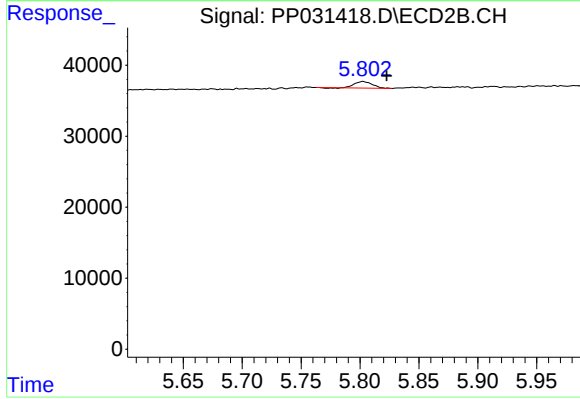

#15 AR-1232-5


R.T.: 5.802 min
Delta R.T.: -0.020 min
Response: 9617
Conc: 24.16 ng/ml

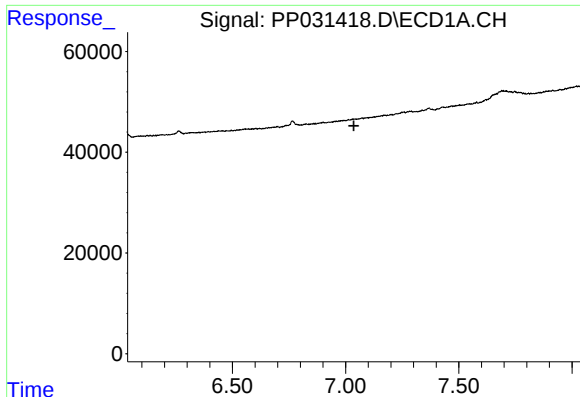

#24 AR-1248-4


R.T.: 0.000 min
Exp R.T. : 7.036 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

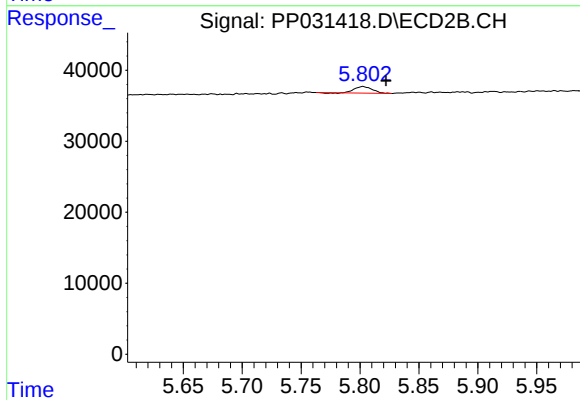


#24 AR-1248-4

R.T.: 5.802 min
Delta R.T.: -0.020 min
Response: 9617
Conc: 7.52 ng/ml

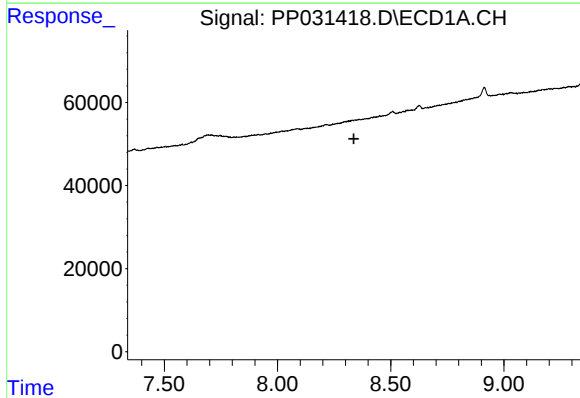


#30 AR-1254-5

R.T.: 0.000 min
Exp R.T. : 8.337 min
Response: 0
Conc: N.D.

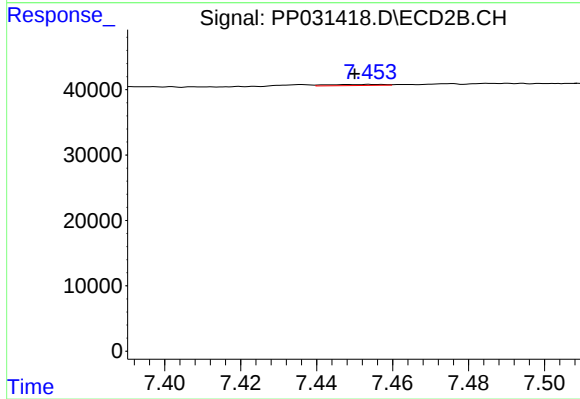

#30 AR-1254-5


R.T.: 7.454 min
Delta R.T.: 0.004 min
Response: 1763
Conc: 0.73 ng/ml

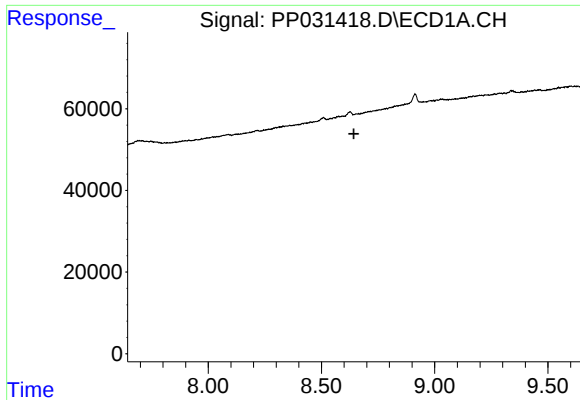

#34 AR-1260-4


R.T.: 0.000 min
Exp R.T.: 8.643 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

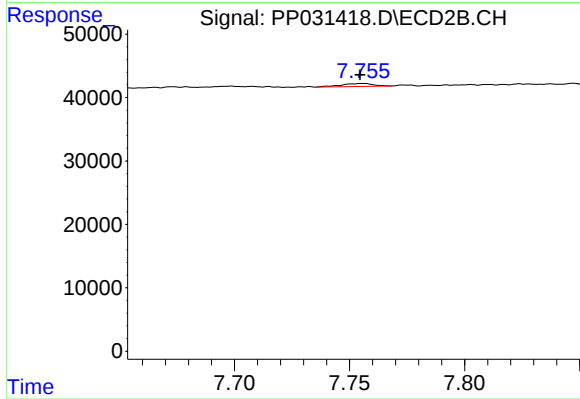


#34 AR-1260-4

R.T.: 7.755 min
Delta R.T.: 0.000 min
Response: 4648
Conc: 2.88 ng/ml

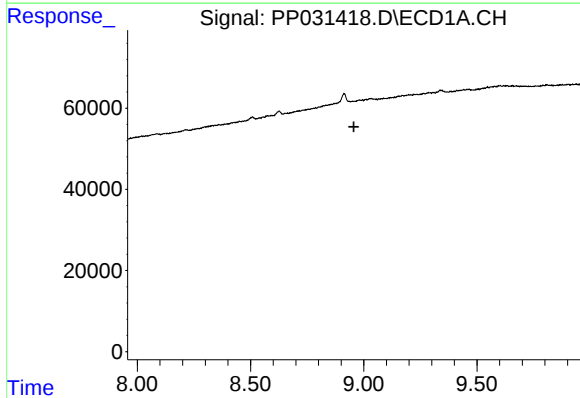


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.957 min
Response: 0
Conc: N.D.

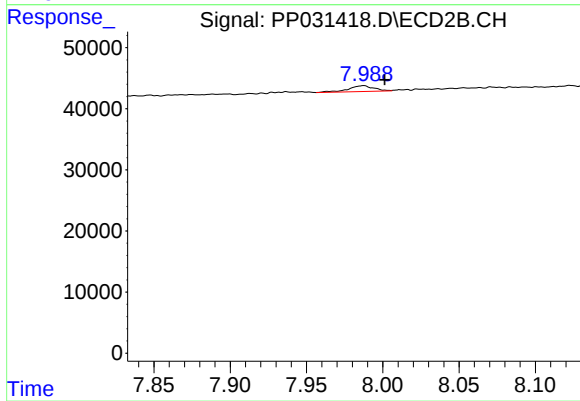

#35 AR-1260-5


R.T.: 7.988 min
Delta R.T.: -0.014 min
Response: 11041
Conc: 2.79 ng/ml

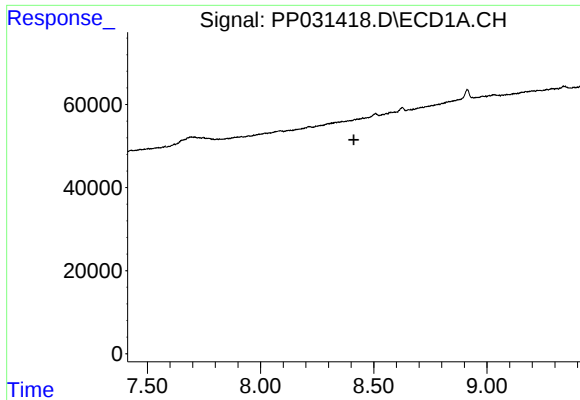

#36 AR-1262-1


R.T.: 0.000 min
Exp R.T. : 8.412 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

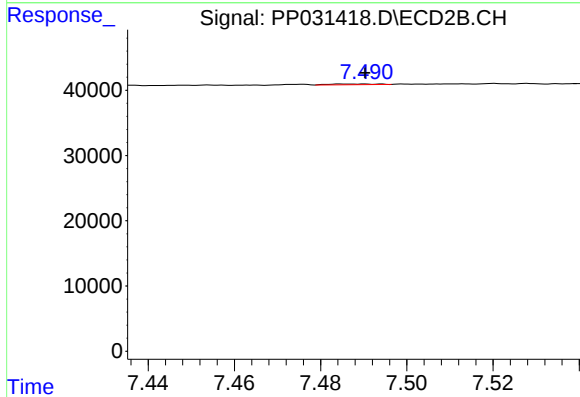


#36 AR-1262-1

R.T.: 7.490 min
Delta R.T.: 0.000 min
Response: 923
Conc: 0.41 ng/ml

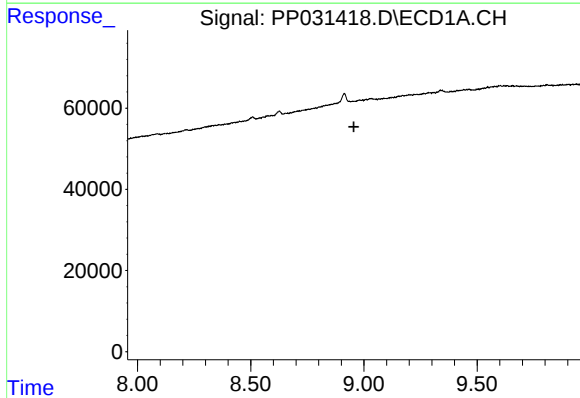


#37 AR-1262-2

R.T.: 0.000 min
Exp R.T. : 8.956 min
Response: 0
Conc: N.D.

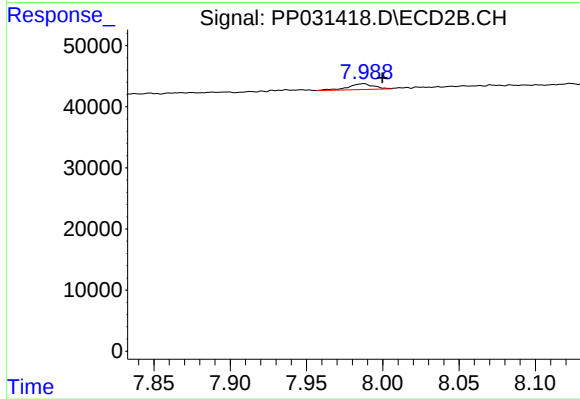

#37 AR-1262-2


R.T.: 7.988 min
Delta R.T.: -0.012 min
Response: 11041
Conc: 2.68 ng/ml

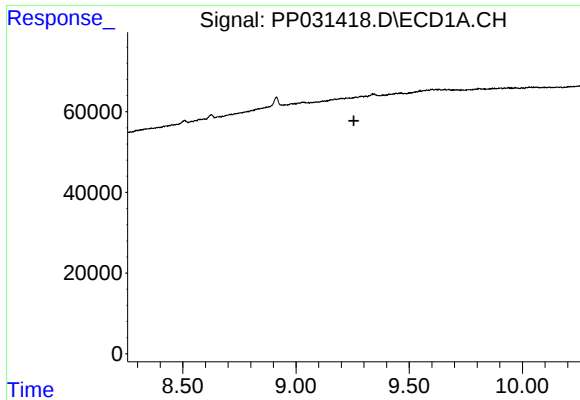

#38 AR-1262-3


R.T.: 0.000 min
Exp R.T. : 9.256 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

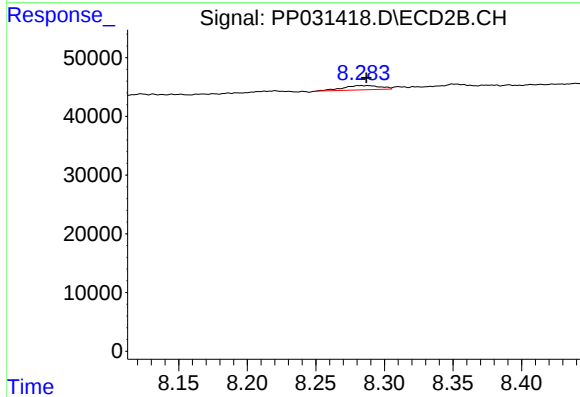


#38 AR-1262-3

R.T.: 8.283 min
Delta R.T.: -0.004 min
Response: 14197
Conc: 8.91 ng/ml

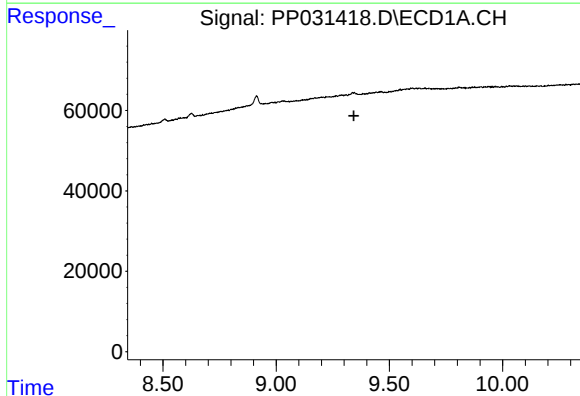


#39 AR-1262-4

R.T.: 0.000 min
Exp R.T. : 9.343 min
Response: 0
Conc: N.D.

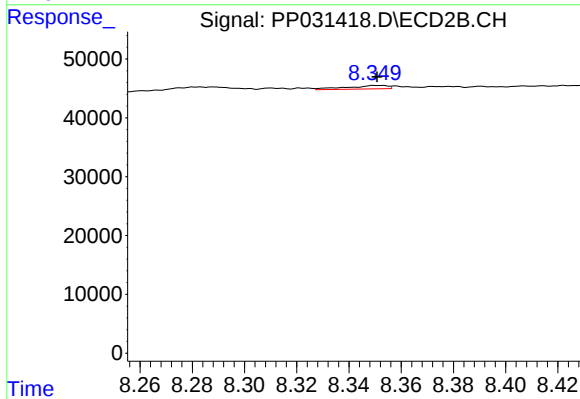

#39 AR-1262-4


R.T.: 8.350 min
Delta R.T.: -0.001 min
Response: 6261
Conc: 2.00 ng/ml

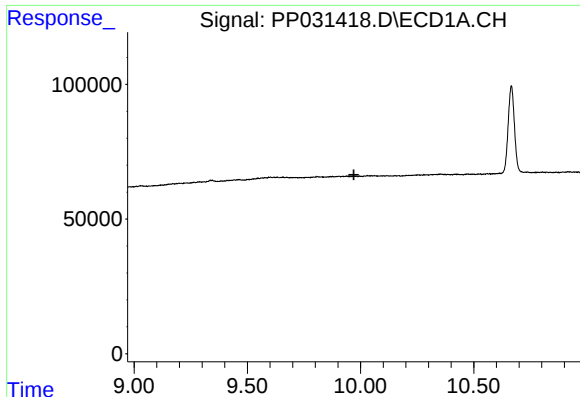

#40 AR-1262-5


R.T.: 0.000 min
Exp R.T. : 9.971 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

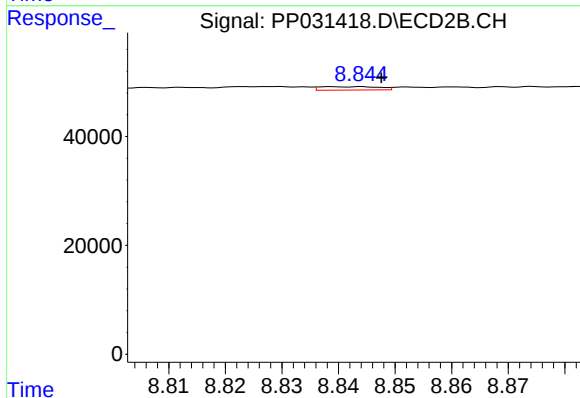


#40 AR-1262-5

R.T.: 8.839 min
Delta R.T.: -0.009 min
Response: 4604
Conc: 3.26 ng/ml

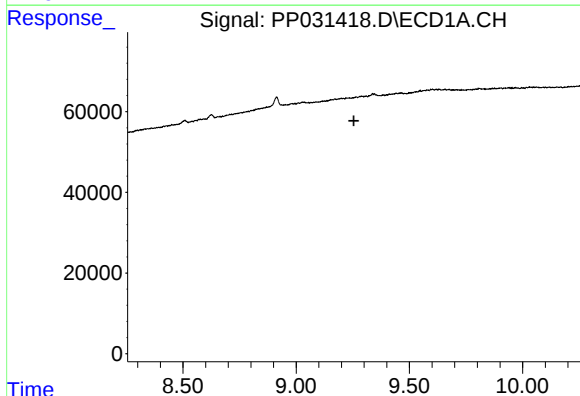


#41 AR-1268-1

R.T.: 0.000 min
Exp R.T. : 9.255 min
Response: 0
Conc: N.D.

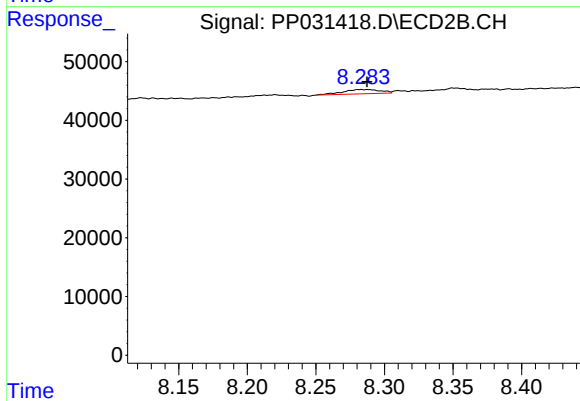

#41 AR-1268-1


R.T.: 8.283 min
Delta R.T.: -0.004 min
Response: 14197
Conc: 2.88 ng/ml

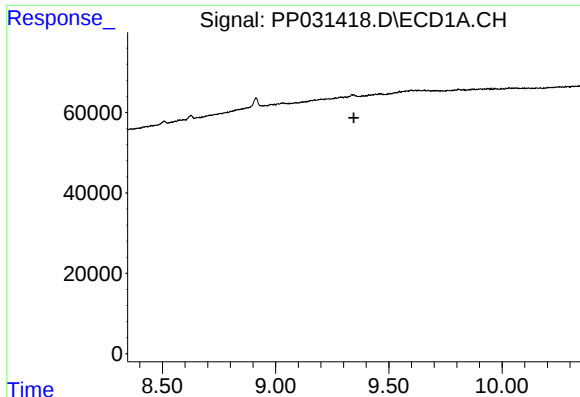

#42 AR-1268-2


R.T.: 0.000 min
Exp R.T.: 9.346 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

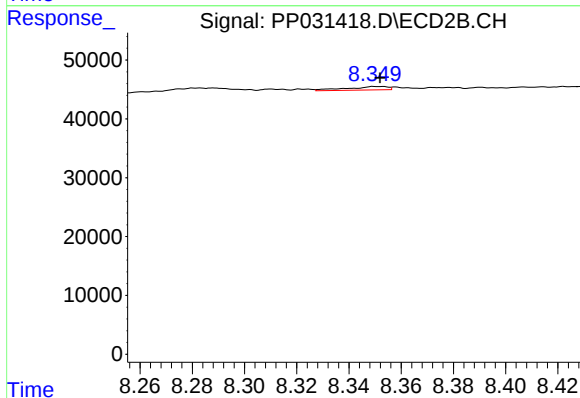


#42 AR-1268-2

R.T.: 8.350 min
Delta R.T.: -0.002 min
Response: 6261
Conc: 1.29 ng/ml

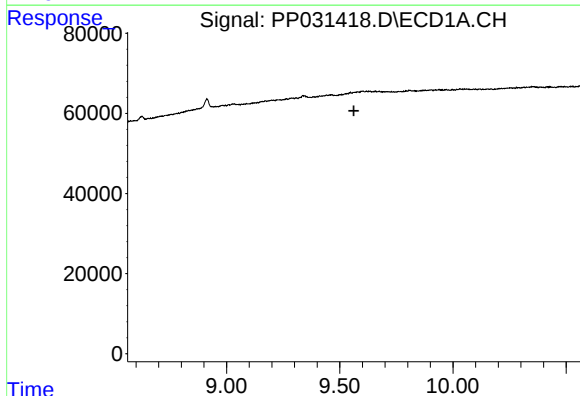


#43 AR-1268-3

R.T.: 0.000 min
Exp R.T.: 9.562 min
Response: 0
Conc: N.D.

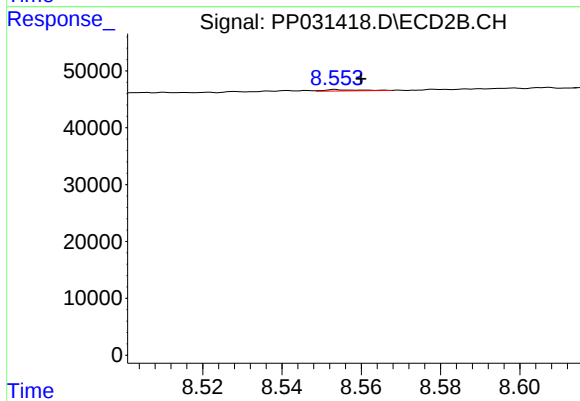

#43 AR-1268-3


R.T.: 8.554 min
Delta R.T.: -0.006 min
Response: 1320
Conc: 0.32 ng/ml

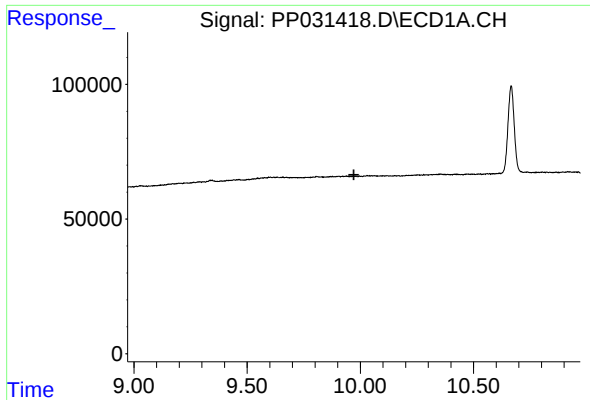

#44 AR-1268-4


R.T.: 0.000 min
Exp R.T. : 9.972 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-04-012-ABCD

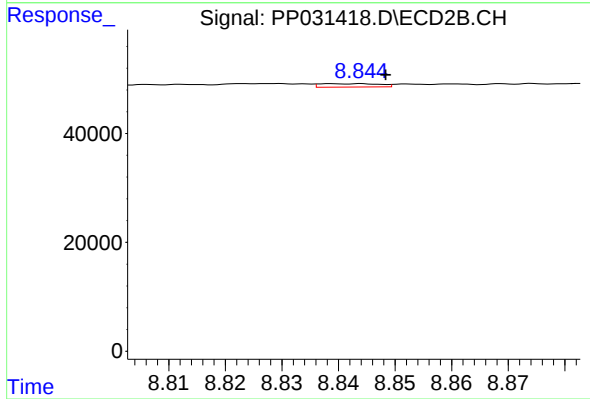


#44 AR-1268-4

R.T.: 8.839 min
Delta R.T.: -0.010 min
Response: 4604
Conc: 2.76 ng/ml

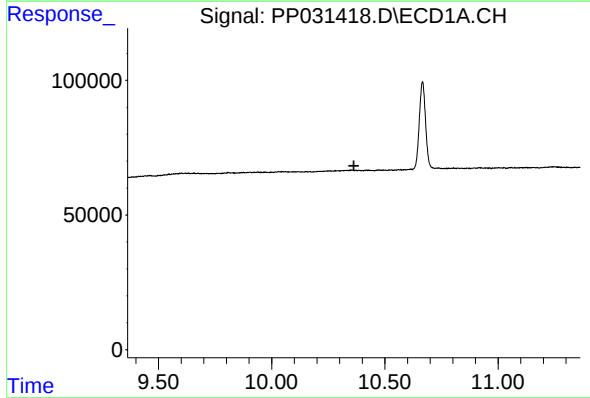

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T. : 10.363 min
Response: 0
Conc: N.D.

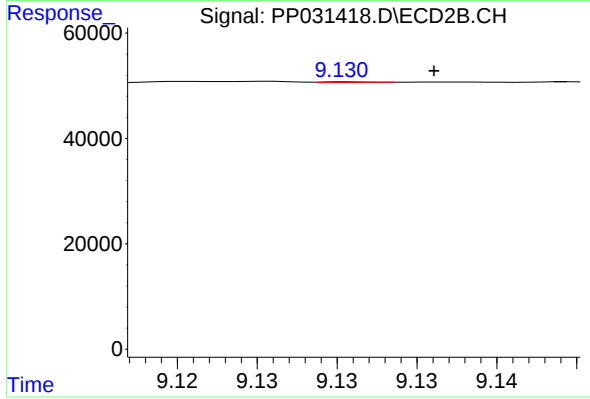

#45 AR-1268-5

R.T.: 9.131 min
Delta R.T.: -0.006 min
Response: 241
Conc: 0.02 ng/ml