

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
 Data File : PP031419.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Nov 2020 15:22
 Operator : DD\AJ
 Sample : L4803-01
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_P
 ClientSampleId :
 FK-BPM-01-C5-D5-C5A-D5A

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Nov 19 17:37:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
 Quant Title : GC EXTRACTABLES
 QLast Update : Wed Nov 18 01:50:50 2020
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	4.792	4.066	980553	943556	24.069	22.569
2)	SA Decachlor...	10.665	9.374	659670	759845	21.478	22.692
Target Compounds							
9)	L2 AR-1221-2	0.000	4.418	0	11556	N.D.	32.725 #
35)	L7 AR-1260-5	0.000	8.010	0	841	N.D.	0.213 #
37)	L8 AR-1262-2	0.000	8.010	0	841	N.D.	0.204 #
38)	L8 AR-1262-3	0.000	8.281	0	2963	N.D.	1.859 #
39)	L8 AR-1262-4	0.000	8.367f	0	3088	N.D.	0.986 #
40)	L8 AR-1262-5	0.000	8.847	0	1392	N.D.	0.987 #
41)	L9 AR-1268-1	0.000	8.281	0	2963	N.D.	0.602 #
42)	L9 AR-1268-2	0.000	8.367f	0	3088	N.D.	0.635 #
43)	L9 AR-1268-3	0.000	8.552	0	1690	N.D.	0.406 #
44)	L9 AR-1268-4	0.000	8.847	0	1392	N.D.	0.835 #
45)	L9 AR-1268-5	0.000	9.128	0	3980	N.D.	0.305 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_P\Data\PP111920\
Data File : PP031419.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Nov 2020 15:22
Operator : DD\AJ
Sample : L4803-01
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Nov 19 17:37:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_P\methods\PP111720.M
Quant Title : GC EXTRACTABLES
QLast Update : Wed Nov 18 01:50:50 2020
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Small noise peaks clipped

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30Mx0.32mmx 0.50µ Signal #2 Info : 30M x 0.32mm x 0.25µm

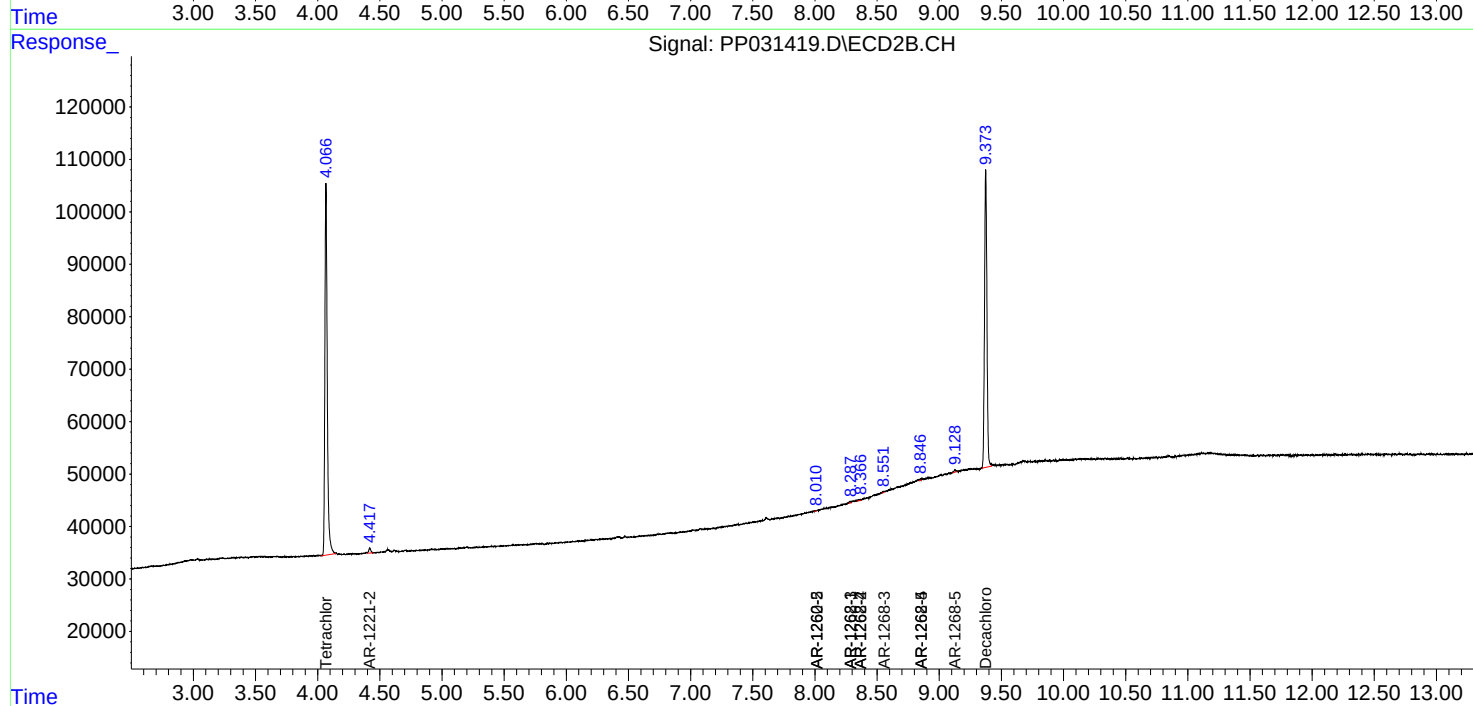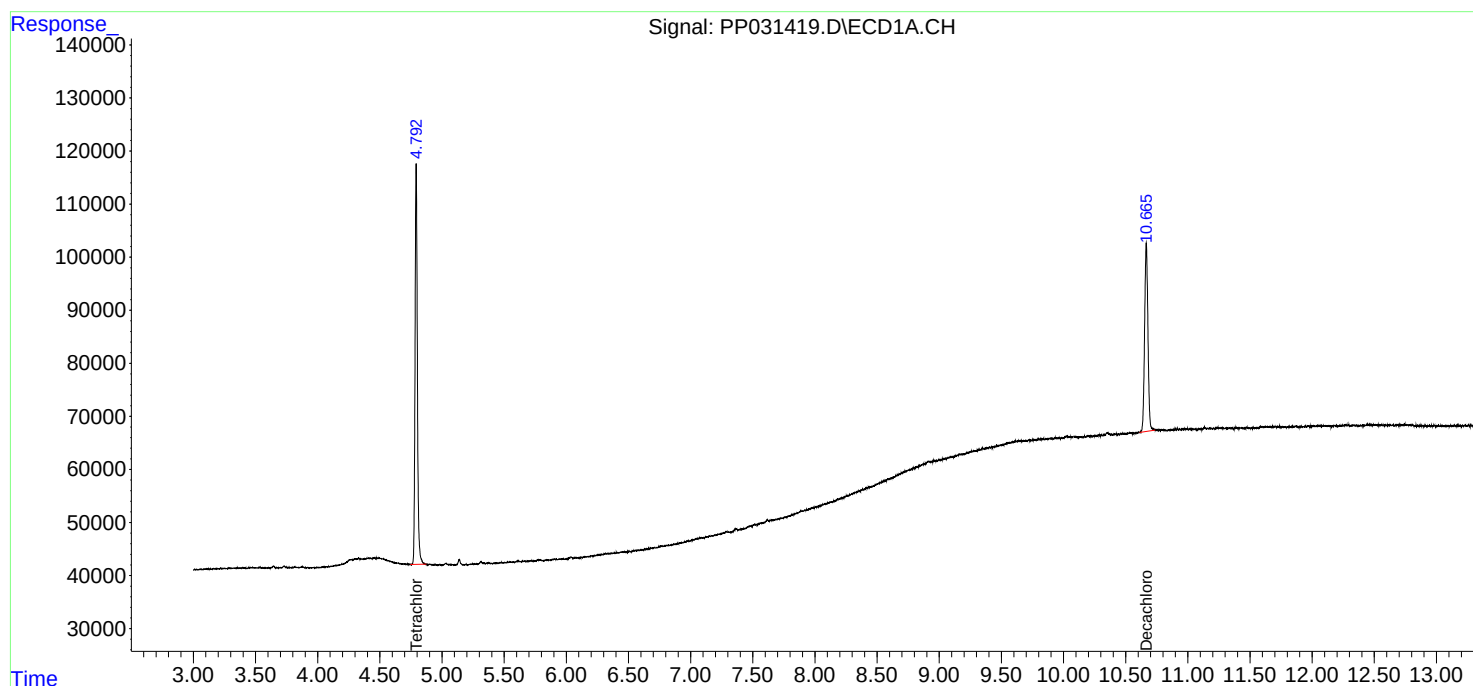


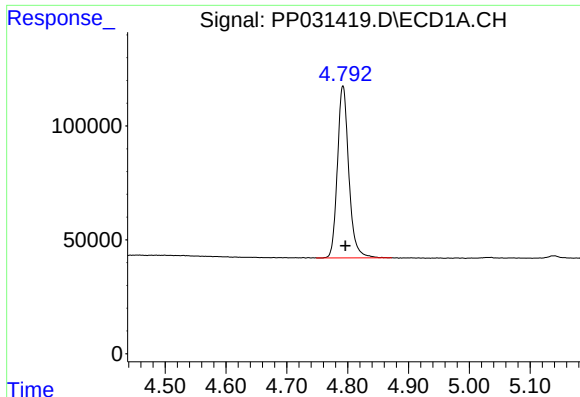

#1 Tetrachloro-m-xylene


R.T.: 4.792 min
Delta R.T.: -0.004 min
Response: 980553
Conc: 24.07 ng/ml

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

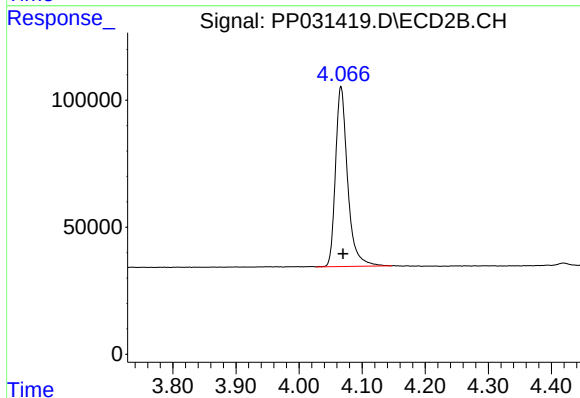


#1 Tetrachloro-m-xylene

R.T.: 4.066 min
Delta R.T.: -0.004 min
Response: 943556
Conc: 22.57 ng/ml

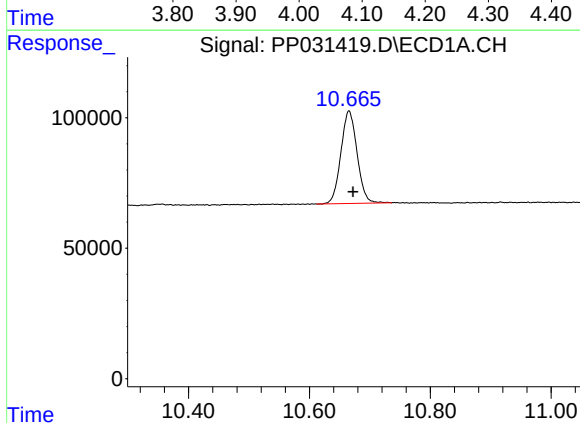


#2 Decachlorobiphenyl

R.T.: 10.665 min
Delta R.T.: -0.007 min
Response: 659670
Conc: 21.48 ng/ml

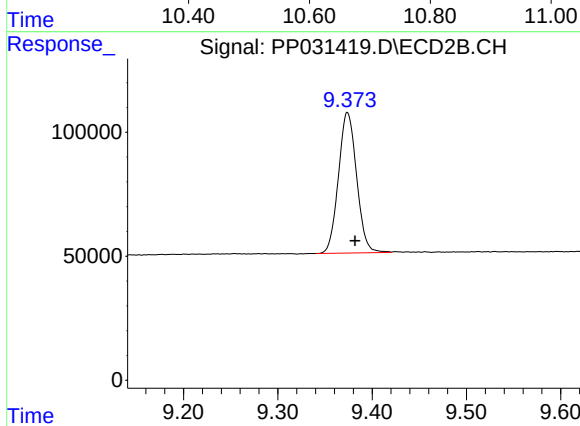

#2 Decachlorobiphenyl


R.T.: 9.374 min
Delta R.T.: -0.008 min
Response: 759845
Conc: 22.69 ng/ml

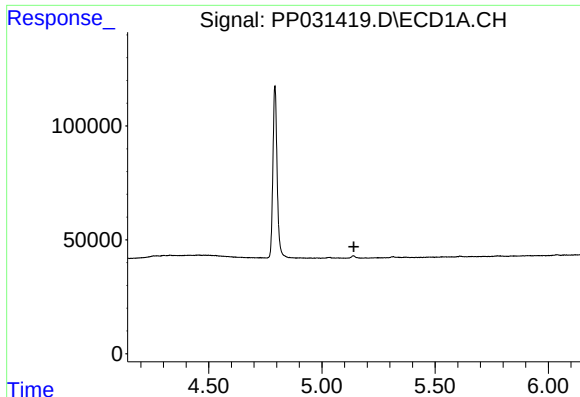

#9 AR-1221-2


R.T.: 0.000 min
Exp R.T.: 5.141 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

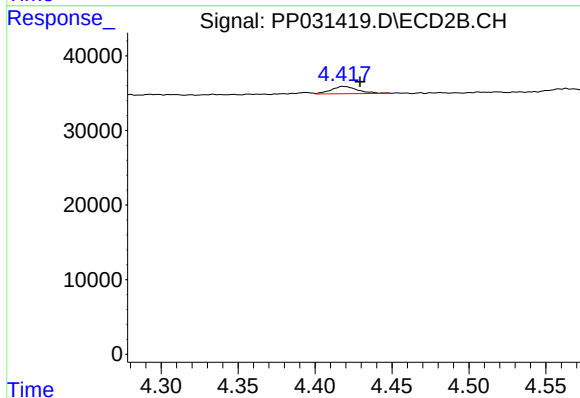


#9 AR-1221-2

R.T.: 4.418 min
Delta R.T.: -0.011 min
Response: 11556
Conc: 32.73 ng/ml

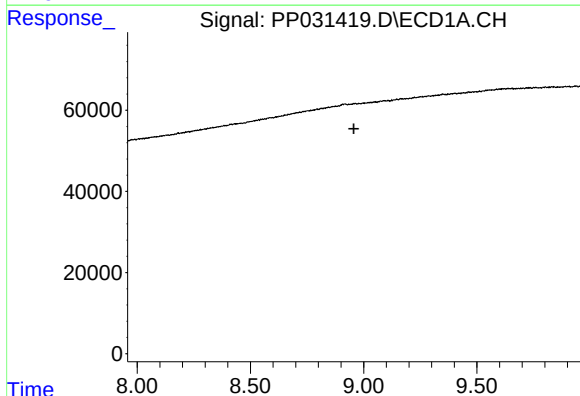


#35 AR-1260-5

R.T.: 0.000 min
Exp R.T.: 8.957 min
Response: 0
Conc: N.D.

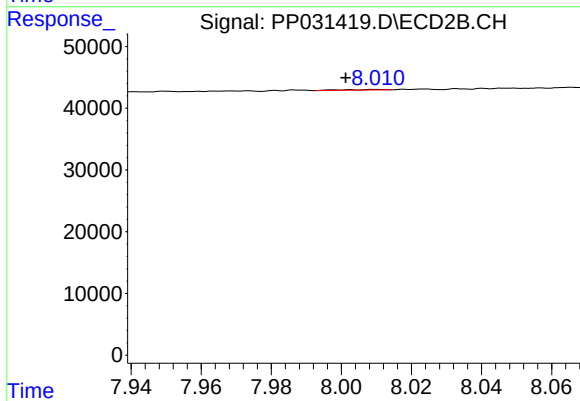

#35 AR-1260-5


R.T.: 8.010 min
Delta R.T.: 0.008 min
Response: 841
Conc: 0.21 ng/ml

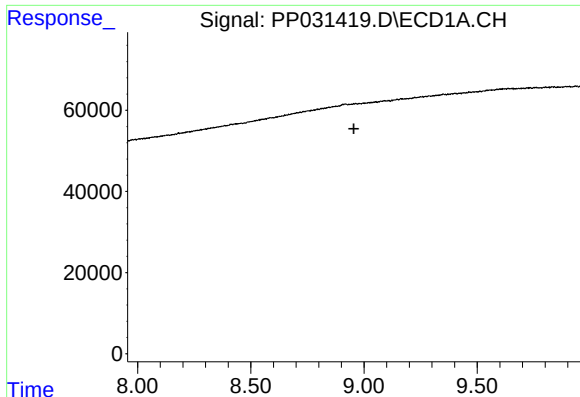

#37 AR-1262-2


R.T.: 0.000 min
Exp R.T.: 8.956 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

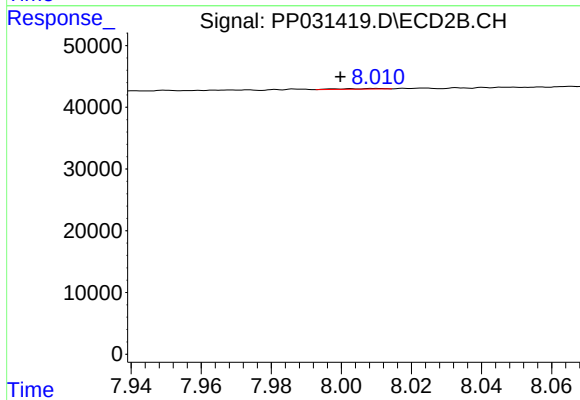


#37 AR-1262-2

R.T.: 8.010 min
Delta R.T.: 0.010 min
Response: 841
Conc: 0.20 ng/ml

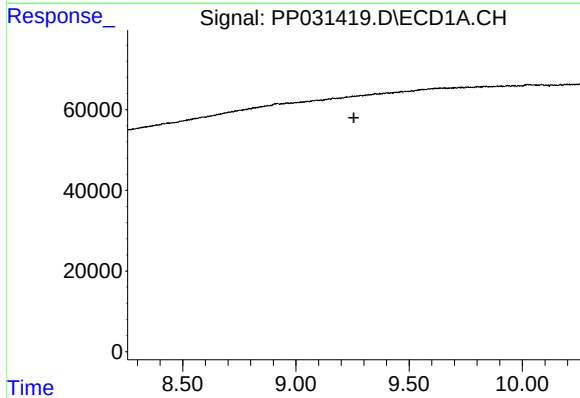


#38 AR-1262-3

R.T.: 0.000 min
Exp R.T.: 9.256 min
Response: 0
Conc: N.D.

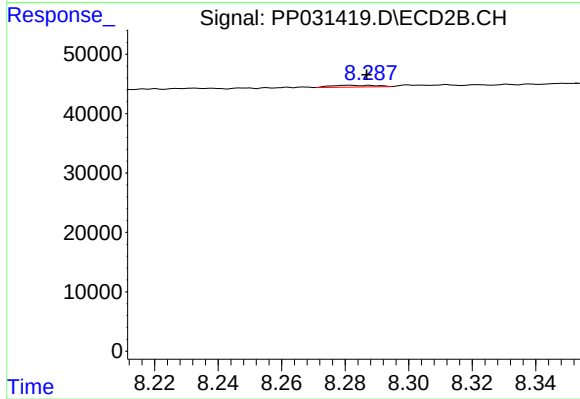

#38 AR-1262-3


R.T.: 8.281 min
Delta R.T.: -0.005 min
Response: 2963
Conc: 1.86 ng/ml

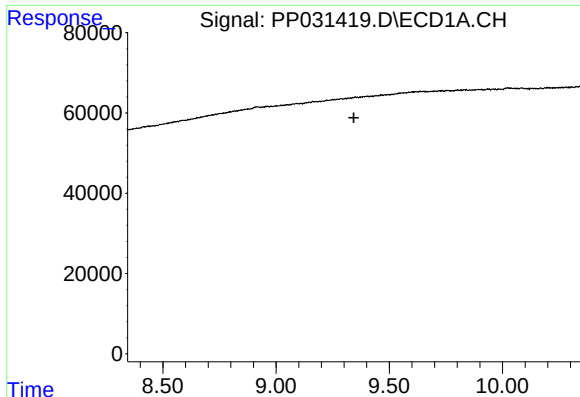

#39 AR-1262-4


R.T.: 0.000 min
Exp R.T.: 9.343 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

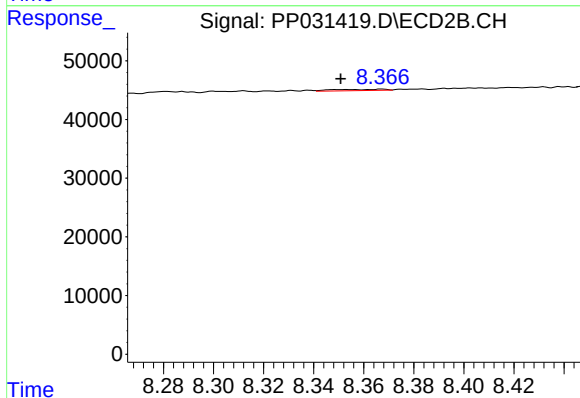


#39 AR-1262-4

R.T.: 8.367 min
Delta R.T.: 0.016 min
Response: 3088
Conc: 0.99 ng/ml

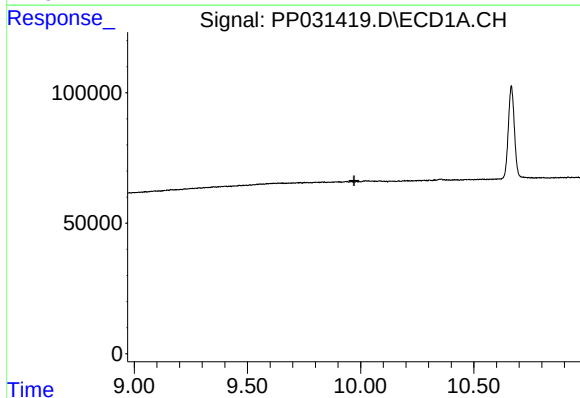


#40 AR-1262-5

R.T.: 0.000 min
Exp R.T.: 9.971 min
Response: 0
Conc: N.D.

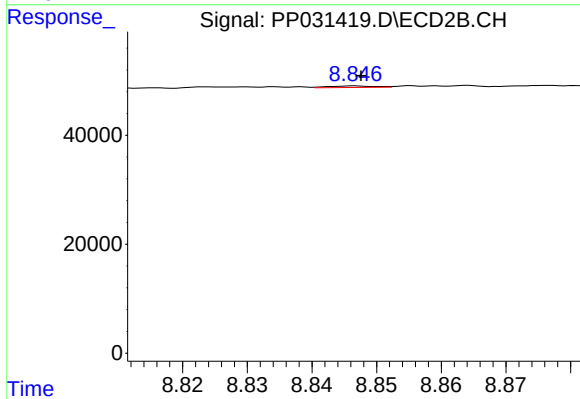

#40 AR-1262-5


R.T.: 8.847 min
Delta R.T.: 0.000 min
Response: 1392
Conc: 0.99 ng/ml

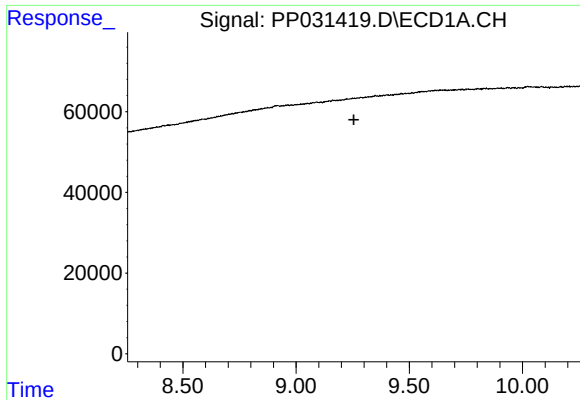

#41 AR-1268-1


R.T.: 0.000 min
Exp R.T.: 9.255 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

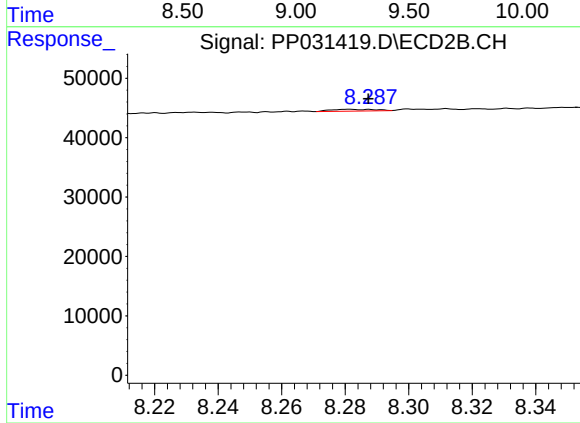


#41 AR-1268-1

R.T.: 8.281 min
Delta R.T.: -0.006 min
Response: 2963
Conc: 0.60 ng/ml

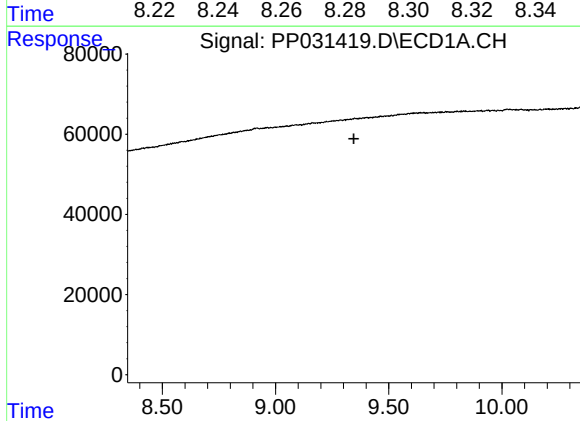


#42 AR-1268-2

R.T.: 0.000 min
Exp R.T.: 9.346 min
Response: 0
Conc: N.D.

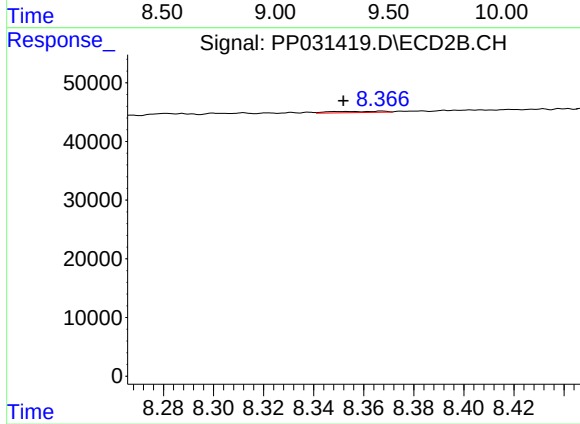

#42 AR-1268-2


R.T.: 8.367 min
Delta R.T.: 0.015 min
Response: 3088
Conc: 0.64 ng/ml

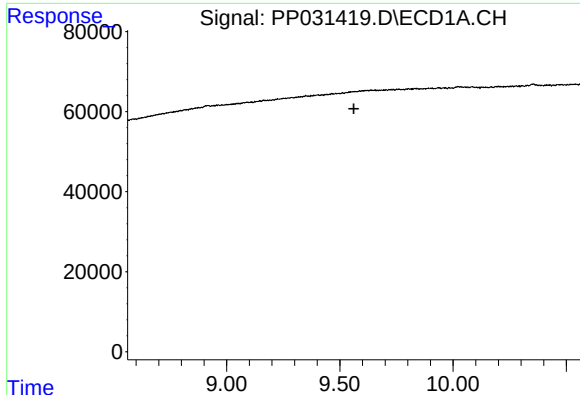

#43 AR-1268-3


R.T.: 0.000 min
Exp R.T.: 9.562 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

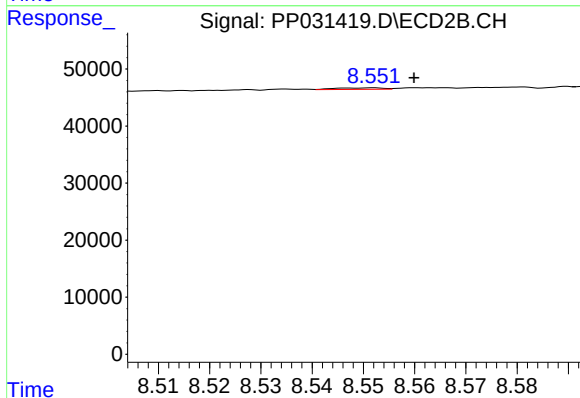


#43 AR-1268-3

R.T.: 8.552 min
Delta R.T.: -0.008 min
Response: 1690
Conc: 0.41 ng/ml

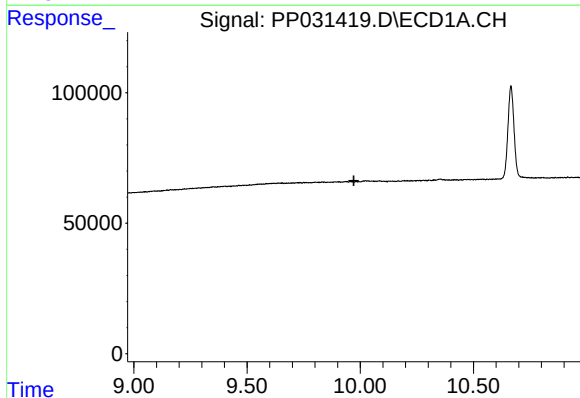


#44 AR-1268-4

R.T.: 0.000 min
Exp R.T.: 9.972 min
Response: 0
Conc: N.D.

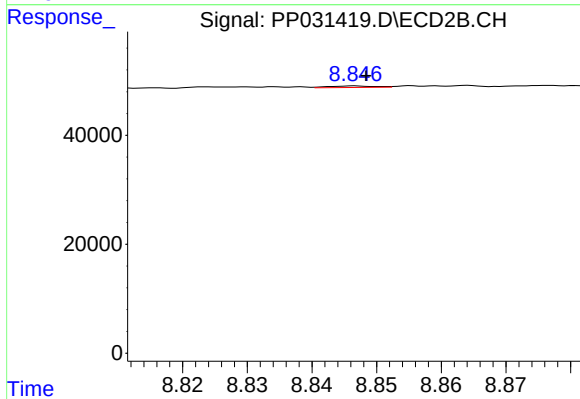

#44 AR-1268-4


R.T.: 8.847 min
Delta R.T.: -0.002 min
Response: 1392
Conc: 0.84 ng/ml

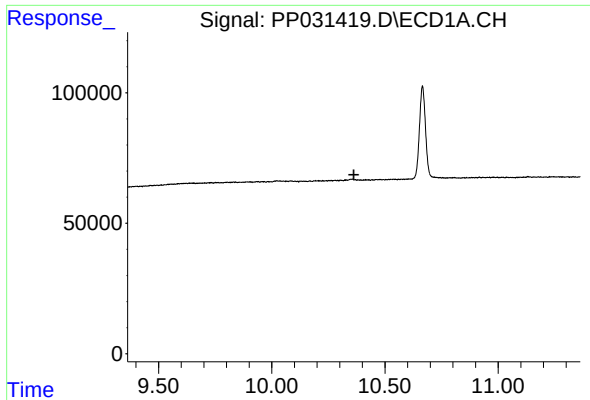

#45 AR-1268-5

R.T.: 0.000 min
Exp R.T.: 10.363 min
Response: 0
Conc: N.D.

Instrument :
ECD_P
ClientSampleId :
FK-BPM-01-C5-D5-C5A-D5A

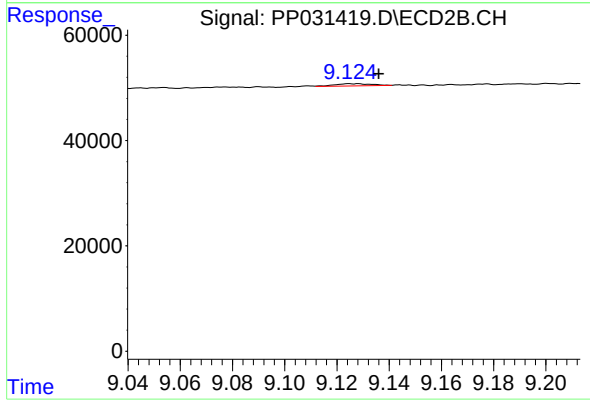

#45 AR-1268-5

R.T.: 9.128 min
Delta R.T.: -0.008 min
Response: 3980
Conc: 0.30 ng/ml